

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022522\
 Data File : BN018724.D
 Acq On : 25 Feb 2022 11:07
 Operator : CG/JU
 Sample : PB142906BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK906

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN021622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN018724.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.017	3	5	18	rVB	79857	124638	2.00%	0.190%
2	3.281	46	50	58	rVB	76029	110310	1.77%	0.168%
3	3.699	117	121	140	rBV	965573	1522458	24.45%	2.324%
4	4.058	177	182	186	rVB	17535	26447	0.42%	0.040%
5	7.058	684	692	706	rBV	1153048	1824950	29.31%	2.786%
6	7.234	715	722	731	rBV	900982	1455958	23.38%	2.223%
7	7.434	748	756	767	rBV	1147843	1840389	29.55%	2.810%
8	7.910	830	837	845	rBV	920528	1468575	23.58%	2.242%
9	8.610	948	956	970	rBV	1408093	2215936	35.58%	3.383%
10	9.063	1024	1033	1042	rBV	1065403	1737964	27.91%	2.653%
11	9.793	1149	1157	1170	rBV	889313	1423651	22.86%	2.174%
12	10.334	1241	1249	1260	rBV	1346112	2243723	36.03%	3.426%
13	10.716	1307	1314	1323	rBV	1269779	2123444	34.10%	3.242%
14	10.846	1328	1336	1354	rVV	1367045	2297112	36.89%	3.507%
15	12.304	1579	1584	1590	rVB	23739	36826	0.59%	0.056%
16	13.945	1857	1863	1870	rBV	2370991	3369156	54.10%	5.144%
17	13.992	1870	1871	1875	rVB4	7334	6405	0.10%	0.010%
18	14.239	1906	1913	1928	rBV	2784978	4031148	64.73%	6.154%
19	14.545	1958	1965	1972	rBV	1952056	2828918	45.43%	4.319%
20	14.722	1988	1995	2014	rBV	1004566	1438490	23.10%	2.196%
21	14.945	2030	2033	2040	rVB6	4466	7616	0.12%	0.012%
22	15.534	2126	2133	2146	rBV	3434191	4949698	79.48%	7.557%
23	15.639	2146	2151	2166	rVV	973555	1338001	21.49%	2.043%
24	15.775	2170	2174	2180	rVB2	18465	27110	0.44%	0.041%
25	16.175	2235	2242	2245	rBV3	8937	11252	0.18%	0.017%
26	16.245	2250	2254	2258	rVB3	8552	11522	0.19%	0.018%
27	16.310	2263	2265	2271	rVB5	4291	6865	0.11%	0.010%
28	16.569	2305	2309	2314	rVB4	7041	10310	0.17%	0.016%
29	16.628	2314	2319	2323	rBV3	15852	21425	0.34%	0.033%
30	16.681	2323	2328	2332	rVB2	13294	17682	0.28%	0.027%
31	17.069	2387	2394	2400	rVB2	8715	14508	0.23%	0.022%
32	17.286	2424	2431	2441	rBV	2216917	3327833	53.44%	5.081%
33	17.380	2441	2447	2460	rBV	3790928	5440505	87.36%	8.306%
34	19.239	2758	2763	2769	rBV	45276	60780	0.98%	0.093%
35	19.310	2770	2775	2783	rVV	43930	61034	0.98%	0.093%
36	19.674	2831	2837	2849	rBV	4689364	6227414	100.00%	9.508%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022522\
Data File : BN018724.D
Acq On : 25 Feb 2022 11:07
Operator : CG/JU
Sample : PB142906BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK906

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN021622.M
Title : SVOA CALIBRATION

37	21.463	3135	3141	3154	rBV	2721908	3365313	54.04%	5.138%
38	23.710	3514	3523	3540	rBV	2672938	5366962	86.18%	8.194%
39	23.863	3541	3549	3567	rVB	1545955	3107391	49.90%	4.744%


Sum of corrected areas: 65499719

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022522\
Data File : BN018724.D
Acq On : 25 Feb 2022 11:07
Operator : CG/JU
Sample : PB142906BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK906

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN021622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

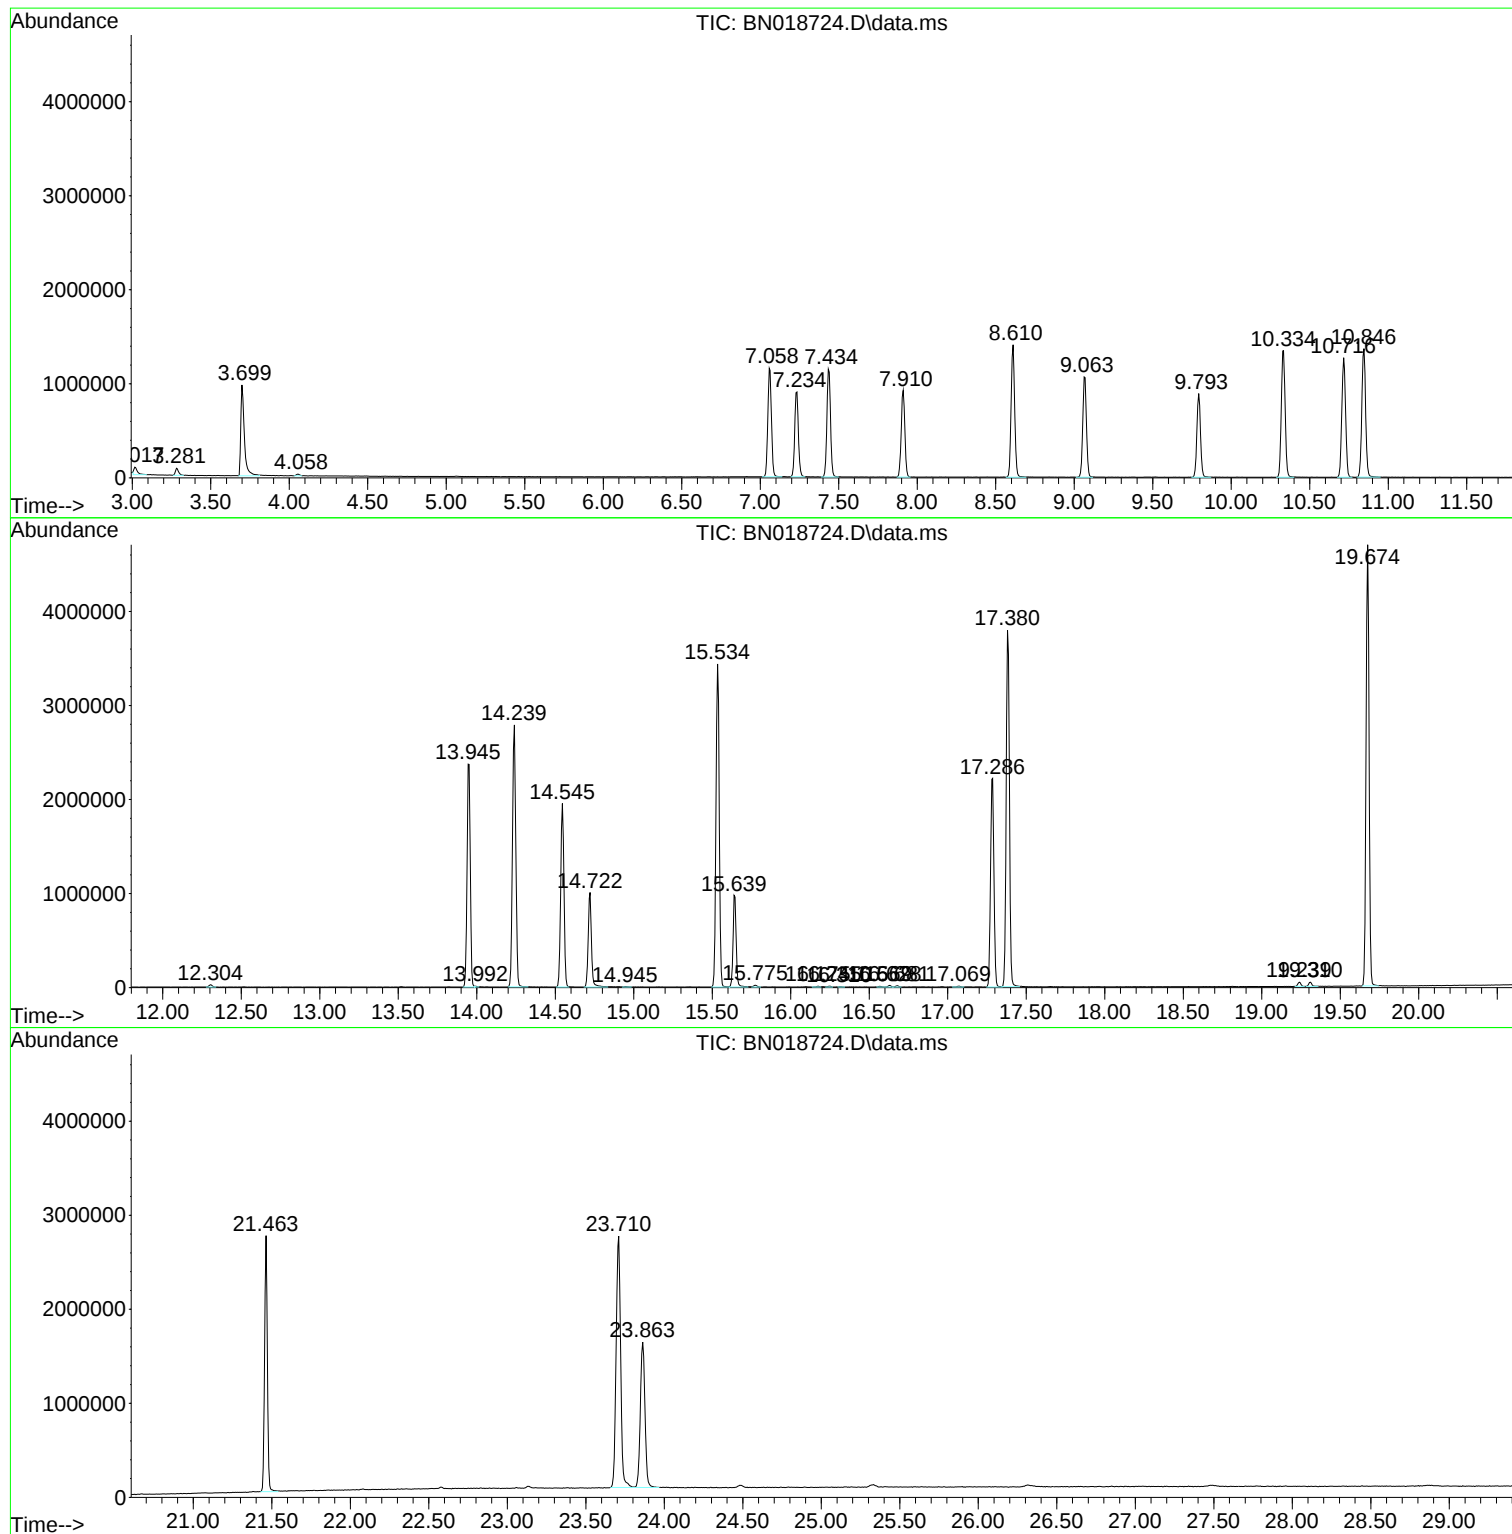

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022522\
Data File : BN018724.D
Acq On : 25 Feb 2022 11:07
Operator : CG/JU
Sample : PB142906BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK906

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN021622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022522\
Data File : BN018724.D
Acq On : 25 Feb 2022 11:07
Operator : CG/JU
Sample : PB142906BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK906

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN021622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc