

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022522\
 Data File : BN018741.D
 Acq On : 25 Feb 2022 21:52
 Operator : CG/JU
 Sample : PB142928BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK928

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN021622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN018741.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.017	3	5	11	rVB	46463	57861	1.14%	0.104%
2	3.281	46	50	59	rVB	65390	92423	1.82%	0.166%
3	3.699	117	121	139	rBV	845387	1259514	24.85%	2.263%
4	4.058	178	182	188	rVB	17165	27478	0.54%	0.049%
5	7.063	686	693	707	rVB	979233	1559056	30.76%	2.801%
6	7.234	715	722	733	rVB	754992	1227034	24.21%	2.204%
7	7.434	749	756	766	rBV	980994	1573354	31.04%	2.827%
8	7.910	829	837	845	rBV	933669	1458449	28.77%	2.620%
9	8.610	949	956	970	rBV	1206681	1891023	37.31%	3.397%
10	9.069	1026	1034	1043	rBV	905960	1475999	29.12%	2.652%
11	9.793	1150	1157	1171	rBV	764653	1225071	24.17%	2.201%
12	10.334	1241	1249	1261	rBV	1148759	1922013	37.92%	3.453%
13	10.716	1306	1314	1325	rVB	1227627	2085284	41.14%	3.746%
14	10.846	1327	1336	1351	rBV	1135231	1938178	38.24%	3.482%
15	12.304	1579	1584	1590	rBV2	19517	32691	0.64%	0.059%
16	13.516	1785	1790	1796	rVB6	4044	6823	0.13%	0.012%
17	13.945	1857	1863	1870	rBV	1976956	2809851	55.43%	5.048%
18	14.240	1906	1913	1922	rBV	2302844	3359771	66.28%	6.036%
19	14.545	1958	1965	1973	rBV	1891499	2740998	54.08%	4.924%
20	14.722	1987	1995	2009	rBV	814126	1201688	23.71%	2.159%
21	14.951	2030	2034	2039	rVB6	2755	5086	0.10%	0.009%
22	15.534	2126	2133	2144	rBV	2896436	4106810	81.02%	7.378%
23	15.645	2144	2152	2161	rBV	812708	1121219	22.12%	2.014%
24	15.769	2169	2173	2183	rVB	15260	22098	0.44%	0.040%
25	17.075	2390	2395	2401	rVB	8922	13724	0.27%	0.025%
26	17.281	2424	2430	2439	rBV	2145386	3123380	61.62%	5.611%
27	17.381	2441	2447	2462	rBV2	3095909	4510997	89.00%	8.104%
28	19.239	2758	2763	2768	rBV2	36875	54200	1.07%	0.097%
29	19.310	2770	2775	2779	rVV	37254	47671	0.94%	0.086%
30	19.675	2830	2837	2850	rBV	3675486	5068762	100.00%	9.106%
31	21.463	3135	3141	3152	rBV	2304637	2970612	58.61%	5.337%
32	23.704	3514	3522	3530	rBV2	2032199	4029528	79.50%	7.239%
33	23.863	3541	3549	3562	rVB2	1248212	2643384	52.15%	4.749%




Sum of corrected areas: 55662030

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022522\
Data File : BN018741.D
Acq On : 25 Feb 2022 21:52
Operator : CG/JU
Sample : PB142928BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK928

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN021622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

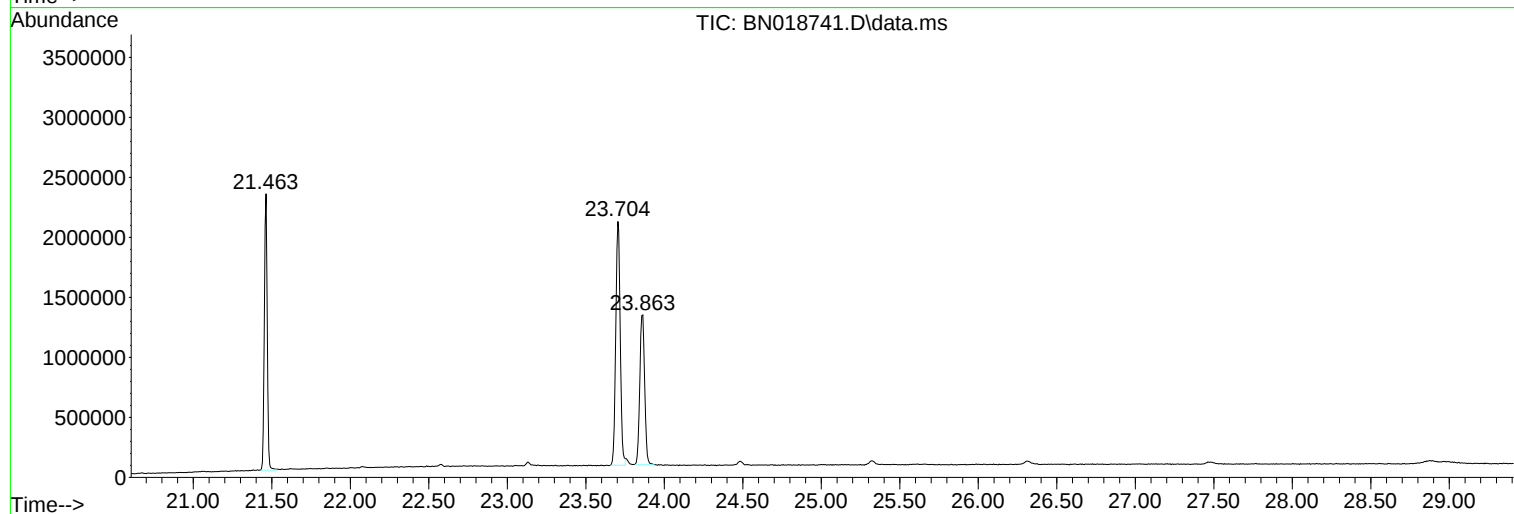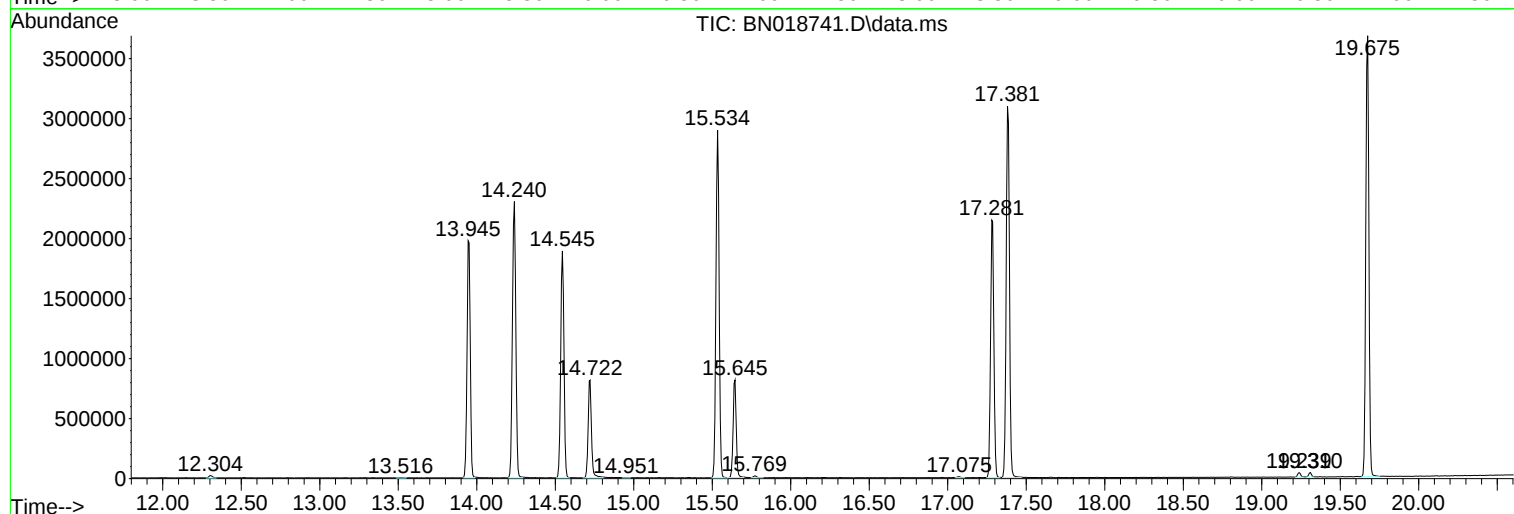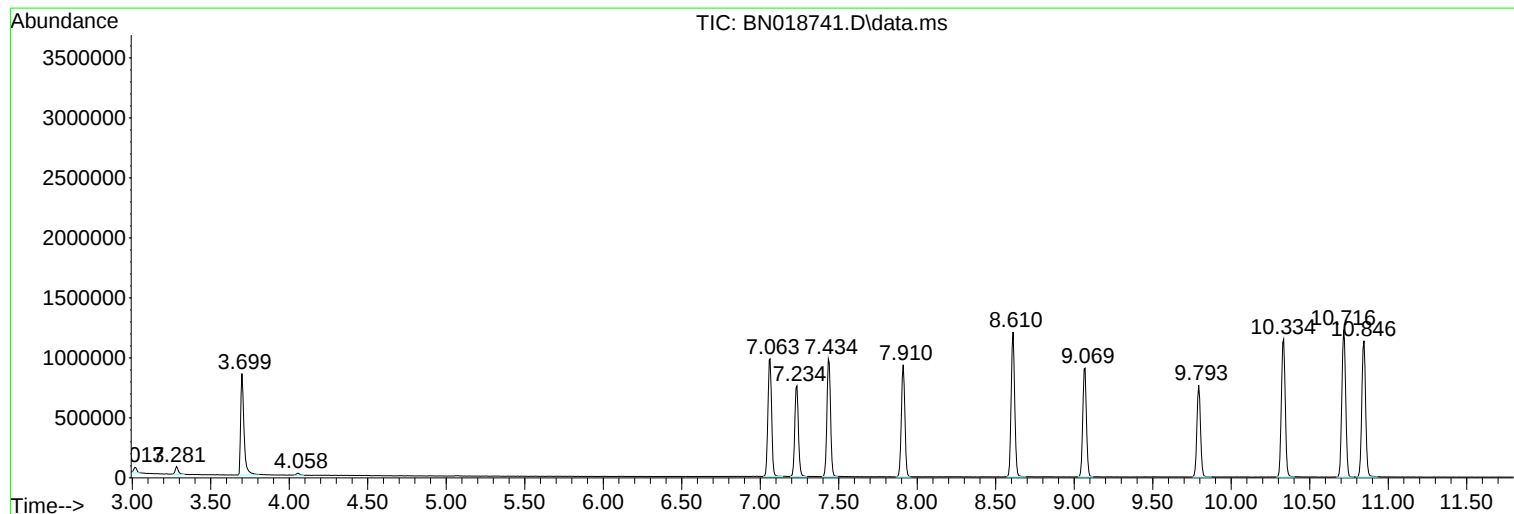

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022522\
Data File : BN018741.D
Acq On : 25 Feb 2022 21:52
Operator : CG/JU
Sample : PB142928BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK928

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN021622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022522\
Data File : BN018741.D
Acq On : 25 Feb 2022 21:52
Operator : CG/JU
Sample : PB142928BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK928

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN021622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc