

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022522\
 Data File : BN018742.D
 Acq On : 25 Feb 2022 22:28
 Operator : CG/JU
 Sample : PB142930BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK930

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN021622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN018742.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.017	3	5	17	rVB	50873	71854	1.47%	0.134%
2	3.281	46	50	59	rVB	68546	93614	1.92%	0.174%
3	3.699	117	121	143	rBV	861760	1284825	26.33%	2.389%
4	4.052	178	181	188	rVB	16191	23934	0.49%	0.045%
5	7.058	685	692	701	rBV	1000826	1579853	32.38%	2.938%
6	7.228	715	721	734	rVB	773501	1252901	25.68%	2.330%
7	7.434	748	756	767	rBV	1013971	1600024	32.80%	2.975%
8	7.911	830	837	845	rBV	843423	1335001	27.36%	2.482%
9	8.611	948	956	967	rBV	1202506	1906366	39.07%	3.545%
10	9.069	1026	1034	1043	rBV	902021	1487519	30.49%	2.766%
11	9.793	1149	1157	1168	rBV	763719	1221405	25.04%	2.271%
12	10.334	1239	1249	1266	rBV	1155036	1946938	39.91%	3.620%
13	10.716	1307	1314	1325	rBV	1145893	1908654	39.12%	3.549%
14	10.846	1327	1336	1350	rBV	1169863	1953974	40.05%	3.633%
15	12.304	1579	1584	1591	rVB	19972	31068	0.64%	0.058%
16	13.951	1856	1864	1870	rBV	1982999	2803973	57.47%	5.214%
17	13.993	1870	1871	1880	rVB7	6202	7691	0.16%	0.014%
18	14.240	1906	1913	1926	rBV	2311211	3393791	69.56%	6.310%
19	14.545	1958	1965	1973	rBV	1670591	2477393	50.78%	4.606%
20	14.722	1986	1995	2014	rBV	811076	1168720	23.96%	2.173%
21	15.534	2126	2133	2145	rBV	2796739	4083979	83.71%	7.594%
22	15.640	2145	2151	2162	rBV	796978	1094832	22.44%	2.036%
23	15.775	2170	2174	2179	rVB3	14879	19856	0.41%	0.037%
24	16.210	2243	2248	2252	rVB7	2725	5331	0.11%	0.010%
25	17.069	2391	2394	2397	rBV2	7544	8077	0.17%	0.015%
26	17.287	2424	2431	2440	rBV	1948804	2799260	57.38%	5.205%
27	17.381	2441	2447	2466	rVB2	3131213	4453763	91.29%	8.281%
28	19.239	2758	2763	2768	rVB2	36344	50031	1.03%	0.093%
29	19.310	2768	2775	2780	rBV	36352	51878	1.06%	0.096%
30	19.675	2830	2837	2852	rBV	3730006	4878785	100.00%	9.072%
31	21.463	3135	3141	3151	rBV	2046067	2537795	52.02%	4.719%
32	23.704	3514	3522	3530	rBV2	1990629	3936062	80.68%	7.319%
33	23.857	3541	3548	3563	rVB2	1112292	2311538	47.38%	4.298%




Sum of corrected areas: 53780685

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022522\
Data File : BN018742.D
Acq On : 25 Feb 2022 22:28
Operator : CG/JU
Sample : PB142930BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK930

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN021622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

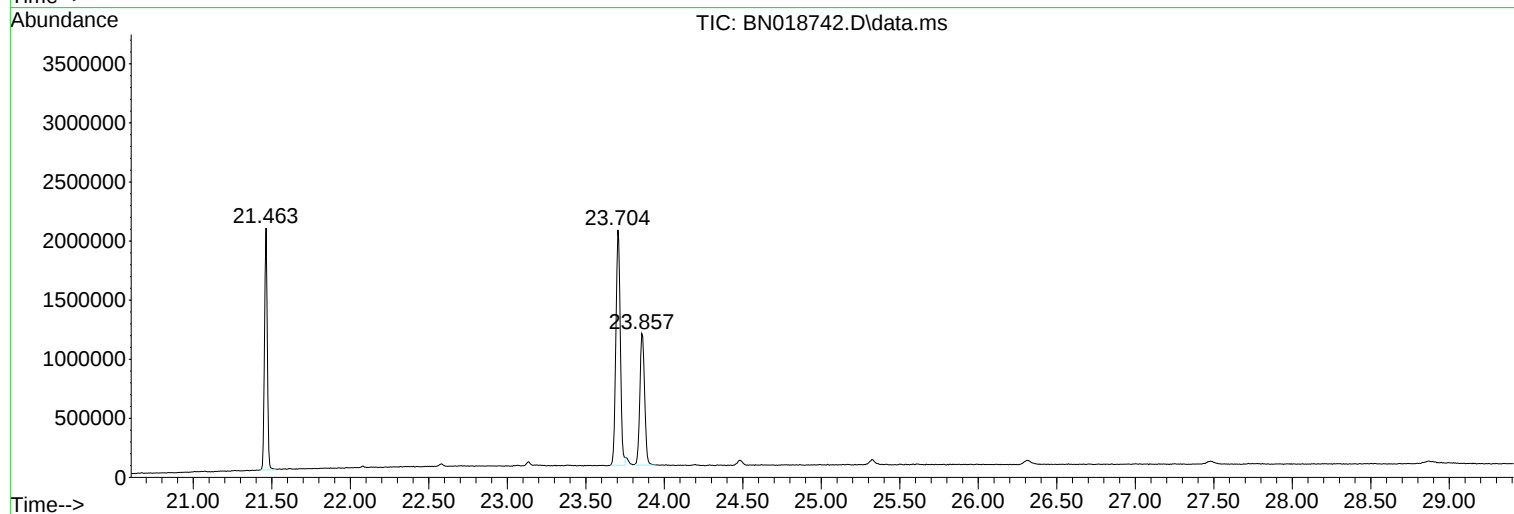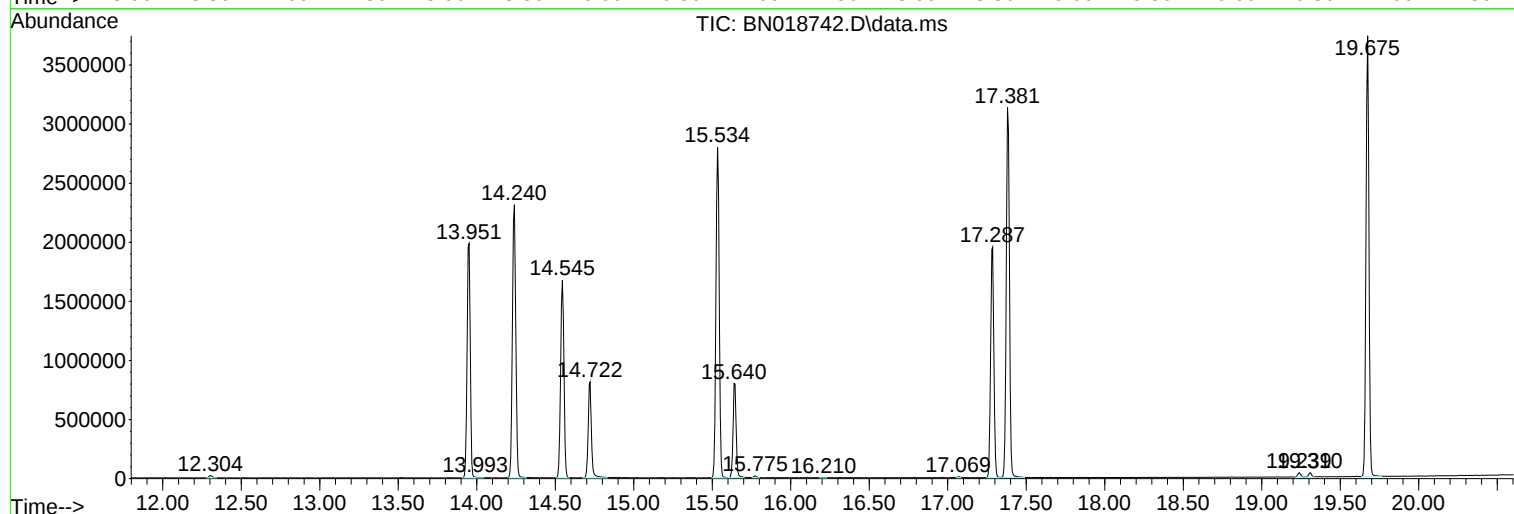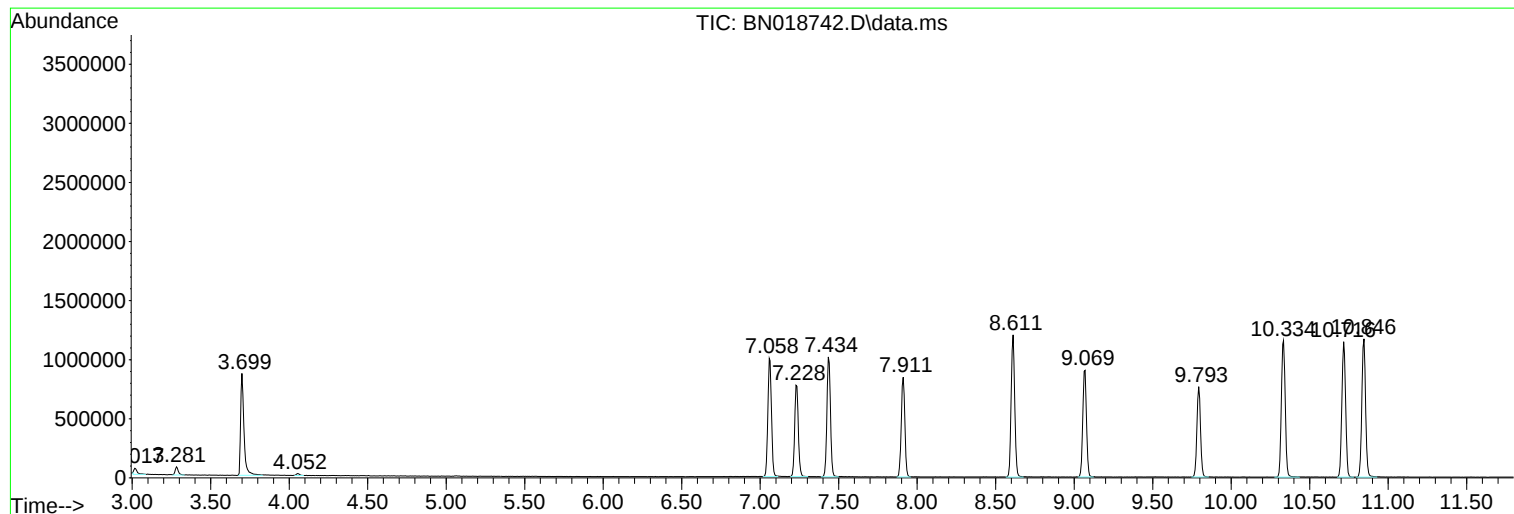

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022522\
Data File : BN018742.D
Acq On : 25 Feb 2022 22:28
Operator : CG/JU
Sample : PB142930BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK930

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN021622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022522\
Data File : BN018742.D
Acq On : 25 Feb 2022 22:28
Operator : CG/JU
Sample : PB142930BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK930

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN021622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc