

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022620\
 Data File : BN009936.D
 Acq On : 26 Feb 2020 19:55
 Operator : CG/JU
 Sample : L1612-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBDK9

Quant Time: Feb 27 07:17:52 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 26 07:56:07 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	95039	20.00	ng/ul	0.00
18) Naphthalene-d8	10.13	136	419743	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.02	164	266677	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.78	188	574702	20.00	ng/ul	0.00
78) Chrysene-d12	21.00	240	545013	20.00	ng/ul	0.00
86) Perylene-d12	23.10	264	568586	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.02	96	11266	4.88	ng/uL	0.00
5) Phenol-d5	6.59	99	208341	25.77	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.74	67	165981	29.75	ng/ul	0.00
9) 2-Chlorophenol-d4	6.92	132	173448	28.50	ng/ul	0.00
13) 4-Methylphenol-d8	8.10	113	174448	27.13	ng/ul	0.00
19) Nitrobenzene-d5	8.53	128	85578	27.87	ng/ul	0.00
22) 2-Nitrophenol-d4	9.24	143	93730	27.90	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.78	165	172376	26.69	ng/ul	0.00
29) 4-Chloroaniline-d4	10.29	131	221964	30.59	ng/ul	0.00
44) Dimethylphthalate-d6	13.45	166	567898	28.51	ng/ul	0.00
47) Acenaphthylene-d8	13.71	160	680741	29.02	ng/ul	0.00
52) 4-Nitrophenol-d4	14.27	143	65266	17.94	ng/ul	0.00
58) Fluorene-d10	15.03	176	503965	29.30	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.19	200	61649	17.27	ng/ul	0.00
71) Anthracene-d10	16.88	188	758958	28.81	ng/ul	0.00
79) Pyrene-d10	19.19	212	829169	29.11	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.97	264	851883	30.00	ng/ul	0.00


Target Compounds				Ovalue	
45) Dimethylphthalate	13.50	163	47907	2.305	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022620\
Data File : BN009936.D
Acq On : 26 Feb 2020 19:55
Operator : CG/JU
Sample : L1612-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBDK9

Quant Time: Feb 27 07:17:52 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 26 07:56:07 2020
Response via : Initial Calibration

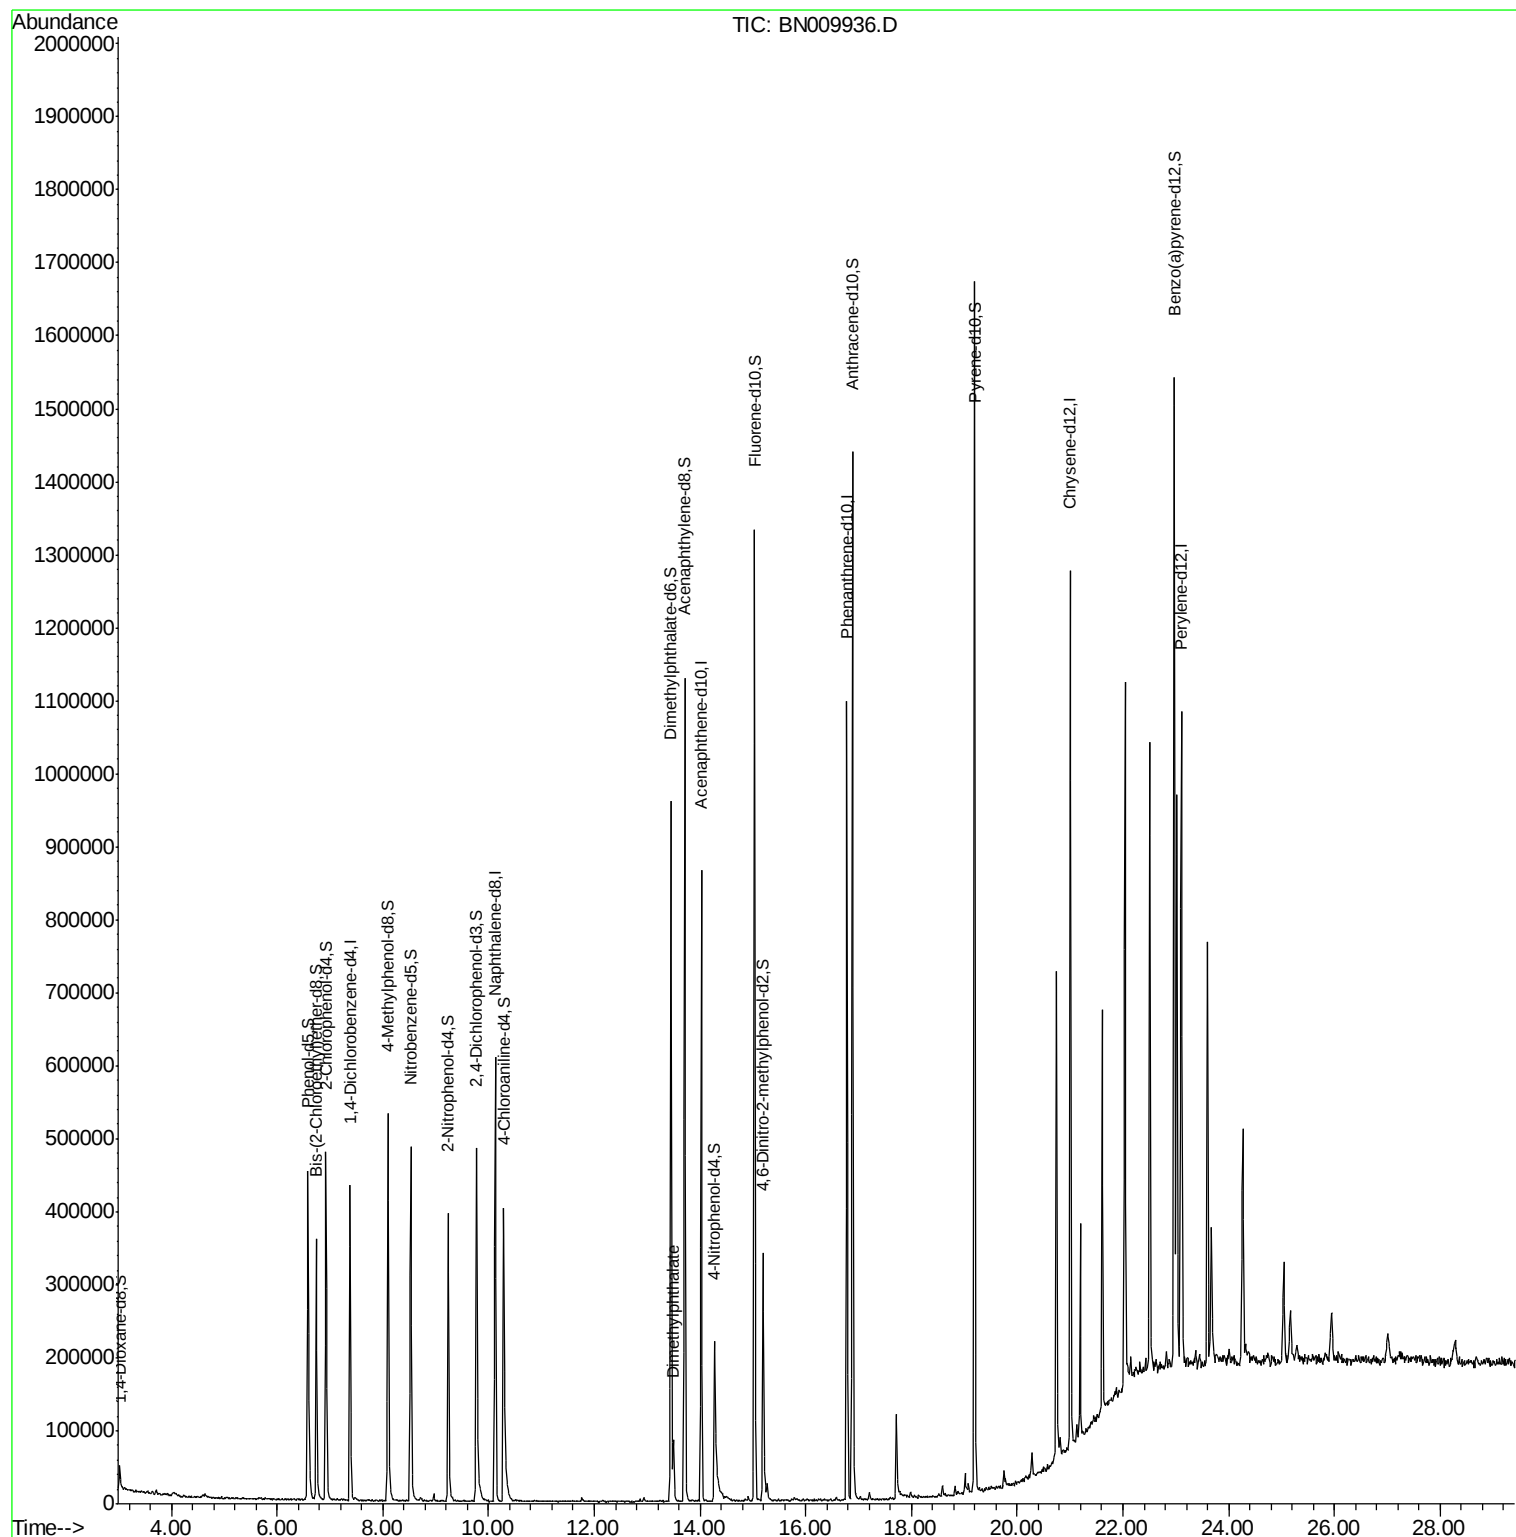

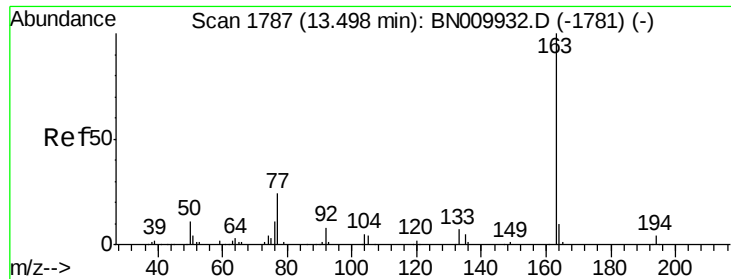

#45

Dimethylphthalate

Concen: 2.305 ng/ul

RT: 13.50 min Scan# 1787

Delta R.T. 0.00 min

Lab File: BN009936.D

Acq: 26 Feb 2020 19:55

Instrument :

BNA_N

ClientSampleId :

DBDK9


Tot Ion:163 Resp: 47907

Ion Ratio Lower Upper

163 100

194 3.7 3.4 5.0

164 10.4 8.0 12.0

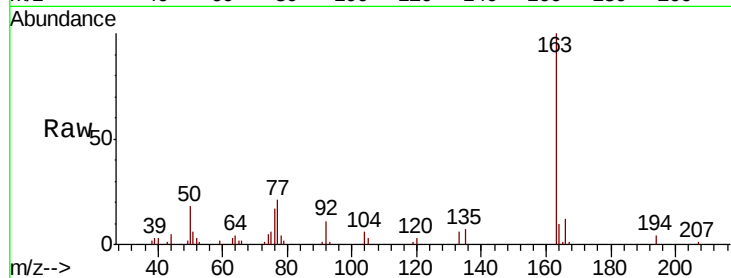

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

