

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022620\
 Data File : BN009937.D
 Acq On : 26 Feb 2020 20:31
 Operator : CG/JU
 Sample : L1612-08
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBDL0

Quant Time: Feb 27 07:53:34 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 26 07:56:07 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	90610	20.00	ng/ul	0.00
18) Naphthalene-d8	10.13	136	390695	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.02	164	254176	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.78	188	535807	20.00	ng/ul	0.00
78) Chrysene-d12	21.00	240	525288	20.00	ng/ul	0.00
86) Perylene-d12	23.10	264	544842	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.03	96	14442	6.56	ng/uL	0.00
5) Phenol-d5	6.59	99	260660	33.82	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.74	67	200380	37.68	ng/ul	0.00
9) 2-Chlorophenol-d4	6.92	132	211431	36.44	ng/ul	0.00
13) 4-Methylphenol-d8	8.10	113	202464	33.02	ng/ul	0.00
19) Nitrobenzene-d5	8.53	128	107970	37.77	ng/ul	0.00
22) 2-Nitrophenol-d4	9.24	143	120080	38.40	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.77	165	209108	34.79	ng/ul	0.00
29) 4-Chloroaniline-d4	10.29	131	239402	35.45	ng/ul	0.00
44) Dimethylphthalate-d6	13.45	166	708663	37.33	ng/ul	0.00
47) Acenaphthylene-d8	13.71	160	831426	37.18	ng/ul	0.00
52) 4-Nitrophenol-d4	14.27	143	84353	24.33	ng/ul	0.00
58) Fluorene-d10	15.03	176	608527	37.12	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.19	200	81161	24.38	ng/ul	0.00
71) Anthracene-d10	16.88	188	934734	38.06	ng/ul	0.00
79) Pyrene-d10	19.19	212	1023921	37.29	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.97	264	1026134	37.71	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.50	163	51490	2.599	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022620\
Data File : BN009937.D
Acq On : 26 Feb 2020 20:31
Operator : CG/JU
Sample : L1612-08
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBDL0

Quant Time: Feb 27 07:53:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 26 07:56:07 2020
Response via : Initial Calibration

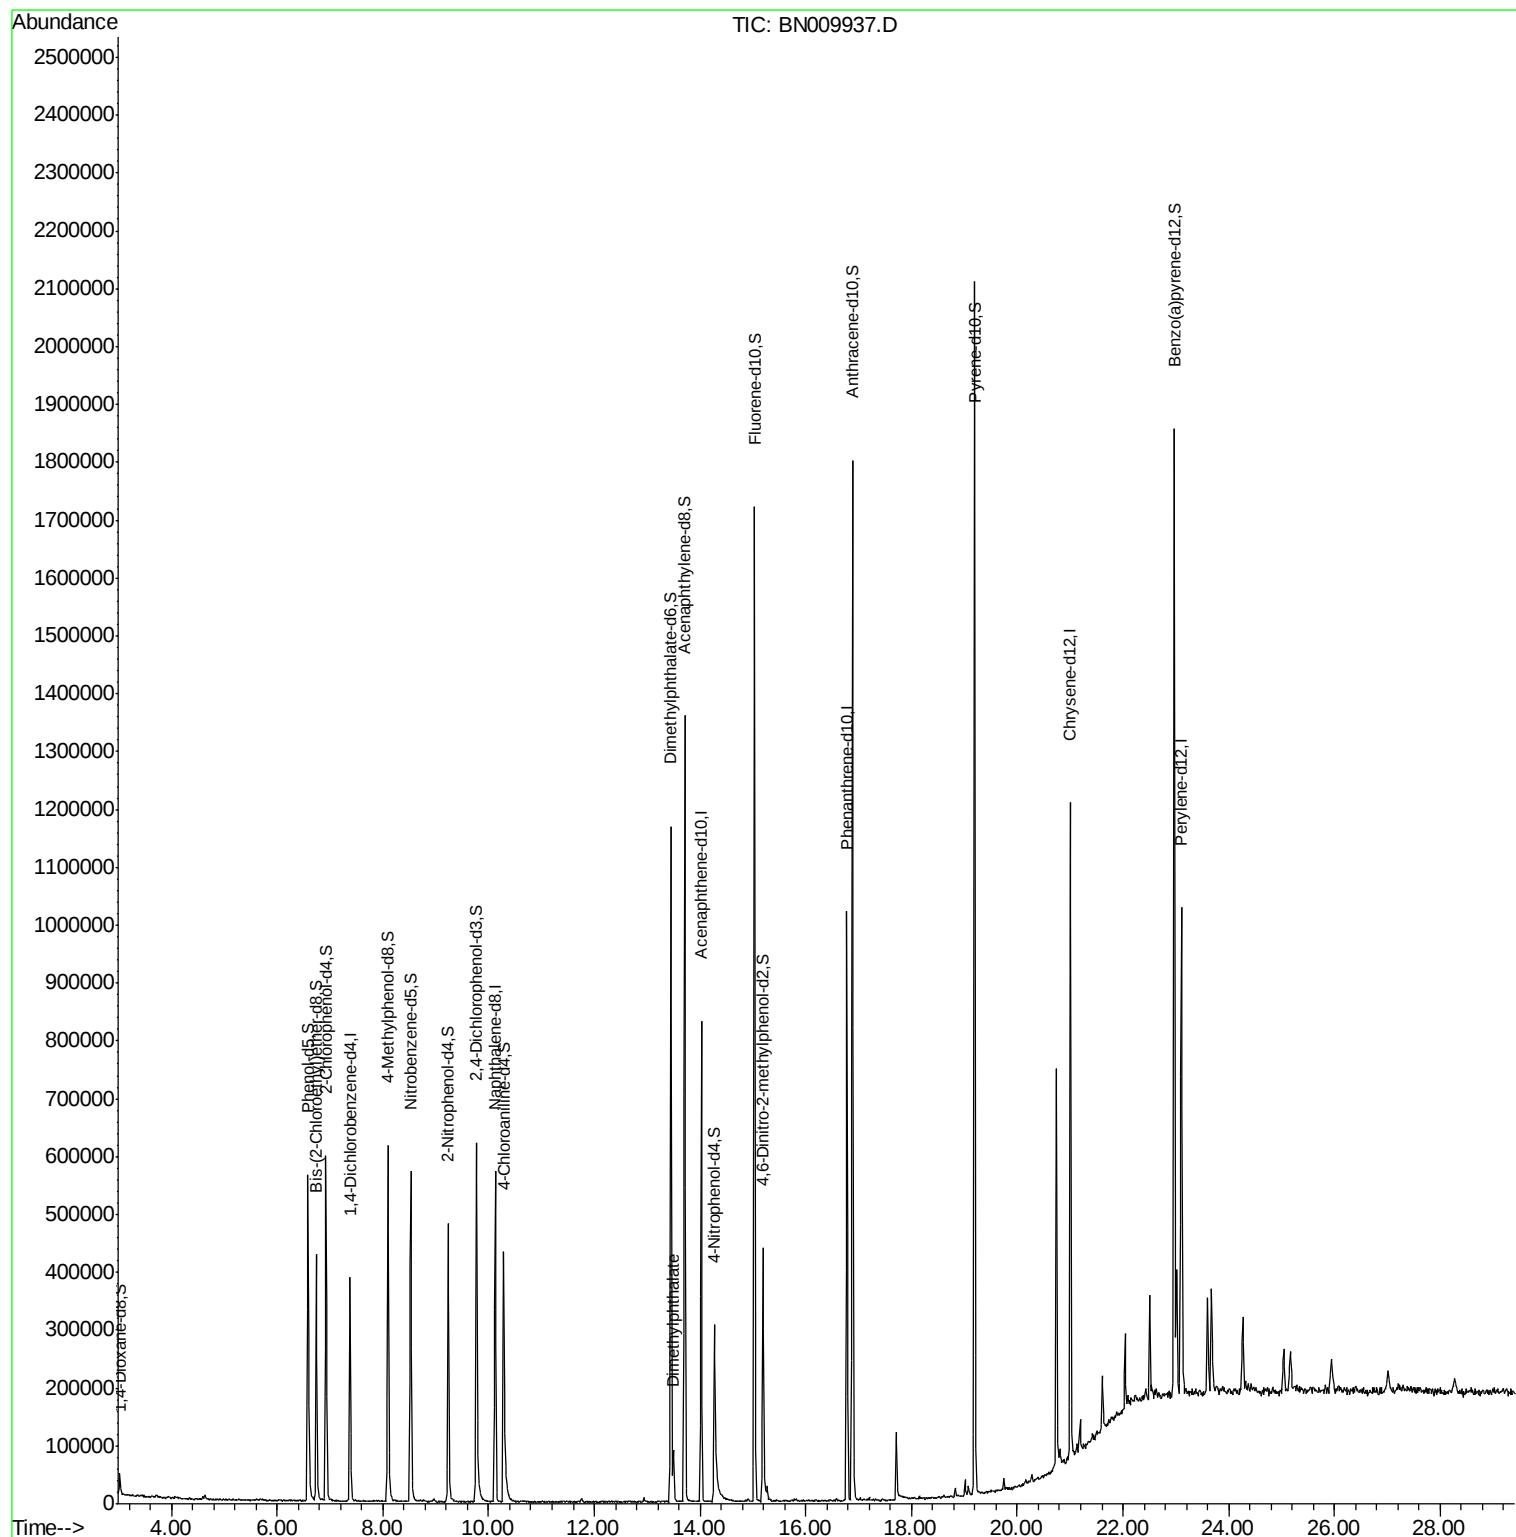

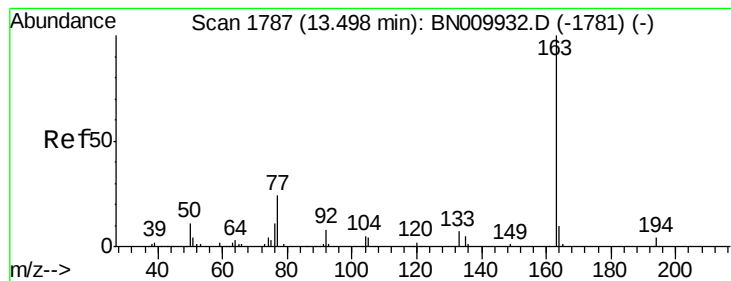

#45

Dimethylphthalate

Concen: 2.599 ng/ul

RT: 13.50 min Scan# 1787

Delta R.T. 0.00 min

Lab File: BN009937.D

Acq: 26 Feb 2020 20:31

Instrument :

BNA_N

ClientSampleId :

DBDL0


Tot Ion:163 Resp: 51490

Ion Ratio Lower Upper

163 100

194 4.2 3.4 5.0

164 11.1 8.0 12.0

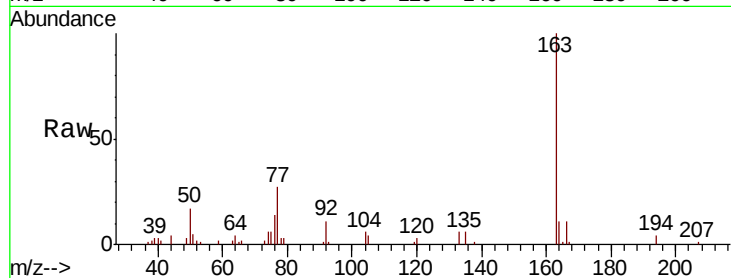

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

