

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN022620\
 Data File : BN009975.D
 Acq On : 27 Feb 2020 21:53
 Operator : CG/JU
 Sample : L1582-05DL3 600X
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBDJ7DL3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	31	33	36	rBV3	2165	1938	0.15%	0.026%
2	3.622	106	108	109	rVB2	2624	1559	0.12%	0.021%
3	3.705	121	122	127	rVB2	3282	3595	0.28%	0.049%
4	3.963	162	166	167	rBV3	1434	1759	0.14%	0.024%
5	4.011	171	174	177	rBV4	1908	3102	0.25%	0.042%
6	4.152	196	198	202	rBV4	1894	3336	0.26%	0.045%
7	4.181	202	203	206	rVV3	2259	1746	0.14%	0.024%
8	4.416	240	243	247	rBV5	2006	2736	0.22%	0.037%
9	4.452	247	249	251	rVB2	2389	1713	0.14%	0.023%
10	4.869	319	320	324	rBV3	1547	1789	0.14%	0.024%
11	5.358	400	403	407	rVB5	1325	1600	0.13%	0.022%
12	5.663	453	455	456	rBV	1697	1670	0.13%	0.023%
13	5.699	460	461	466	rVV4	1485	2194	0.17%	0.030%
14	5.922	496	499	501	rBV4	1450	1635	0.13%	0.022%
15	6.263	555	557	561	rVB4	1838	2104	0.17%	0.029%
16	6.510	594	599	602	rVV4	1604	1984	0.16%	0.027%
17	6.634	617	620	623	rBV5	1793	2359	0.19%	0.032%
18	6.904	664	666	670	rBV3	1529	2354	0.19%	0.032%
19	7.046	686	690	693	rBV3	1758	2562	0.20%	0.035%
20	7.381	741	747	763	rBV	301266	532303	42.05%	7.241%
21	7.599	779	784	785	rBV3	2289	3544	0.28%	0.048%
22	7.752	803	810	817	rBV2	10937	20460	1.62%	0.278%
23	7.910	831	837	845	rBV3	17599	40087	3.17%	0.545%
24	8.334	904	909	910	rVB3	1564	2252	0.18%	0.031%
25	8.351	910	912	916	rBV2	1788	2672	0.21%	0.036%
26	8.557	944	947	948	rBV2	1915	1727	0.14%	0.023%
27	8.604	953	955	959	rVV4	1576	2474	0.20%	0.034%
28	8.646	959	962	964	rVV2	1297	1868	0.15%	0.025%
29	8.869	994	1000	1003	rBV3	1848	3977	0.31%	0.054%
30	8.899	1003	1005	1008	rVB3	1508	1615	0.13%	0.022%
31	9.410	1089	1092	1095	rVB3	1280	1856	0.15%	0.025%
32	9.516	1105	1110	1114	rBV	11307	18476	1.46%	0.251%
33	9.763	1148	1152	1155	rBV2	1908	2353	0.19%	0.032%
34	9.810	1158	1160	1163	rVB3	1487	1632	0.13%	0.022%

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN022620\
 Data File : BN009975.D
 Acq On : 27 Feb 2020 21:53
 Operator : CG/JU
 Sample : L1582-05DL3 600X
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBDJ7DL3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Title : SVOA CALIBRATION

35	10.122	1207	1213	1217	rVV	440752	722115	57.04%	9.822%
36	10.175	1217	1222	1239	rVV	500256	976930	77.17%	13.289%
37	10.298	1239	1243	1256	rVV3	14541	33909	2.68%	0.461%
38	10.628	1297	1299	1302	rVB	1545	1628	0.13%	0.022%
39	10.928	1346	1350	1356	rBV4	1508	2936	0.23%	0.040%
40	11.828	1496	1503	1515	rBV	32836	74569	5.89%	1.014%
41	11.957	1522	1525	1527	rVB2	1600	1663	0.13%	0.023%
42	12.045	1532	1540	1548	rBV2	18067	38763	3.06%	0.527%
43	12.181	1558	1563	1565	rVV2	1067	1784	0.14%	0.024%
44	12.216	1567	1569	1572	rVB4	1825	1899	0.15%	0.026%
45	12.369	1593	1595	1597	rVV2	1402	1641	0.13%	0.022%
46	12.810	1665	1670	1673	rBV4	1222	2093	0.17%	0.028%
47	12.875	1676	1681	1684	rVV3	2919	4245	0.34%	0.058%
48	12.898	1684	1685	1693	rVB5	1727	3254	0.26%	0.044%
49	13.075	1712	1715	1719	rBV4	1265	2117	0.17%	0.029%
50	13.351	1759	1762	1763	rBV3	1896	1906	0.15%	0.026%
51	14.022	1869	1876	1884	rBV	614956	975778	77.08%	13.273%
52	14.086	1884	1887	1896	rVB2	33988	61271	4.84%	0.833%
53	14.239	1909	1913	1915	rBV2	2489	3263	0.26%	0.044%
54	14.334	1924	1929	1930	rVB2	1099	1715	0.14%	0.023%
55	14.463	1946	1951	1959	rBV2	13331	21429	1.69%	0.291%
56	14.616	1973	1977	1980	rVV3	1717	1870	0.15%	0.025%
57	14.981	2038	2039	2042	rBV2	1693	1558	0.12%	0.021%
58	15.045	2047	2050	2052	rVV2	1858	1764	0.14%	0.024%
59	15.110	2056	2061	2067	rVV2	11213	17559	1.39%	0.239%
60	15.575	2134	2140	2141	rVB3	1617	2242	0.18%	0.030%
61	16.092	2227	2228	2234	rVB3	1266	2275	0.18%	0.031%
62	16.316	2263	2266	2269	rVV3	1322	1860	0.15%	0.025%
63	16.357	2269	2273	2275	rVB3	1449	1879	0.15%	0.026%
64	16.516	2296	2300	2303	rBV5	1240	1851	0.15%	0.025%
65	16.575	2307	2310	2314	rVB3	1909	2741	0.22%	0.037%
66	16.745	2336	2339	2340	rBV3	1607	1835	0.14%	0.025%
67	16.780	2340	2345	2364	rVV	678158	1165854	92.09%	15.858%
68	16.910	2364	2367	2368	rVV2	3268	2838	0.22%	0.039%
69	16.951	2371	2374	2376	rVB4	1758	1776	0.14%	0.024%
70	17.045	2389	2390	2394	rBV4	1544	1628	0.13%	0.022%
71	17.239	2418	2423	2432	rBV4	7487	19160	1.51%	0.261%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022620\
 Data File : BN009975.D
 Acq On : 27 Feb 2020 21:53
 Operator : CG/JU
 Sample : L1582-05DL3 600X
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBDJ7DL3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Title : SVOA CALIBRATION

72	17.333	2435	2439	2442	rBV4	1722	1933	0.15%	0.026%
73	17.580	2477	2481	2483	rVB3	1385	2053	0.16%	0.028%
74	17.704	2498	2502	2505	rVB3	1058	1588	0.13%	0.022%
75	18.004	2549	2553	2558	rBV3	1950	3741	0.30%	0.051%
76	18.216	2586	2589	2594	rVB3	1359	1970	0.16%	0.027%
77	18.257	2594	2596	2599	rVB4	2303	2931	0.23%	0.040%
78	18.298	2599	2603	2606	rBV4	1992	3933	0.31%	0.053%
79	18.457	2627	2630	2633	rBV2	1423	2146	0.17%	0.029%
80	18.510	2637	2639	2641	rBV3	1811	2148	0.17%	0.029%
81	18.598	2651	2654	2656	rVB3	1927	1749	0.14%	0.024%
82	18.710	2671	2673	2675	rVB2	2031	1739	0.14%	0.024%
83	18.763	2681	2682	2684	rBV	2245	1773	0.14%	0.024%
84	18.786	2684	2686	2689	rBV4	1924	1906	0.15%	0.026%
85	18.892	2701	2704	2706	rVV3	3272	3529	0.28%	0.048%
86	18.910	2706	2707	2709	rVV2	1985	1701	0.13%	0.023%
87	18.963	2713	2716	2717	rVV3	2228	1896	0.15%	0.026%
88	18.980	2717	2719	2722	rVV2	1942	2487	0.20%	0.034%
89	19.057	2729	2732	2734	rBV2	1701	2147	0.17%	0.029%
90	19.110	2739	2741	2746	rBV4	1913	2303	0.18%	0.031%
91	19.163	2748	2750	2753	rVB3	2374	2550	0.20%	0.035%
92	19.210	2755	2758	2759	rBV3	2719	2638	0.21%	0.036%
93	19.398	2787	2790	2791	rBV3	2348	2062	0.16%	0.028%
94	19.510	2806	2809	2811	rBV3	2789	2839	0.22%	0.039%
95	19.586	2820	2822	2824	rBV3	2253	2997	0.24%	0.041%
96	19.769	2851	2853	2856	rVB3	2741	1978	0.16%	0.027%
97	19.927	2878	2880	2881	rBV2	4012	2254	0.18%	0.031%
98	20.121	2911	2913	2916	rBV3	4281	4388	0.35%	0.060%
99	21.004	3058	3063	3076	rBV	911110	1266001	100.00%	17.221%
100	23.098	3414	3419	3428	rBV	636122	1177637	93.02%	16.019%


Sum of corrected areas: 7351646

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN022620\
Data File : BN009975.D
Acq On : 27 Feb 2020 21:53
Operator : CG/JU
Sample : L1582-05DL3 600X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBDJ7DL3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

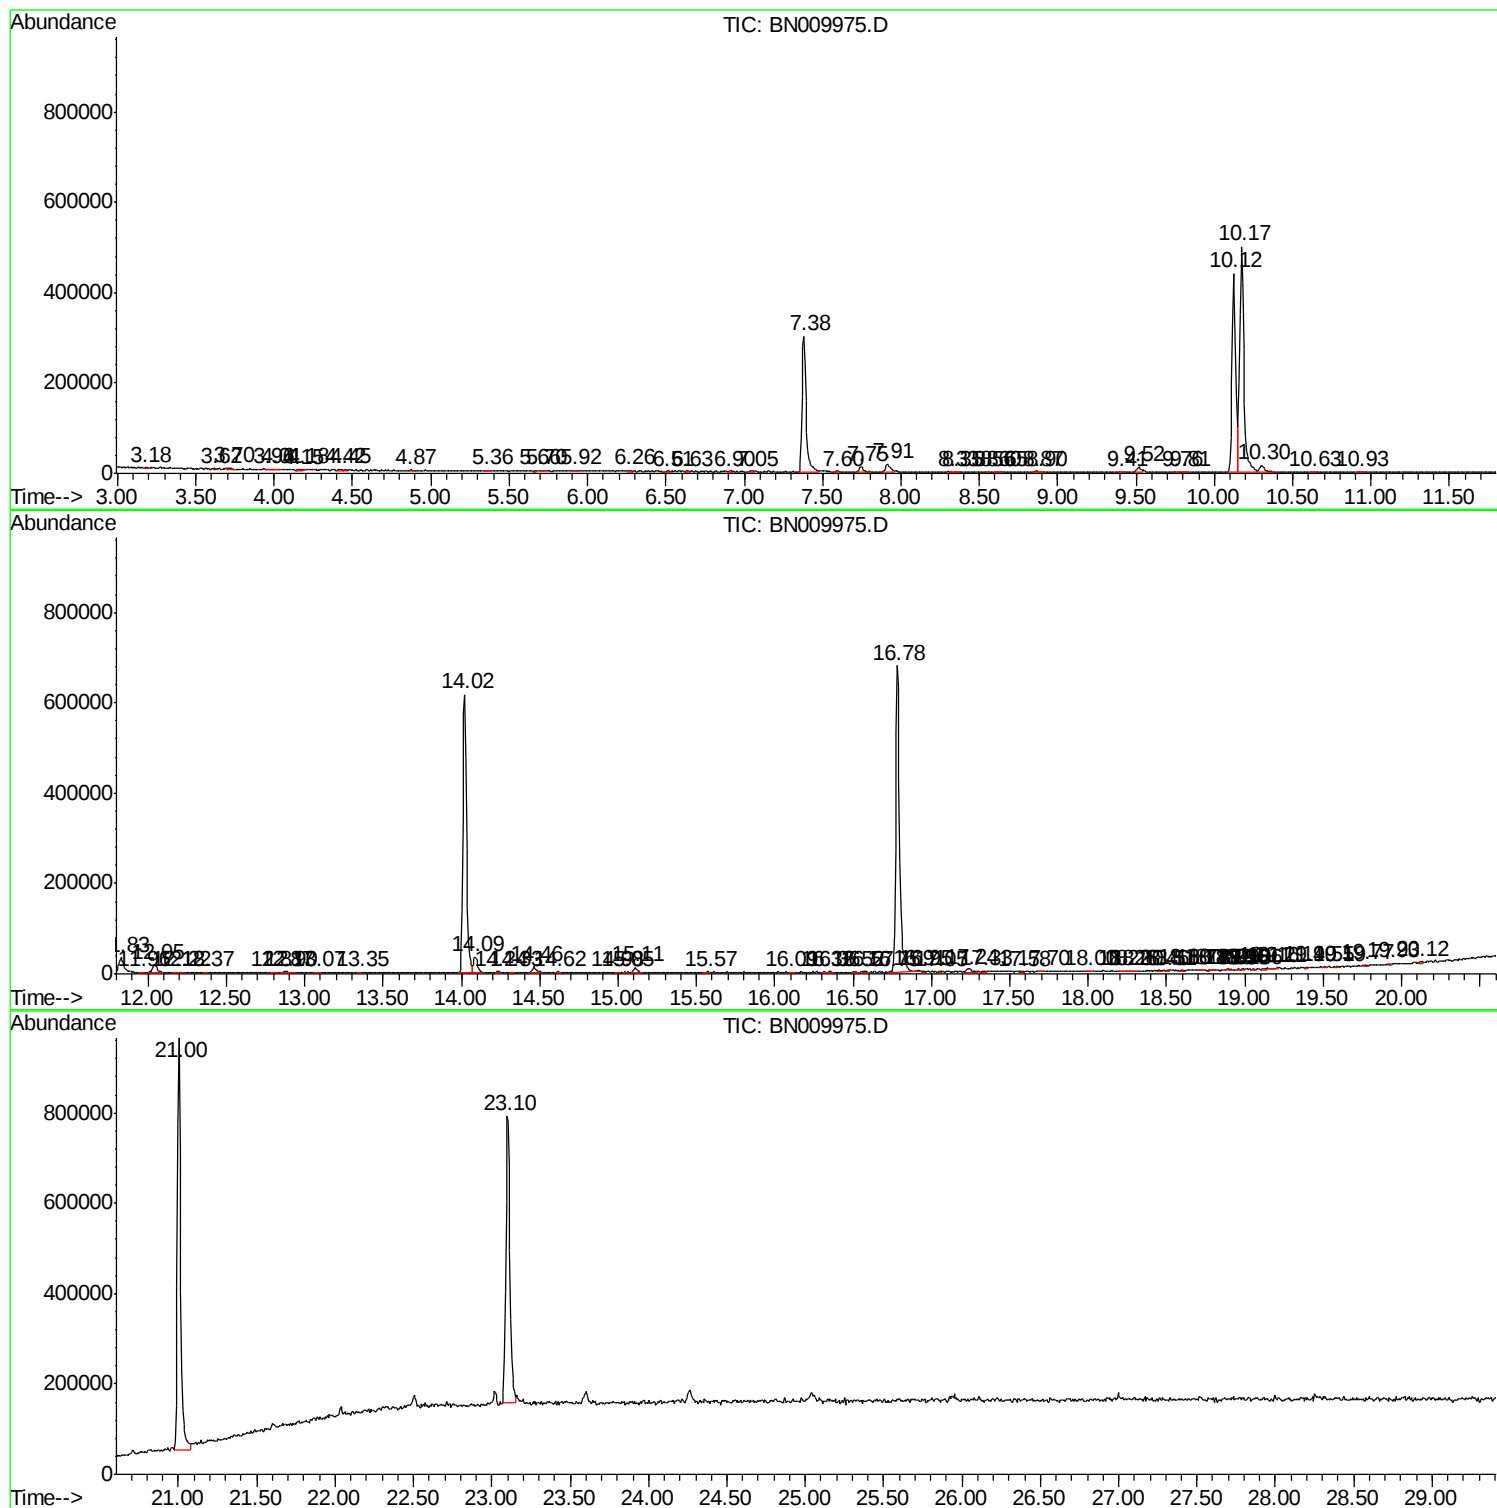

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022620\
Data File : BN009975.D
Acq On : 27 Feb 2020 21:53
Operator : CG/JU
Sample : L1582-05DL3 600X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBDJ7DL3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022620\
Data File : BN009975.D
Acq On : 27 Feb 2020 21:53
Operator : CG/JU
Sample : L1582-05DL3 600X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBDJ7DL3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc