
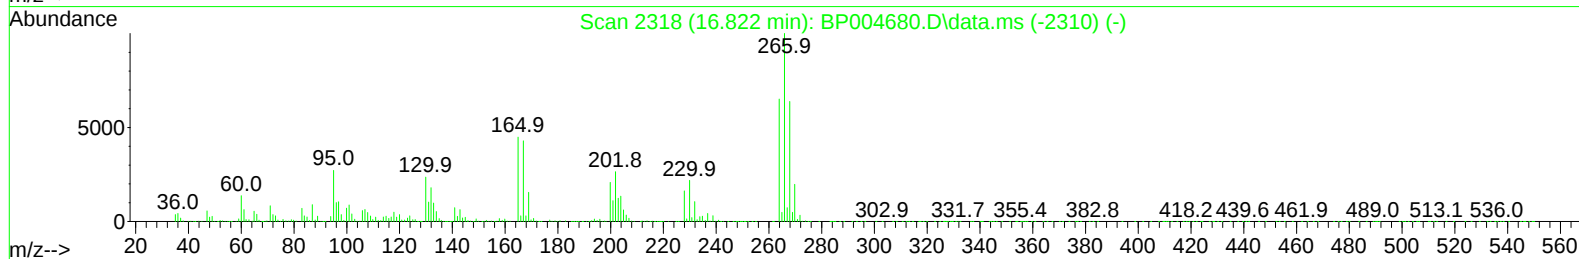
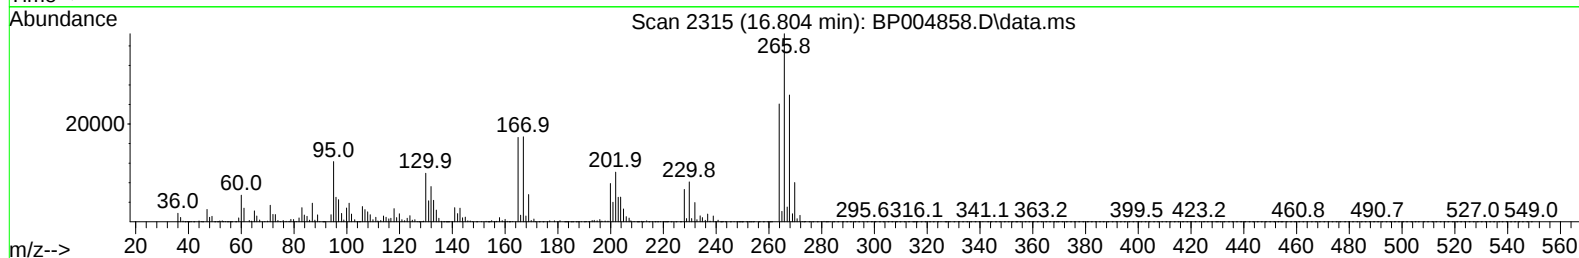


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022621\
Data File : BP004858.D
Acq On : 26 Feb 2021 12:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 26 13:29:19 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP022621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 26 13:23:29 2021
Response via : Initial Calibration

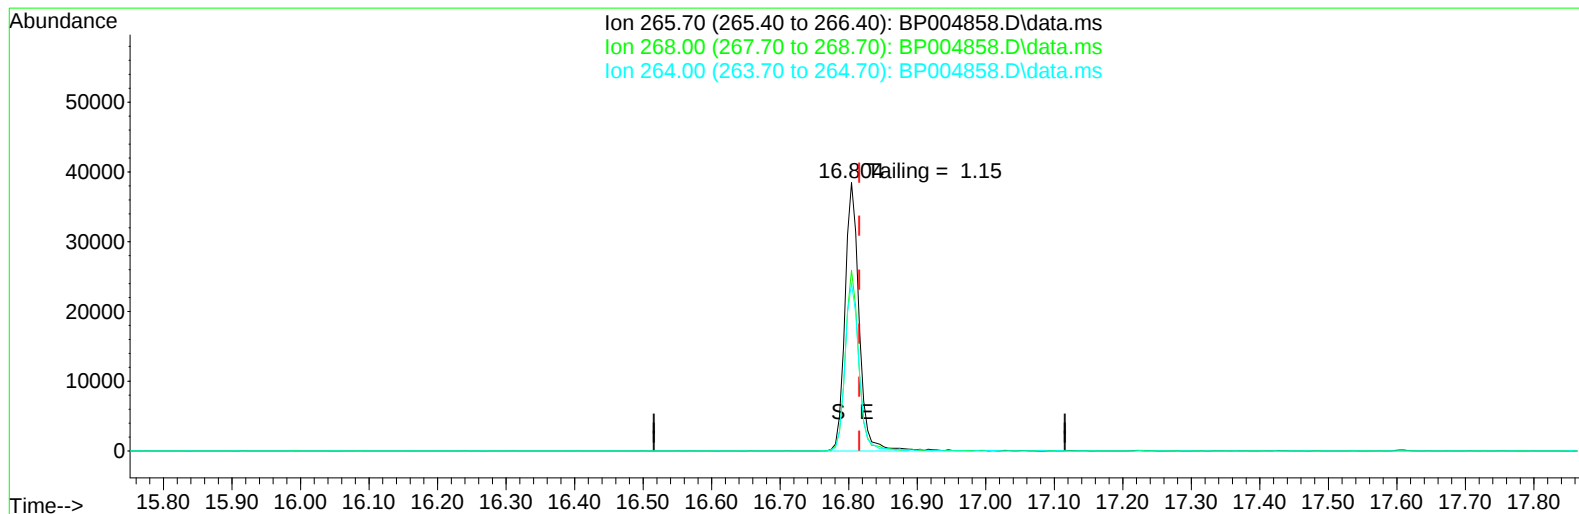

TIC: BP004858.D\data.ms

(70) Pentachlorophenol (C)

16.804min (-0.011) 1095006.19 ng

response 51577

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	67.39
264.00	63.30	62.61
0.00	0.00	0.00