
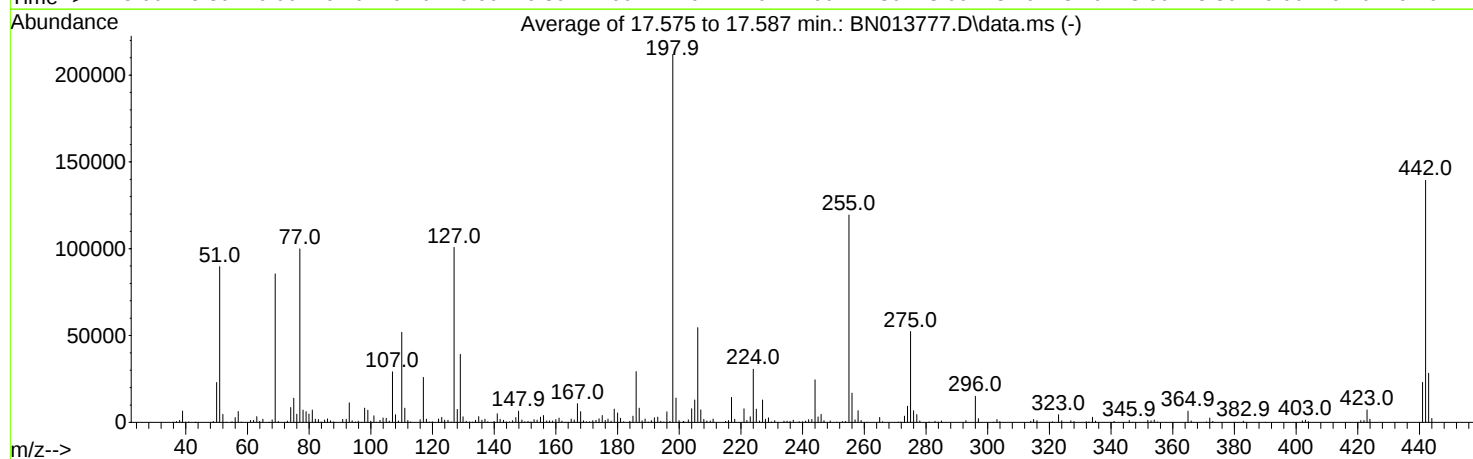


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022621\
 Data File : BN013777.D
 Acq On : 26 Feb 2021 08:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN022421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 25 11:31:11 2021

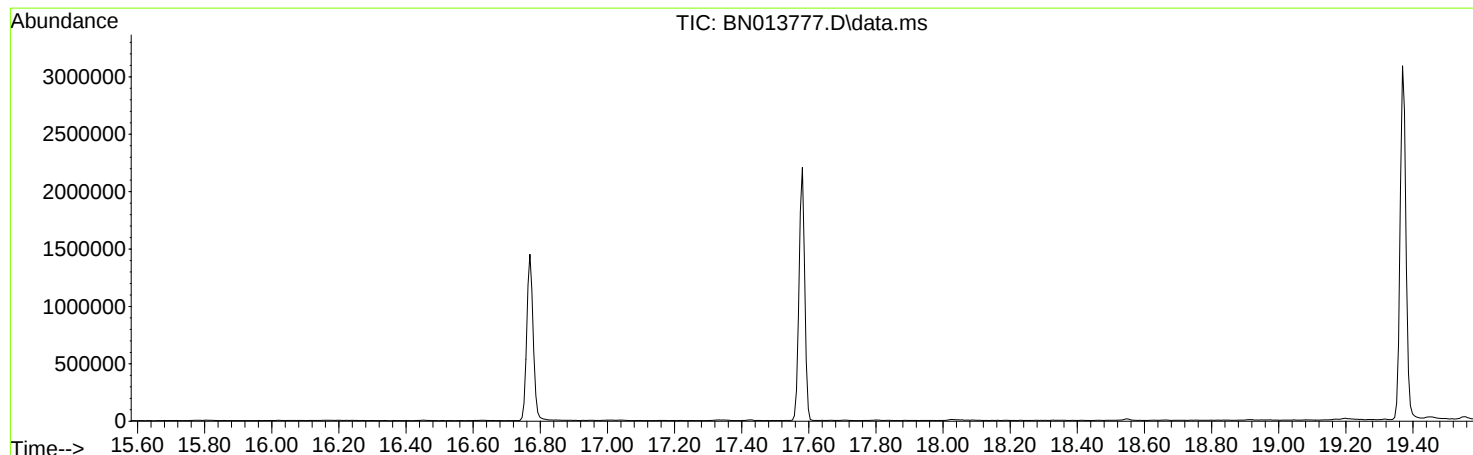

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.3	89707	PASS
68	69	0.00	2	1.7	1446	PASS
69	198	0.00	100	40.4	85557	PASS
70	69	0.00	2	0.6	550	PASS
127	198	10	80	47.6	100811	PASS
197	198	0.00	2	0.3	546	PASS
198	198	100	100	100.0	211861	PASS
199	198	5	9	6.6	14041	PASS
275	198	10	60	24.7	52304	PASS
365	198	1	100	3.1	6469	PASS
441	198	0.01	100	10.9	23059	PASS
442	442	50	100	100.0	139387	PASS
443	442	15	24	20.3	28323	PASS

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/26/2021	BNA_N	<u>BN013777.D</u>
Compound Name	Response	Retention Time
DDT	691187	20.61
DDD	8763	20.16
DDE	744	19.66
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9507	700694	1.36

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022621\
Data File : BN013777.D
Acq On : 26 Feb 2021 08:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 01 06:24:58 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 26 07:31:37 2021
Response via : Initial Calibration

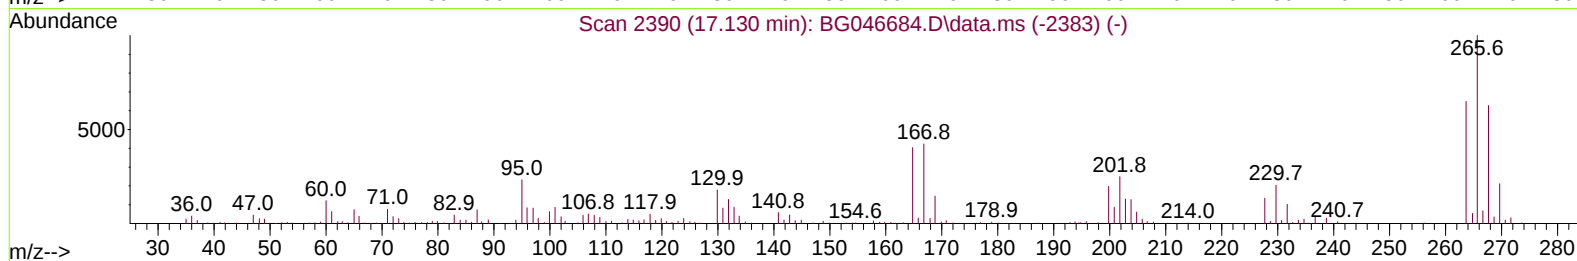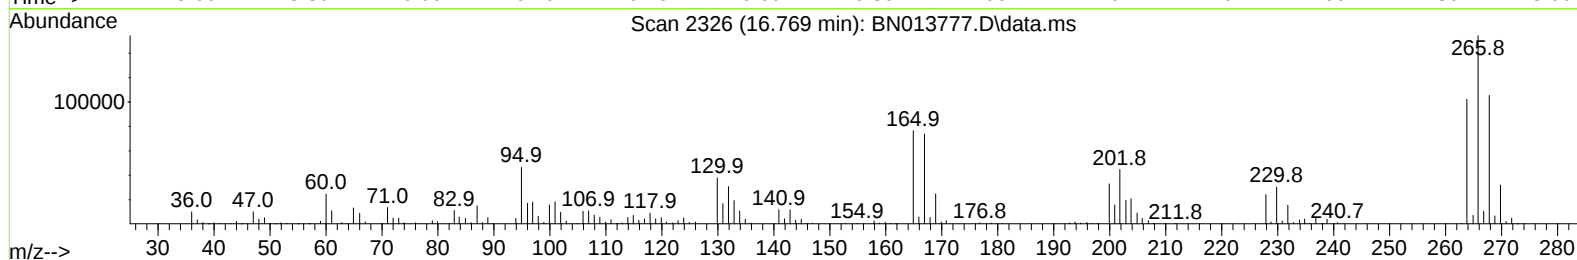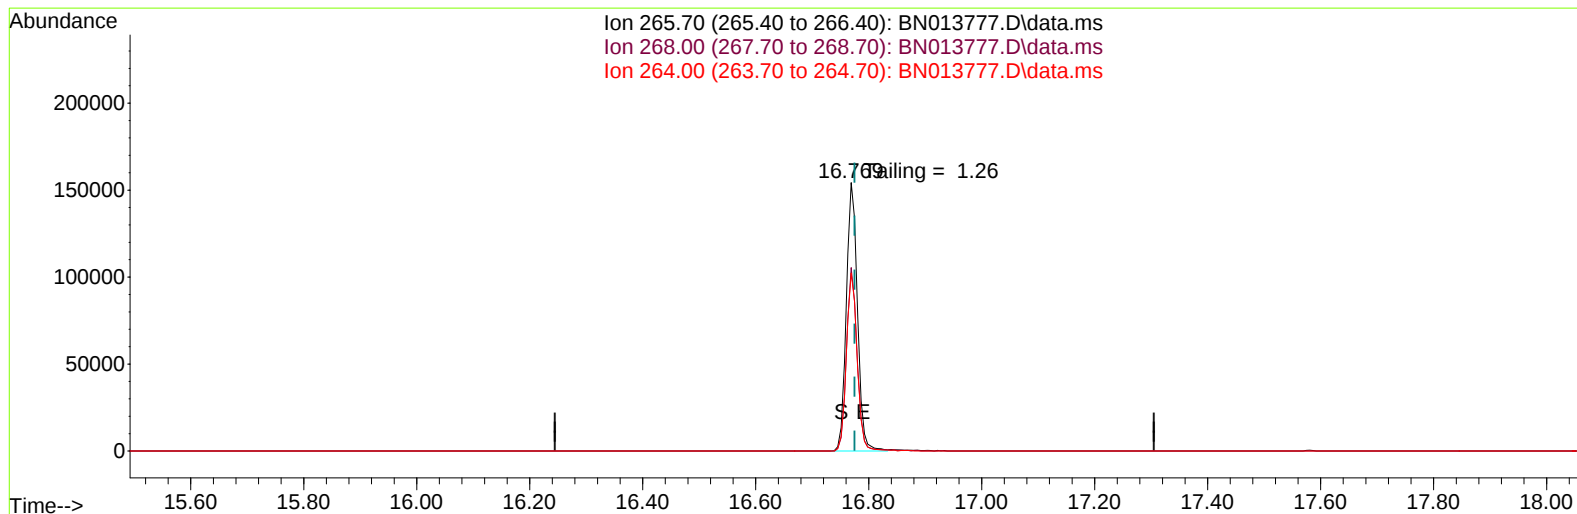

TIC: BN013777.D\data.ms

(70) Pentachlorophenol (C)

16.769min (-0.006) 22169.33 ng




response 210689

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.33
264.00	61.60	66.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022621\
Data File : BN013777.D
Acq On : 26 Feb 2021 08:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 01 06:24:58 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 26 07:31:37 2021
Response via : Initial Calibration

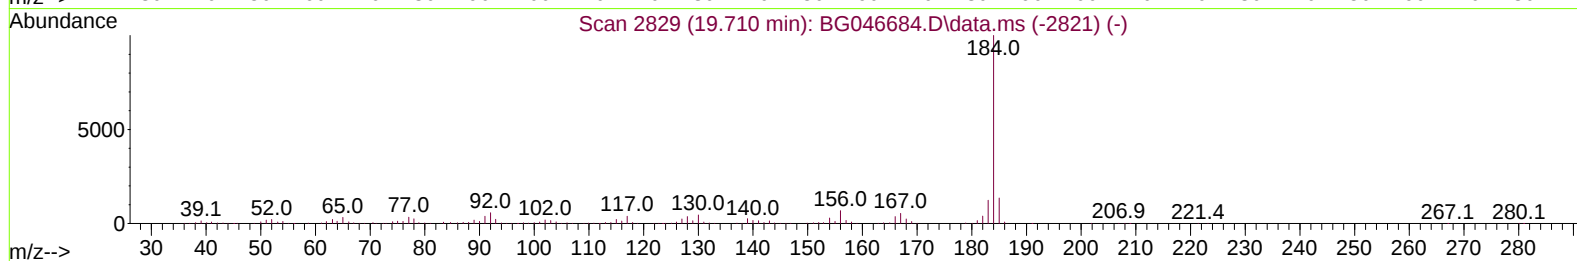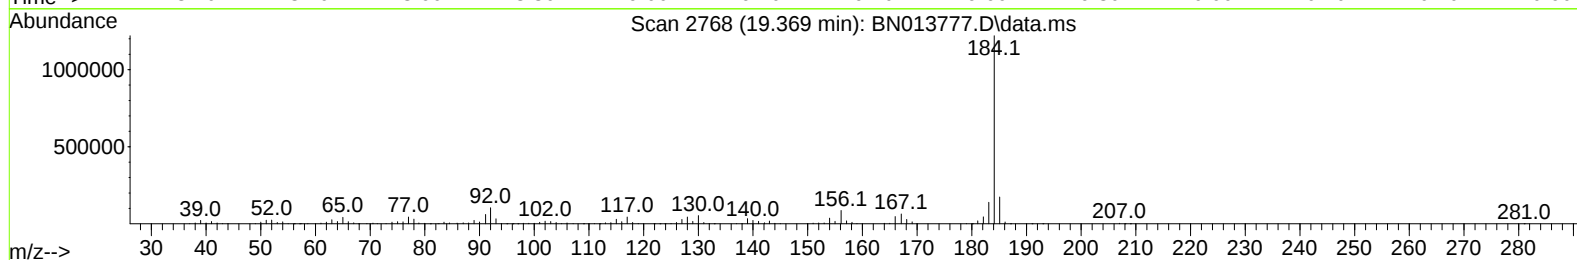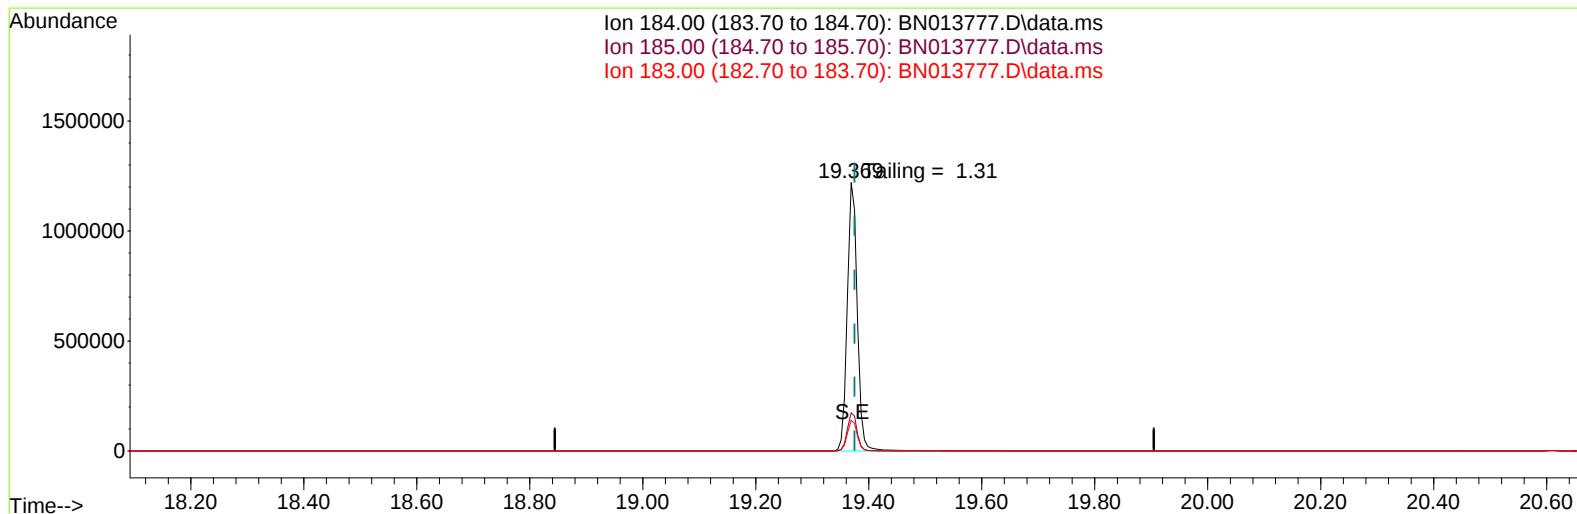

TIC: BN013777.D\data.ms

(77) Benzidine

19.369min (-0.006) 0.00 ng

response 1505843

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.26
183.00	13.20	11.48
0.00	0.00	0.00