
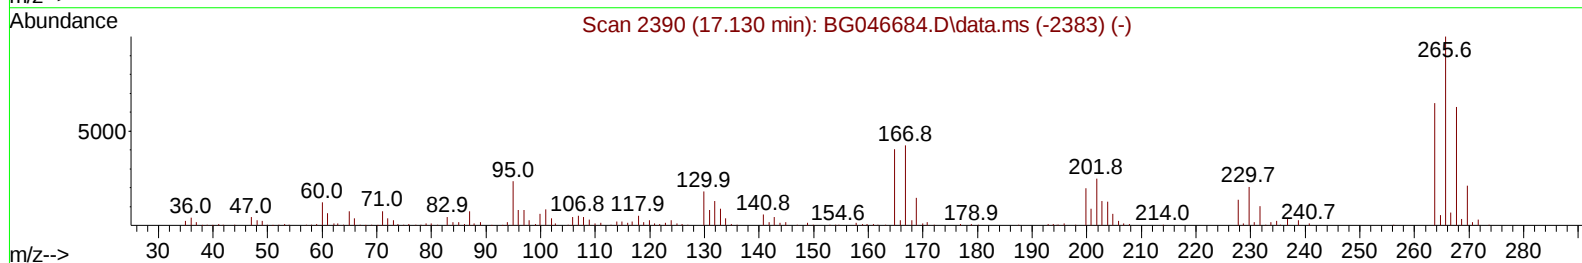
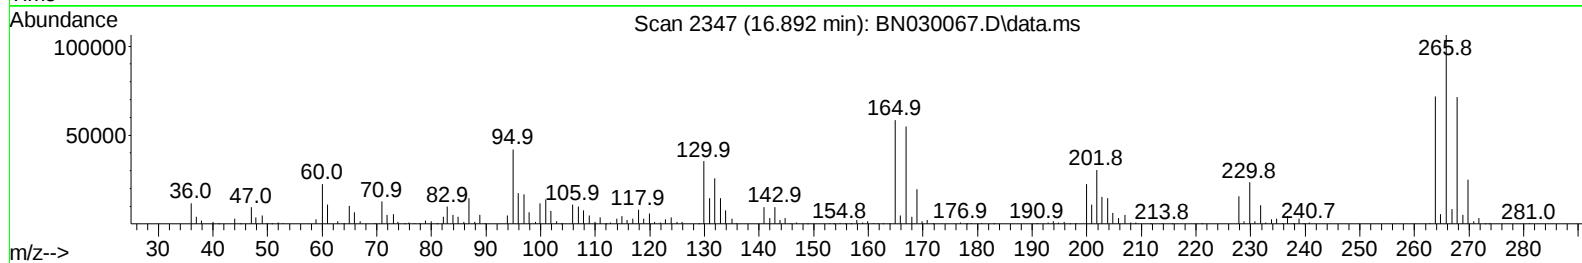


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022624\
Data File : BN030067.D
Acq On : 26 Feb 2024 21:49
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Feb 27 03:32:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 03:29:47 2024
Response via : Initial Calibration

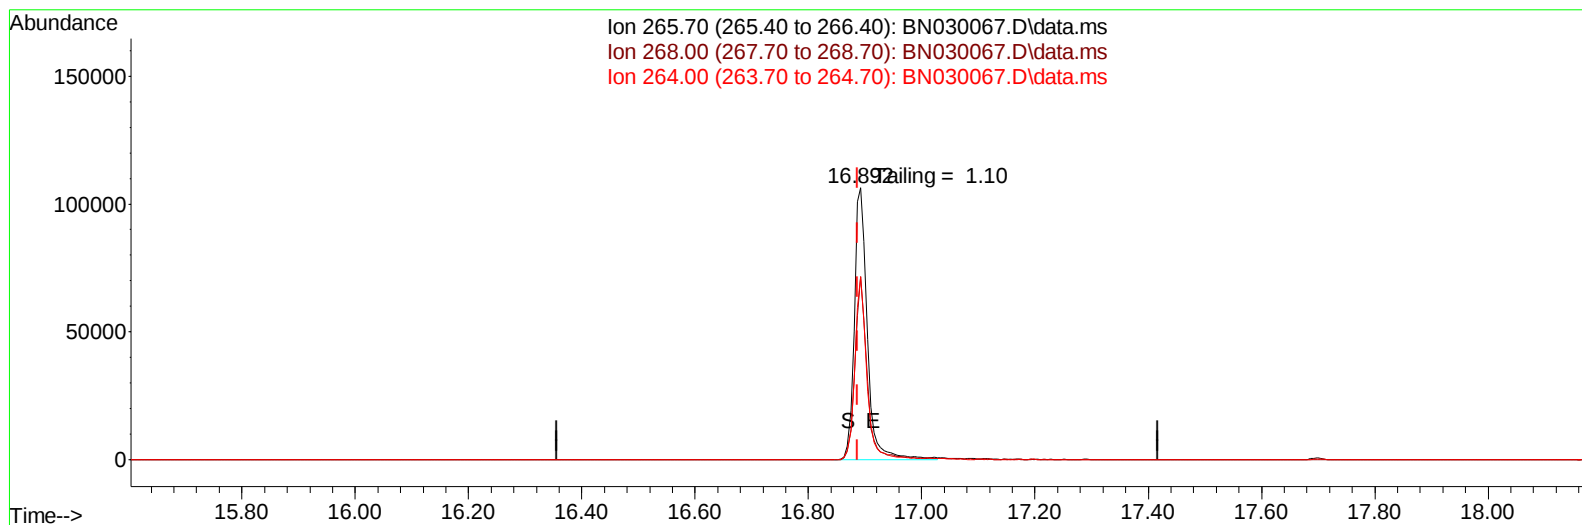




TIC: BN030067.D\data.ms

(70) Pentachlorophenol (C)**16.892min (+ 0.006) 16080.95 ng****response 169107**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.26
264.00	61.60	67.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022624\
Data File : BN030067.D
Acq On : 26 Feb 2024 21:49
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Feb 27 03:32:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 03:29:47 2024
Response via : Initial Calibration

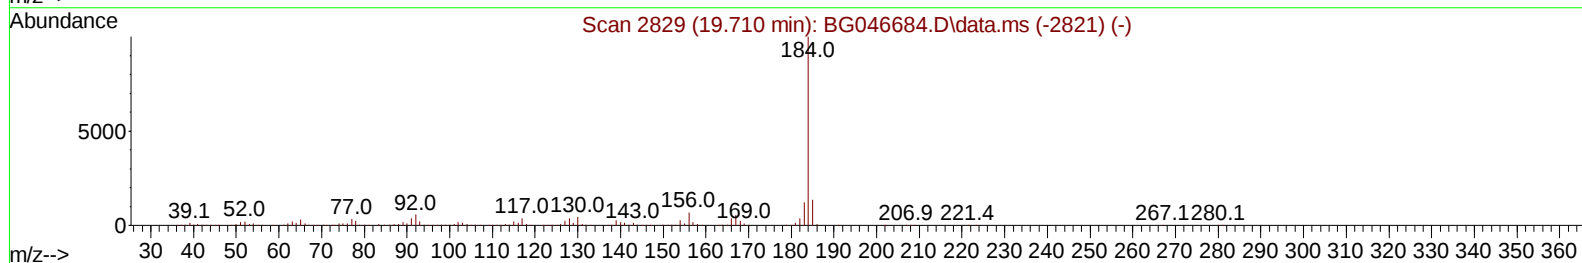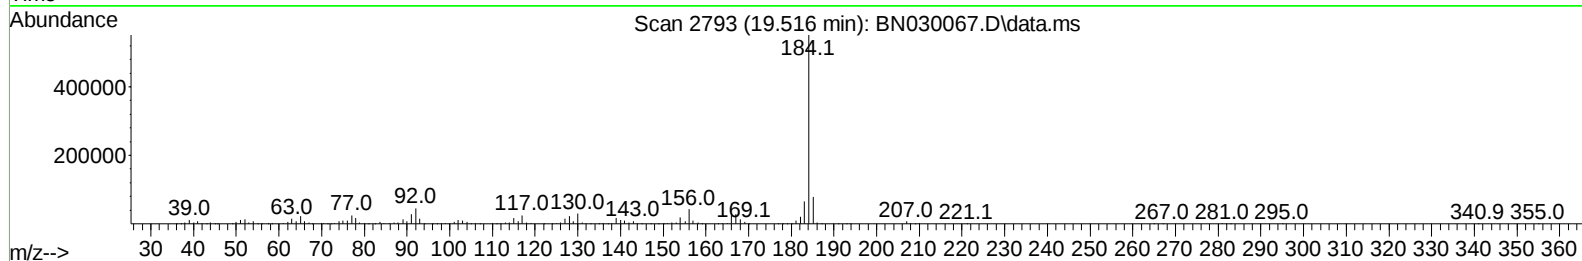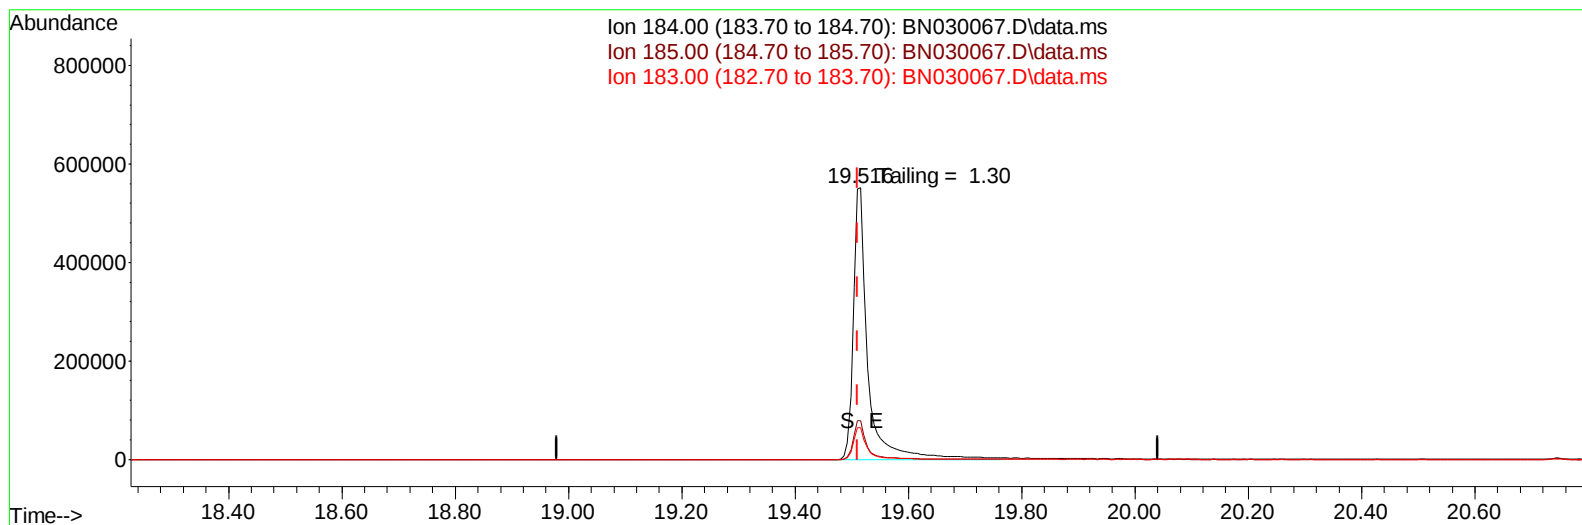

TIC: BN030067.D\data.ms

(77) Benzidine

19.516min (+ 0.006) 0.00 ng

response 992606

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.33
183.00	13.20	11.75
0.00	0.00	0.00