
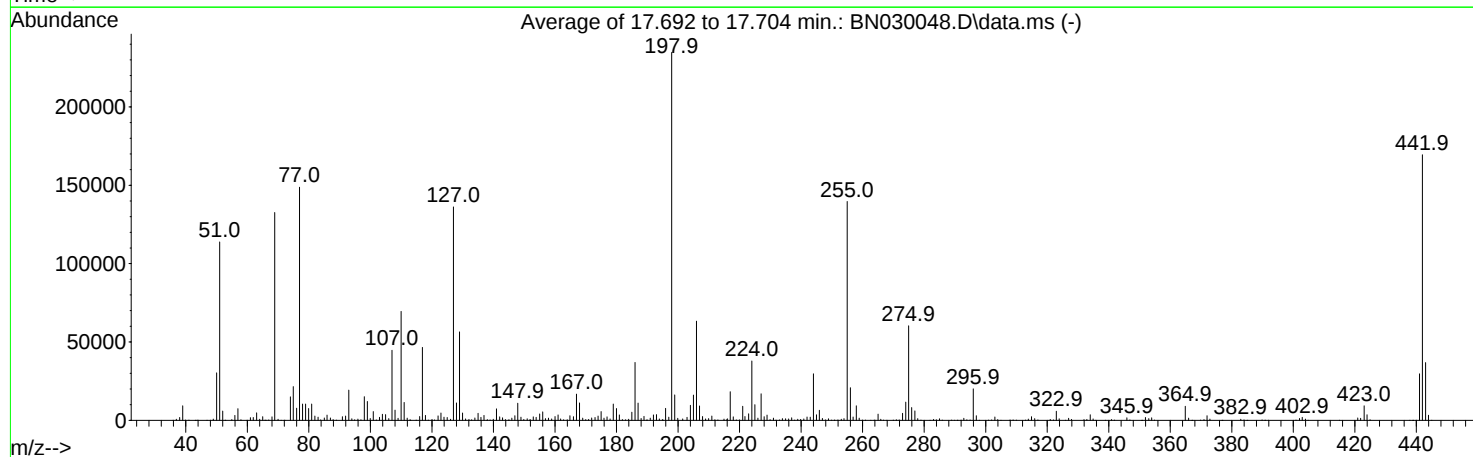


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022624\
Data File : BN030048.D
Acq On : 26 Feb 2024 09:07
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Feb 26 02:39:45 2024

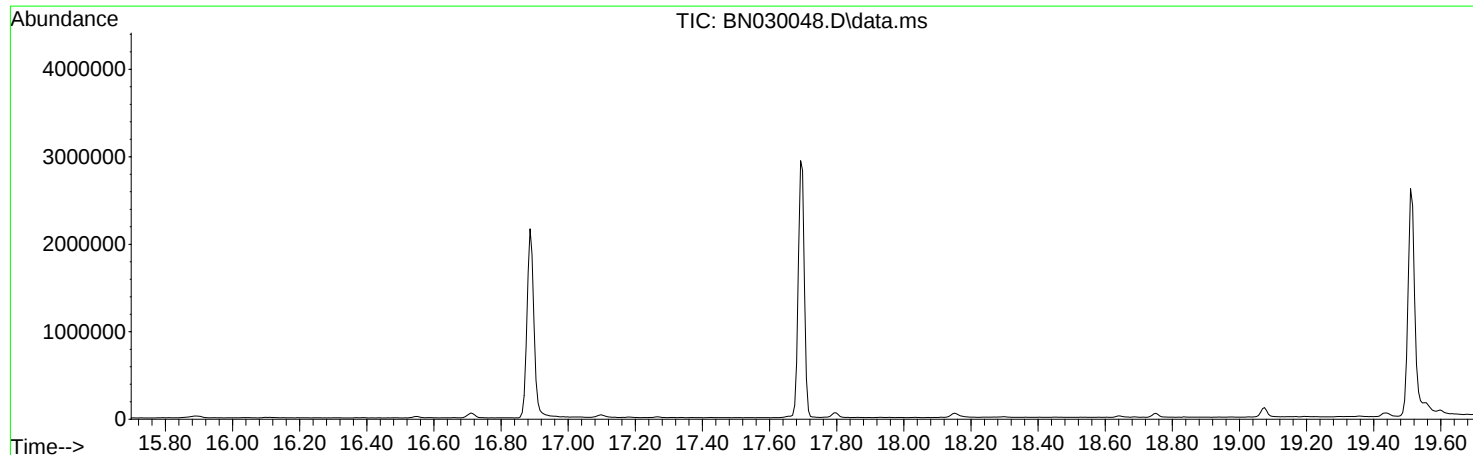




AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.5	113800	PASS
68	69	0.00	2	1.7	2300	PASS
69	198	0.00	100	56.5	132571	PASS
70	69	0.00	2	0.5	712	PASS
127	198	10	80	58.0	136157	PASS
197	198	0.00	2	0.9	2060	PASS
198	198	100	100	100.0	234709	PASS
199	198	5	9	6.9	16218	PASS
275	198	10	60	25.7	60379	PASS
365	198	1	100	3.8	9013	PASS
441	198	0.01	100	12.7	29691	PASS
442	442	50	100	100.0	169472	PASS
443	442	15	24	21.7	36811	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022624\
Data File : BN030048.D
Acq On : 26 Feb 2024 09:07
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 27 03:29:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 03:29:47 2024
Response via : Initial Calibration

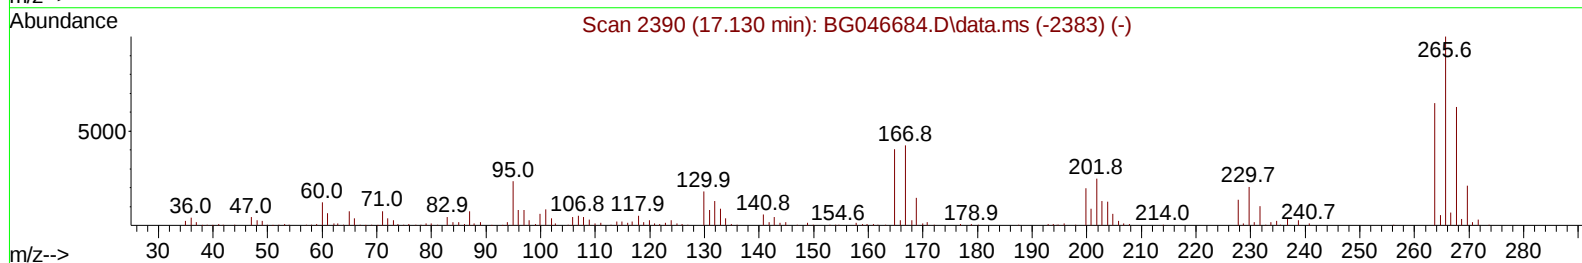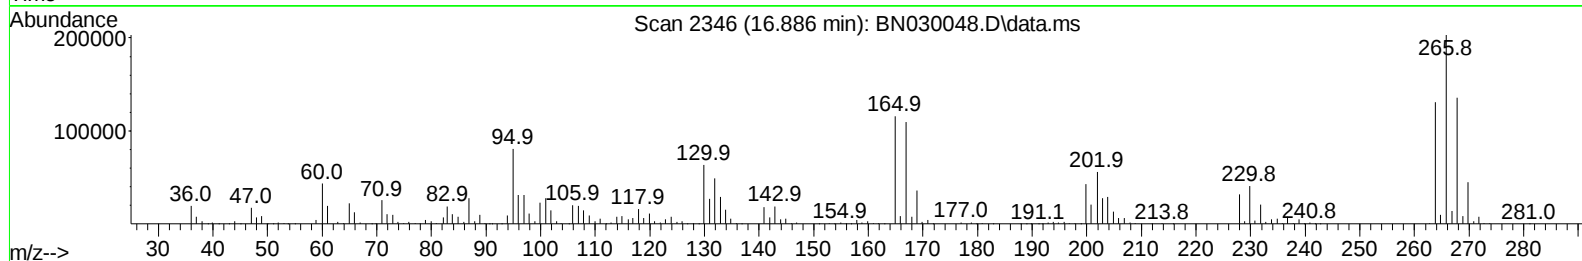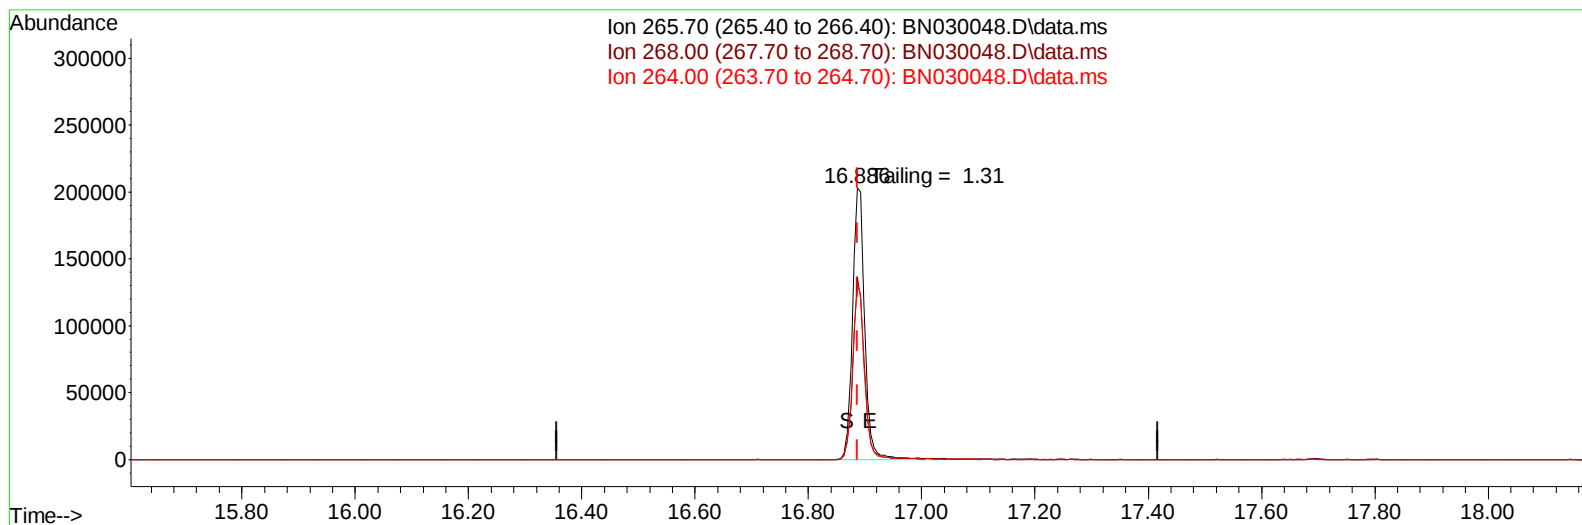

TIC: BN030048.D\data.ms

(70) Pentachlorophenol (C)

16.886min (0.000) 20807.76 ng




response 303727

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.97
264.00	61.60	64.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022624\
Data File : BN030048.D
Acq On : 26 Feb 2024 09:07
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 27 03:29:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 03:29:47 2024
Response via : Initial Calibration

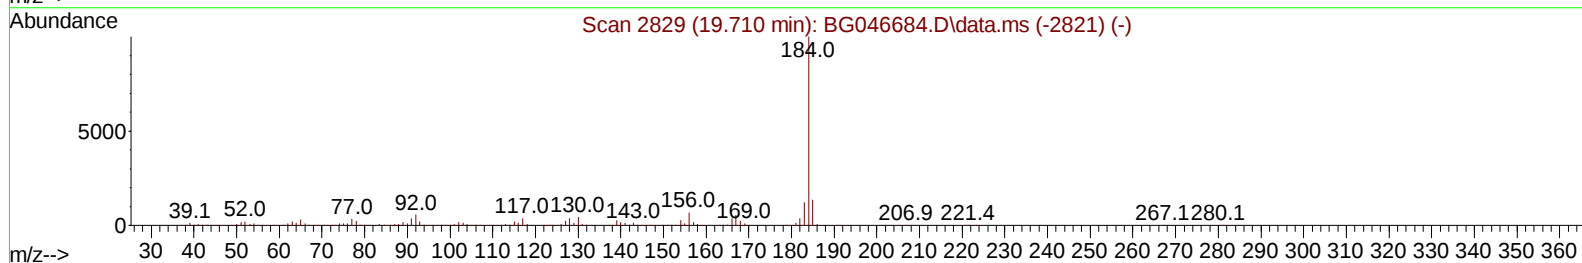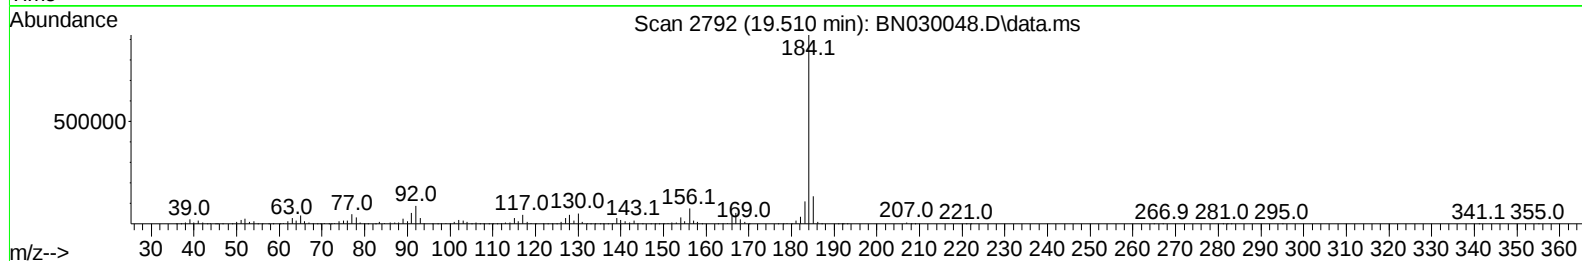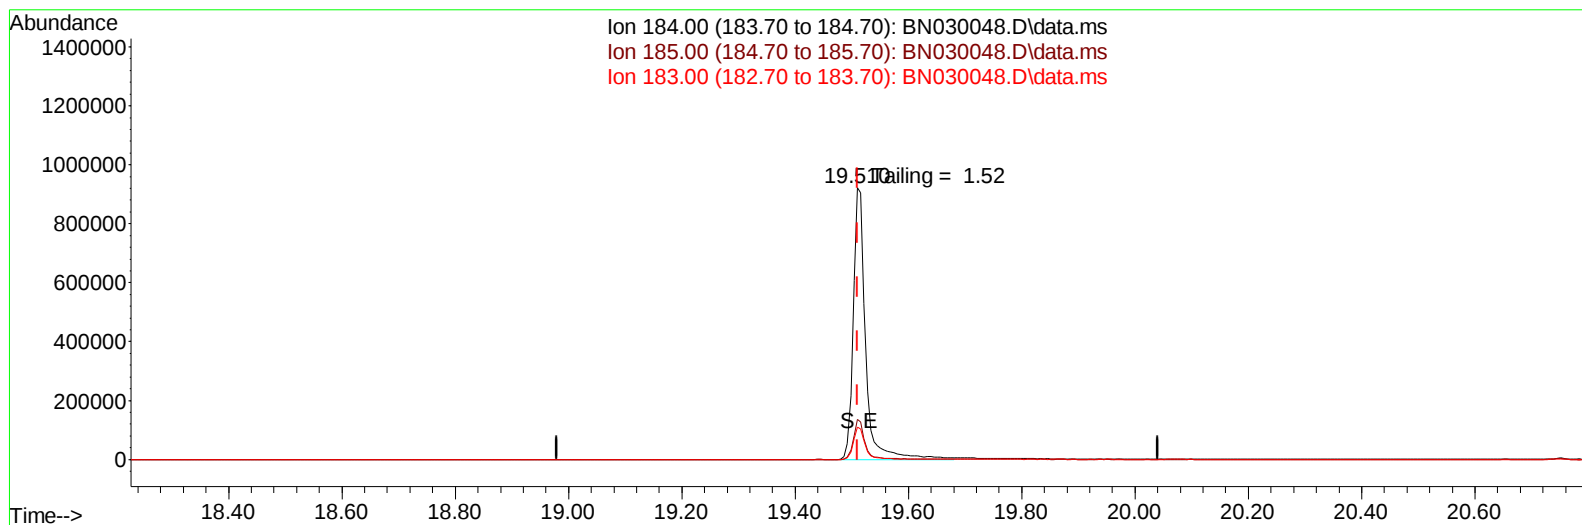

TIC: BN030048.D\data.ms

(77) Benzidine

19.510min (0.000) 0.00 ng

response 1412626

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.69
183.00	13.20	11.92
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/26/2024	BNA_N	<u>BN030048.D</u>
Compound Name	Response	Retention Time
DDT	846009	20.751
DDD	25934	20.31
DDE	1432	19.798
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27366	873375	3.13

Instrument :
BNA_N
ClientSampleId :
DFTPP