
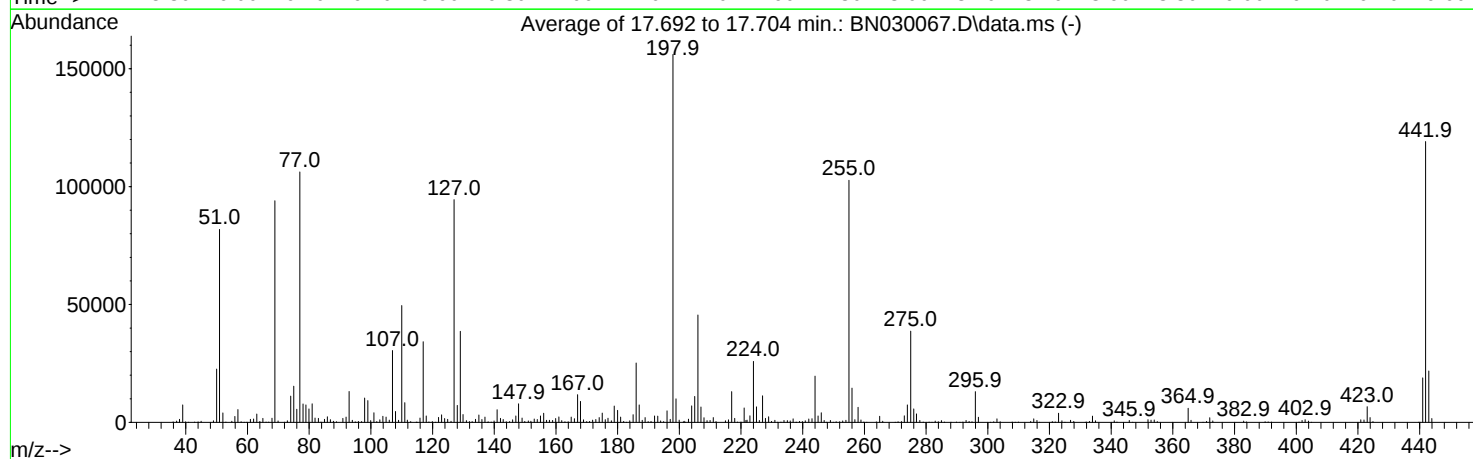


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022624\
Data File : BN030067.D
Acq On : 26 Feb 2024 21:49
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Feb 26 02:39:45 2024

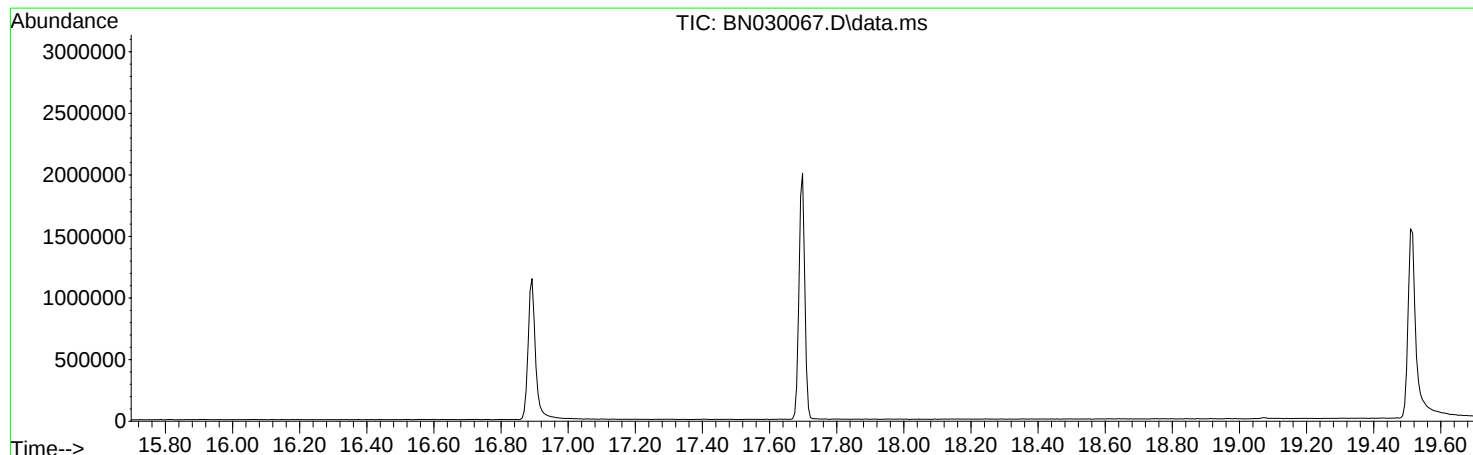




AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.5	81877	PASS
68	69	0.00	2	1.9	1752	PASS
69	198	0.00	100	60.3	94029	PASS
70	69	0.00	2	0.6	605	PASS
127	198	10	80	60.5	94461	PASS
197	198	0.00	2	0.8	1301	PASS
198	198	100	100	100.0	156056	PASS
199	198	5	9	6.4	9992	PASS
275	198	10	60	24.8	38685	PASS
365	198	1	100	3.8	5976	PASS
441	198	0.01	100	12.1	18851	PASS
442	442	50	100	100.0	119120	PASS
443	442	15	24	18.3	21803	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022624\
Data File : BN030067.D
Acq On : 26 Feb 2024 21:49
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 27 03:32:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 03:29:47 2024
Response via : Initial Calibration

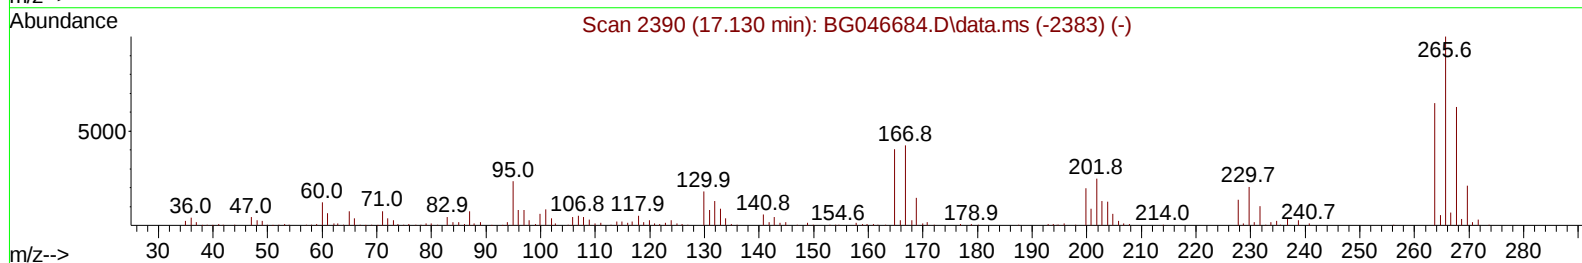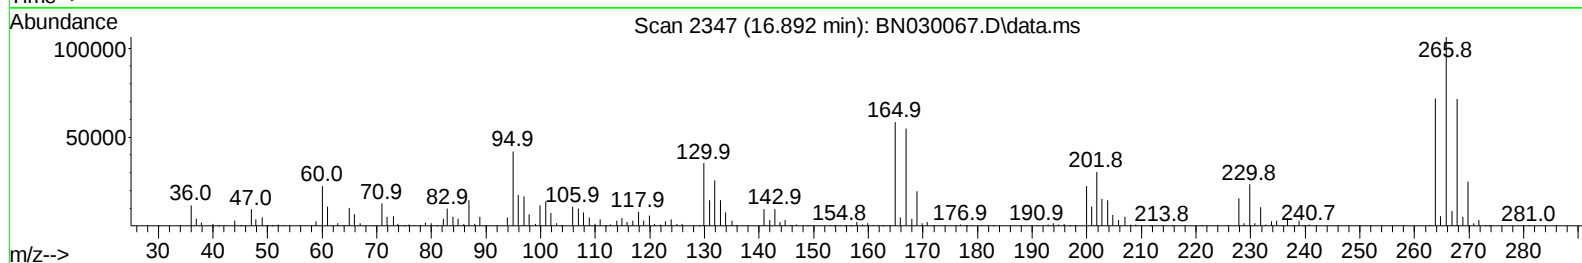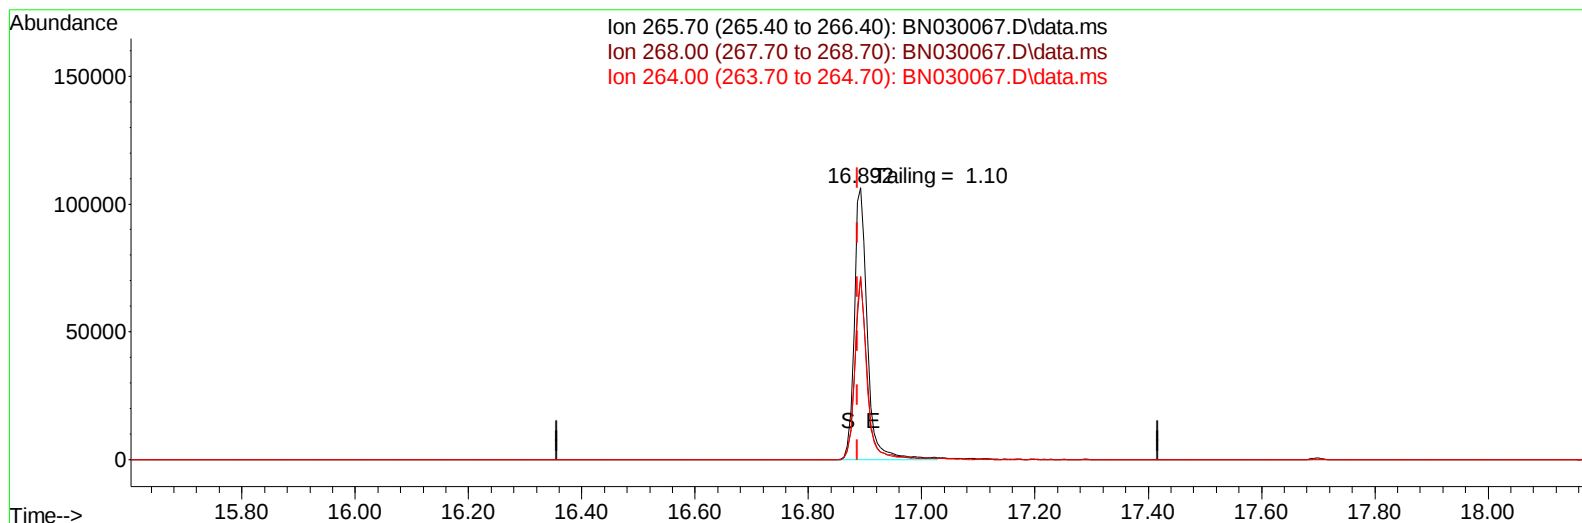

TIC: BN030067.D\data.ms

(70) Pentachlorophenol (C)

16.892min (+ 0.006) 16080.95 ng




response 169107

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.26
264.00	61.60	67.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022624\
Data File : BN030067.D
Acq On : 26 Feb 2024 21:49
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 27 03:32:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 03:29:47 2024
Response via : Initial Calibration

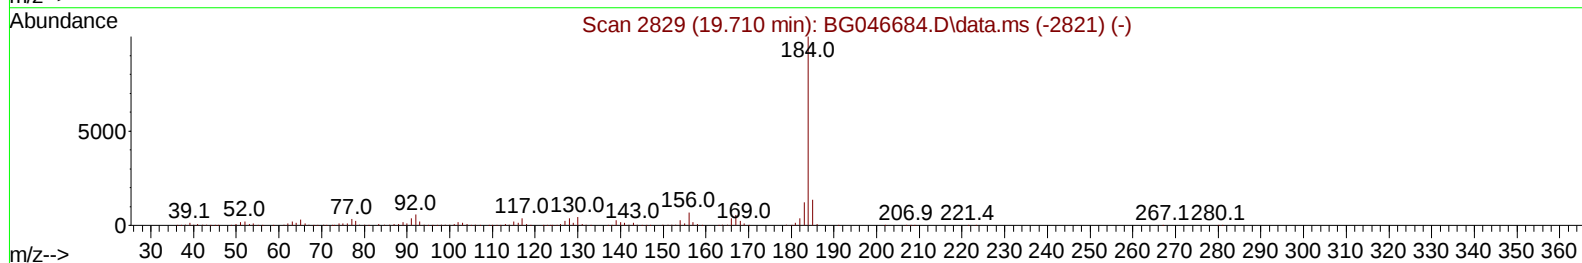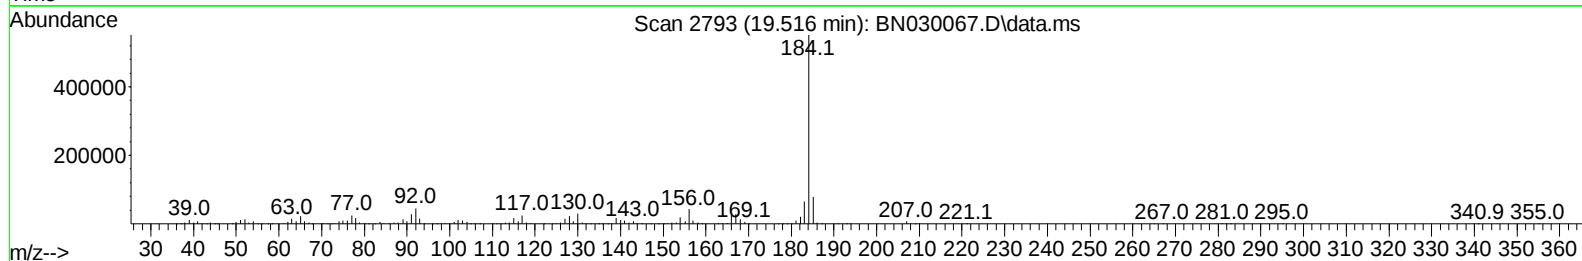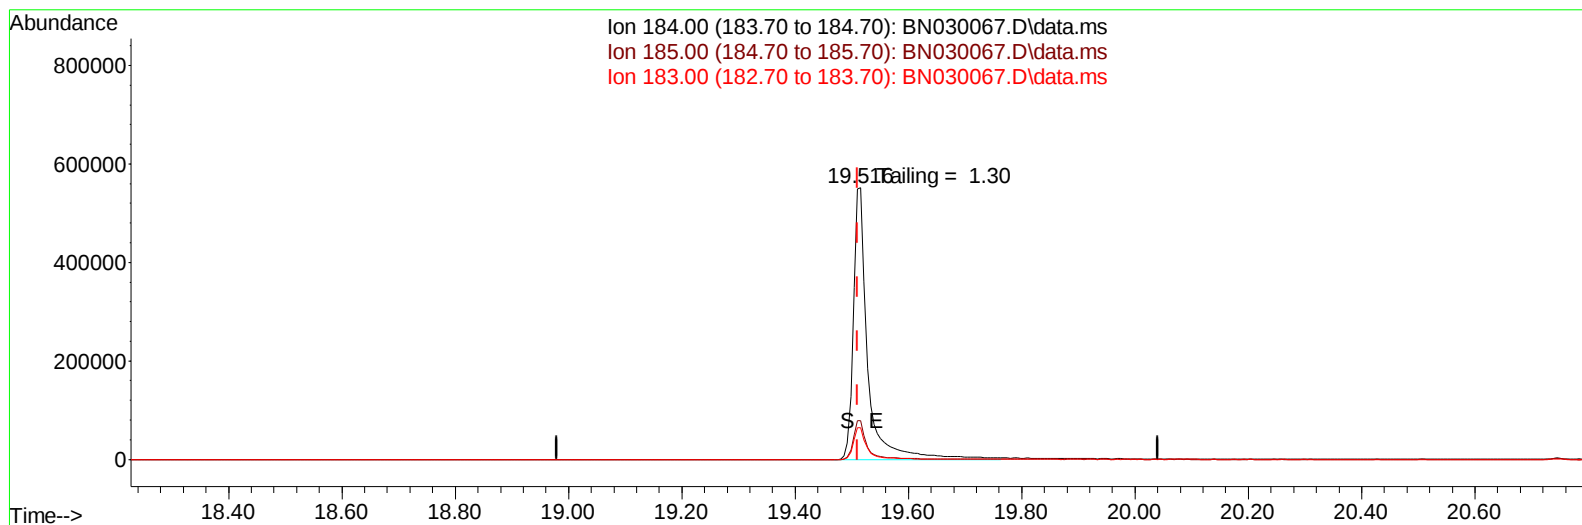

TIC: BN030067.D\data.ms

(77) Benzidine

19.516min (+ 0.006) 0.00 ng

response 992606

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.33
183.00	13.20	11.75
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/26/2024	BNA_N	<u>BN030067.D</u>
Compound Name	Response	Retention Time
DDT	528408	20.745
DDD	17354	20.304
DDE	1219	19.792
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18573	546981	3.40

Instrument :
BNA_N
ClientSampleId :
DFTPP