Quantitation Report (Not Reviewed)

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022625\
Data File : BN036508.D
Acq On : 26 Feb 2025 13:43
Operator : RC/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Quant Time: Feb 26 14:09:37 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN021025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 11 01:17:14 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.739	152	2772	0.400	ng	-0.01
7) Naphthalene-d8	10.530	136	6909	0.400	ng	#-0.01
13) Acenaphthene-d10	14.377	164	4680	0.400	ng	-0.01
19) Phenanthrene-d10	17.124	188	9092	0.400	ng	-0.01
29) Chrysene-d12	21.313	240	6639	0.400	ng	0.00
35) Perylene-d12	23.581	264	6000	0.400	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.334	112	2377	0.363	ng	-0.01
5) Phenol-d6	6.915	99	2776	0.361	ng	-0.02
8) Nitrobenzene-d5	8.886	82	2668	0.391	ng	-0.02
11) 2-Methylnaphthalene-d10	12.126	152	4099	0.386	ng	-0.02
14) 2,4,6-Tribromophenol	15.870	330	719	0.310	ng	-0.01
15) 2-Fluorobiphenyl	13.003	172	7811	0.444	ng	-0.02
27) Fluoranthene-d10	19.160	212	9278	0.367	ng	0.00
31) Terphenyl-d14	19.764	244	6045	0.427	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.261	88	1294	0.427	ng	97
3) n-Nitrosodimethylamine	3.564	42	2267	0.430	ng	92
6) bis(2-Chloroethyl)ether	7.161	93	3244	0.404	ng	98
9) Naphthalene	10.573	128	7777	0.390	ng	99
10) Hexachlorobutadiene	10.872	225	1886	0.389	ng	# 98
12) 2-Methylnaphthalene	12.197	142	5047	0.386	ng	99
16) Acenaphthylene	14.099	152	7894	0.382	ng	99
17) Acenaphthene	14.441	154	5057	0.366	ng	99
18) Fluorene	15.425	166	7106	0.362	ng	100
20) 4,6-Dinitro-2-methylph...	15.510	198	548	0.307	ng	92
21) 4-Bromophenyl-phenylether	16.317	248	2189	0.404	ng	98
22) Hexachlorobenzene	16.441	284	2720	0.406	ng	95
23) Atrazine	16.602	200	1700	0.375	ng	98
24) Pentachlorophenol	16.789	266	1101	0.346	ng	98
25) Phenanthrene	17.161	178	10441	0.397	ng	99
26) Anthracene	17.260	178	9164	0.395	ng	99
28) Fluoranthene	19.188	202	11838	0.367	ng	99
30) Pyrene	19.550	202	11970	0.468	ng	100
32) Benzo(a)anthracene	21.295	228	8384	0.384	ng	98
33) Chrysene	21.349	228	9942	0.420	ng	99
34) Bis(2-ethylhexyl)phtha...	21.232	149	6526	0.479	ng	100
36) Indeno(1,2,3-cd)pyrene	25.879	276	7809	0.372	ng	98
37) Benzo(b)fluoranthene	22.943	252	8277	0.419	ng	99
38) Benzo(k)fluoranthene	22.943	252	8277	0.407	ng	100
39) Benzo(a)pyrene	23.481	252	7264	0.421	ng	# 90
40) Dibenzo(a,h)anthracene	25.896	278	5914	0.357	ng	98
41) Benzo(g,h,i)perylene	26.572	276	6890	0.367	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Not Reviewed)

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022625\
Data File : BN036508.D
Acq On : 26 Feb 2025 13:43
Operator : RC/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Quant Time: Feb 26 14:09:37 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN021025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 11 01:17:14 2025
Response via : Initial Calibration

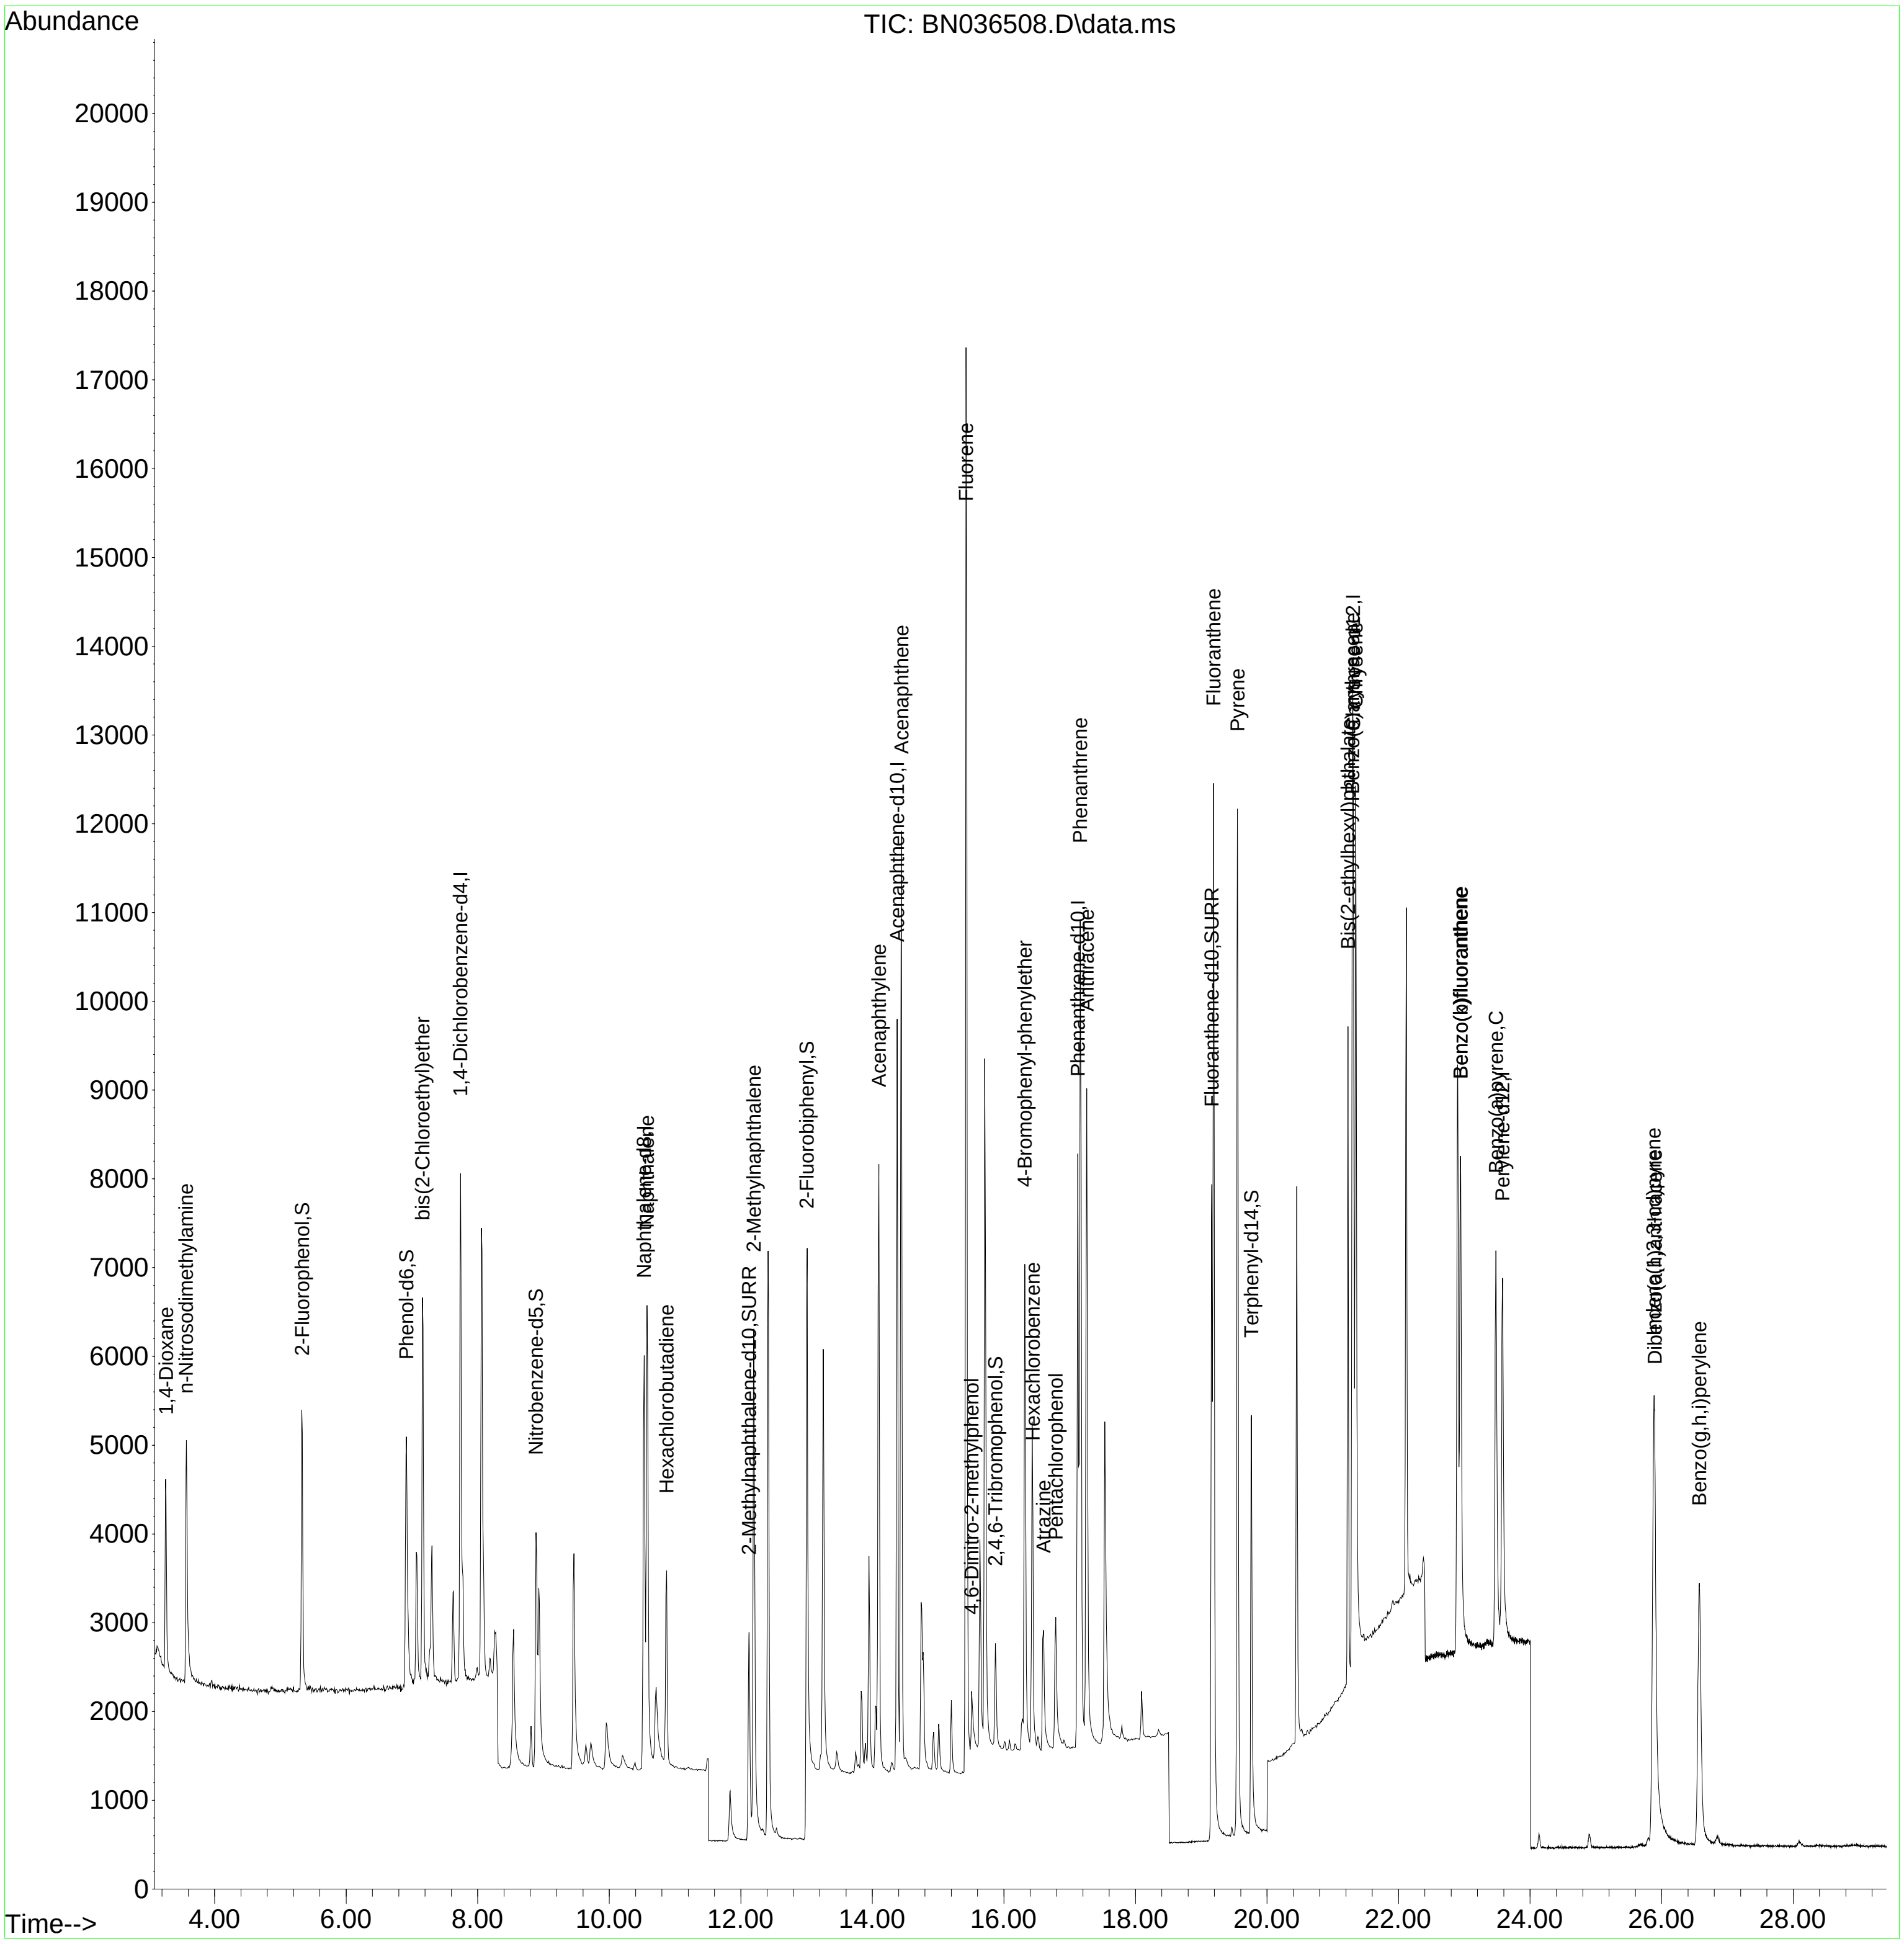

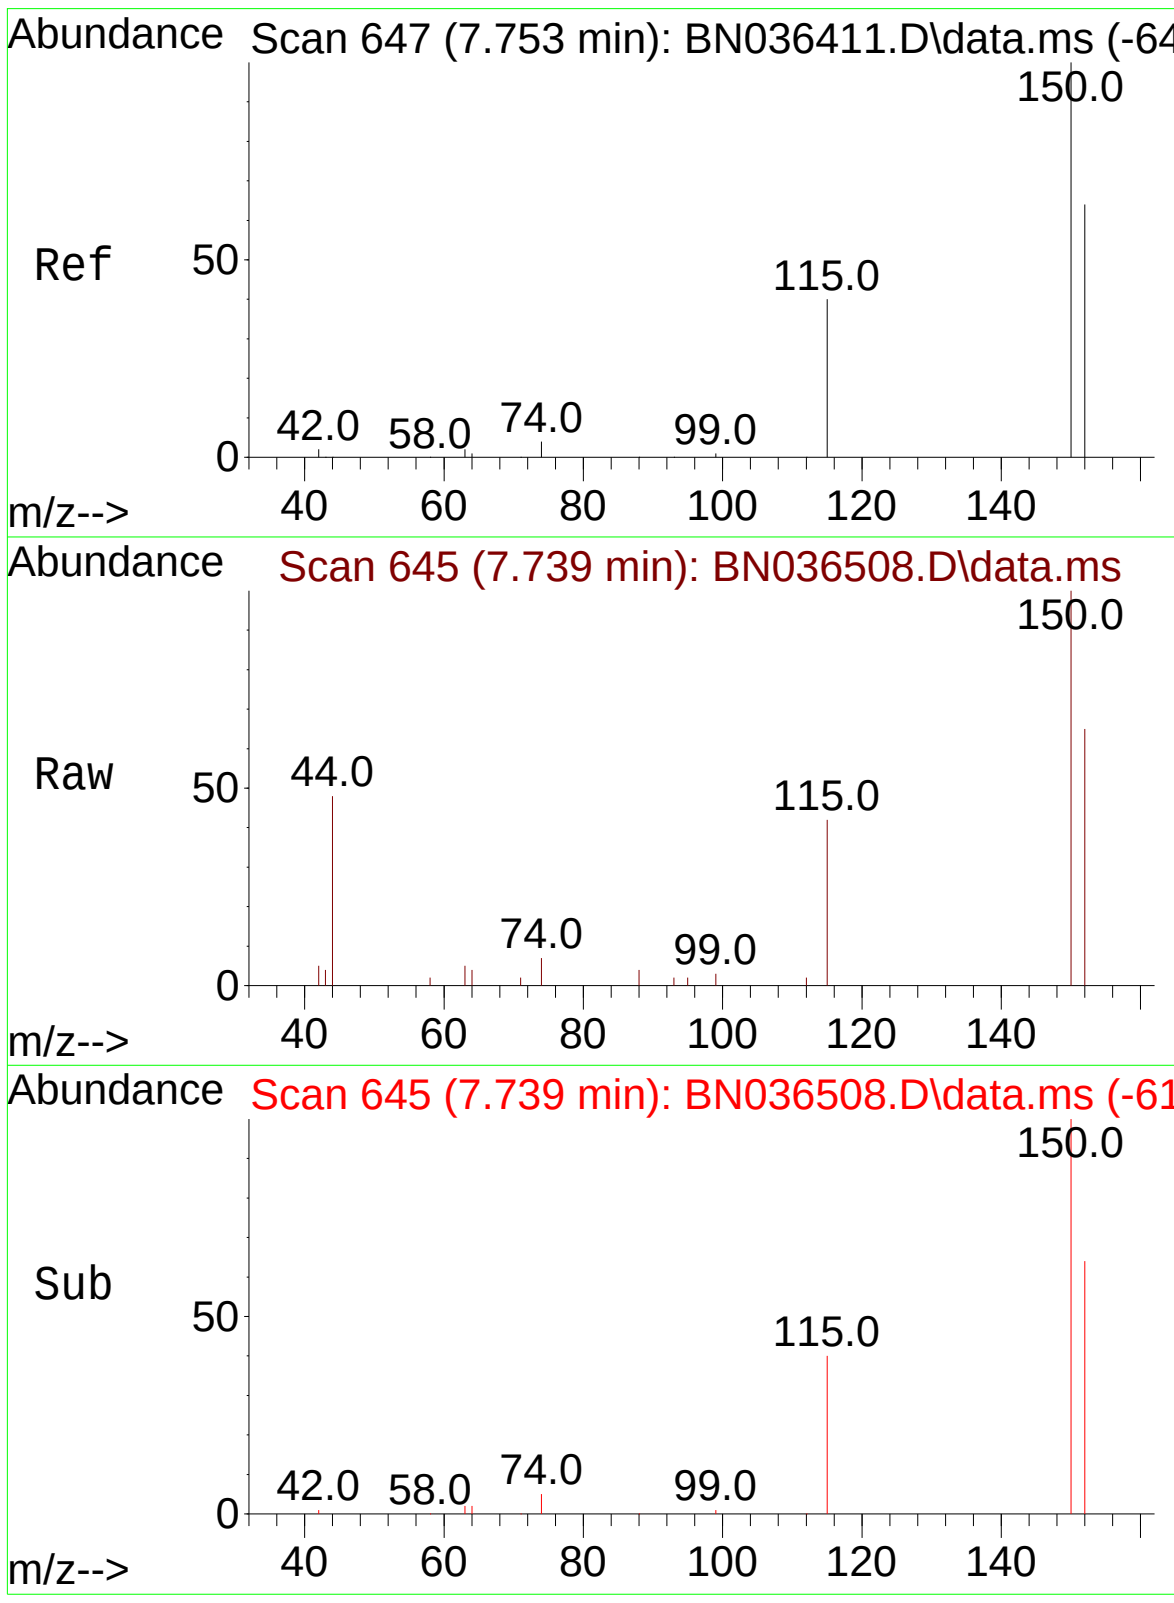

#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.739 min Scan# 64
Delta R.T. -0.014 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:152 Resp: 2772

Ion	Ratio	Lower	Upper
152	100		
150	153.8	123.7	185.5
115	65.1	52.5	78.7

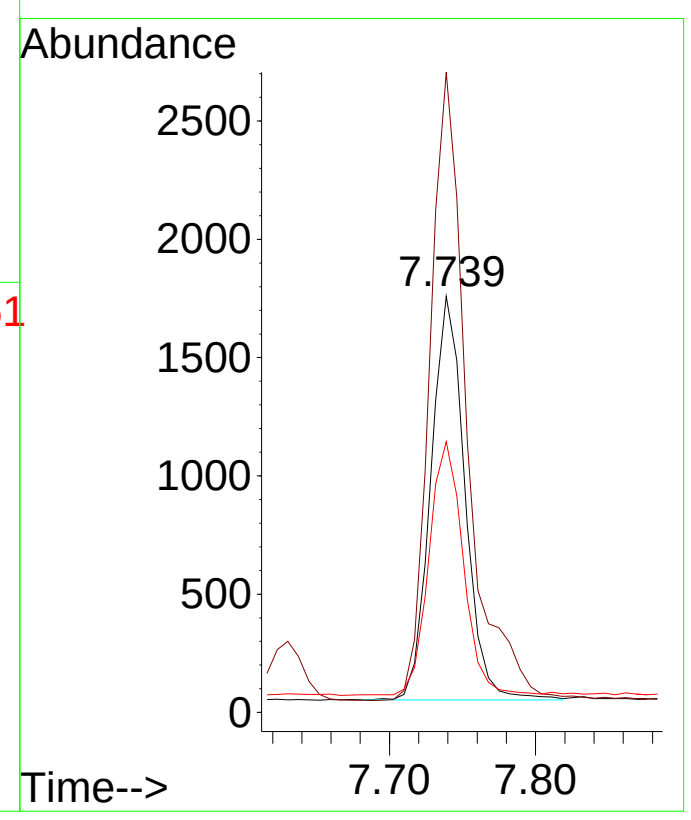

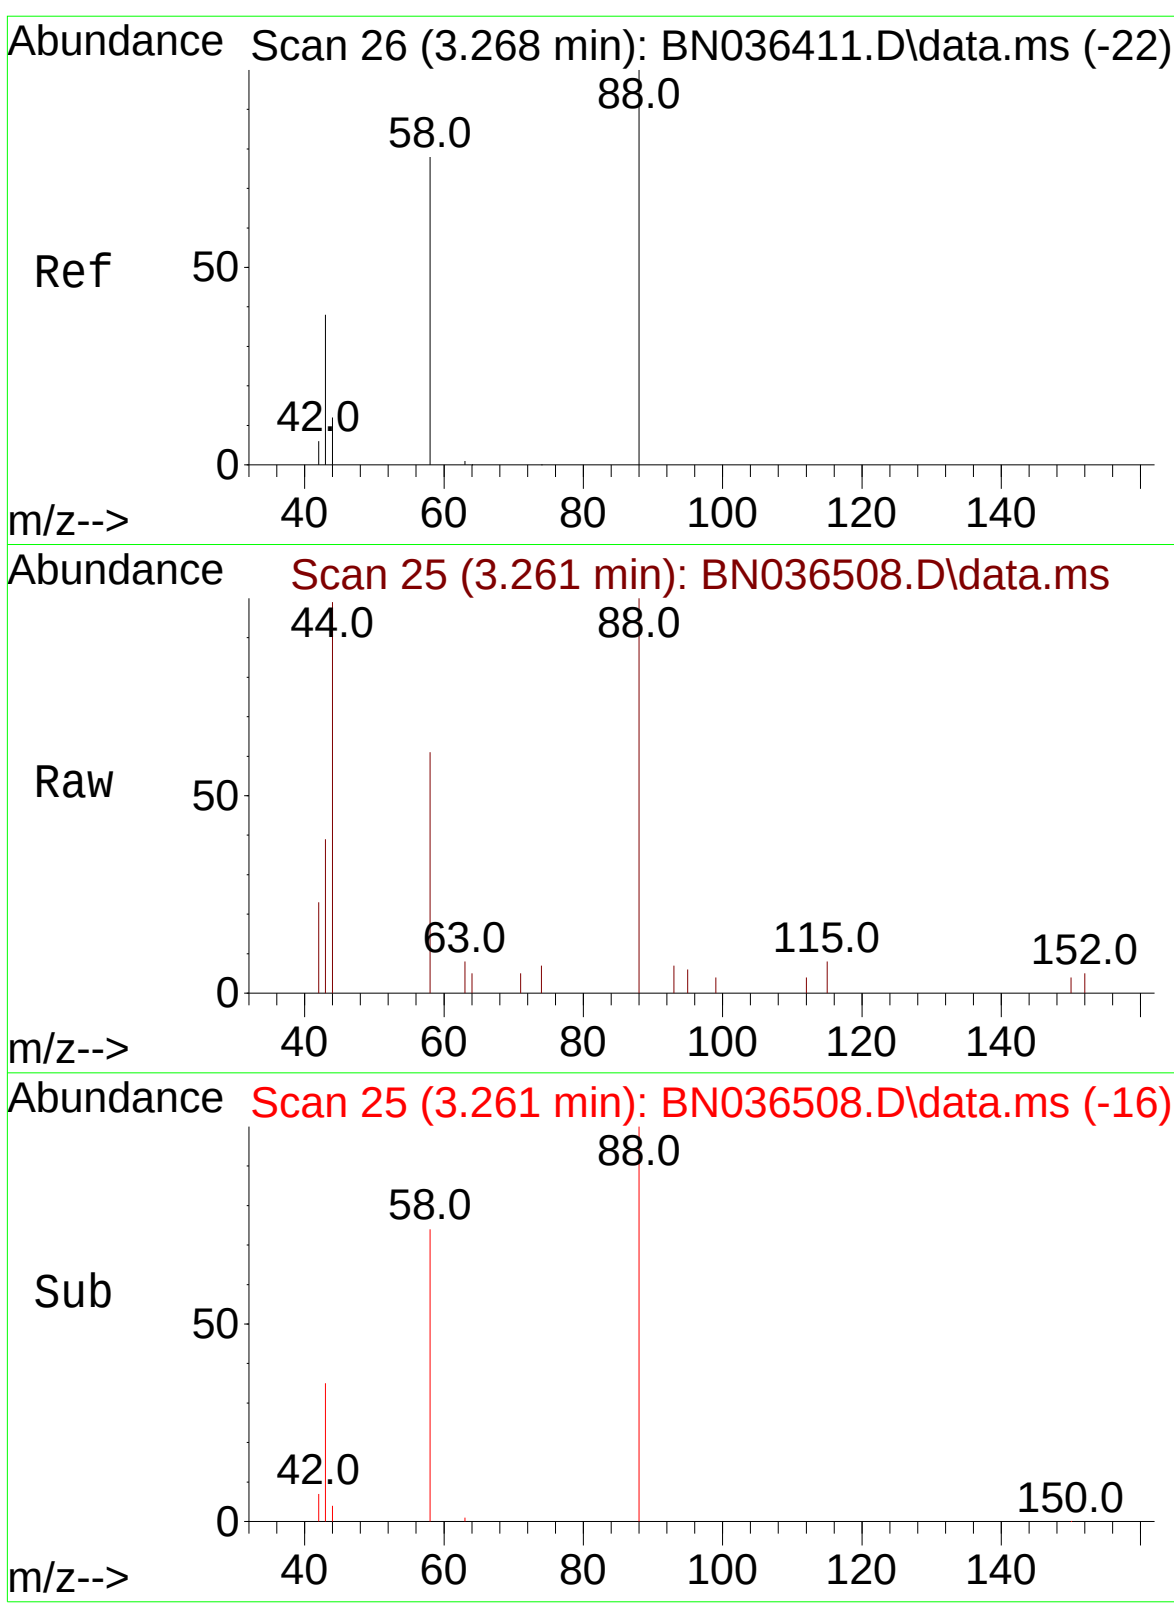

#2
1,4-Dioxane
Concen: 0.427 ng
RT: 3.261 min Scan# 25
Delta R.T. -0.007 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Tgt Ion: 88 Resp: 1294

Ion	Ratio	Lower	Upper
88	100		
43	40.8	33.7	50.5
58	82.4	68.9	103.3

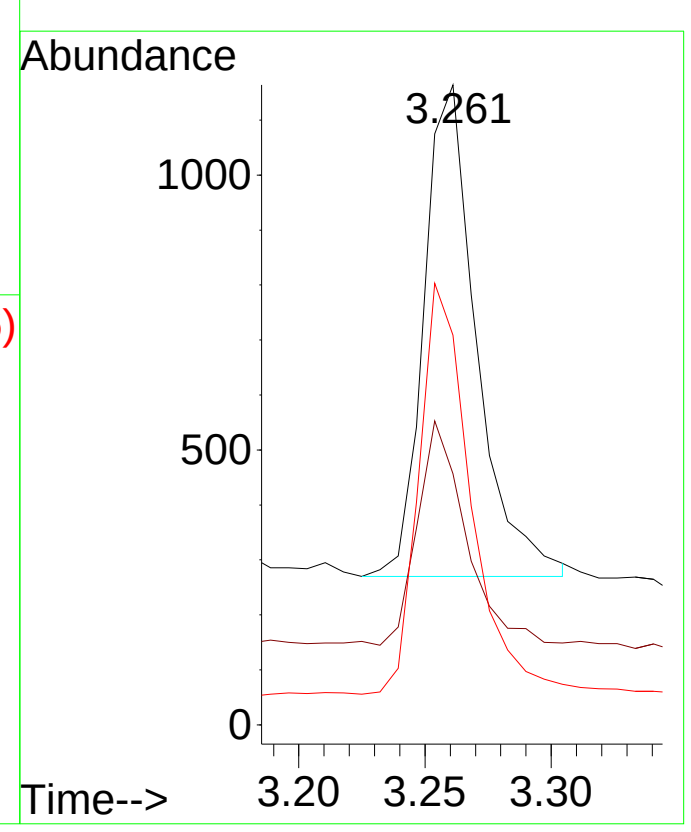

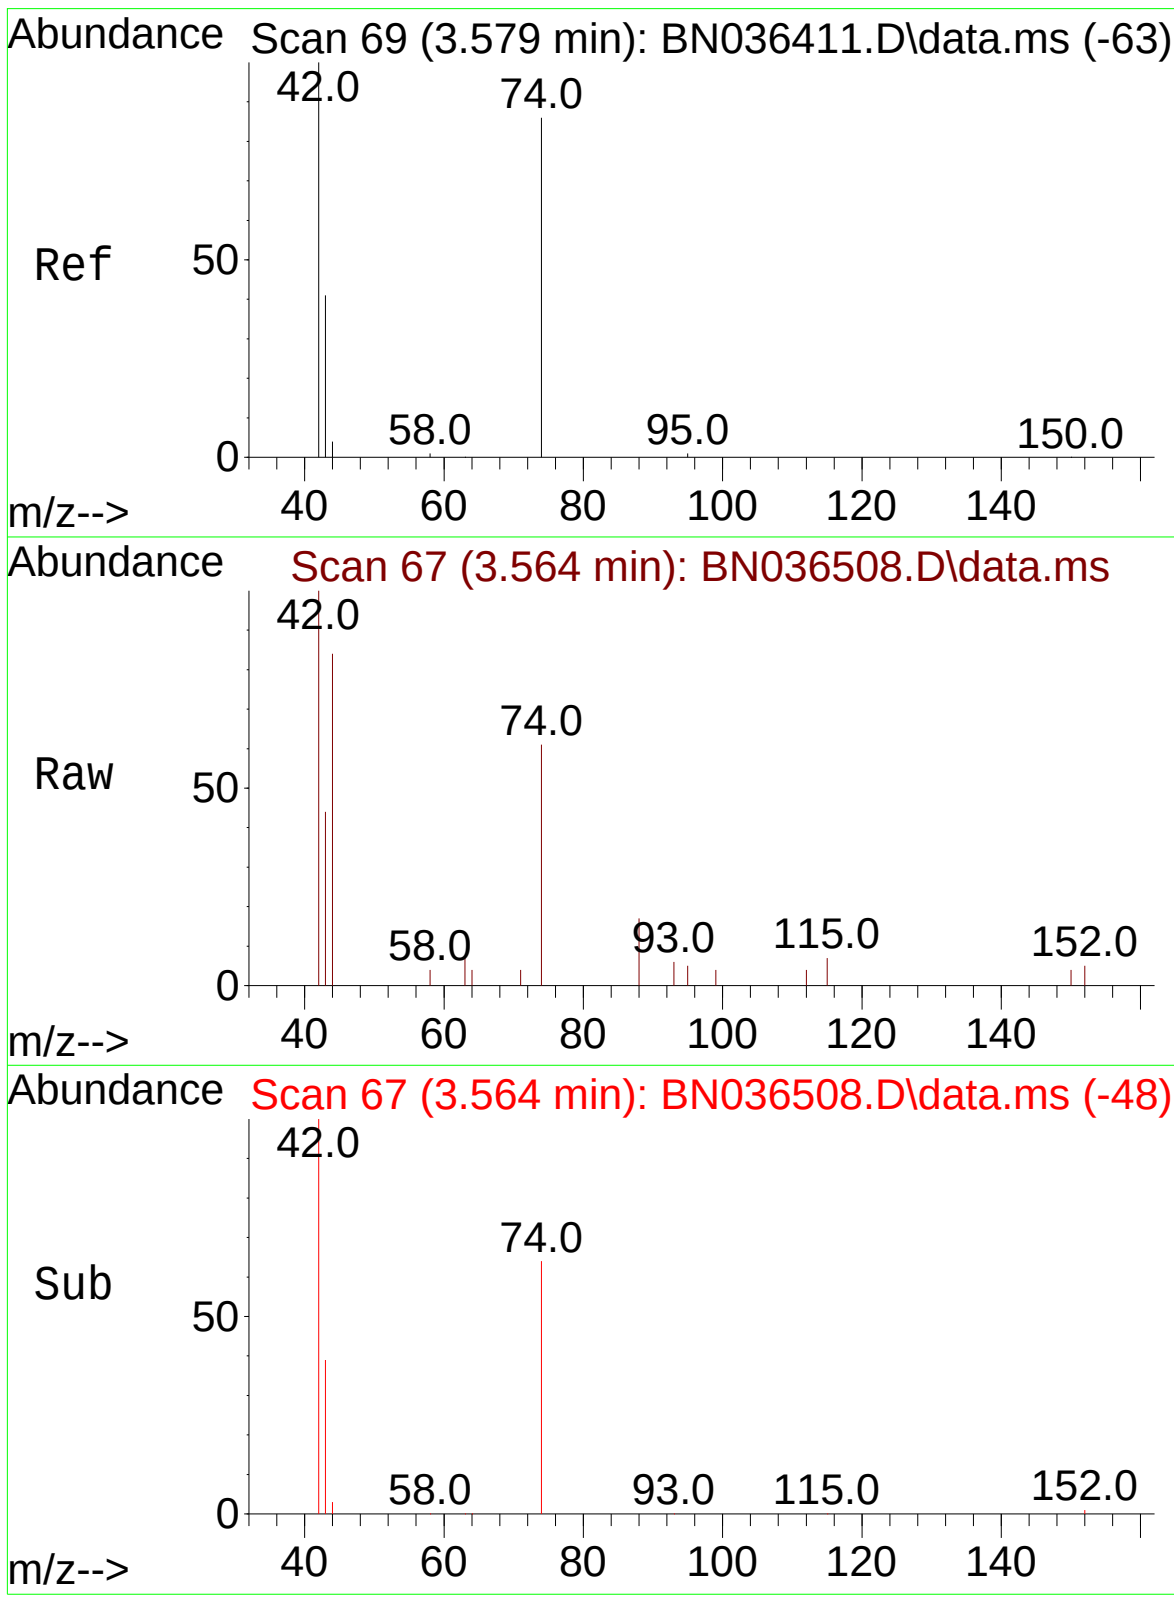

#3
n-Nitrosodimethylamine
Concen: 0.430 ng
RT: 3.564 min Scan# 6

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Delta R.T. -0.014 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Tgt Ion: 42 Resp: 2267

Ion	Ratio	Lower	Upper
42	100		
74	81.6	71.8	107.6
44	8.6	7.8	11.6

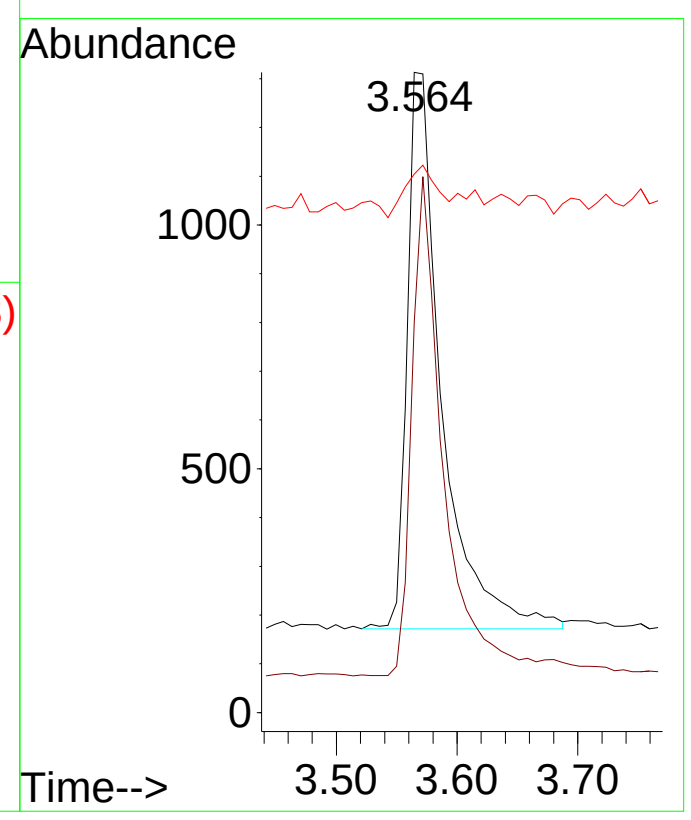

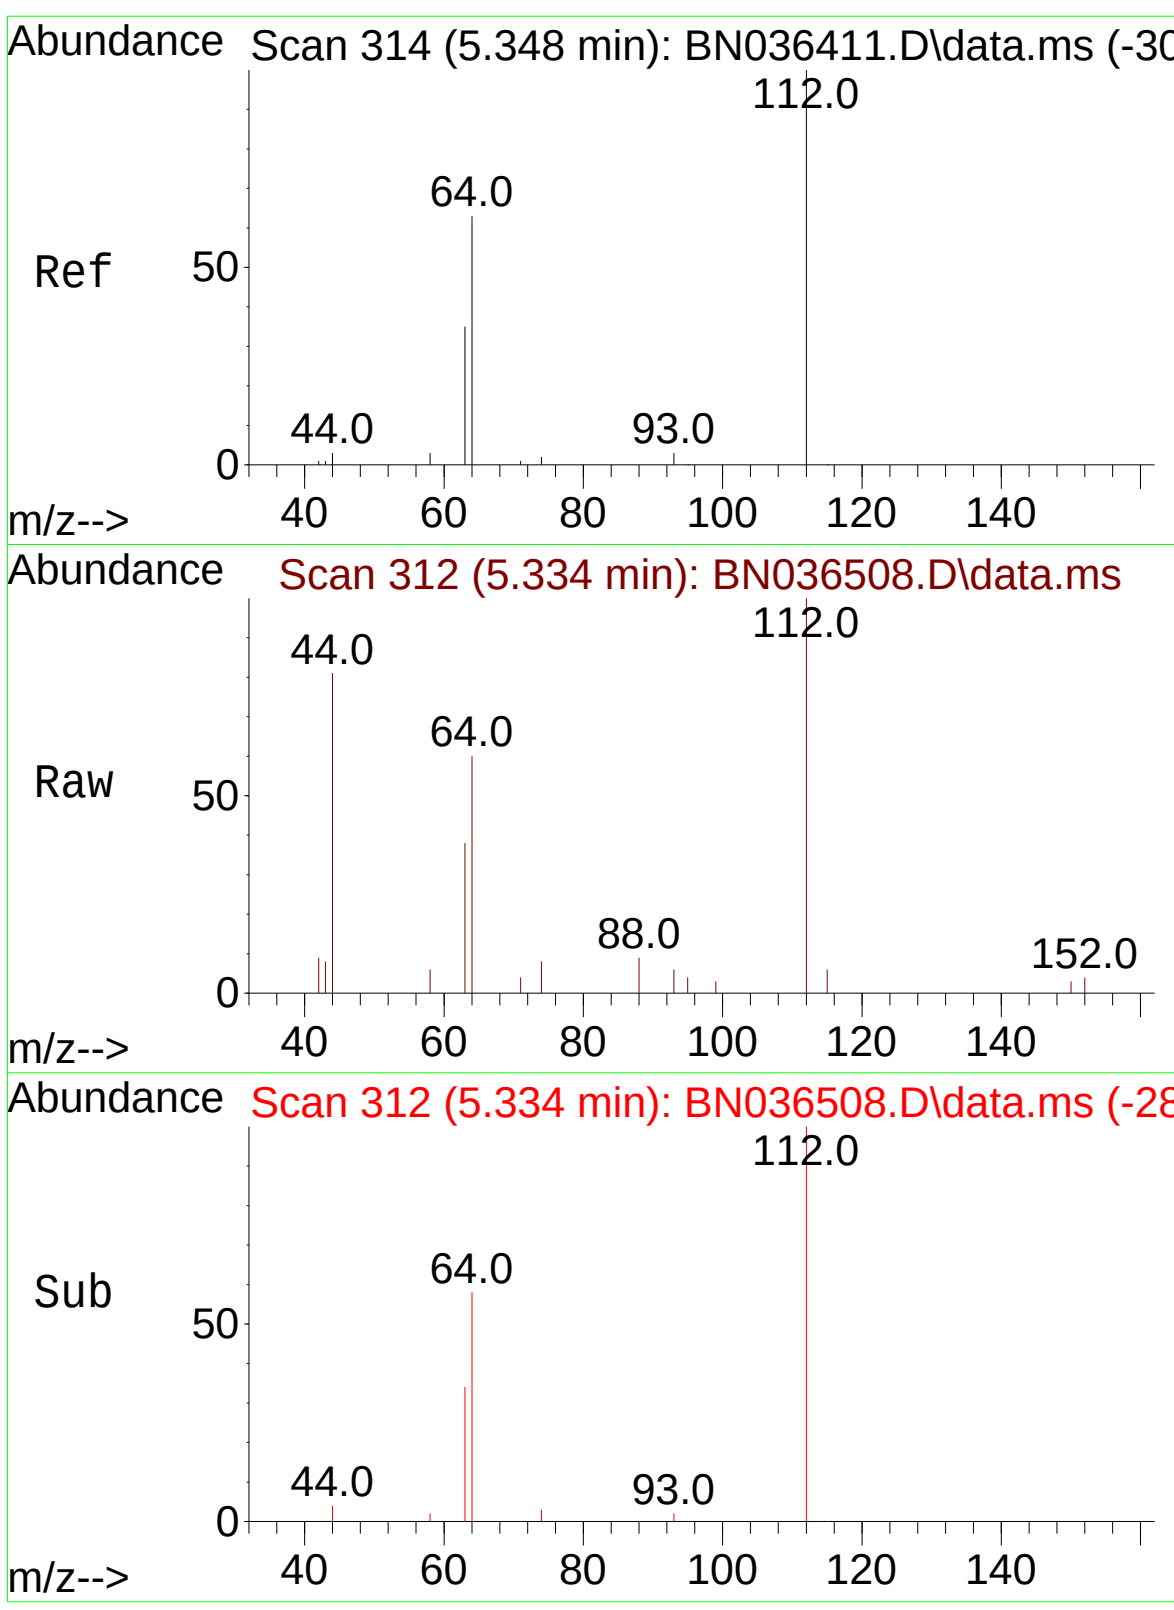

#4
2-Fluorophenol
Concen: 0.363 ng
RT: 5.334 min Scan# 312
Delta R.T. -0.014 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Tgt Ion:112 Resp: 2377

Ion	Ratio	Lower	Upper
112	100		
64	67.5	53.4	80.0
63	40.8	30.3	45.5

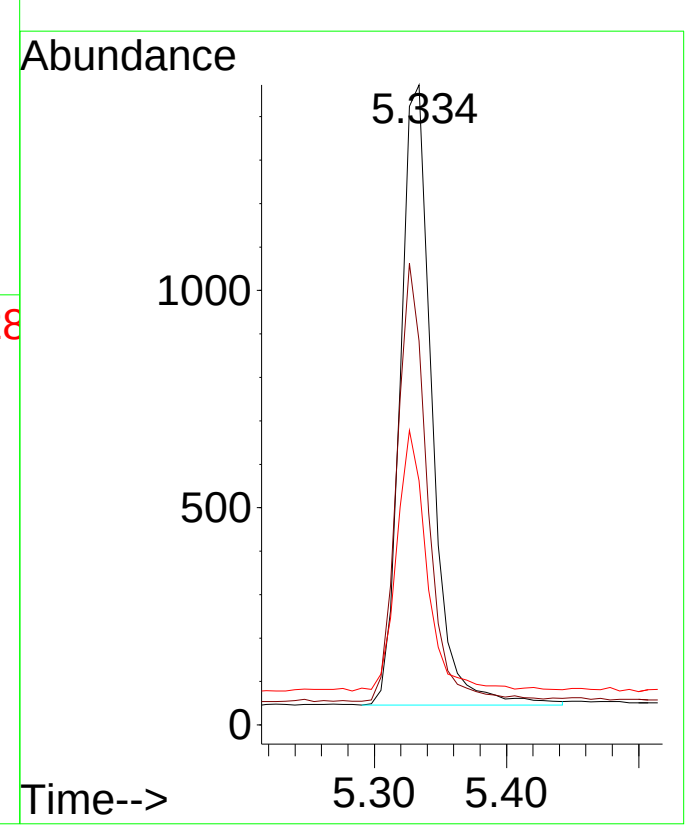

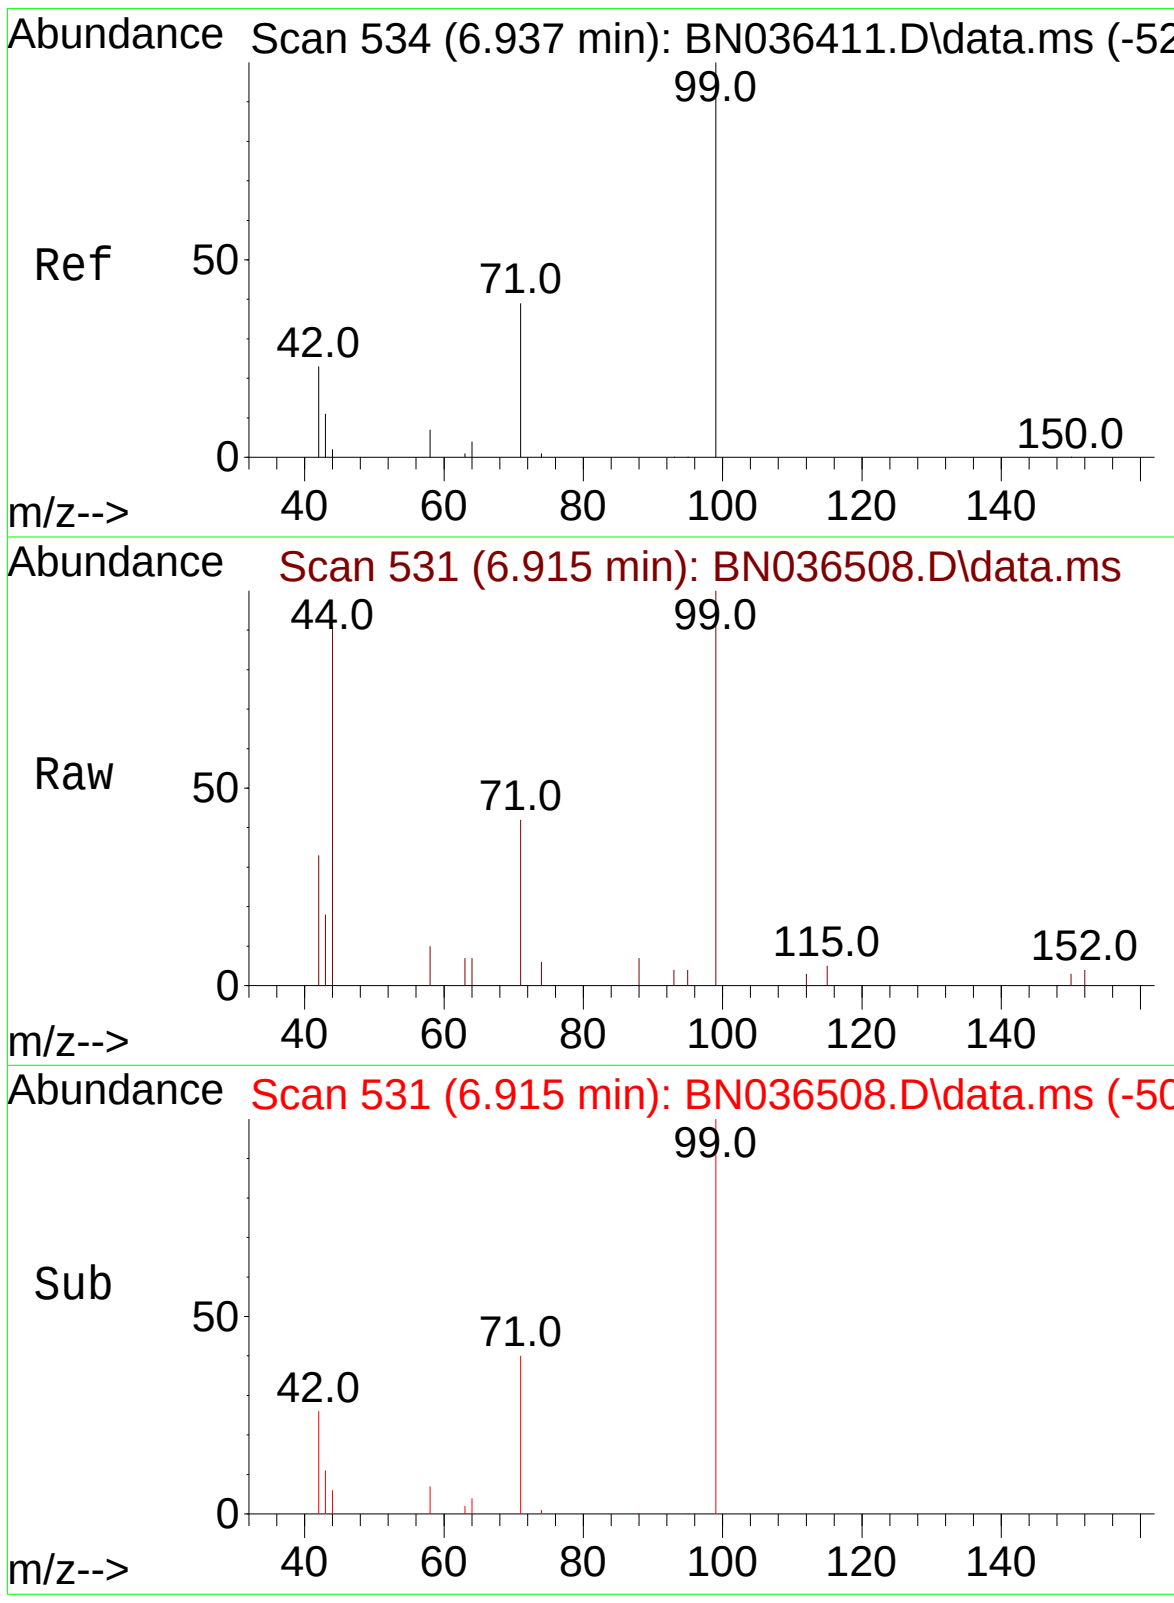

#5
Phenol-d6
Concen: 0.361 ng
RT: 6.915 min   Scan# 5

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Delta R.T.   -0.022 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Tgt Ion: 99 Resp: 2776

Ion	Ratio	Lower	Upper
99	100		
42	30.0	21.7	32.5
71	40.6	32.6	49.0

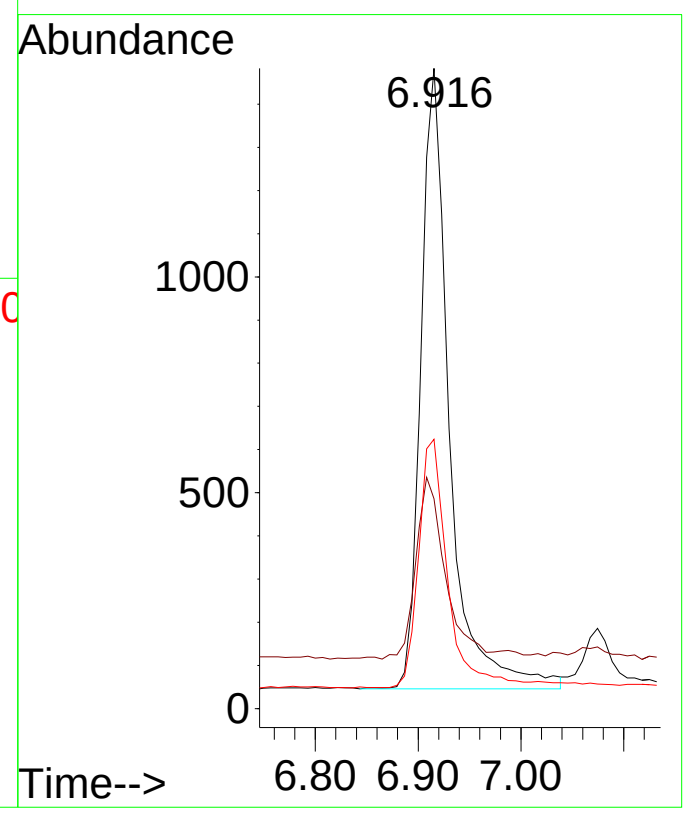

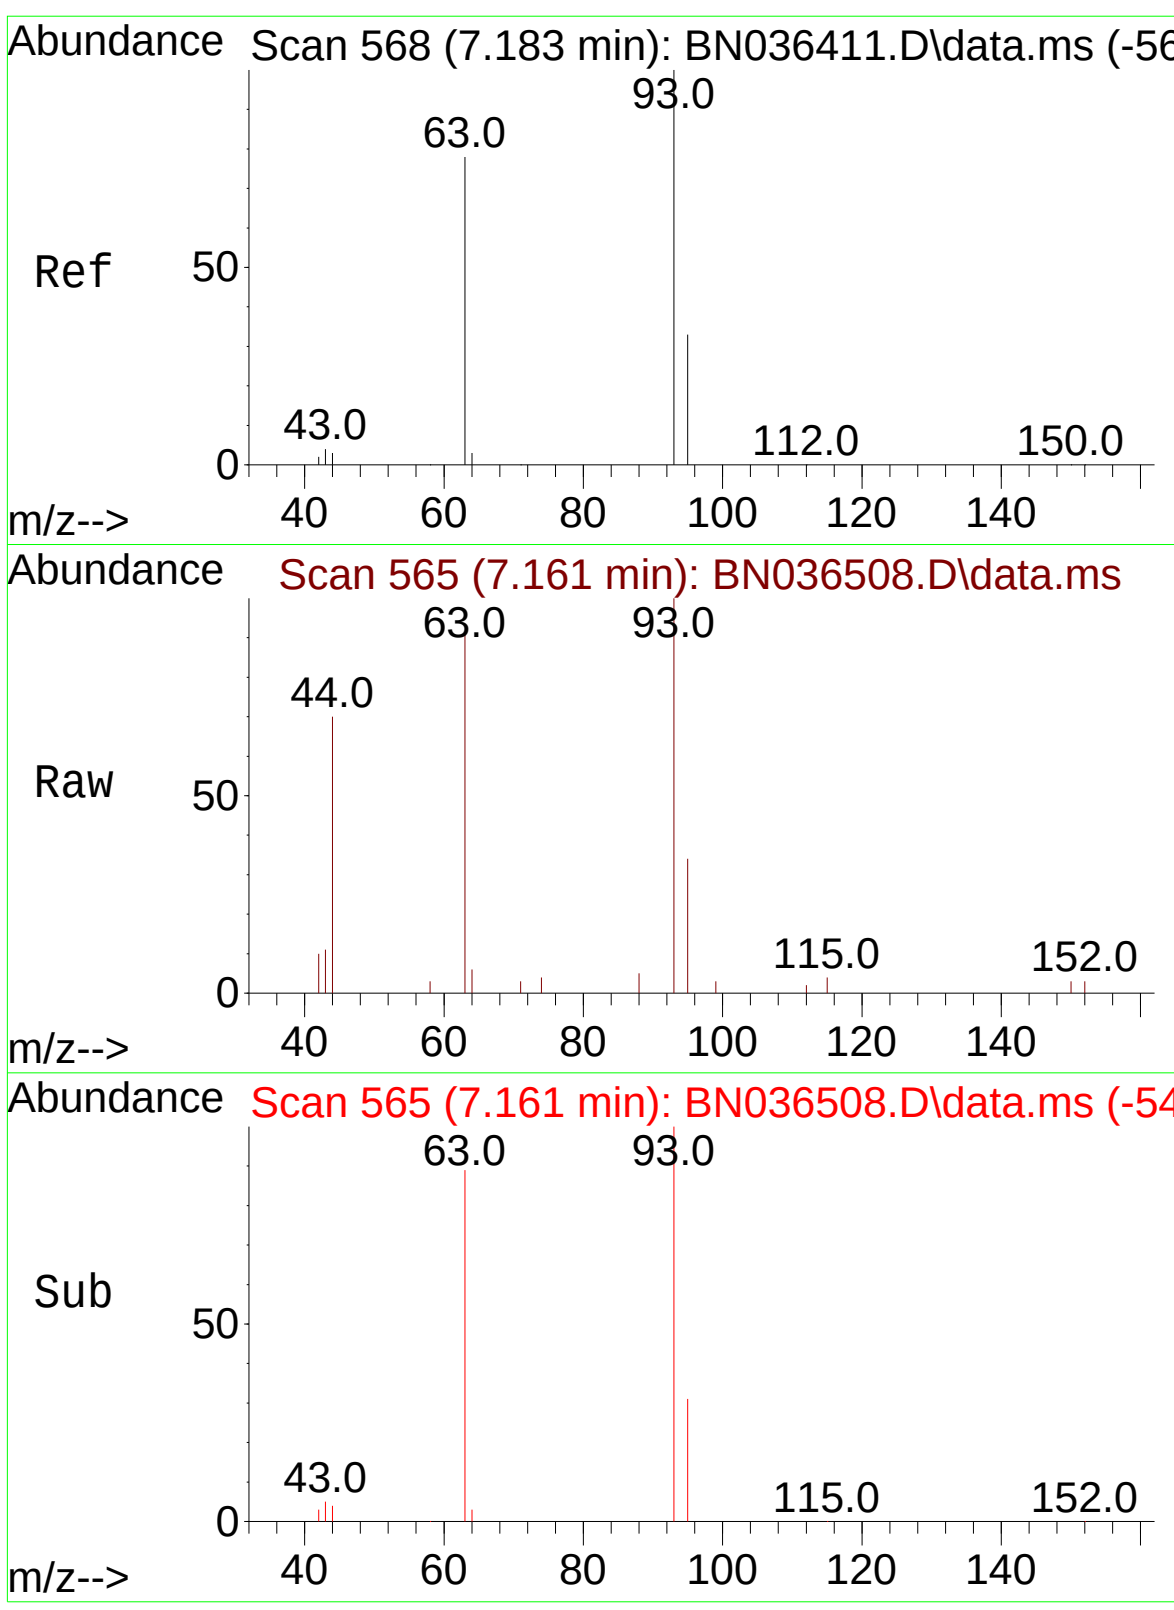

#6
bis(2-Chloroethyl)ether
Concen: 0.404 ng
RT: 7.161 min   Scan# 565
Delta R.T.   -0.022 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Tgt Ion: 93 Resp: 3244

Ion	Ratio	Lower	Upper
93	100		
63	83.8	66.3	99.5
95	31.1	26.2	39.4

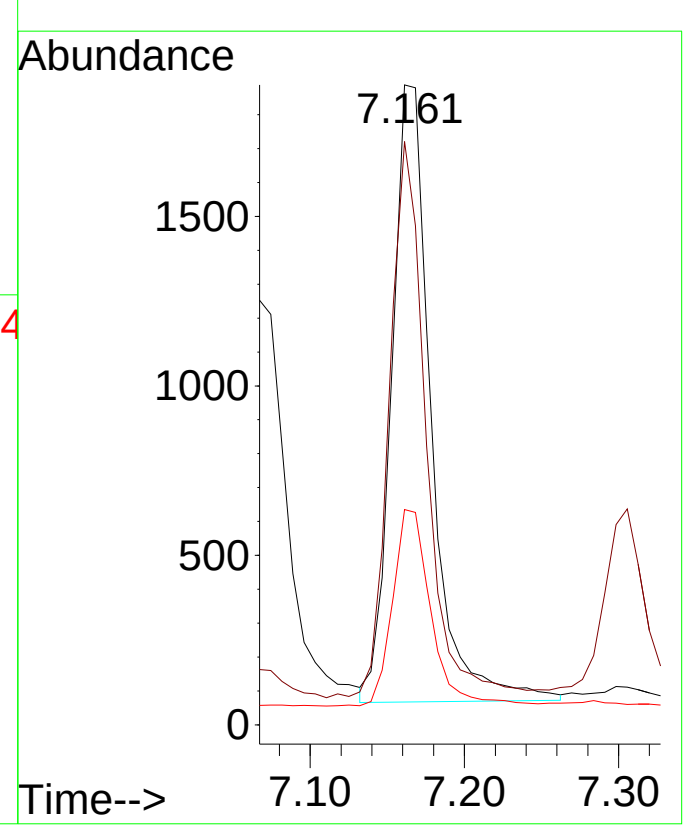

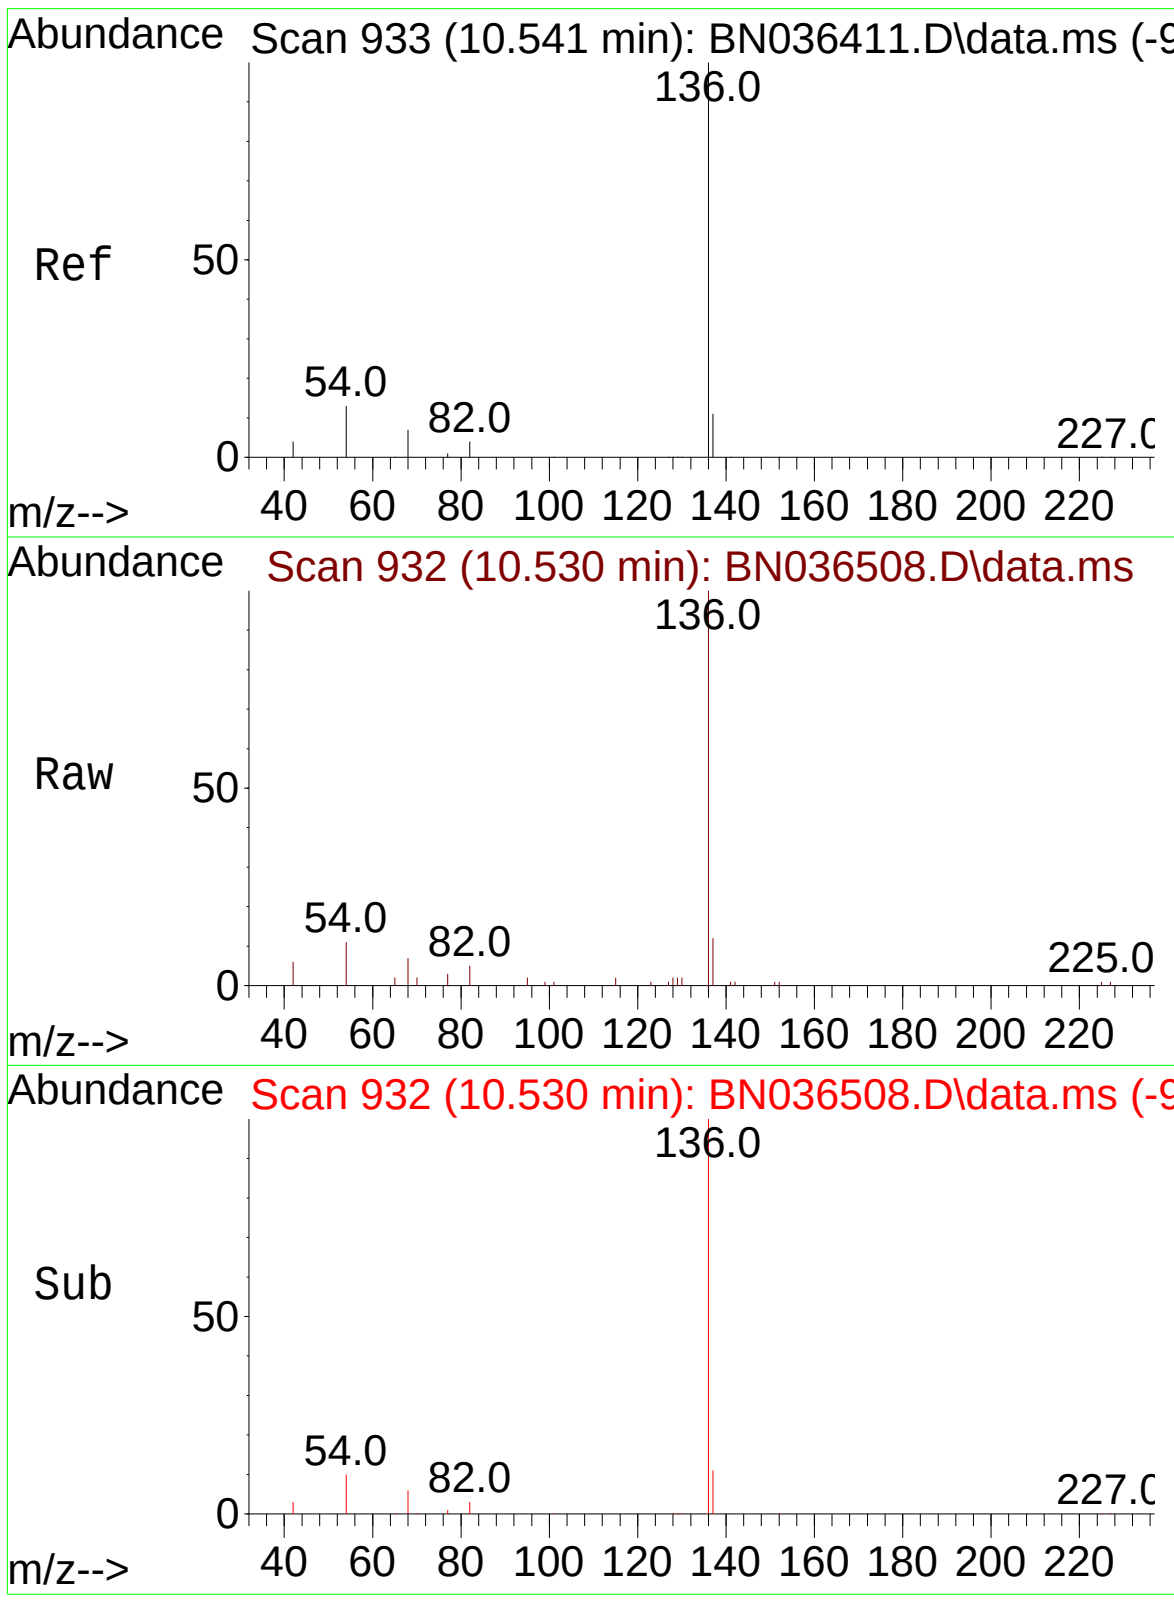

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.530 min   Scan# 9

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Delta R.T.   -0.011 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Tgt Ion:136 Resp: 6909

Ion	Ratio	Lower	Upper
136	100		
137	12.1	10.1	15.1
54	11.2	11.8	17.6#
68	7.3	7.2	10.8

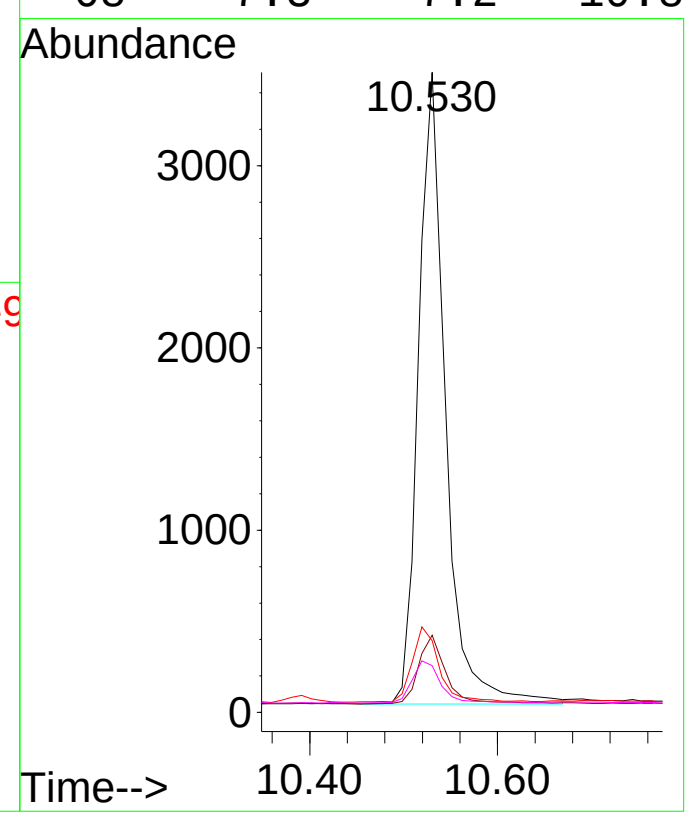

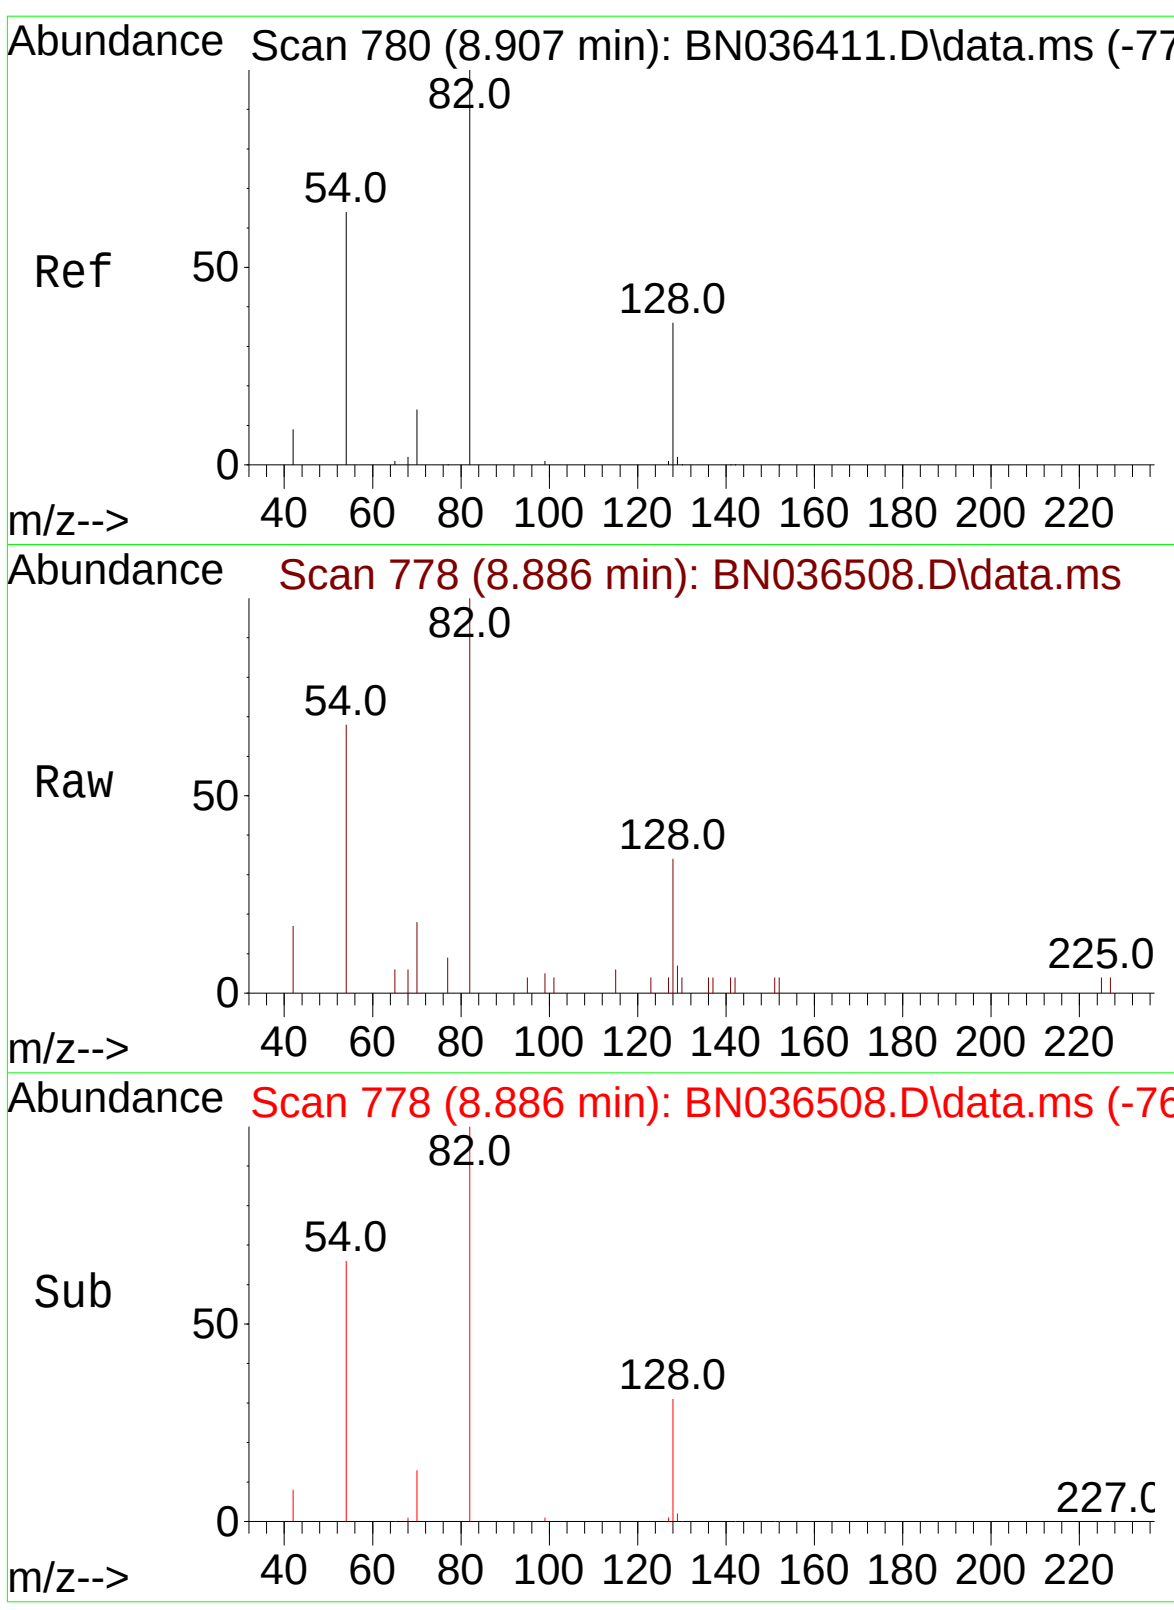

#8
Nitrobenzene-d5
Concen: 0.391 ng
RT: 8.886 min   Scan# 778
Delta R.T.   -0.021 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Tgt Ion: 82 Resp: 2668

Ion	Ratio	Lower	Upper
82	100		
128	34.4	31.9	47.9
54	68.3	53.1	79.7

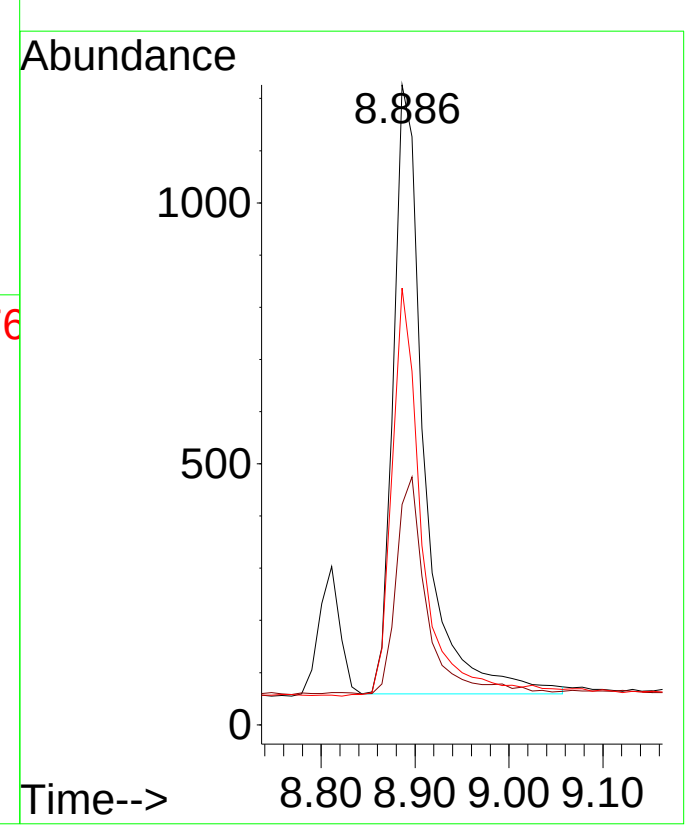

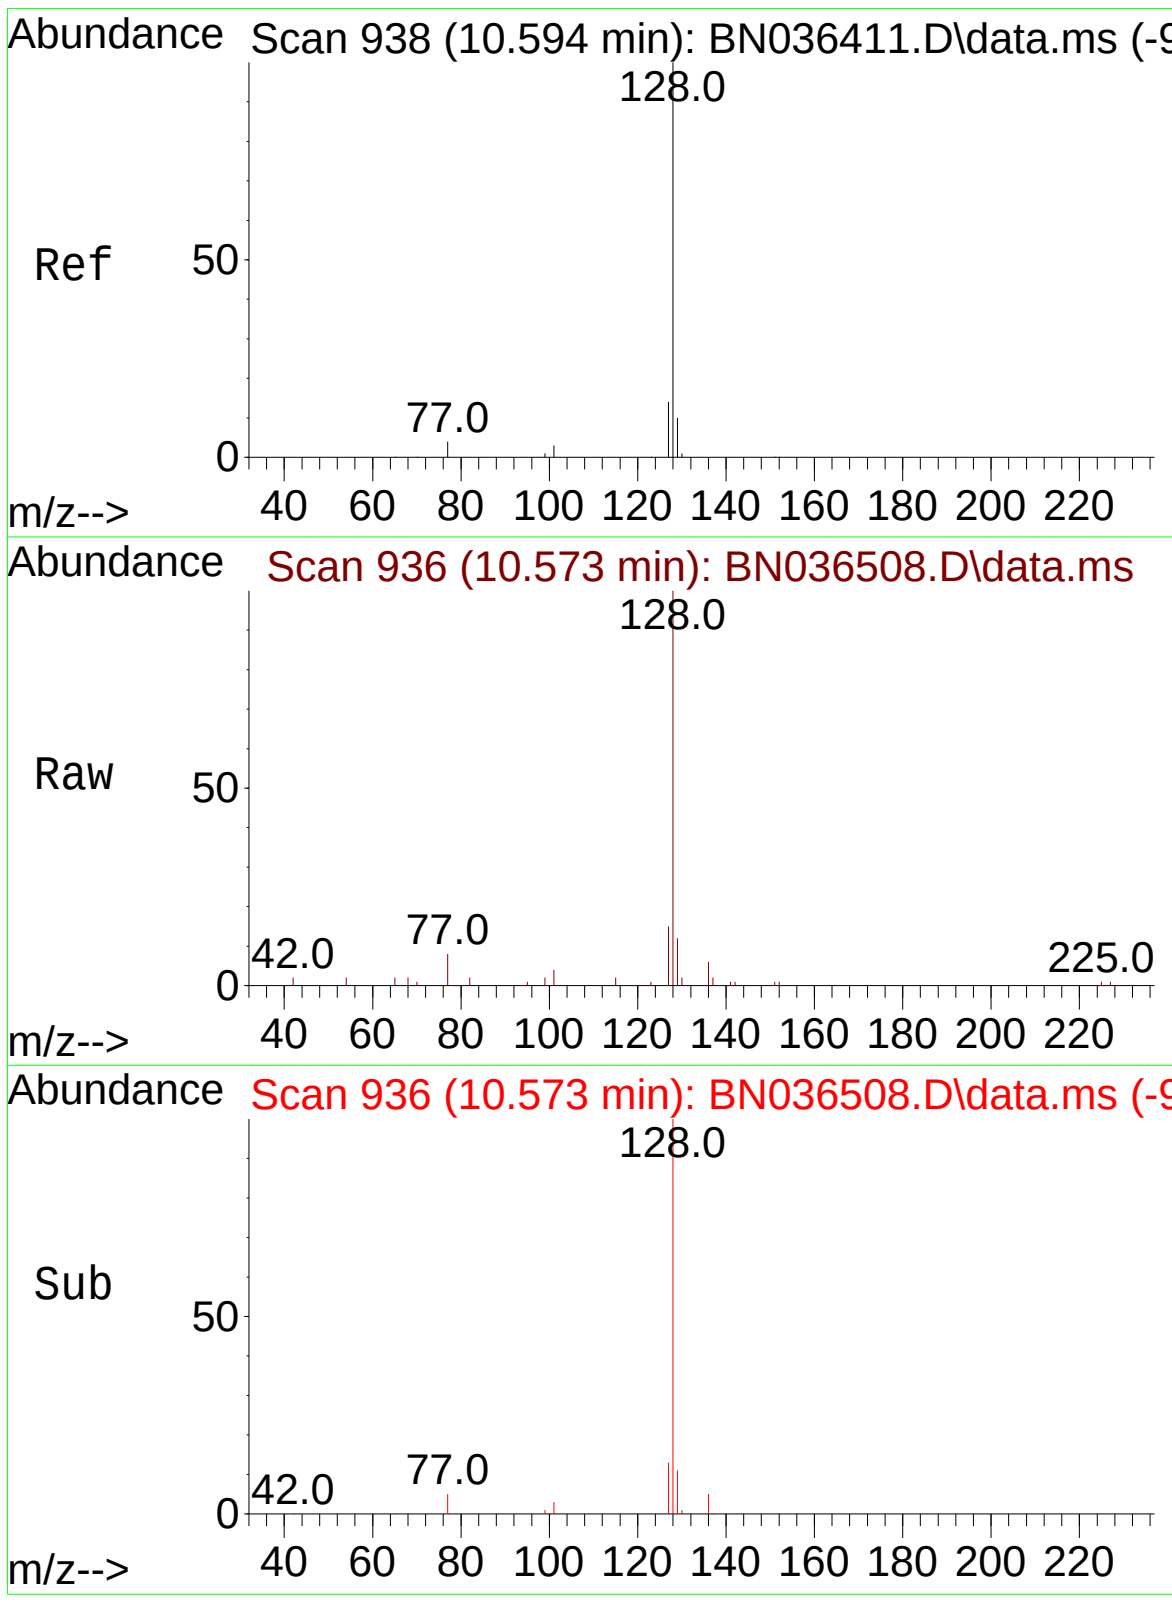

#9
Naphthalene
Concen: 0.390 ng
RT: 10.573 min Scan# 9
Delta R.T. -0.021 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:128 Resp: 7777

Ion	Ratio	Lower	Upper
128	100		
129	12.5	9.6	14.4
127	14.5	12.0	18.0

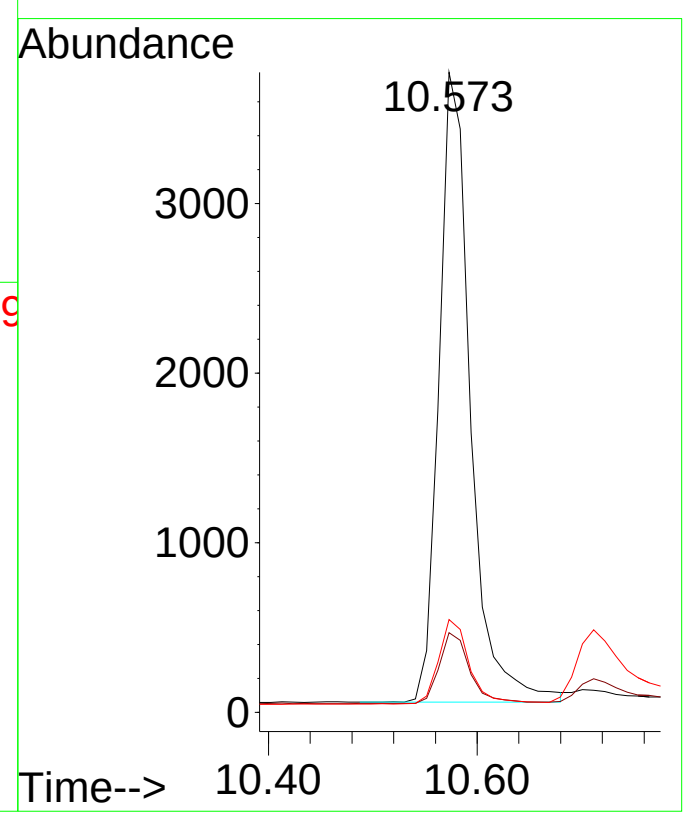

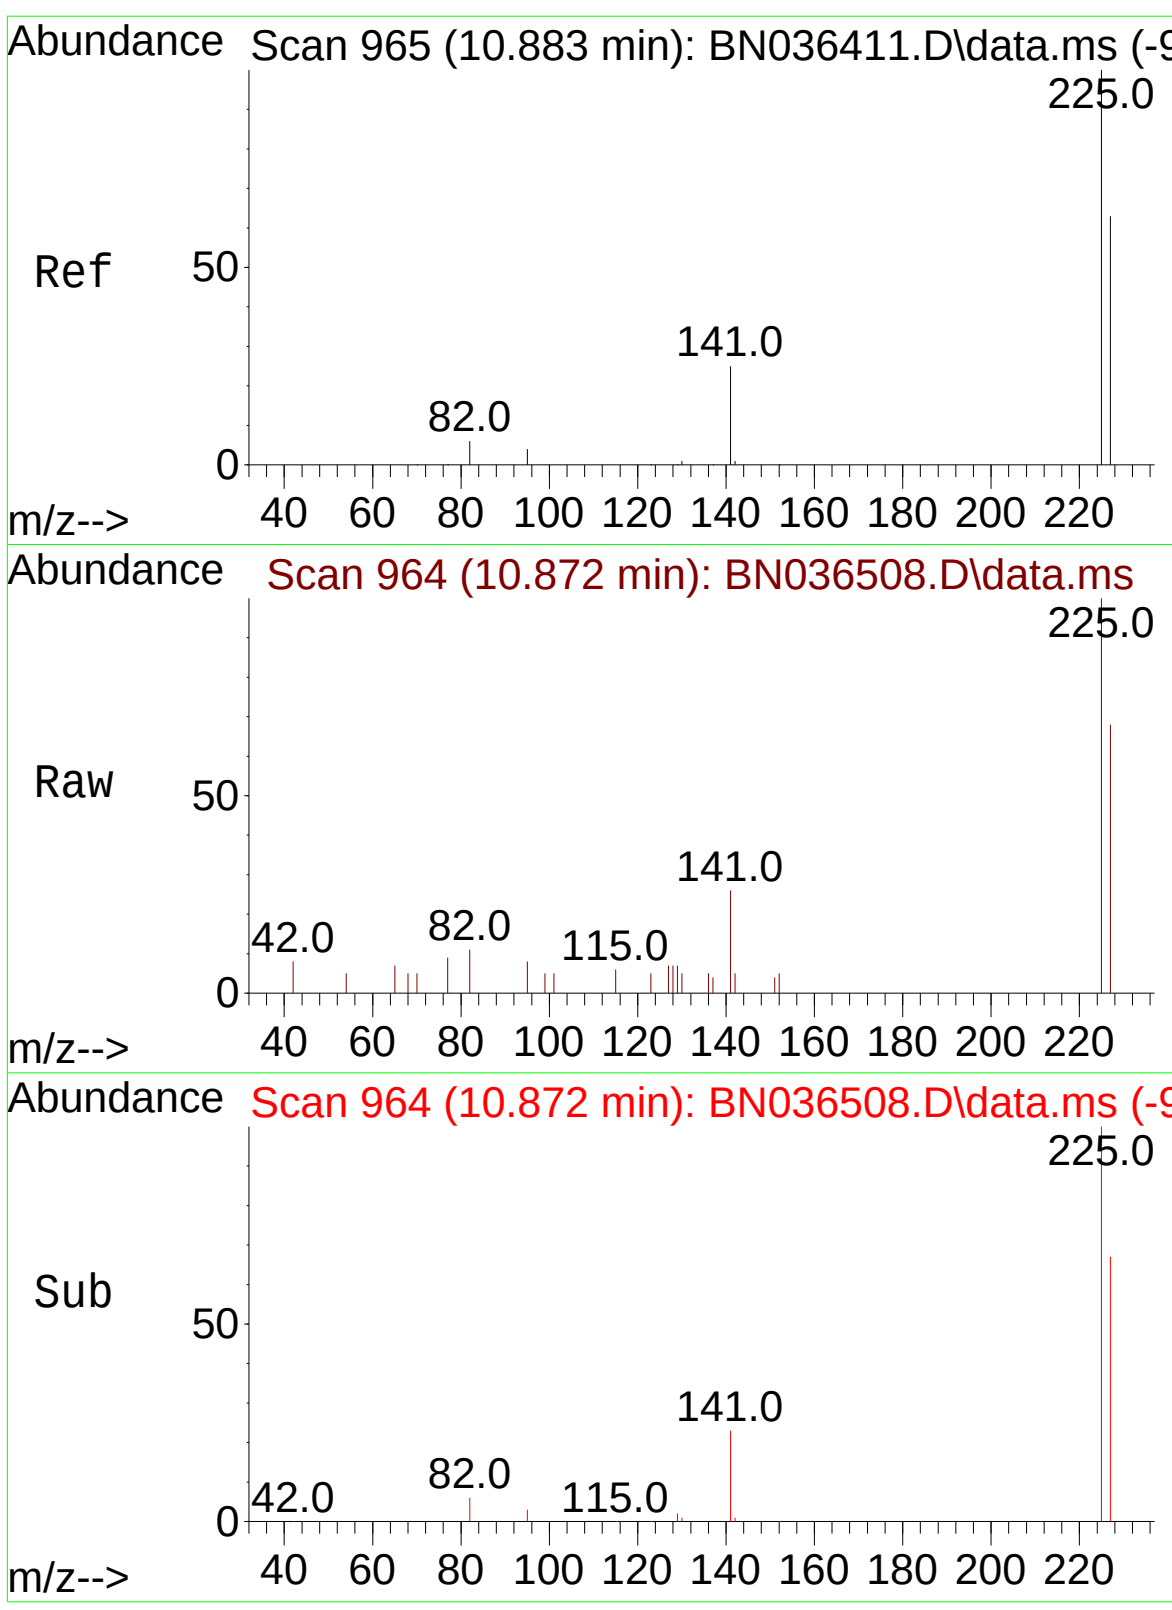

#10
Hexachlorobutadiene
Concen: 0.389 ng
RT: 10.872 min Scan# 964
Delta R.T. -0.011 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Tgt Ion:225 Resp: 1886

Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	64.9	50.9	76.3

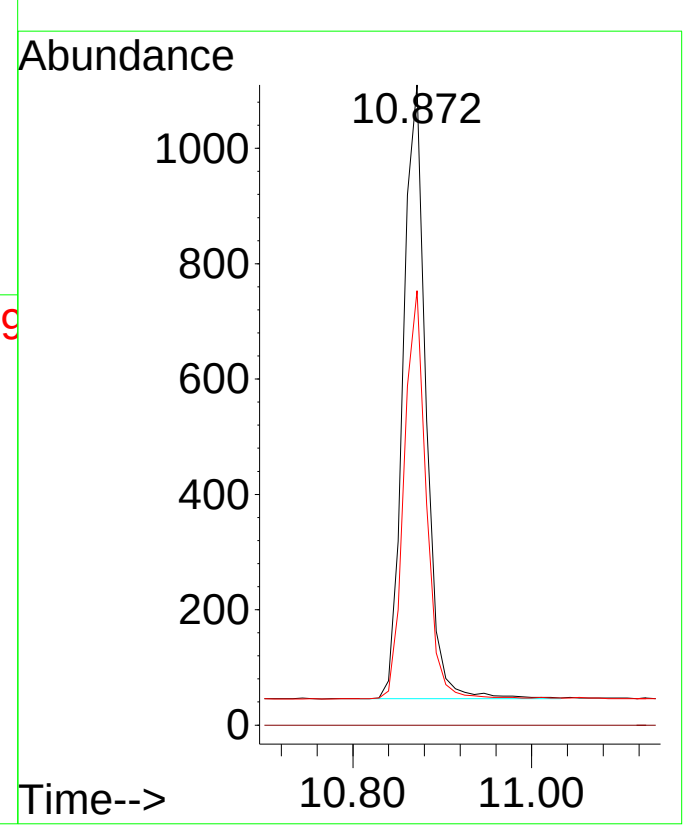

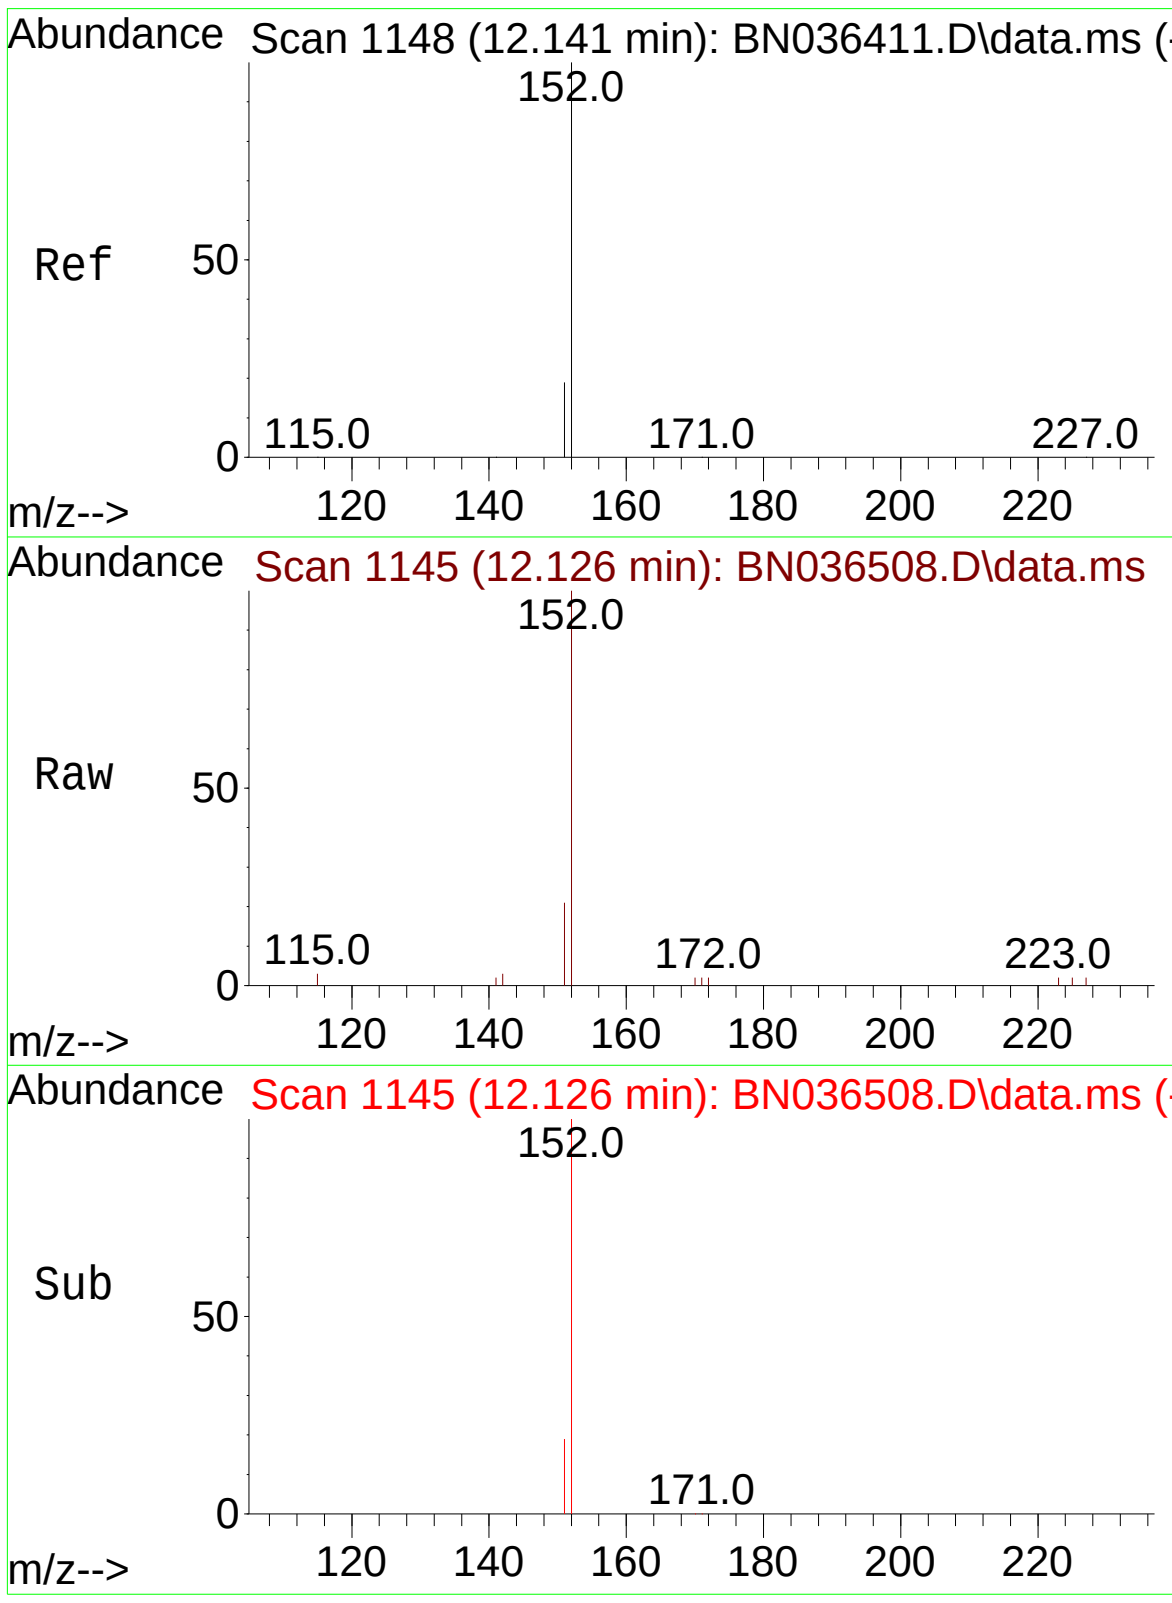

#11
2-Methylnaphthalene-d10
Concen: 0.386 ng
RT: 12.126 min Scan# 1
Delta R.T. -0.015 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:152 Resp: 4099

Ion	Ratio	Lower	Upper
152	100		
151	20.2	16.6	25.0

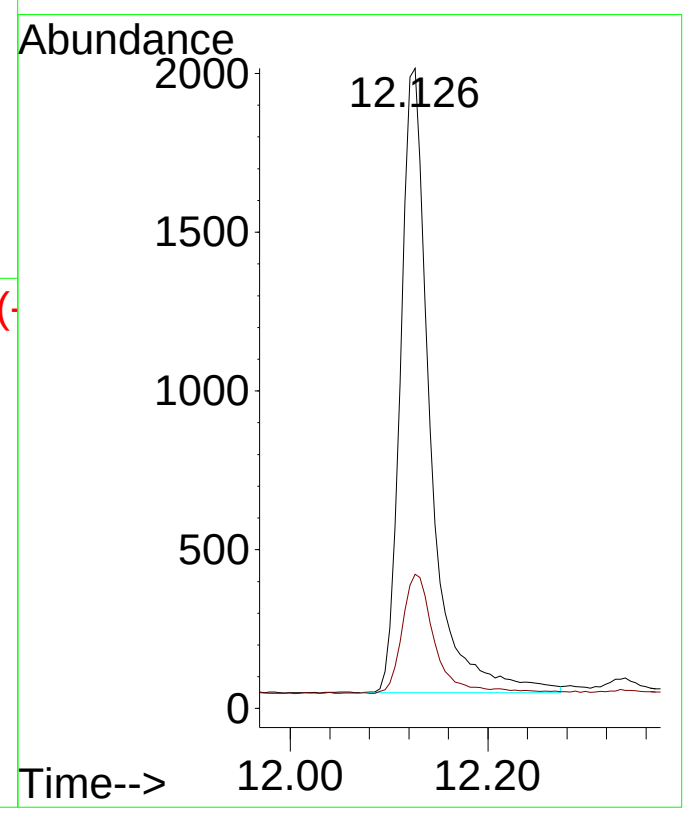

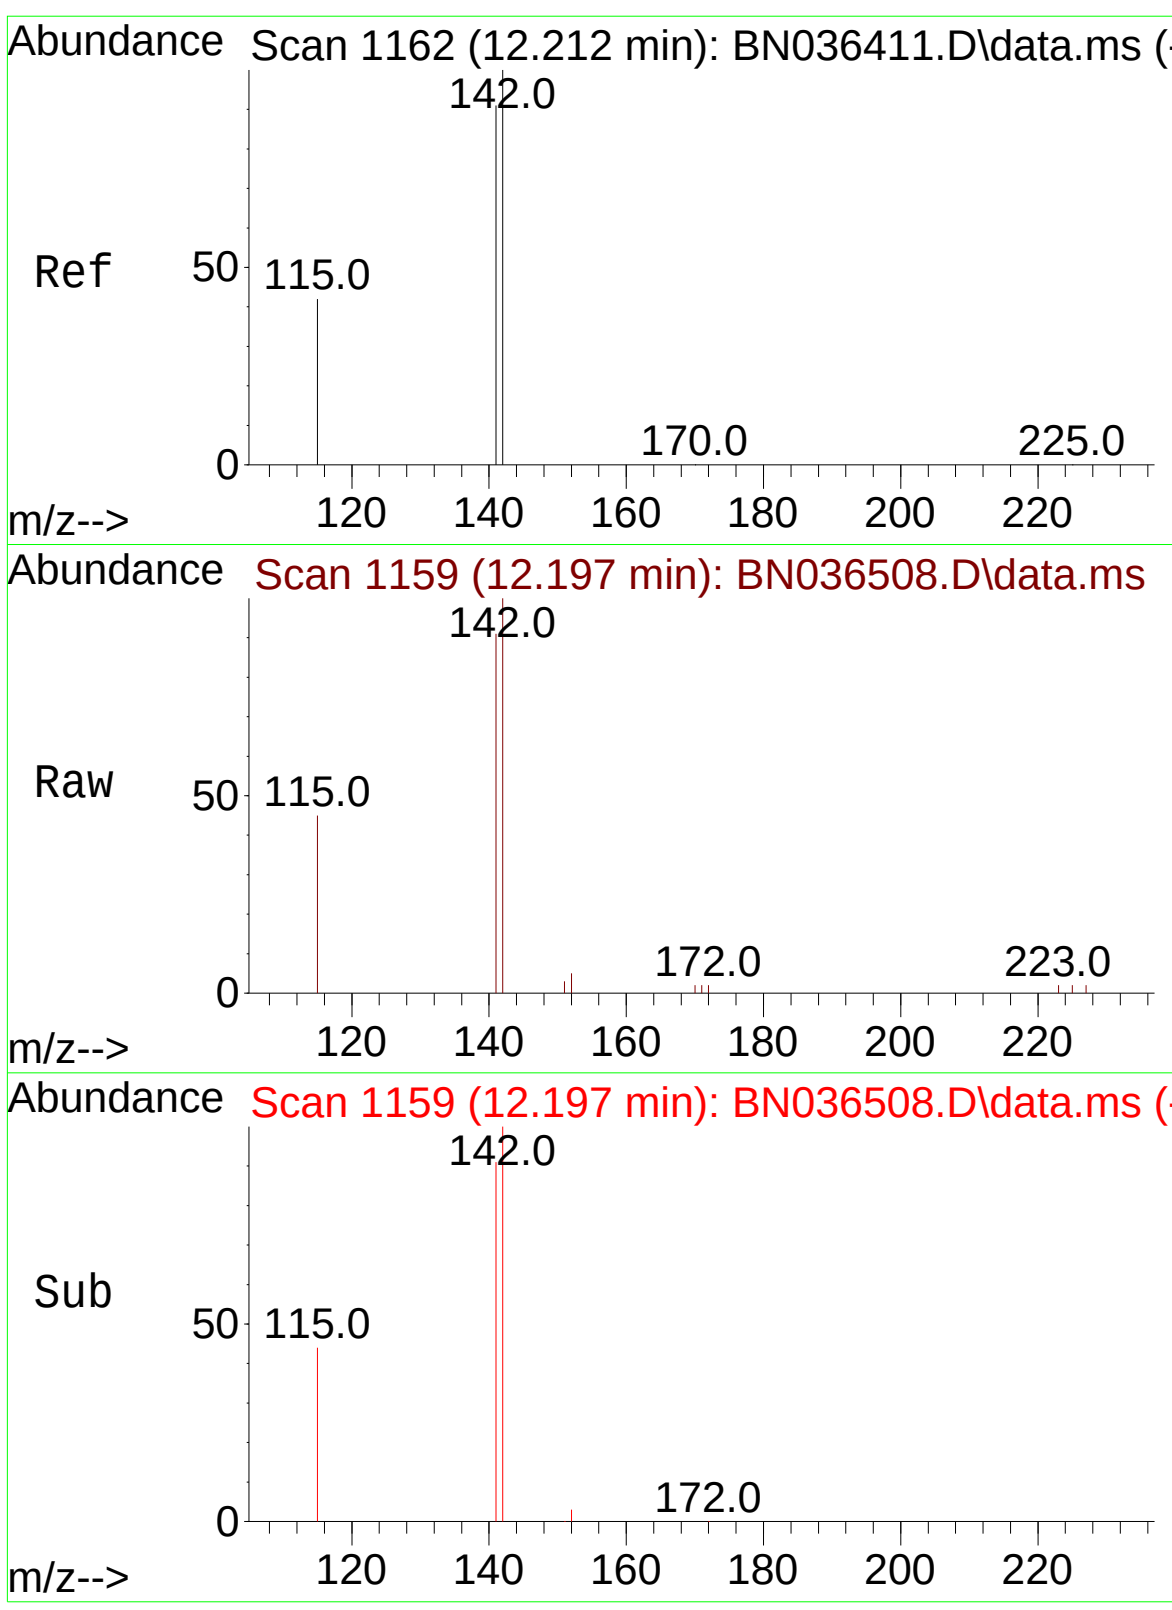

#12
2-Methylnaphthalene
Concen: 0.386 ng
RT: 12.197 min Scan# 1159
Delta R.T. -0.015 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Tgt Ion:142 Resp: 5047

Ion	Ratio	Lower	Upper
142	100		
141	91.2	72.8	109.2
115	45.3	35.5	53.3

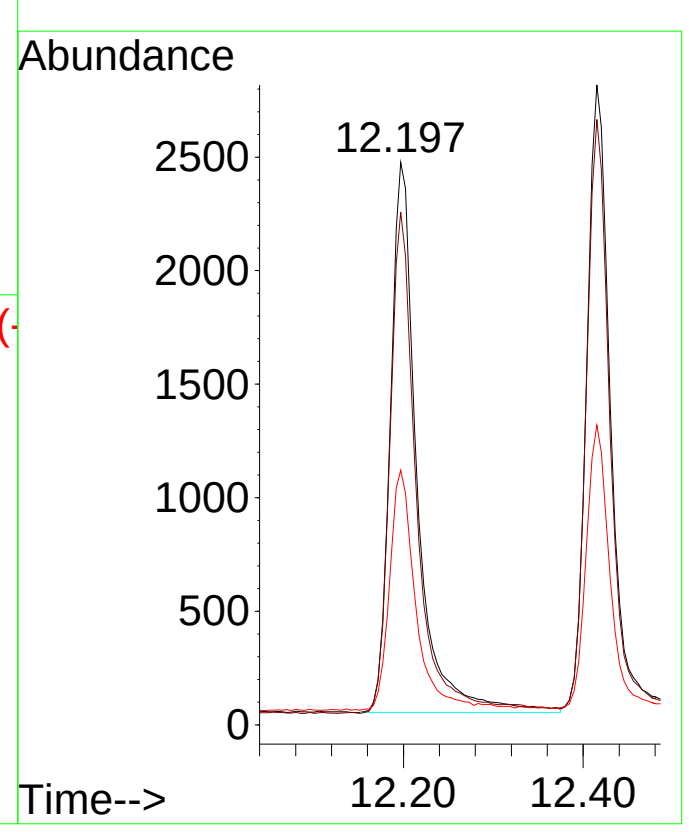

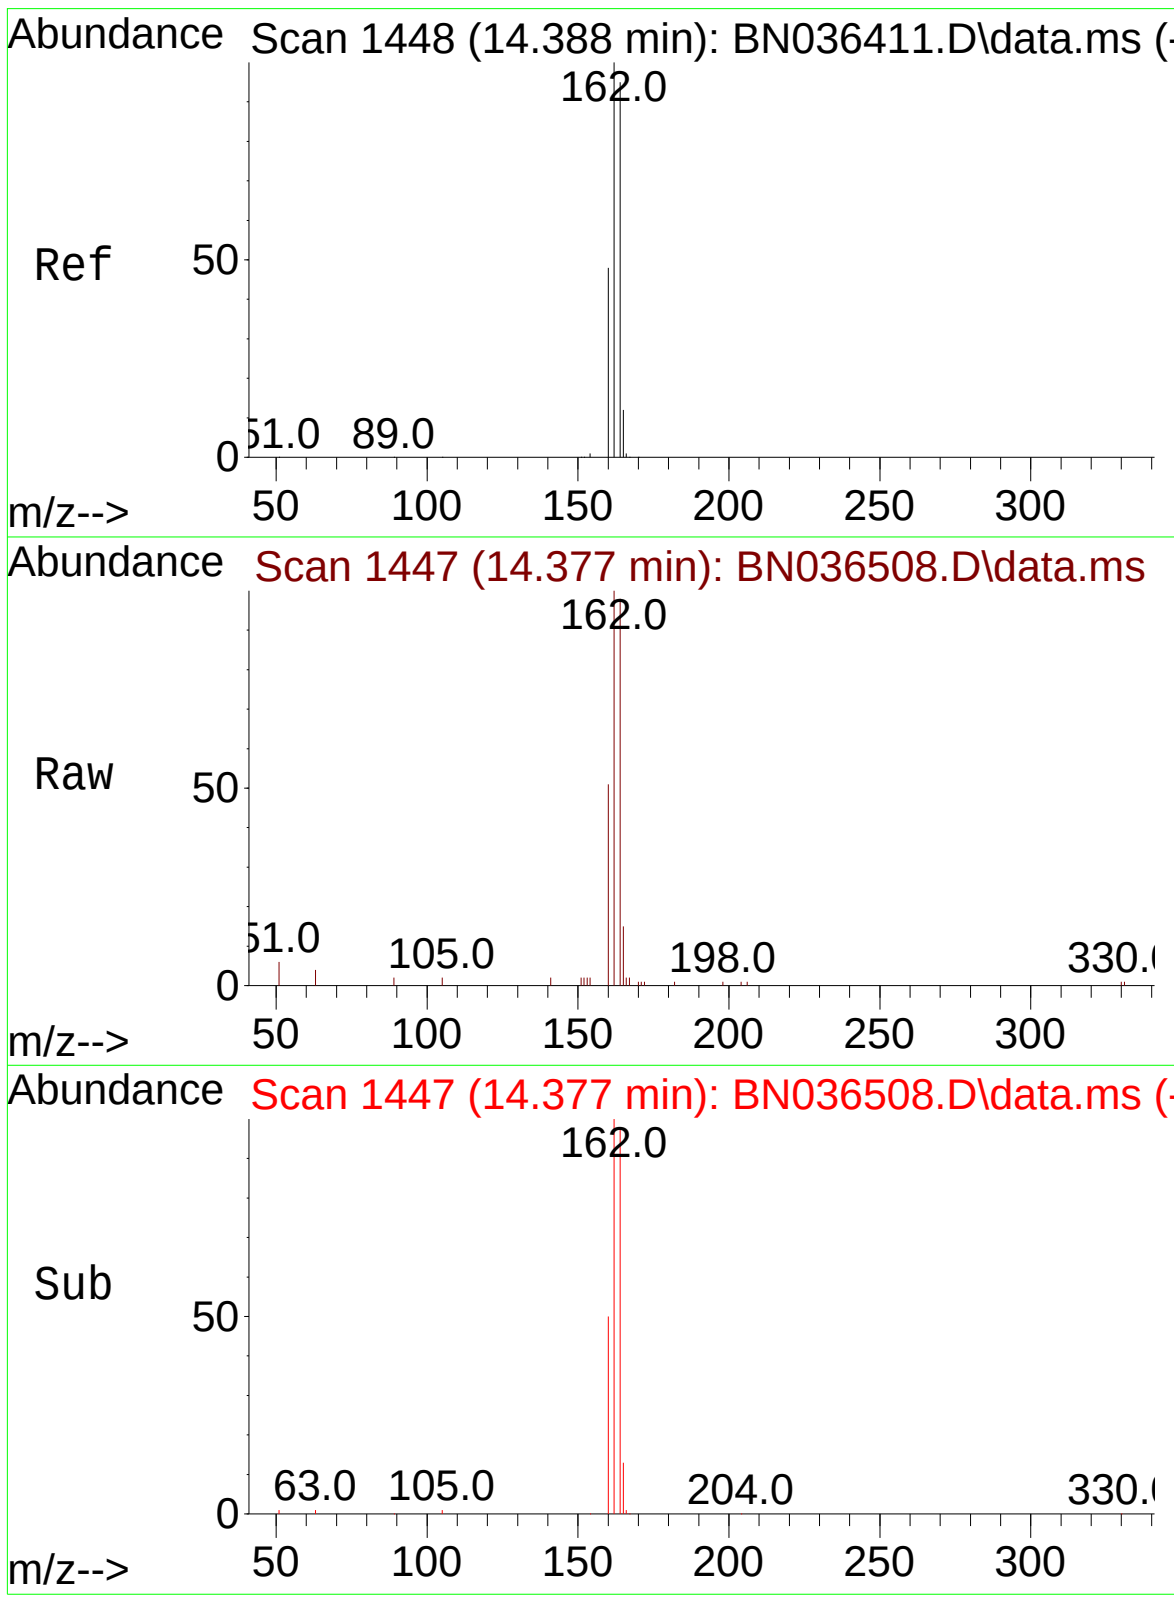

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.377 min Scan# 14
Delta R.T. -0.011 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:164 Resp: 4680

Ion	Ratio	Lower	Upper
164	100		
162	102.2	84.1	126.1
160	51.9	41.4	62.0

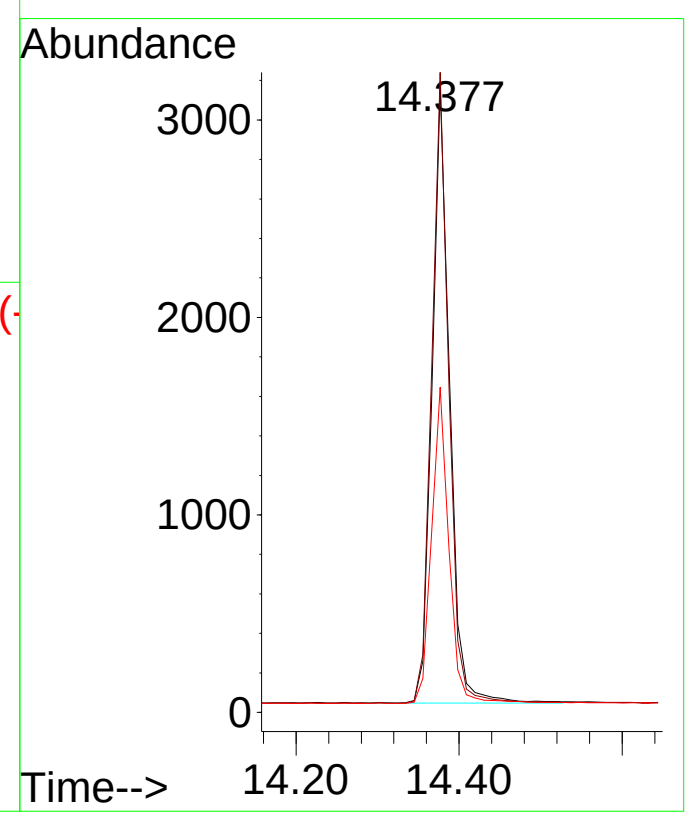

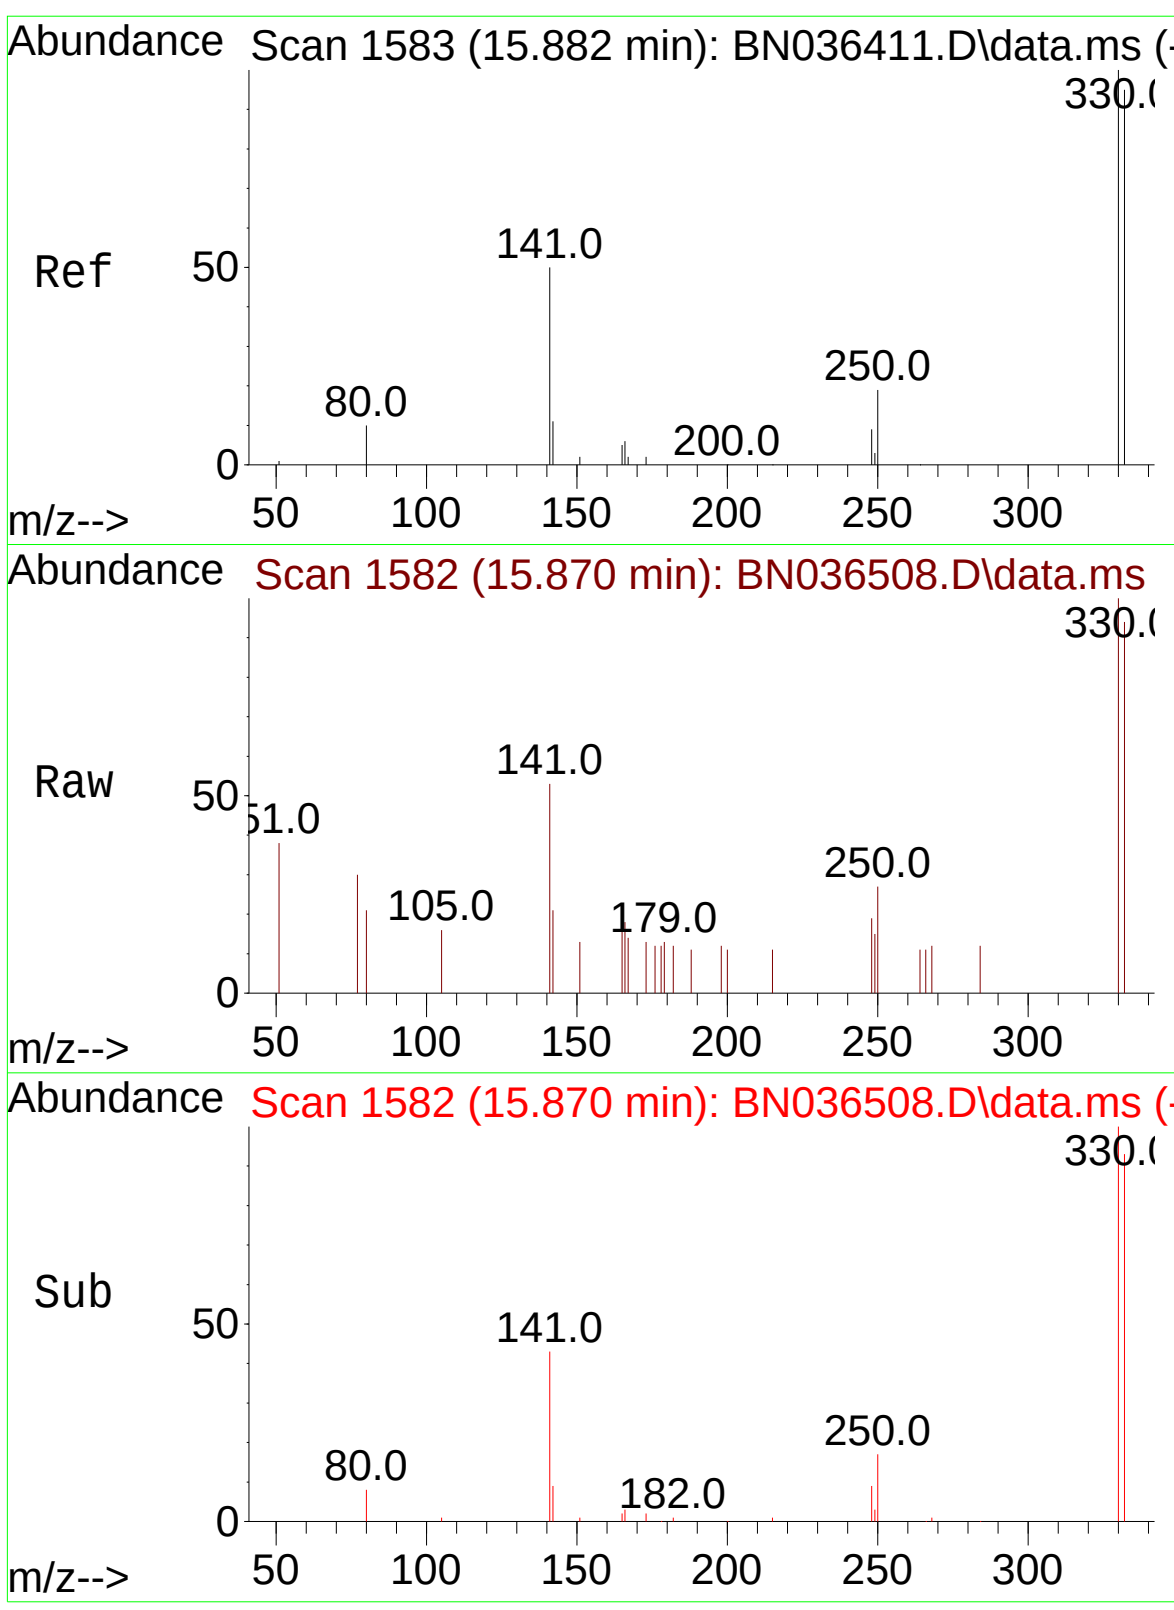

#14
2,4,6-Tribromophenol
Concen: 0.310 ng
RT: 15.870 min Scan# 1582
Delta R.T. -0.012 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Tgt Ion:330 Resp: 719

Ion	Ratio	Lower	Upper
330	100		
332	95.0	76.6	114.8
141	47.8	37.8	56.8

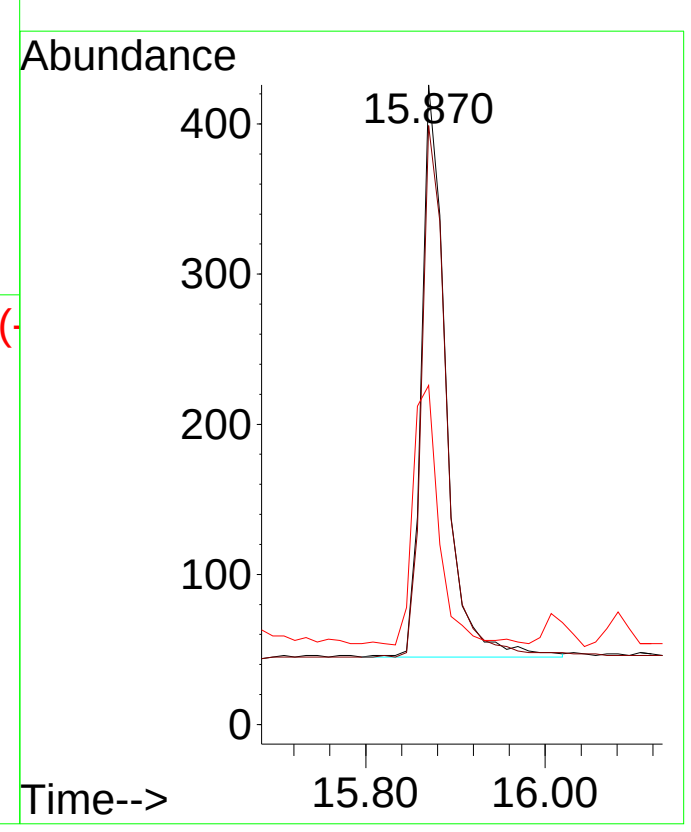

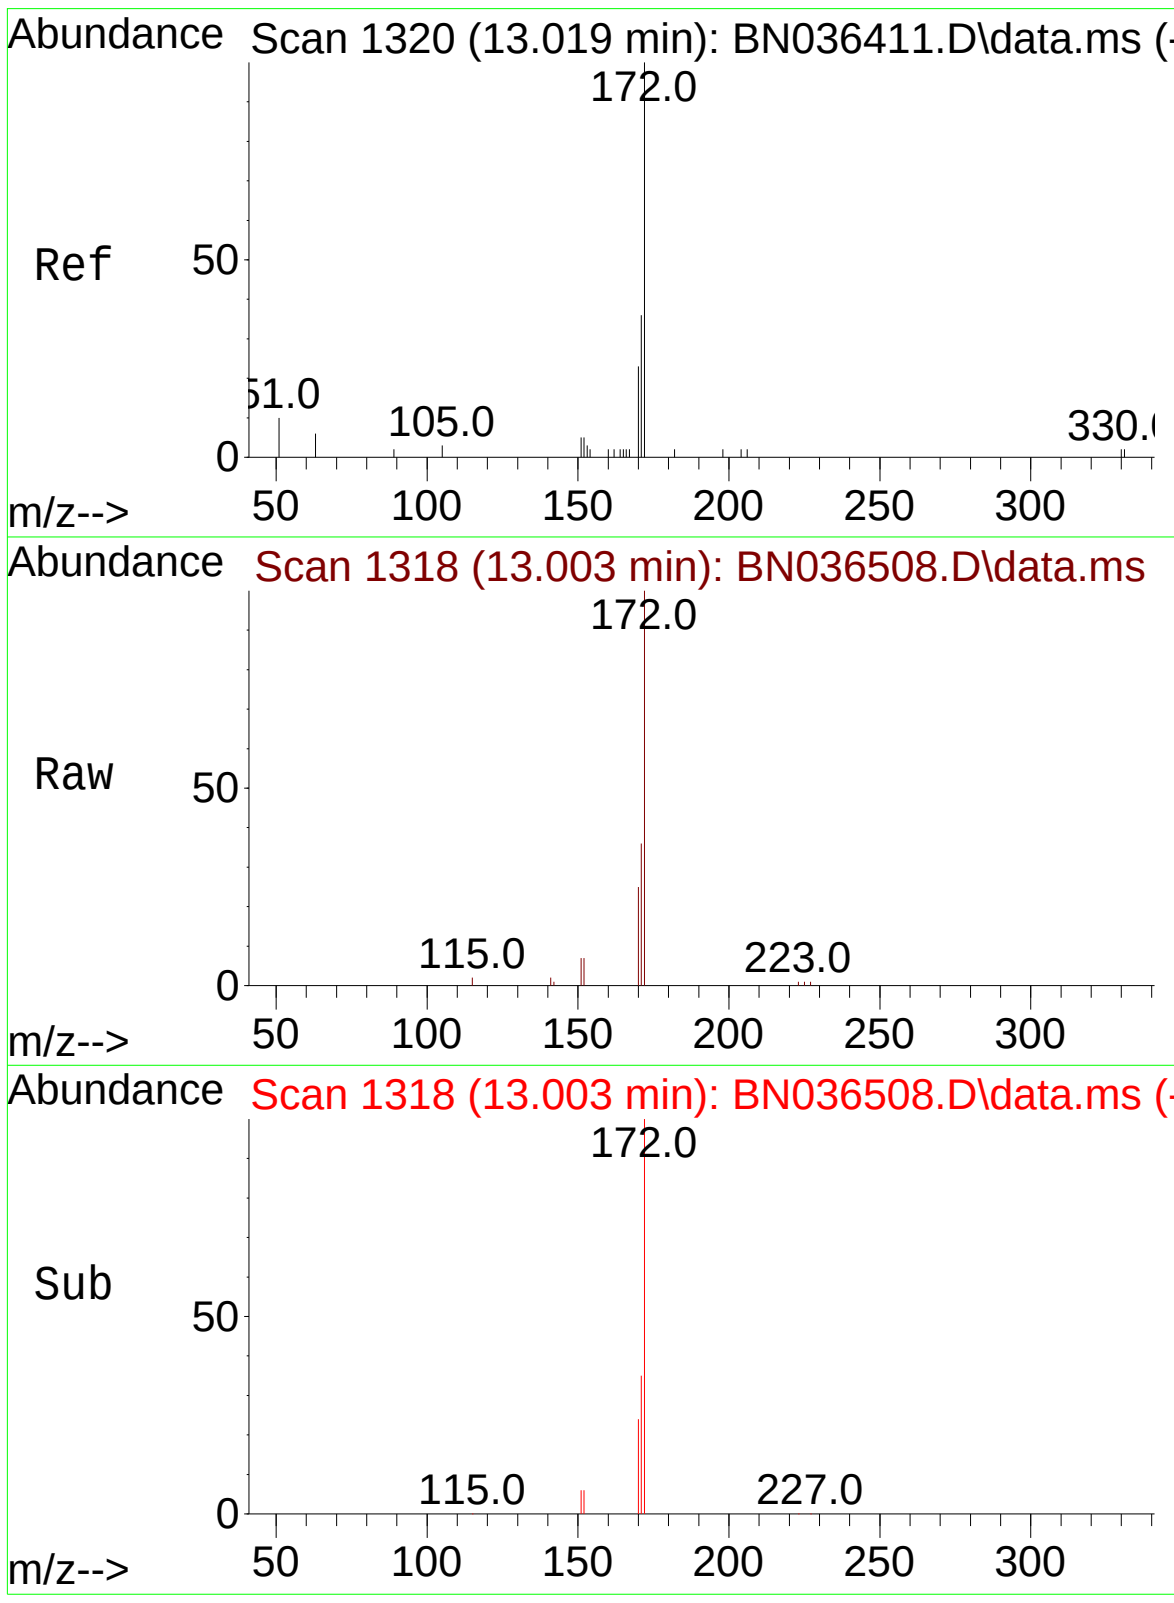

#15
2-Fluorobiphenyl
Concen: 0.444 ng
RT: 13.003 min Scan# 1
Delta R.T. -0.016 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:172 Resp: 7811

Ion	Ratio	Lower	Upper
172	100		
171	36.3	29.6	44.4
170	25.0	19.8	29.6

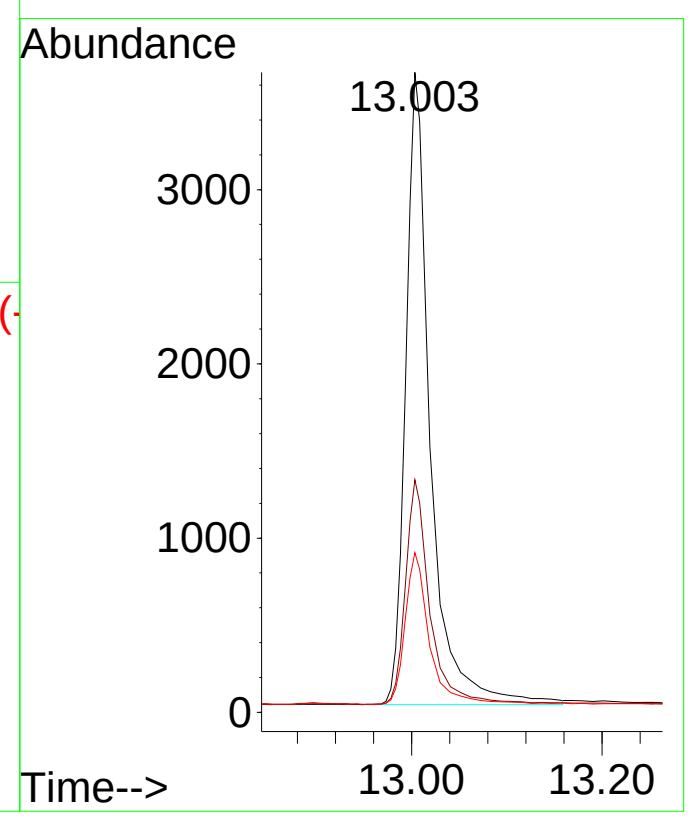

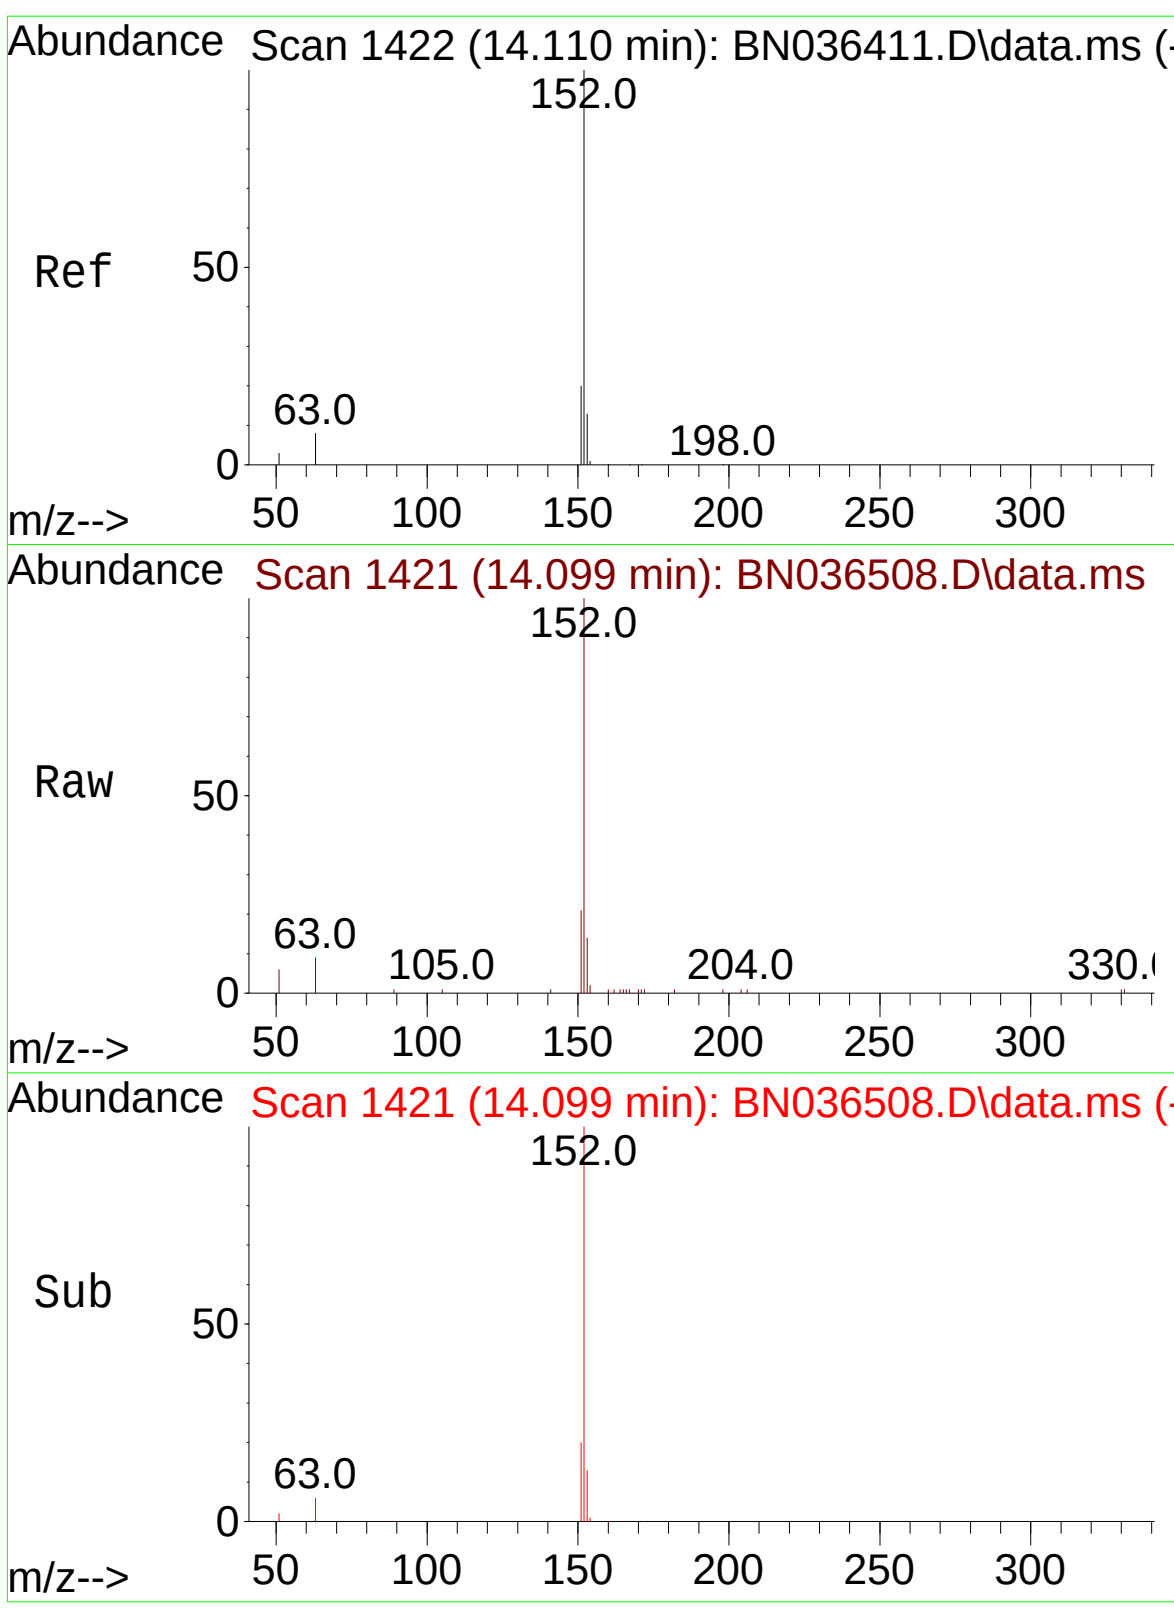

#16
Acenaphthylene
Concen: 0.382 ng
RT: 14.099 min Scan# 1421
Delta R.T. -0.011 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Tgt Ion:152 Resp: 7894

Ion	Ratio	Lower	Upper
152	100		
151	20.1	15.8	23.8
153	12.8	10.2	15.2

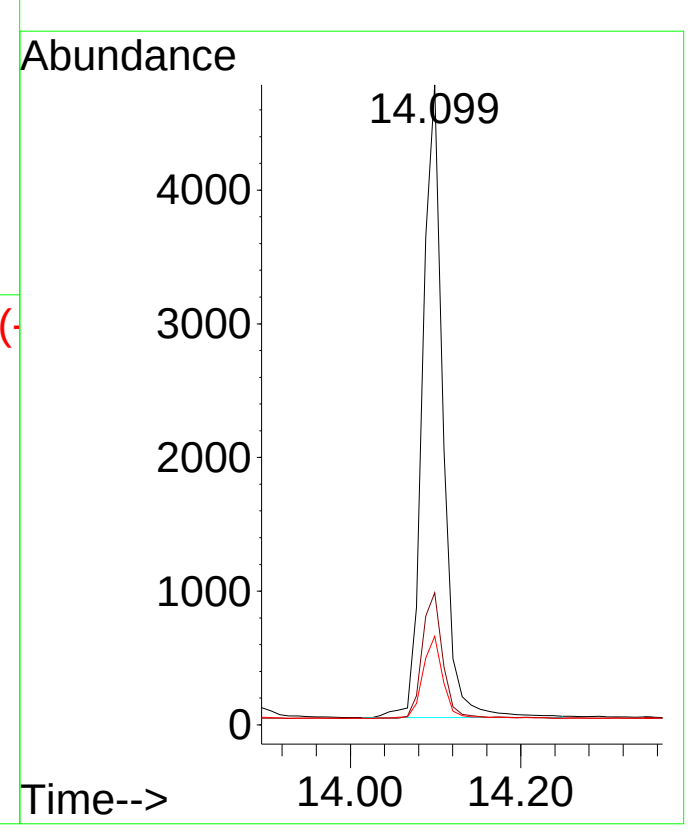

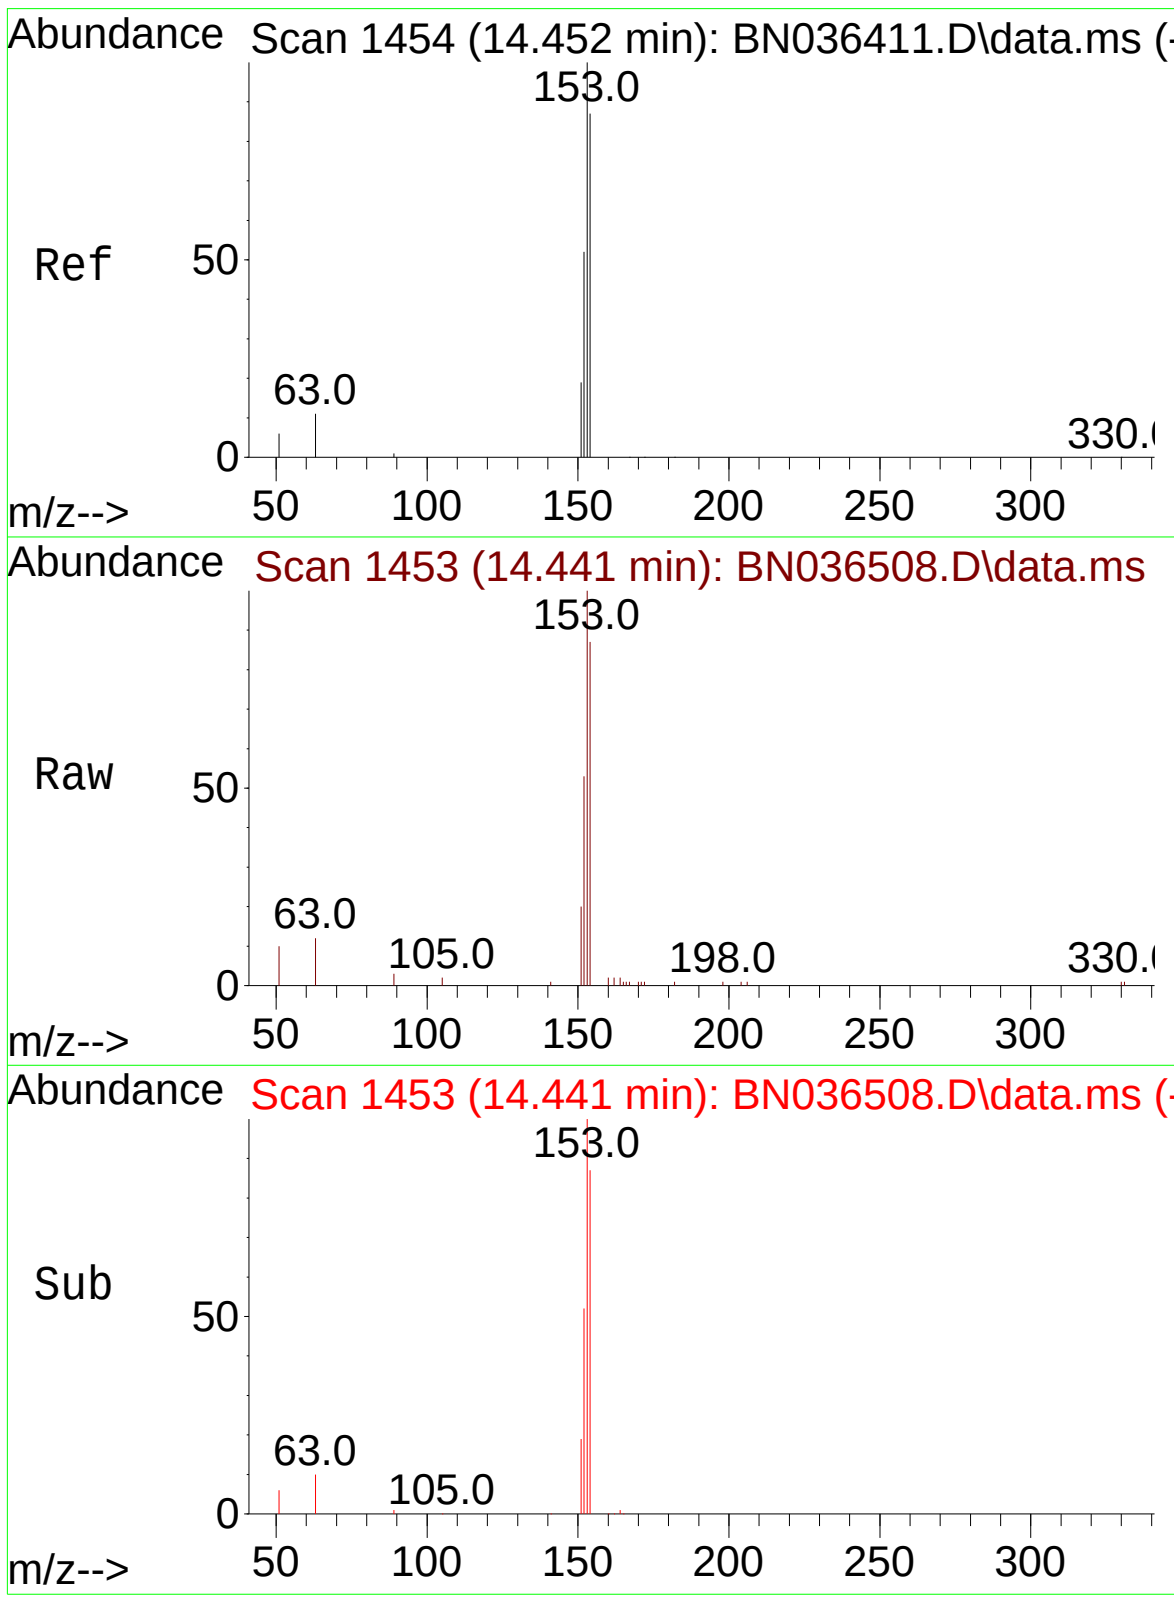

#17
Acenaphthene
Concen: 0.366 ng
RT: 14.441 min Scan# 14
Delta R.T. -0.011 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:154 Resp: 5057

Ion	Ratio	Lower	Upper
154	100		
153	117.0	93.3	139.9
152	63.2	48.8	73.2

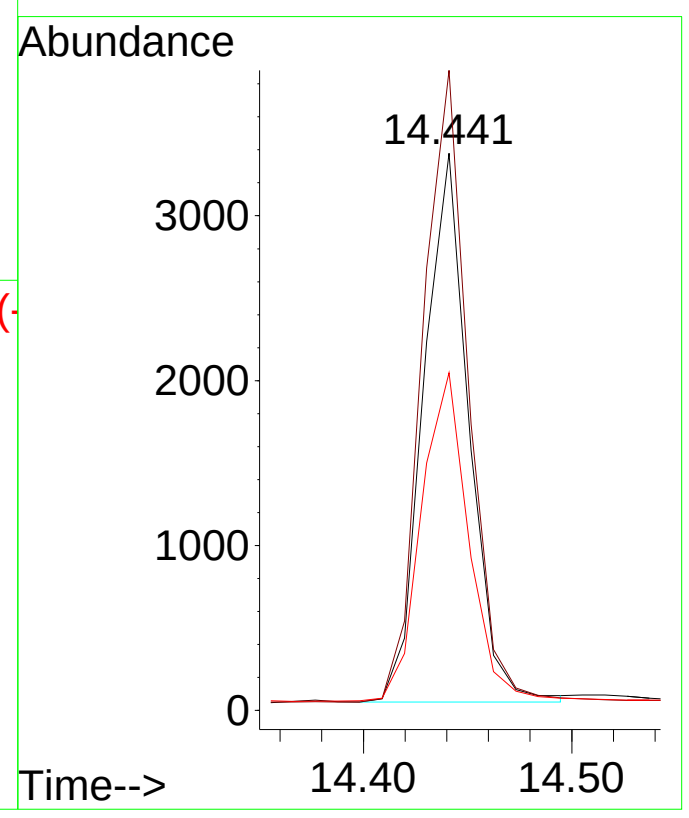

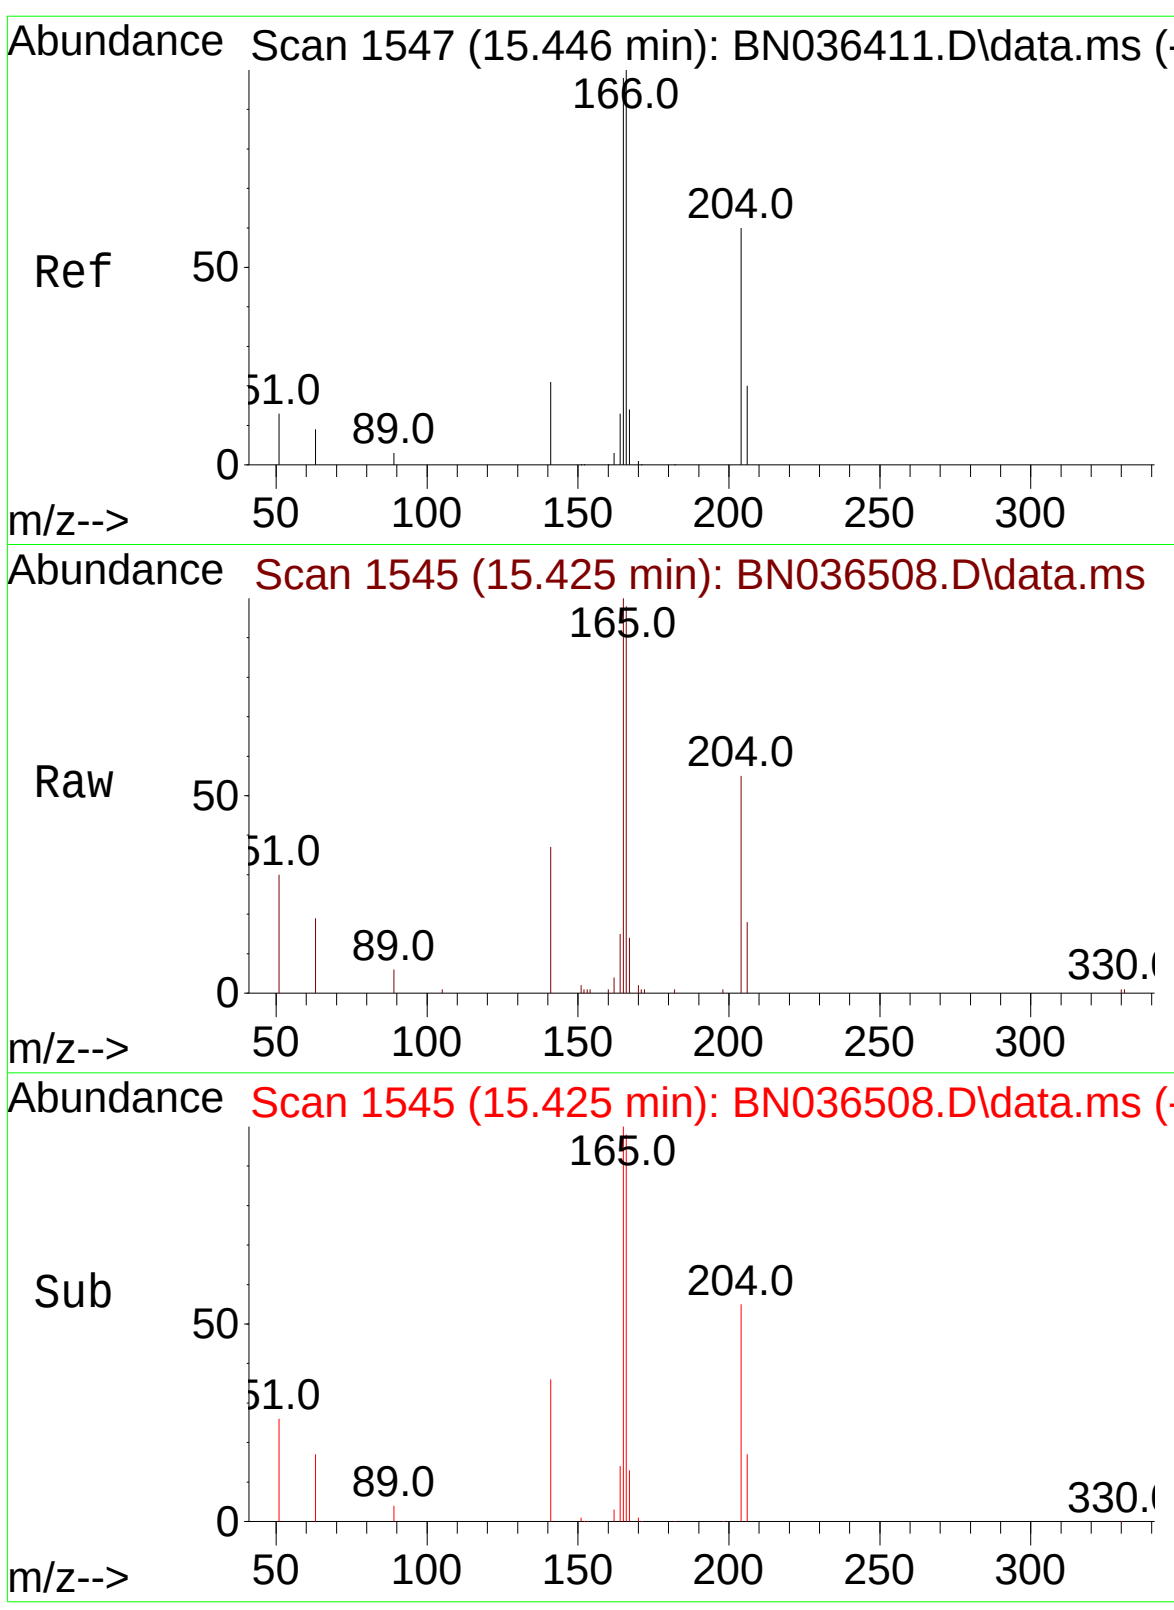

#18
Fluorene
Concen: 0.362 ng
RT: 15.425 min Scan# 1545
Delta R.T. -0.021 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Tgt Ion:166 Resp: 7106

Ion	Ratio	Lower	Upper
166	100		
165	99.3	79.5	119.3
167	12.7	10.4	15.6

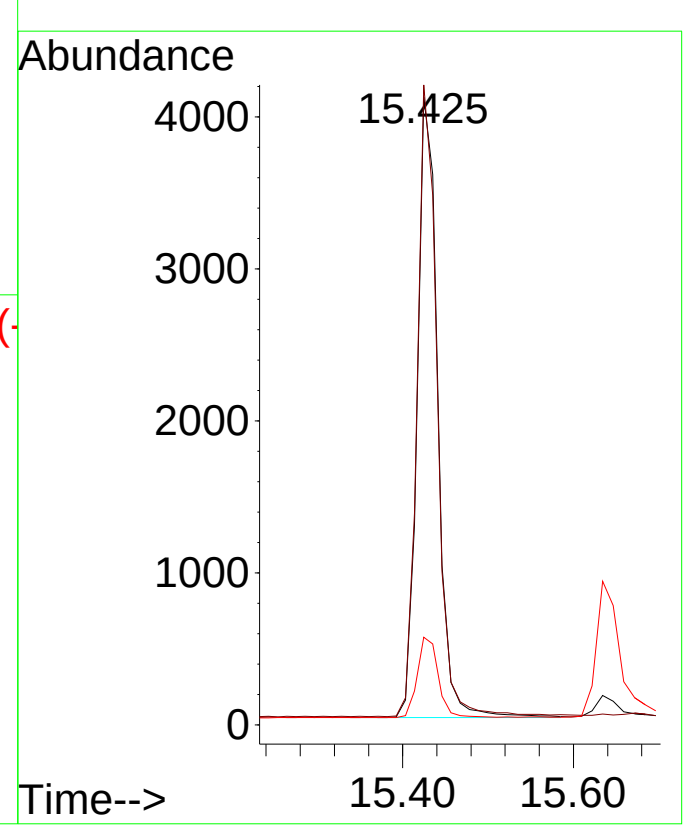

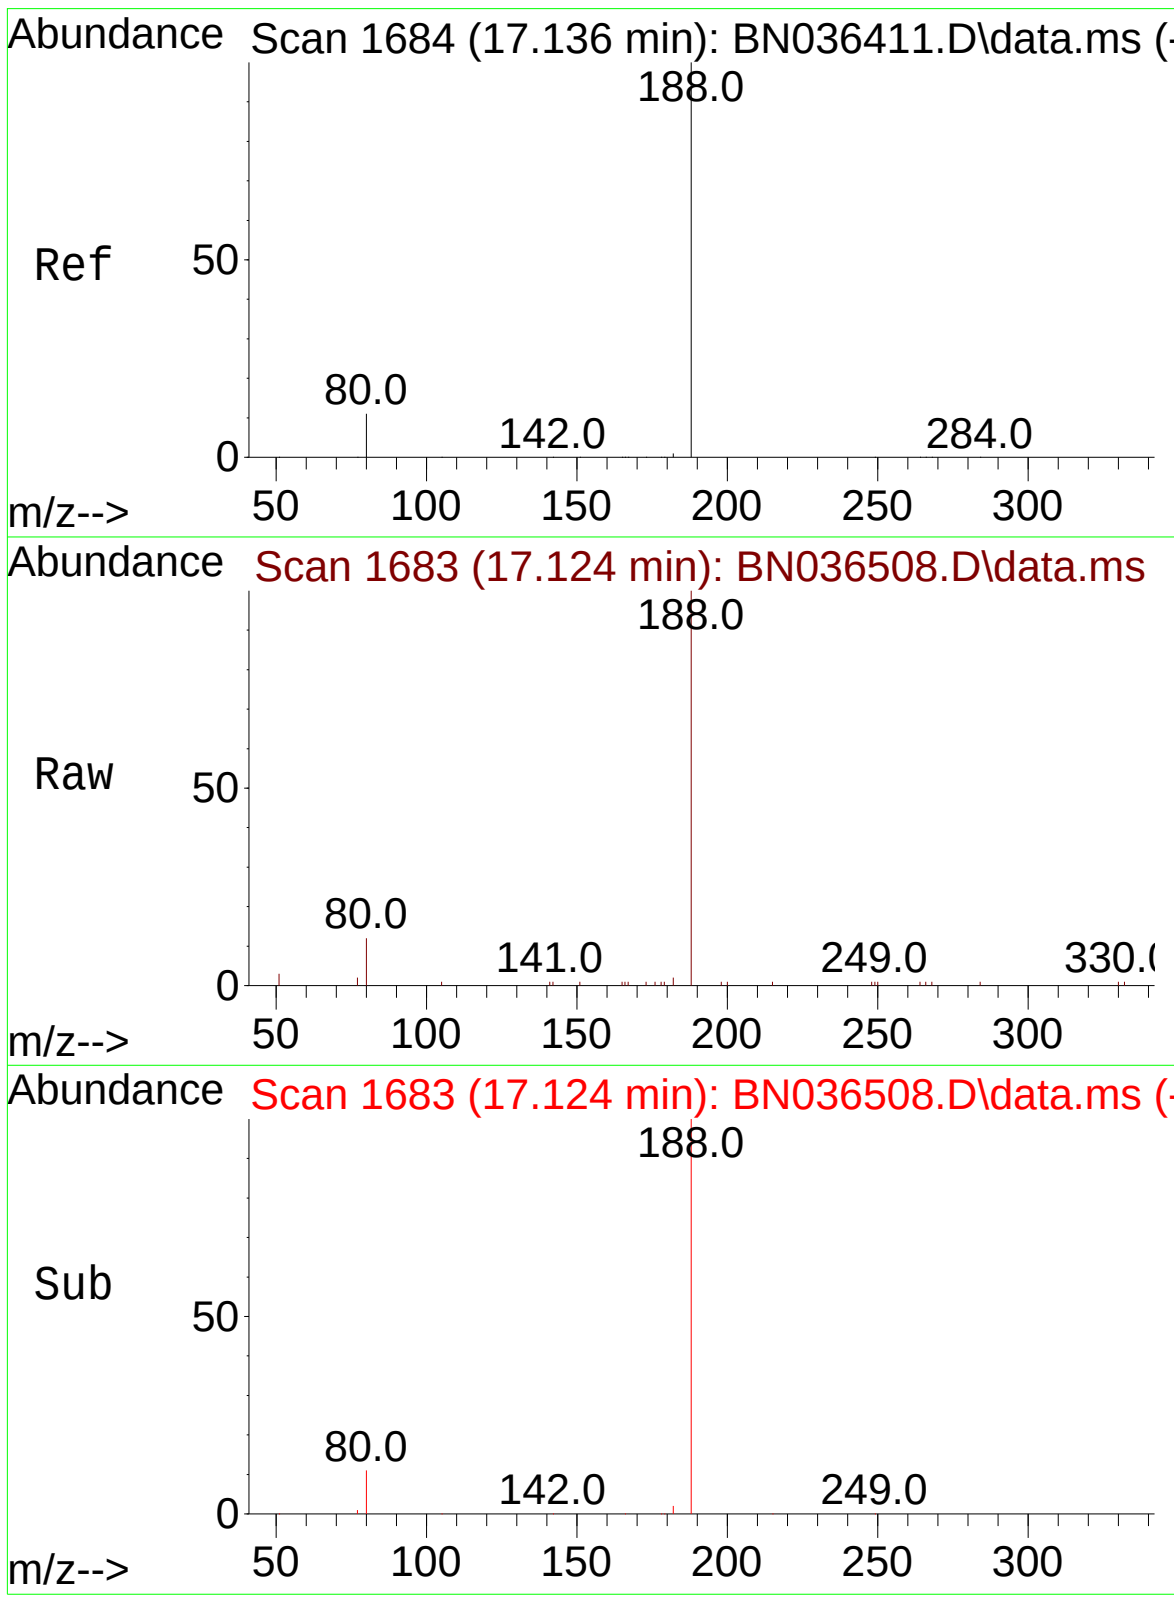

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.124 min Scan# 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Delta R.T. -0.012 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Tgt Ion:188 Resp: 9092

Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	12.1	9.8	14.6

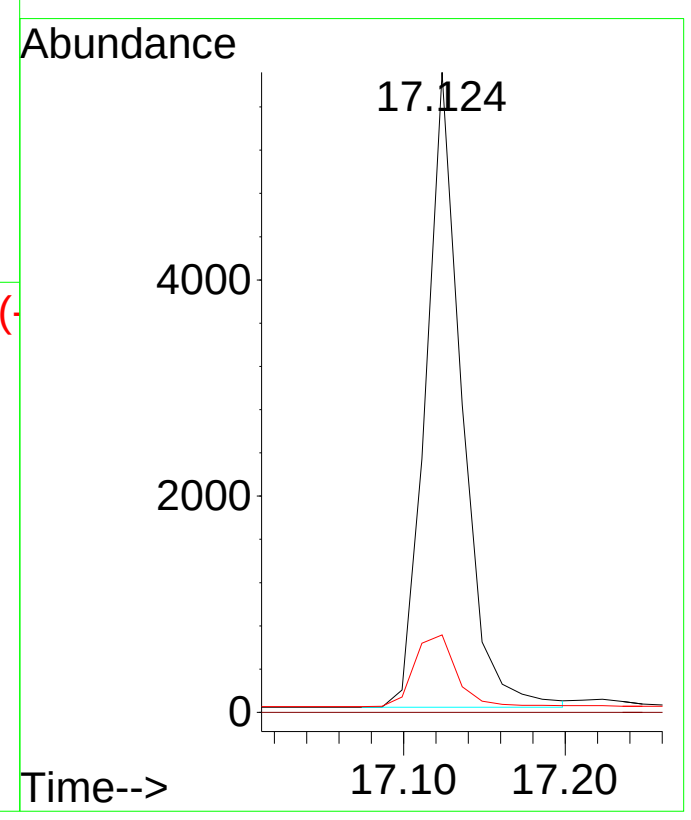

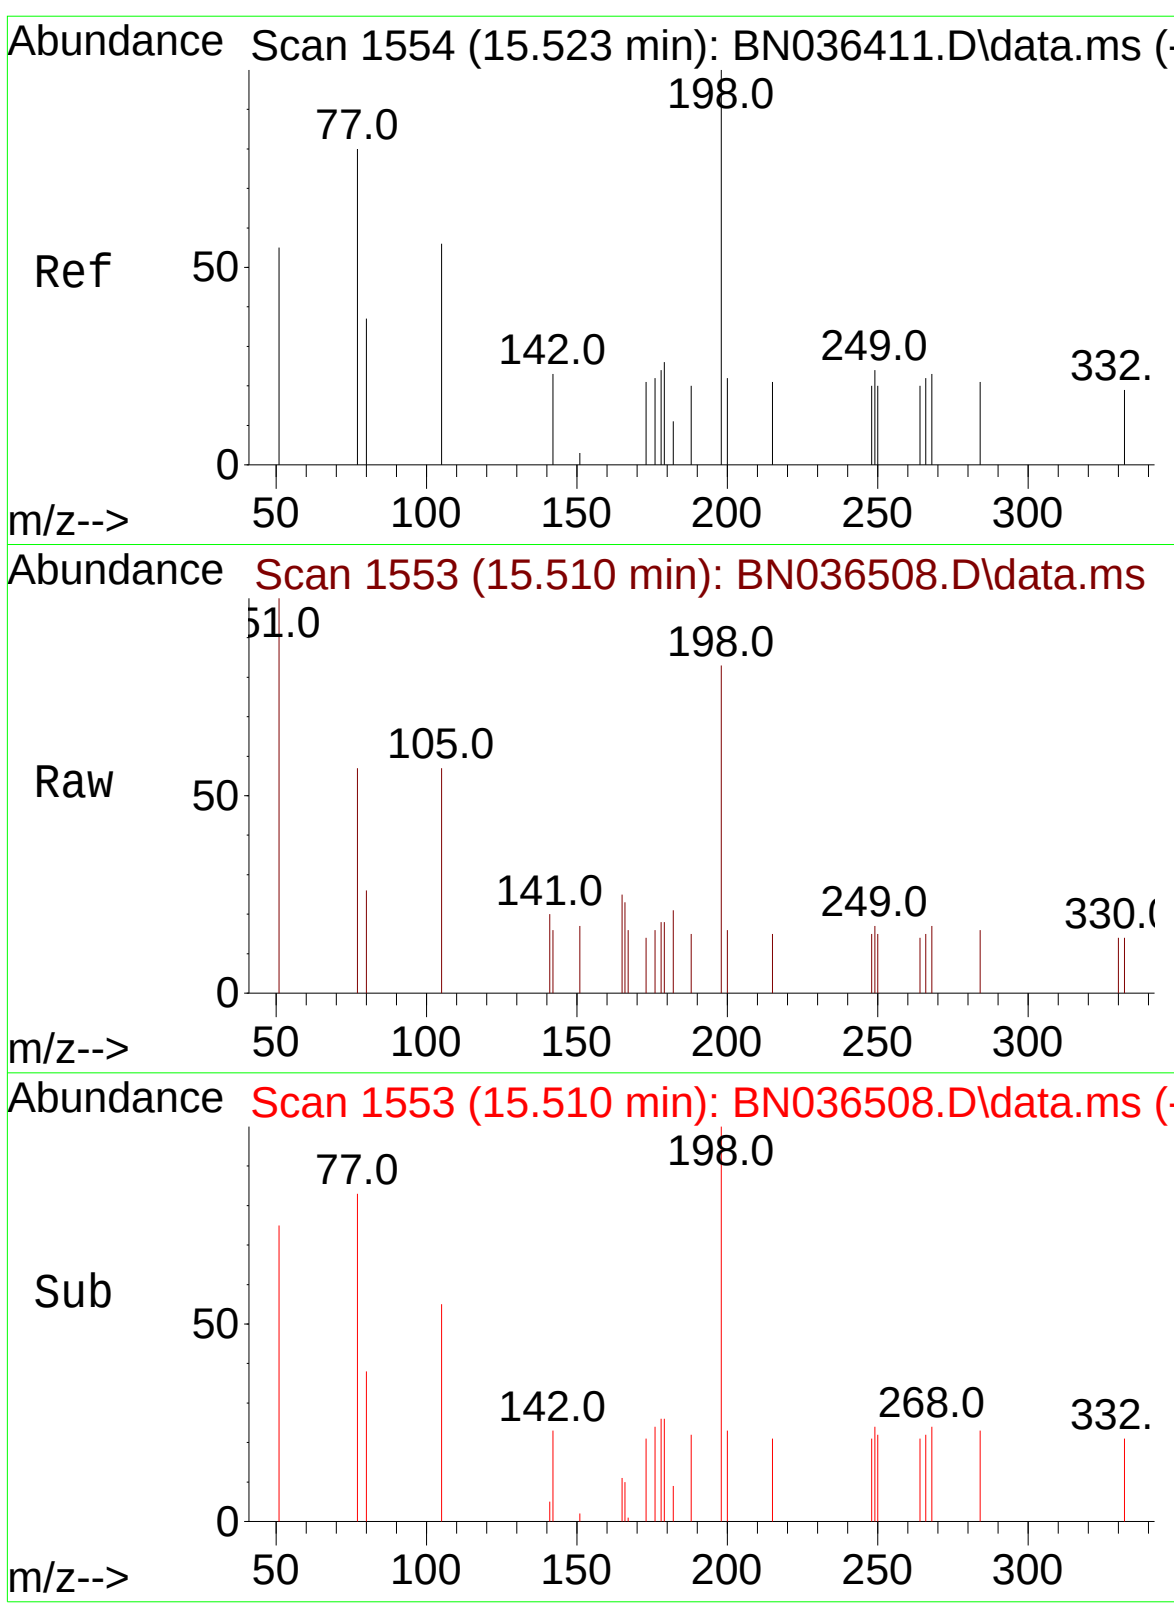

#20
4,6-Dinitro-2-methylphenol
Concen: 0.307 ng
RT: 15.510 min Scan# 1553
Delta R.T. -0.013 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Tgt Ion:198 Resp: 548

Ion	Ratio	Lower	Upper
198	100		
51	120.3	86.6	129.8
105	69.0	57.5	86.3

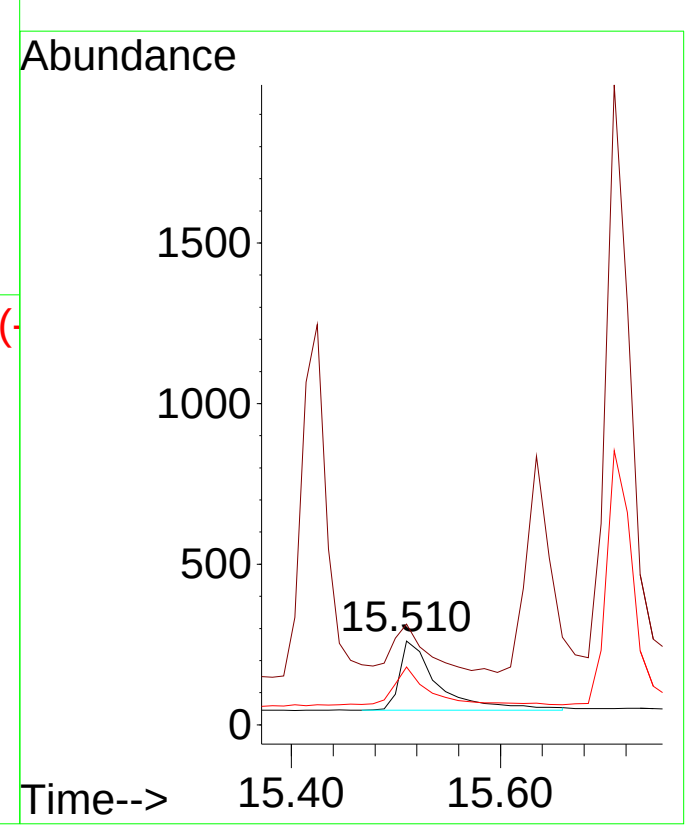

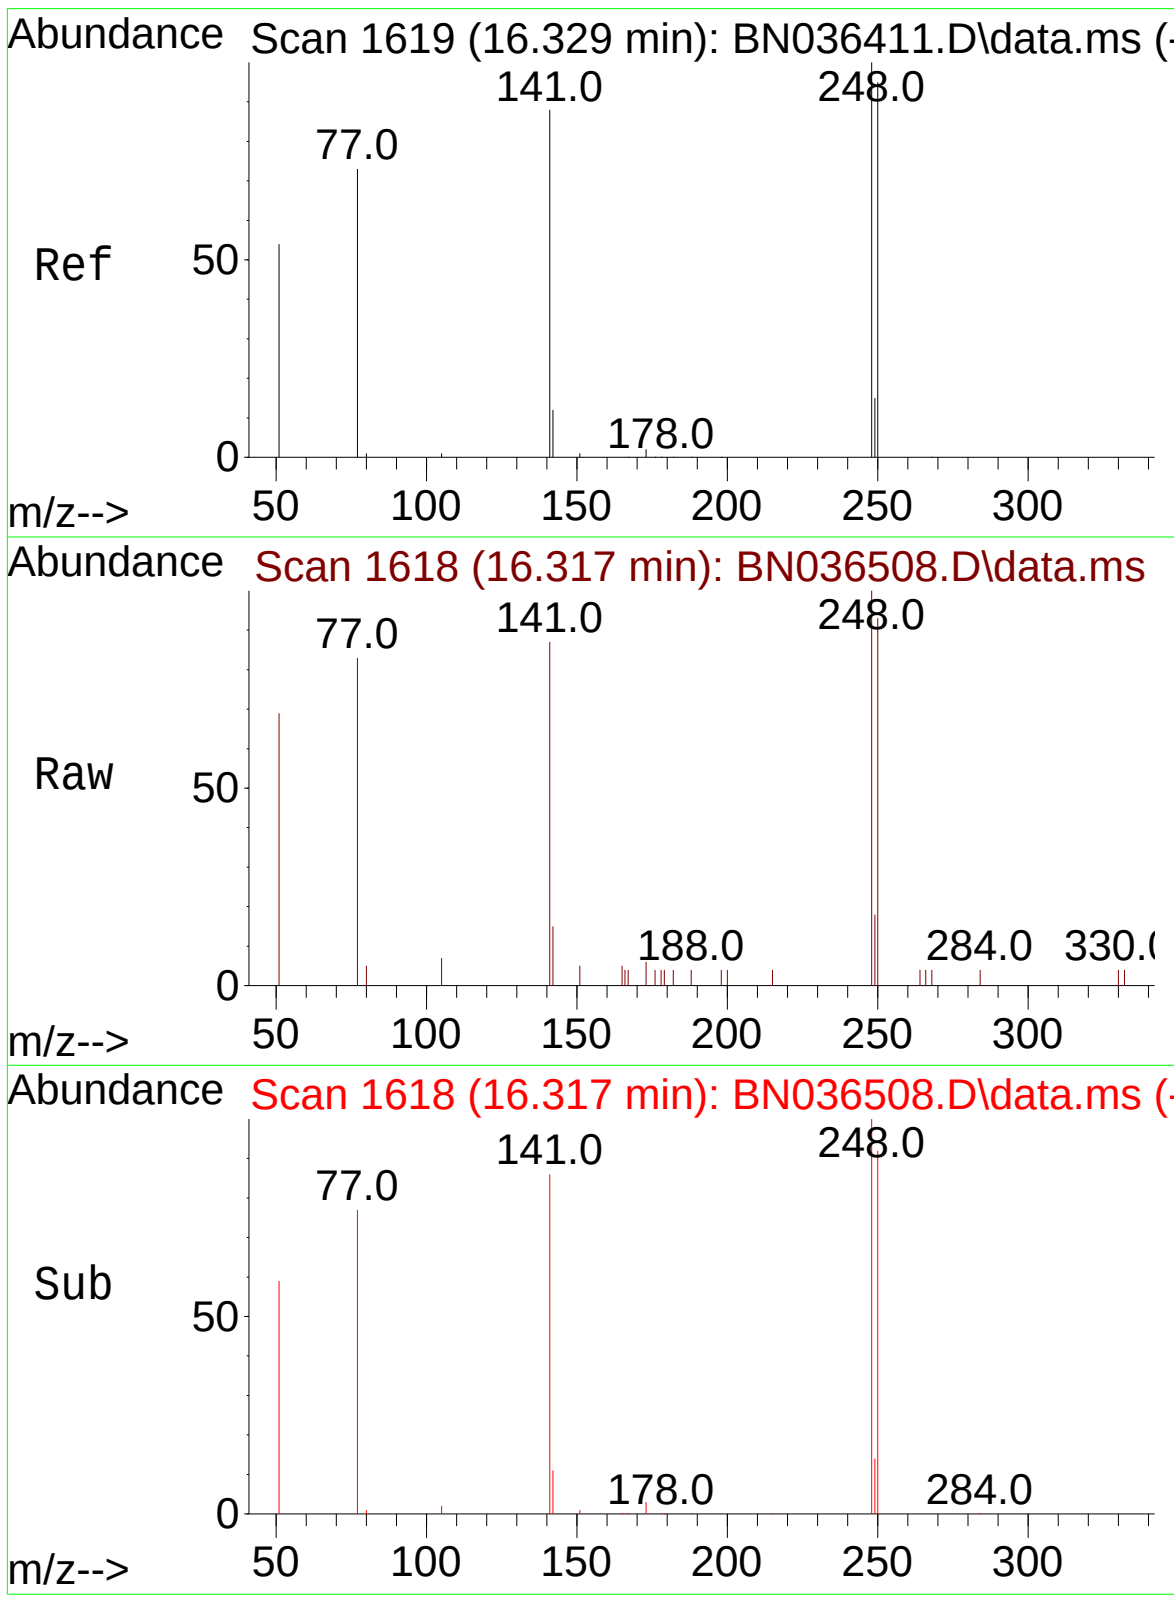

#21
4-Bromophenyl-phenylether
Concen: 0.404 ng
RT: 16.317 min Scan# 1(
Delta R.T.   -0.012 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:248 Resp: 2189

Ion	Ratio	Lower	Upper
248	100		
250	92.7	76.1	114.1
141	87.4	71.7	107.5

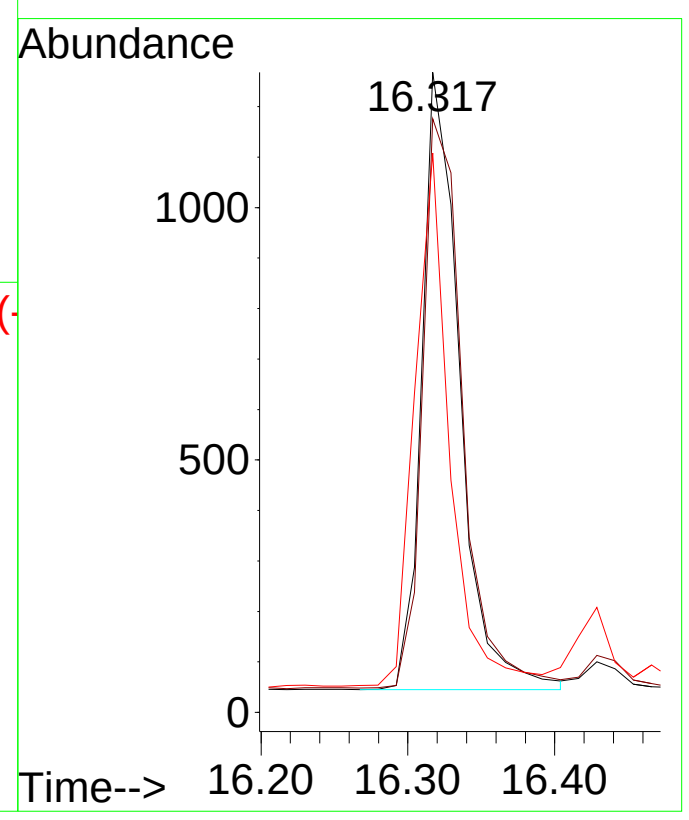

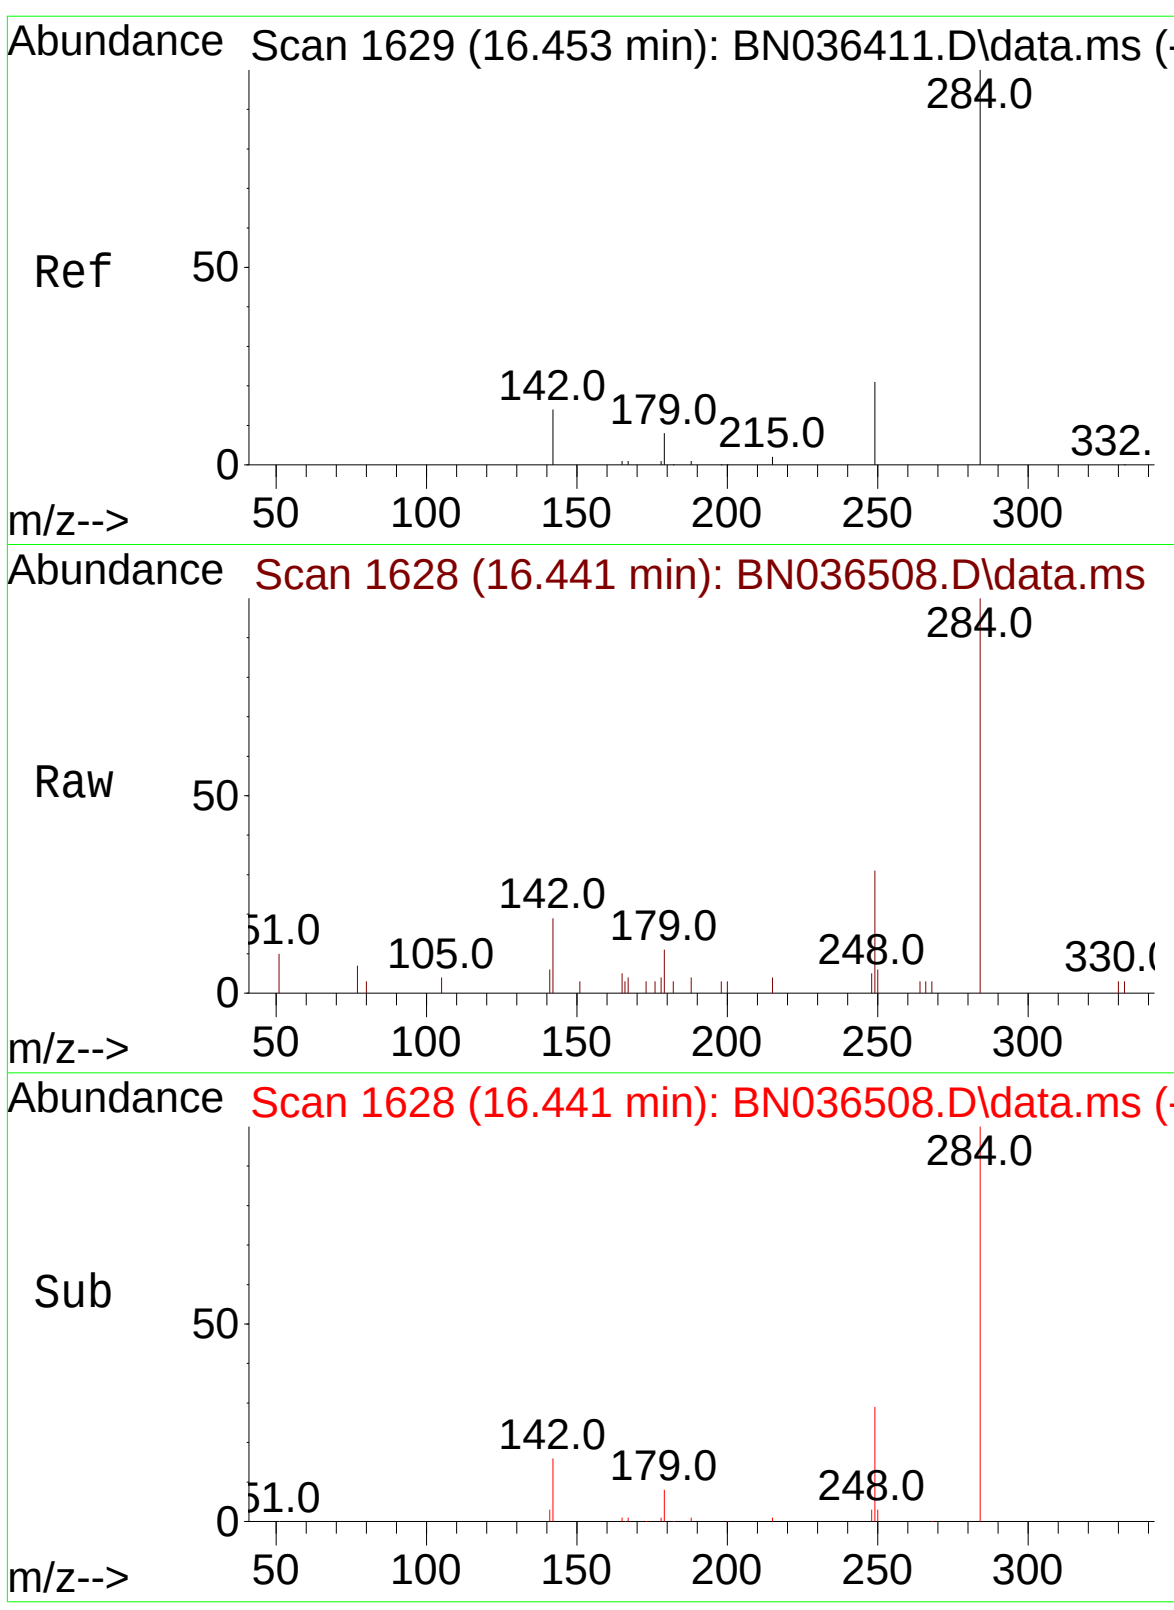

#22
Hexachlorobenzene
Concen: 0.406 ng
RT: 16.441 min Scan# 1628
Delta R.T.   -0.012 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Tgt Ion:284 Resp: 2720

Ion	Ratio	Lower	Upper
284	100		
142	46.4	33.4	50.0
249	34.2	28.6	43.0

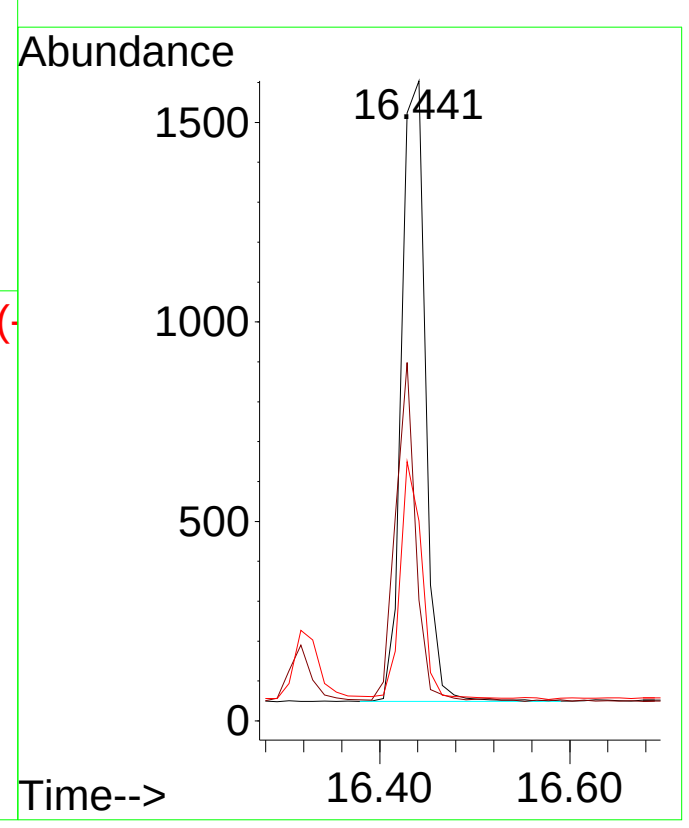

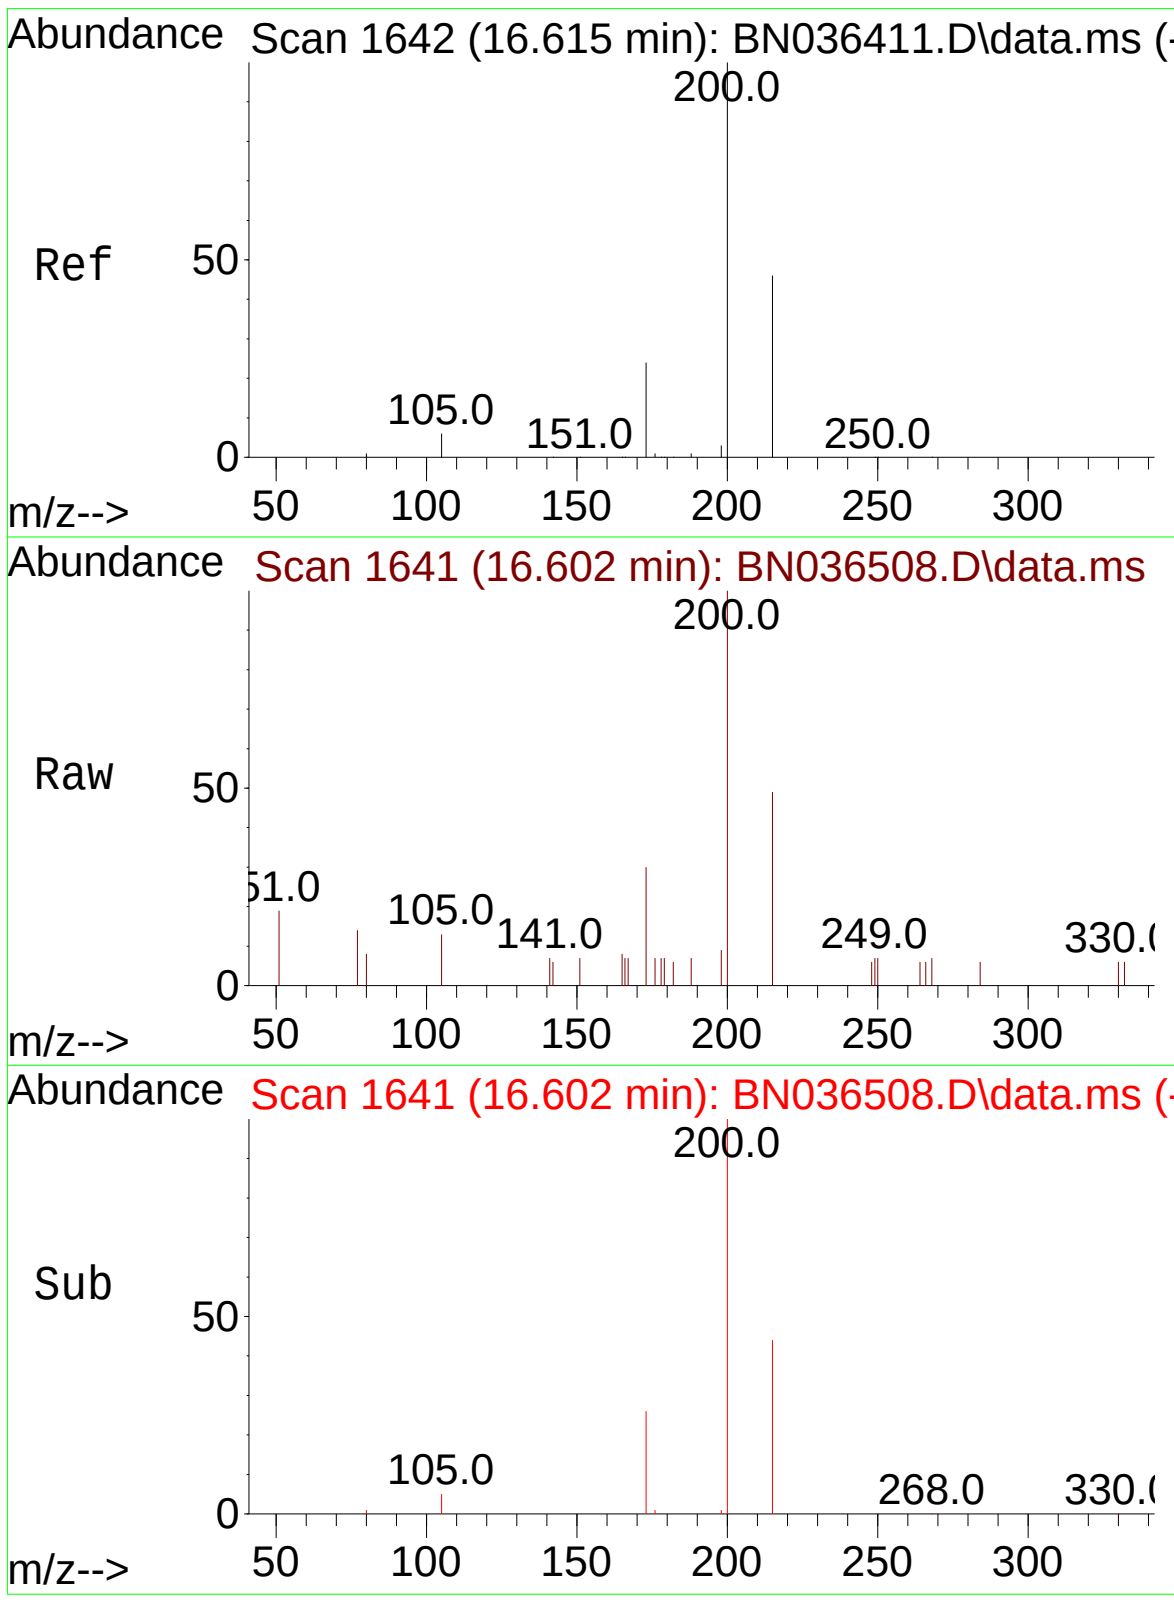

#23
Atrazine
Concen: 0.375 ng
RT: 16.602 min Scan# 1
Delta R.T. -0.012 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:200 Resp: 1700

Ion	Ratio	Lower	Upper
200	100		
173	30.1	23.2	34.8
215	48.9	40.0	60.0

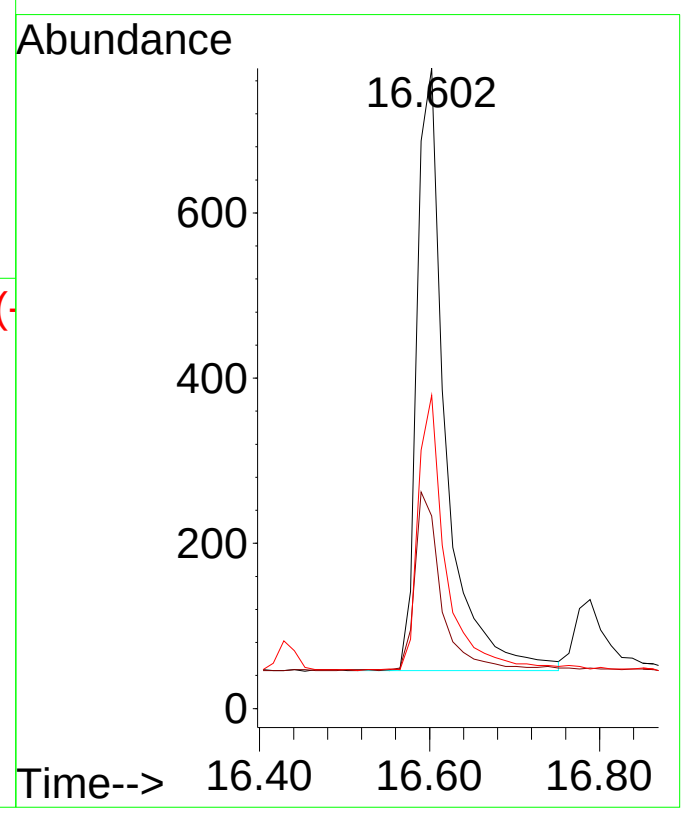

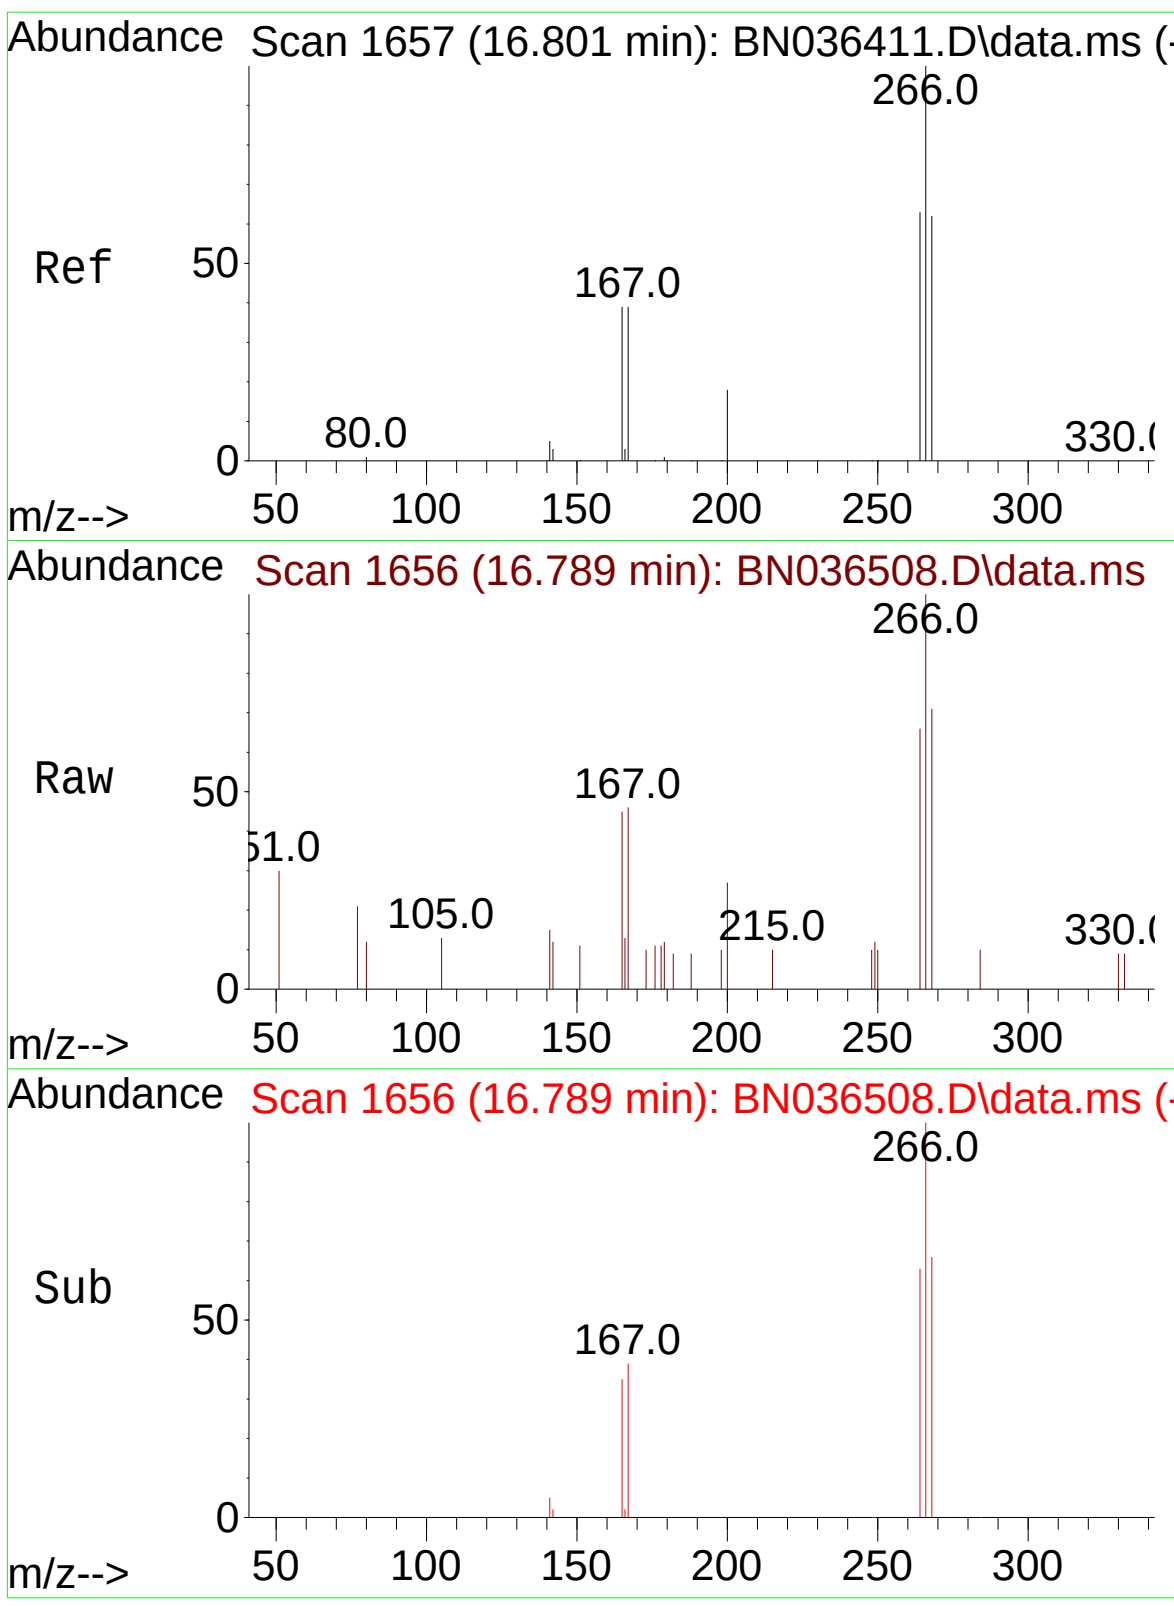

#24
Pentachlorophenol
Concen: 0.346 ng
RT: 16.789 min Scan# 1656
Delta R.T. -0.012 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Tgt Ion:266 Resp: 1101

Ion	Ratio	Lower	Upper
266	100		
264	61.3	50.6	76.0
268	63.4	51.9	77.9

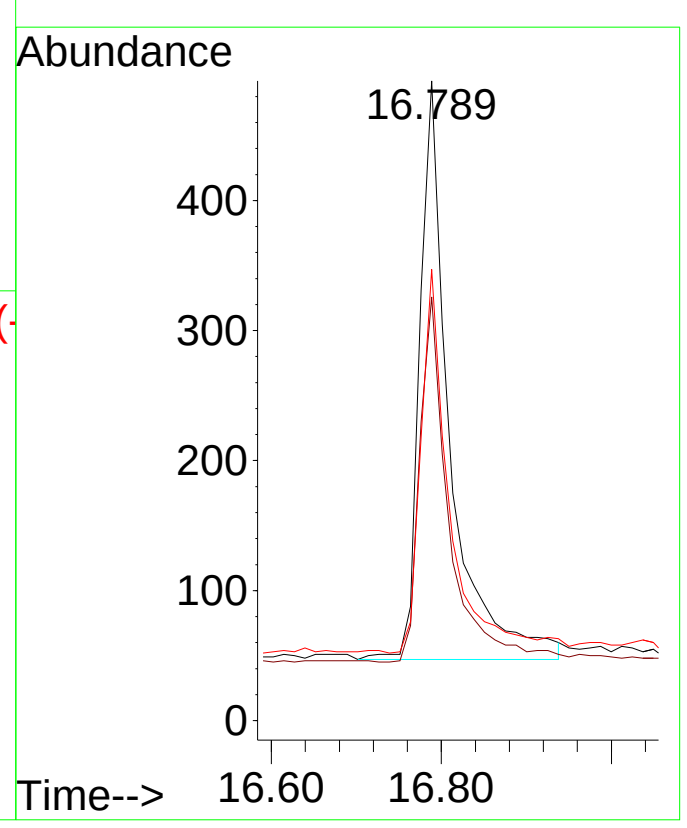

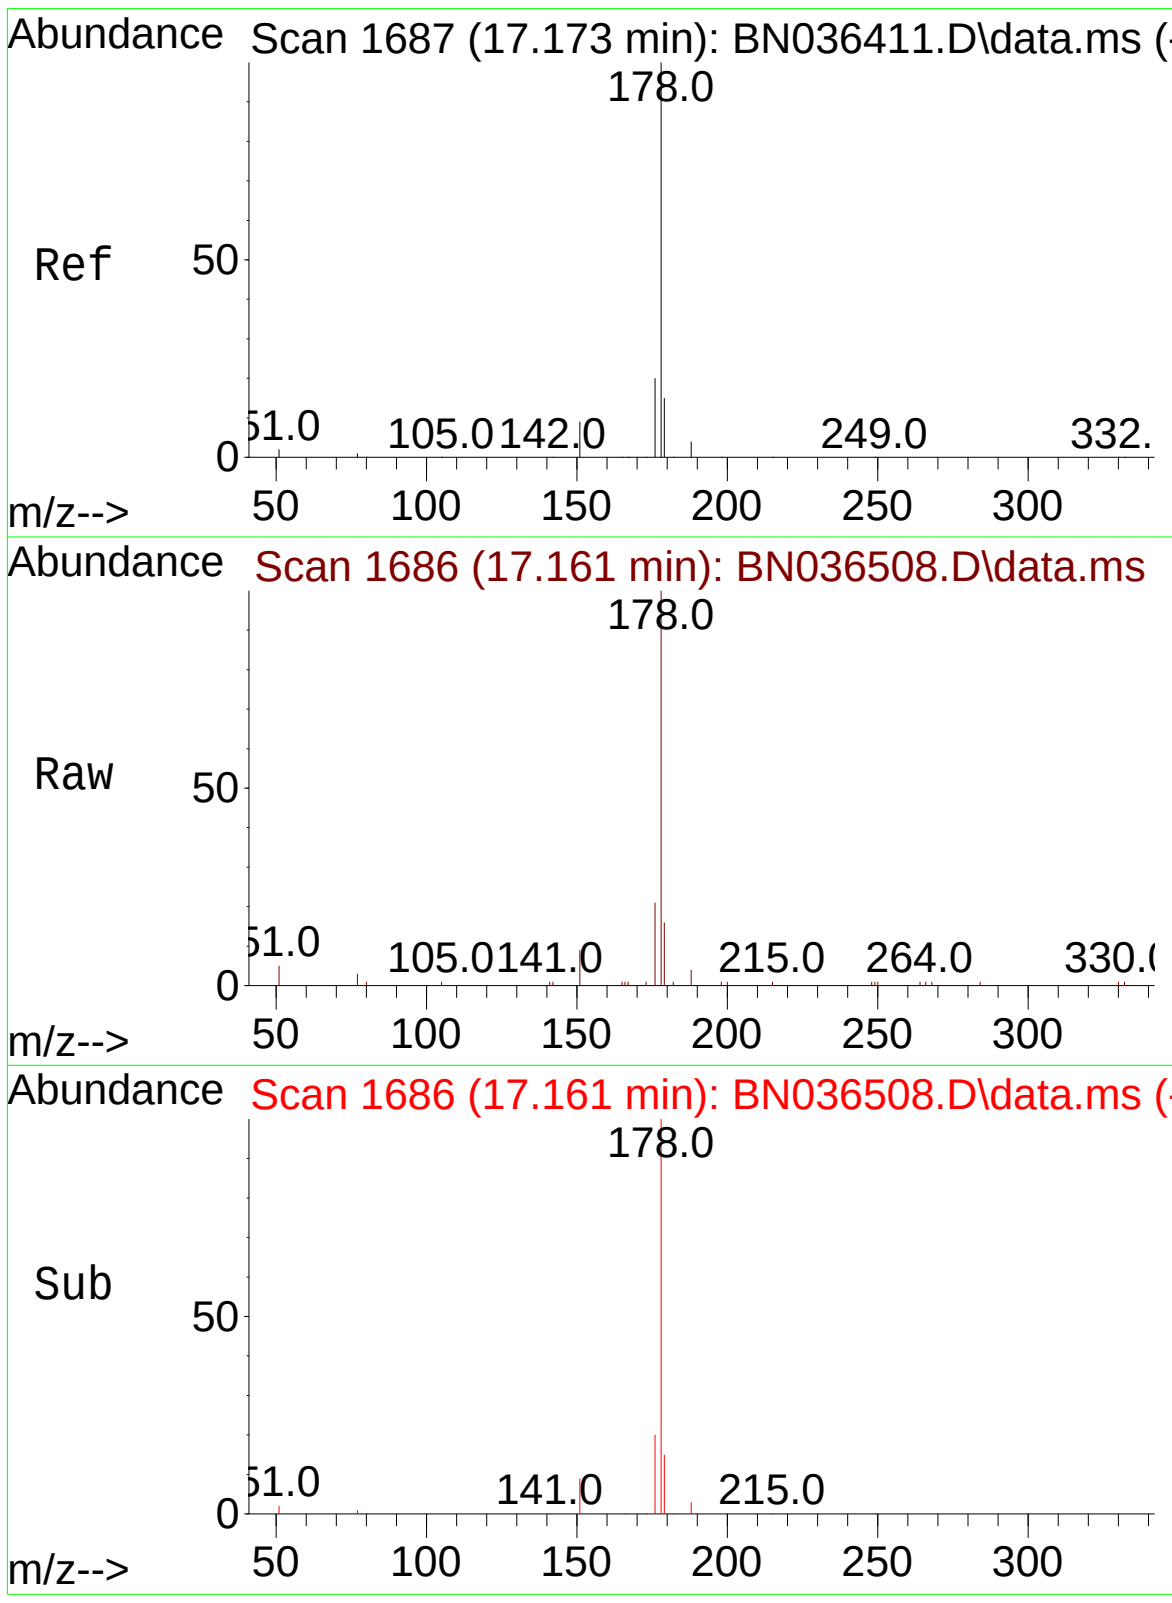

#25
Phenanthrene
Concen: 0.397 ng
RT: 17.161 min Scan# 1(
Delta R.T. -0.012 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:178 Resp: 10441

Ion	Ratio	Lower	Upper
178	100		
176	19.8	15.7	23.5
179	15.2	12.4	18.6

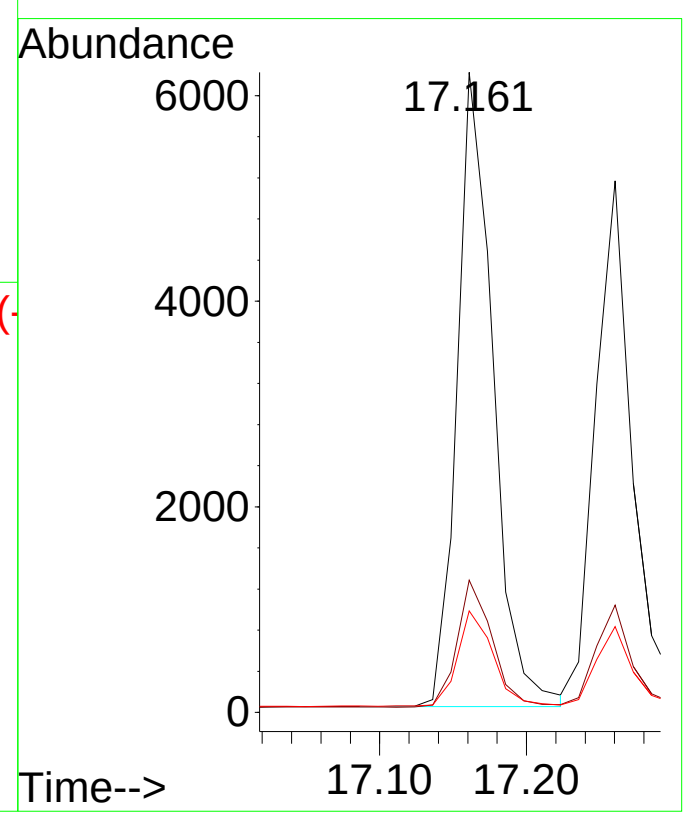

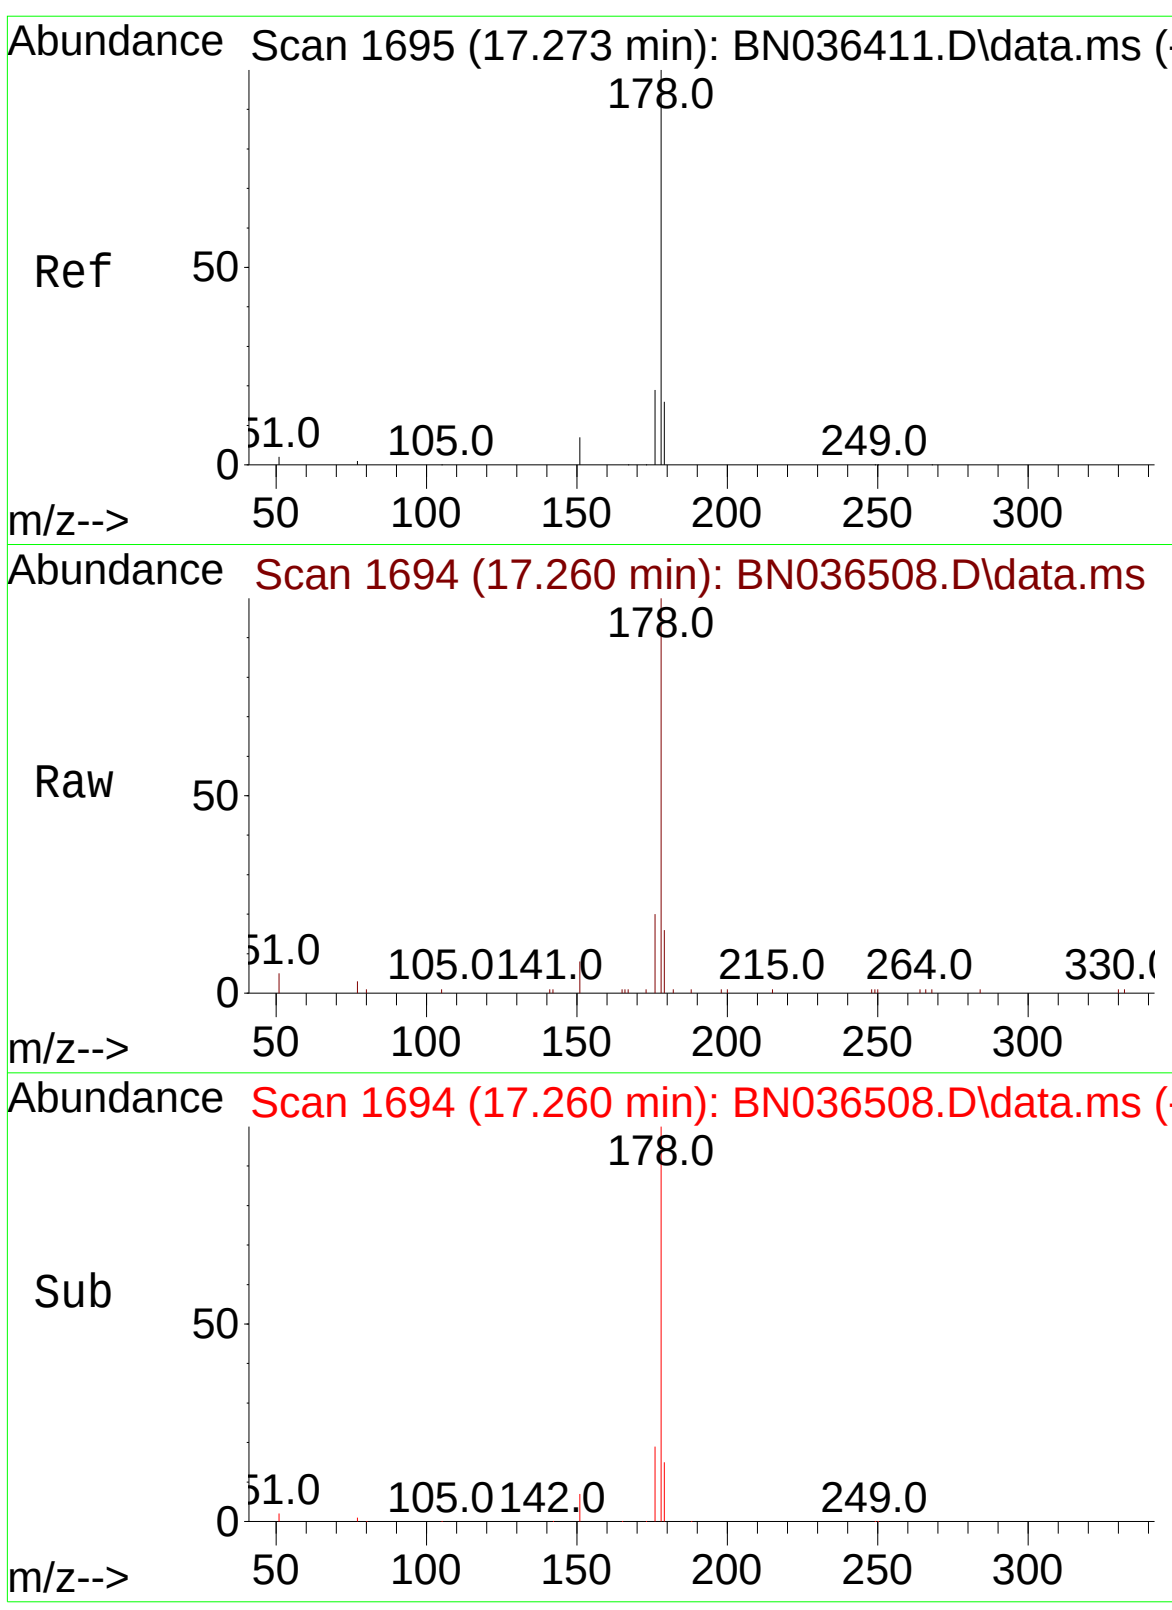

#26
Anthracene
Concen: 0.395 ng
RT: 17.260 min Scan# 1694
Delta R.T. -0.012 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Tgt Ion:178 Resp: 9164

Ion	Ratio	Lower	Upper
178	100		
176	18.9	14.9	22.3
179	15.0	12.4	18.6

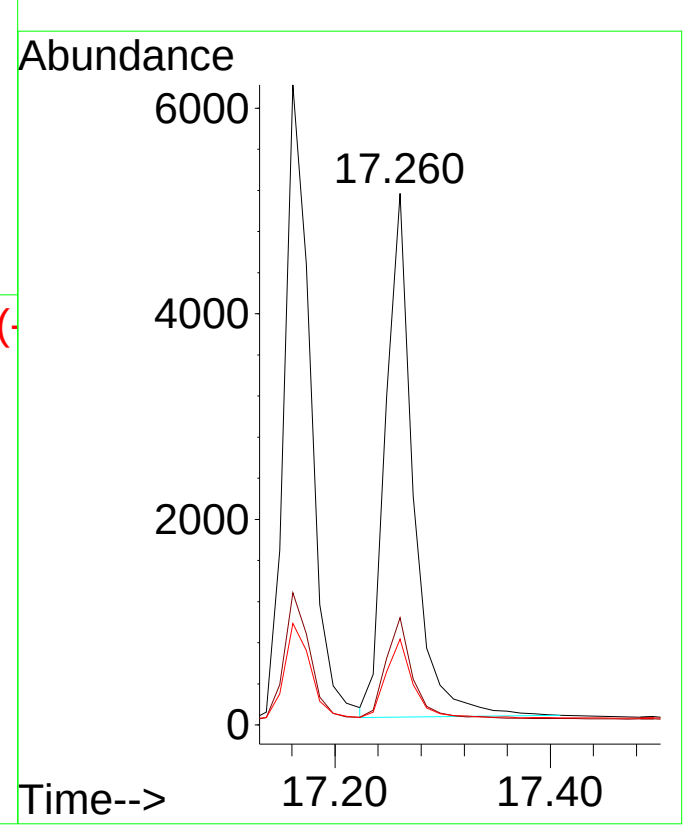

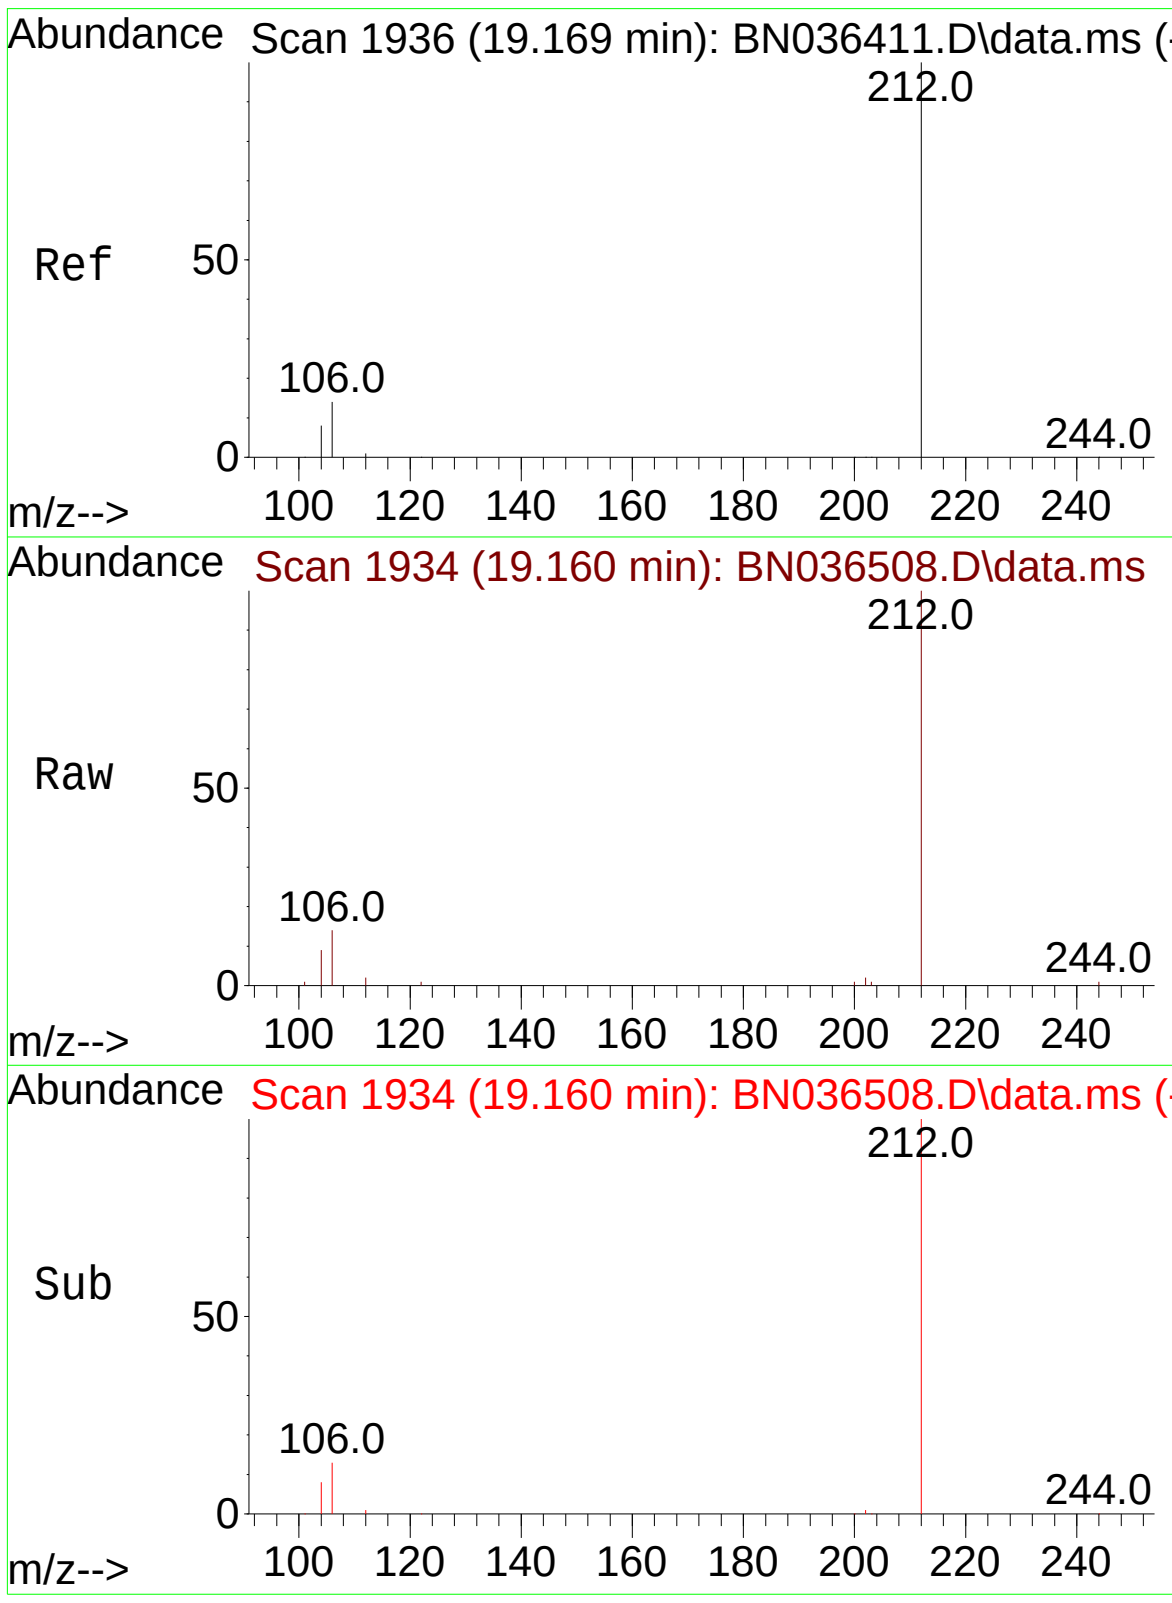

#27
Fluoranthene-d10
Concen: 0.367 ng
RT: 19.160 min Scan# 1
Delta R.T. -0.009 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:212 Resp: 9278

Ion	Ratio	Lower	Upper
212	100		
106	14.5	11.5	17.3
104	9.0	7.1	10.7

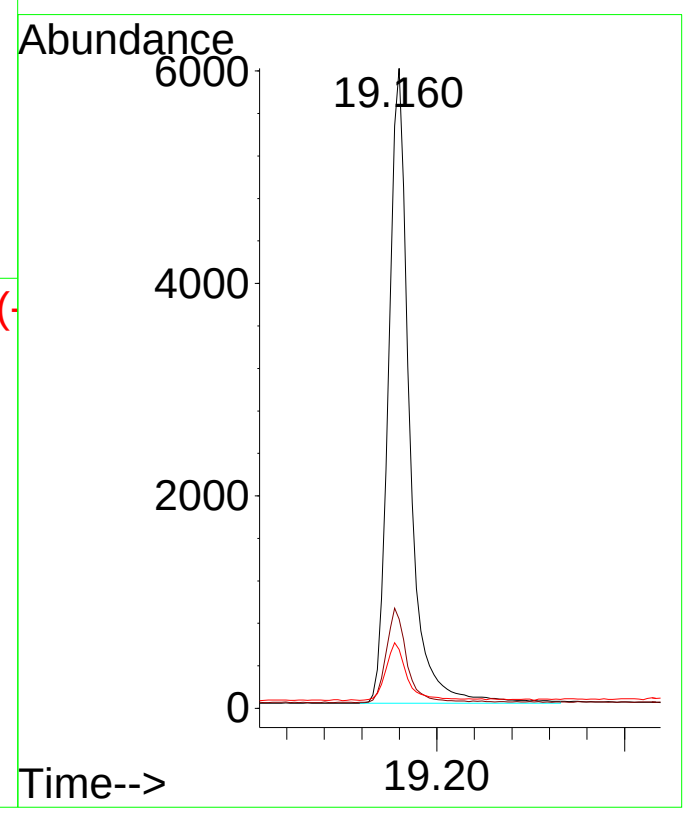

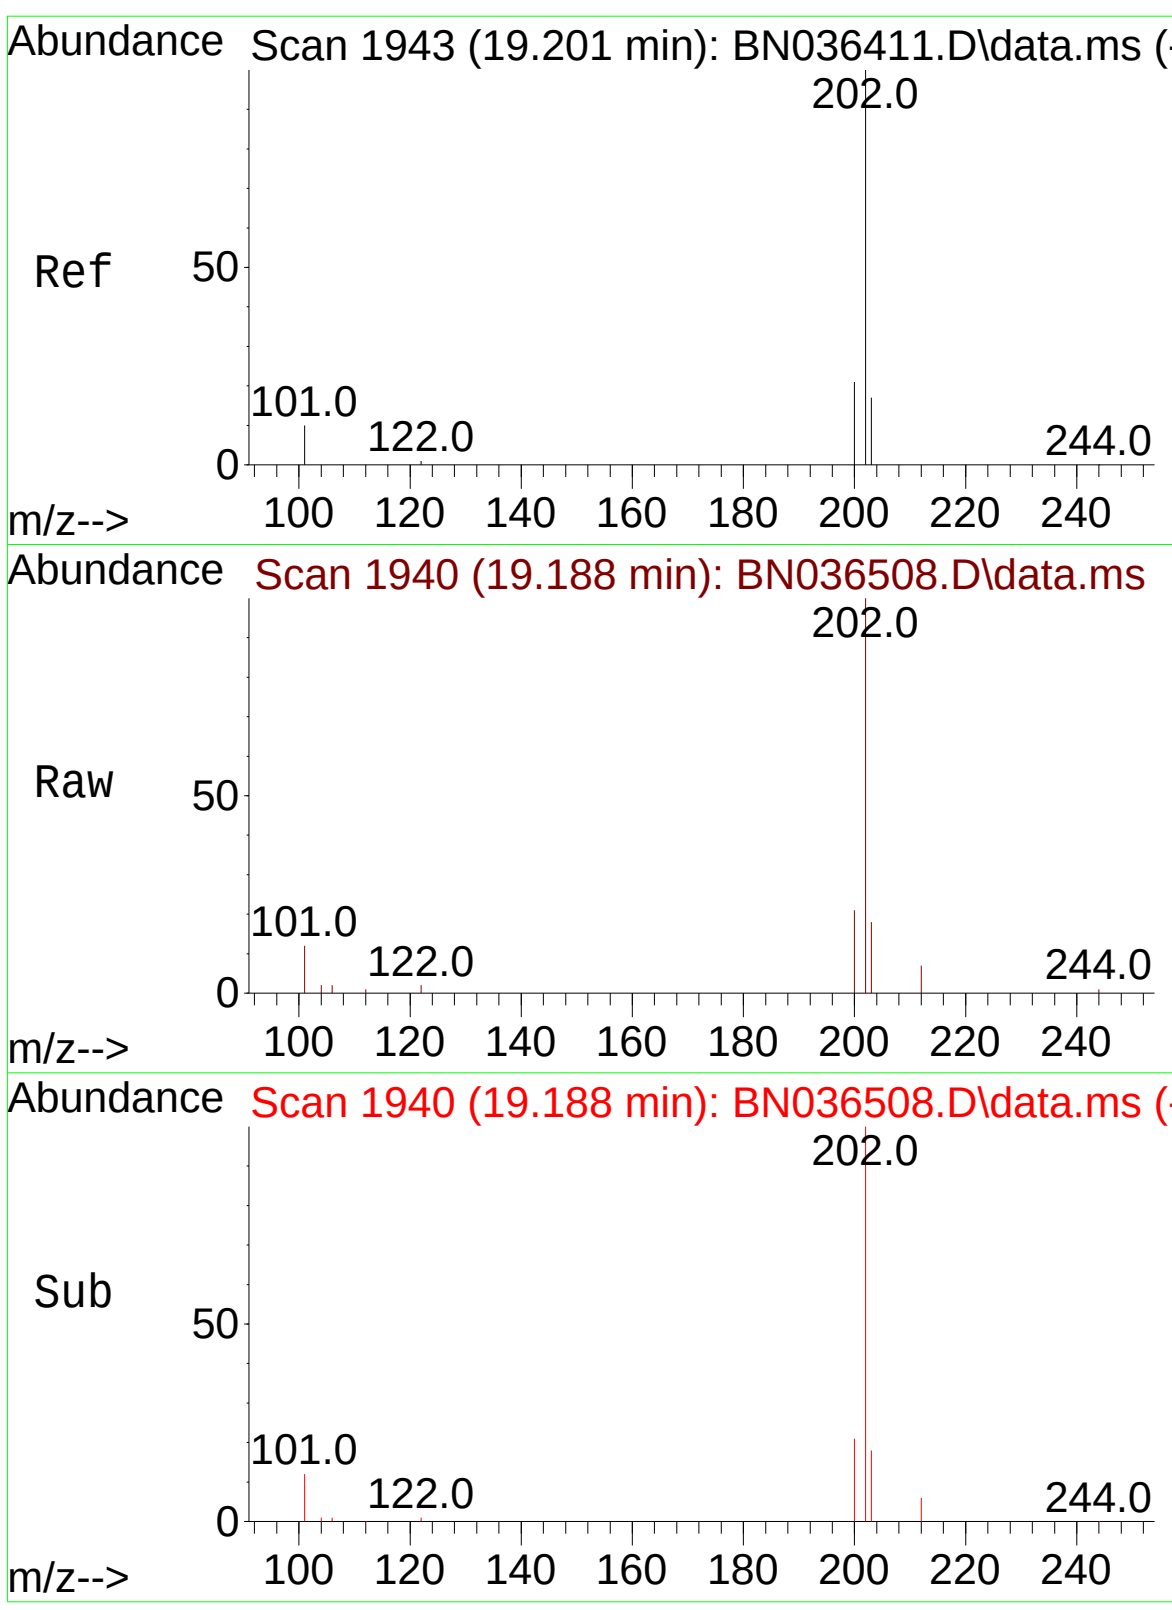

#28
Fluoranthene
Concen: 0.367 ng
RT: 19.188 min Scan# 1940
Delta R.T. -0.014 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Tgt Ion:202 Resp: 11838

Ion	Ratio	Lower	Upper
202	100		
101	11.8	9.2	13.8
203	17.1	13.4	20.0

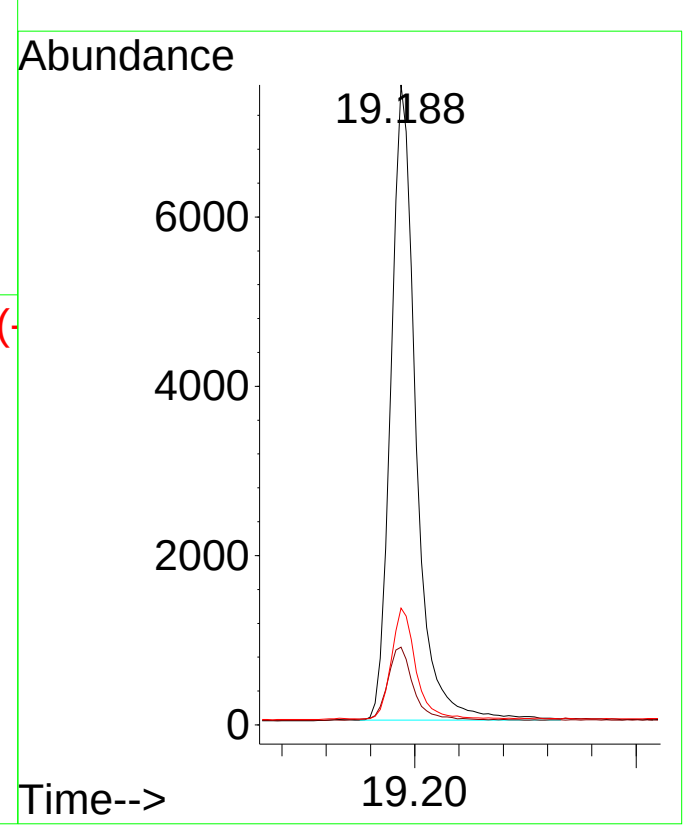

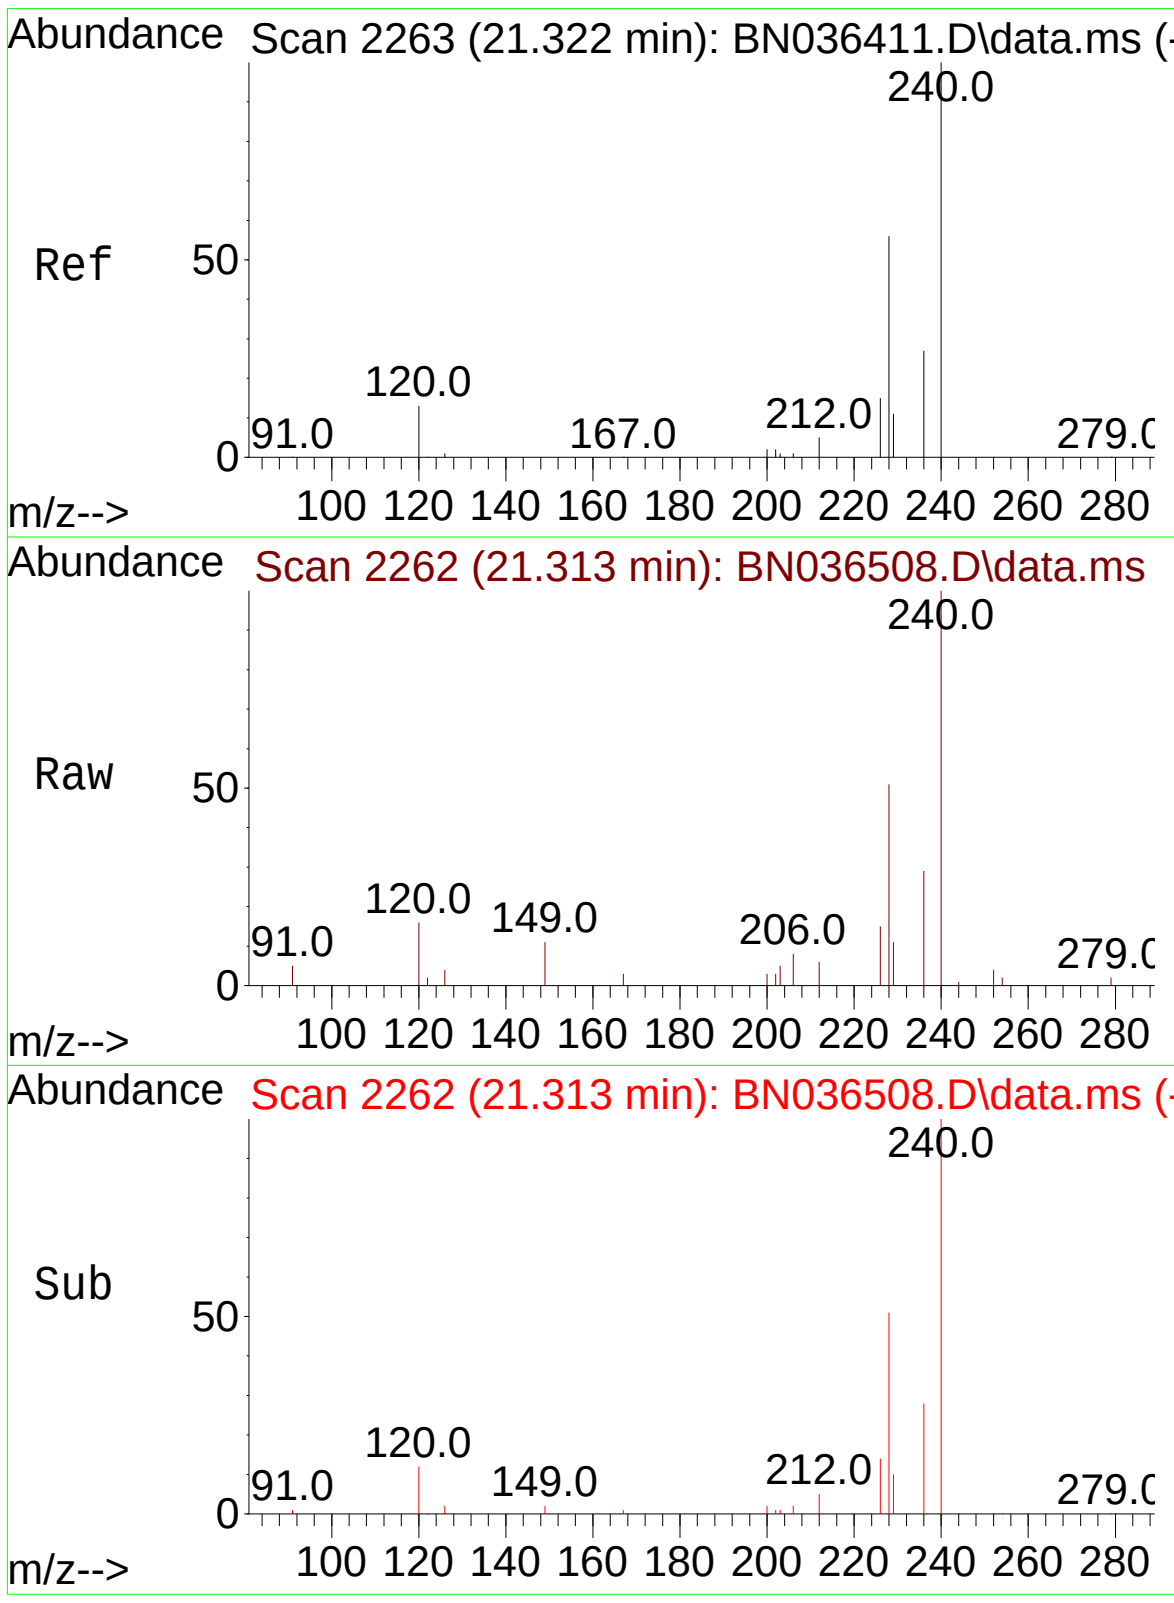

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.313 min Scan# 2

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Delta R.T. -0.009 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Tgt Ion:240 Resp: 6639

Ion	Ratio	Lower	Upper
240	100		
120	15.7	13.3	19.9
236	29.1	23.0	34.6

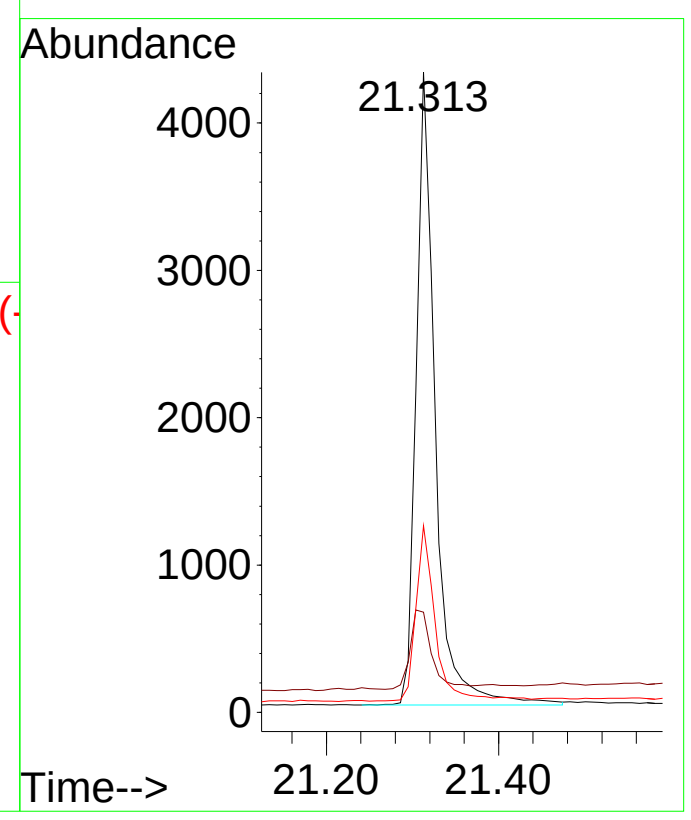

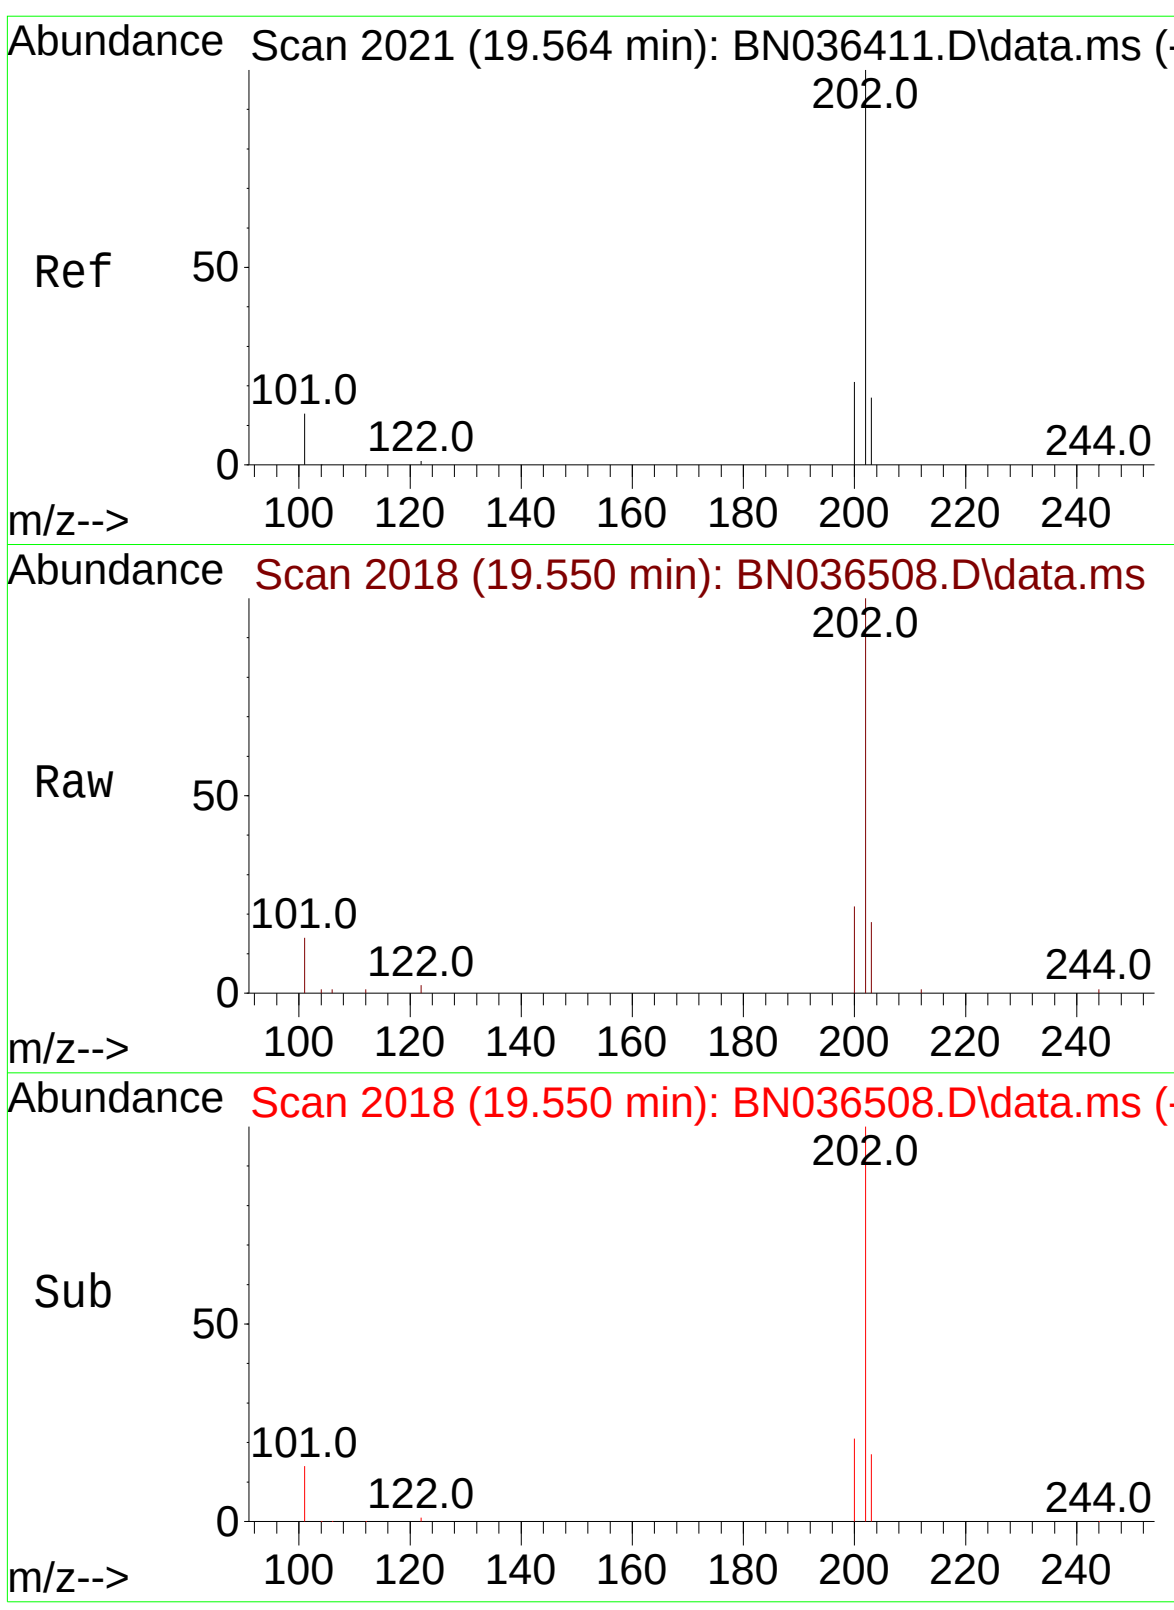

#30
Pyrene
Concen: 0.468 ng
RT: 19.550 min Scan# 2018
Delta R.T. -0.014 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Tgt Ion:202 Resp: 11970

Ion	Ratio	Lower	Upper
202	100		
200	21.3	16.9	25.3
203	17.7	13.9	20.9

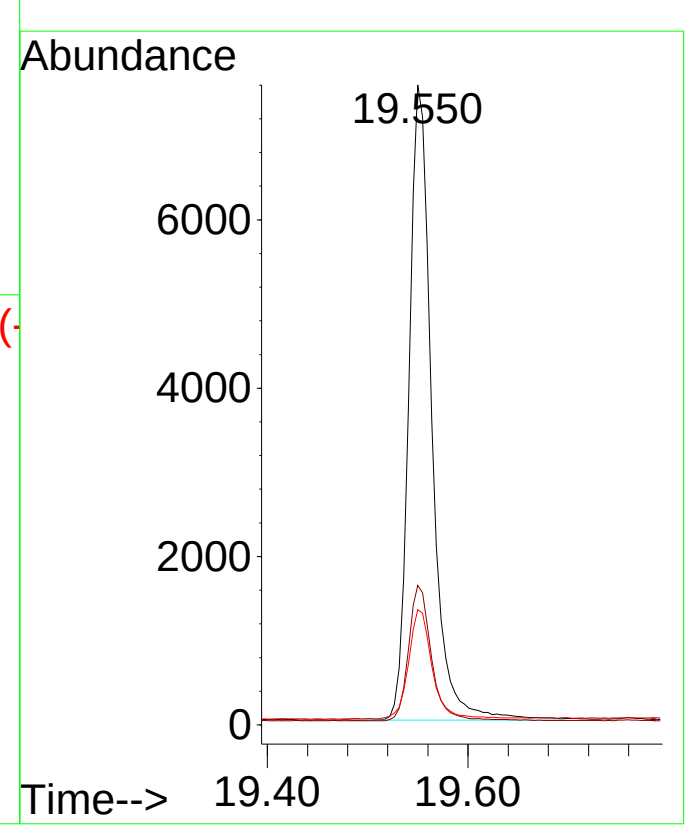

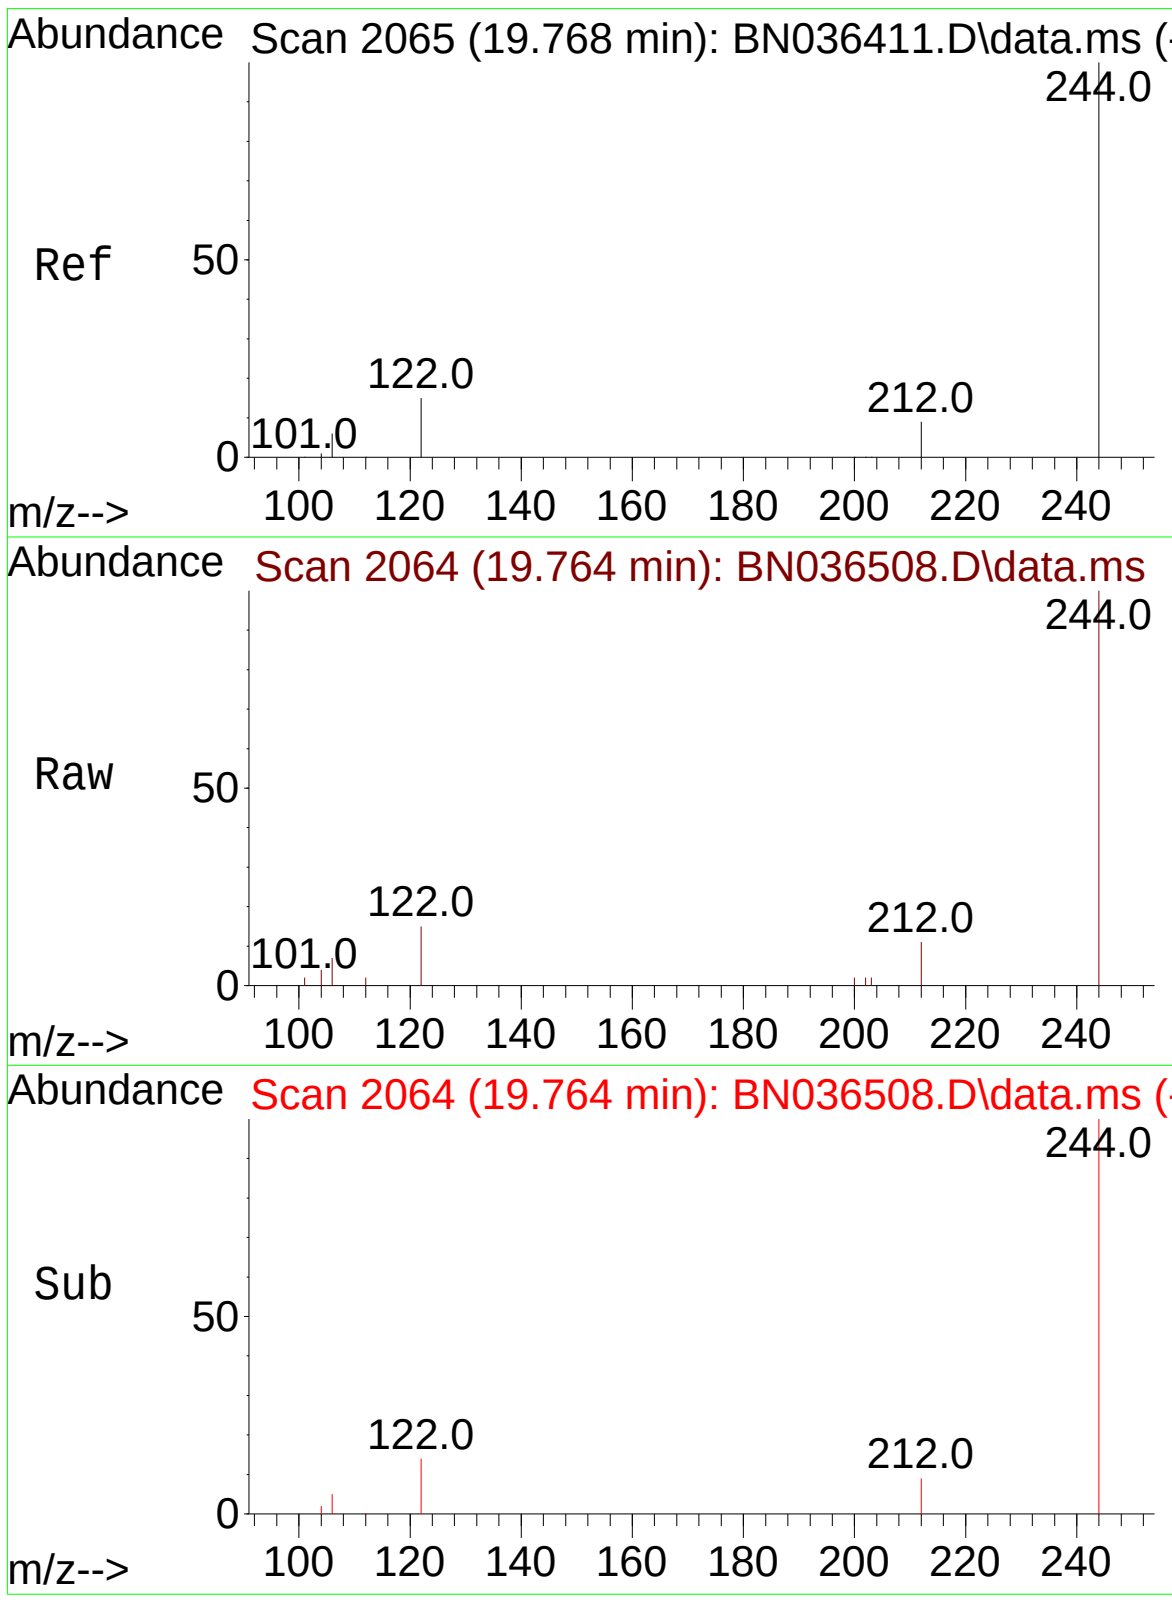

#31
Terphenyl-d14
Concen: 0.427 ng
RT: 19.764 min Scan# 2(
Delta R.T. -0.005 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:244 Resp: 6045

Ion	Ratio	Lower	Upper
244	100		
212	10.8	8.1	12.1
122	15.4	12.8	19.2

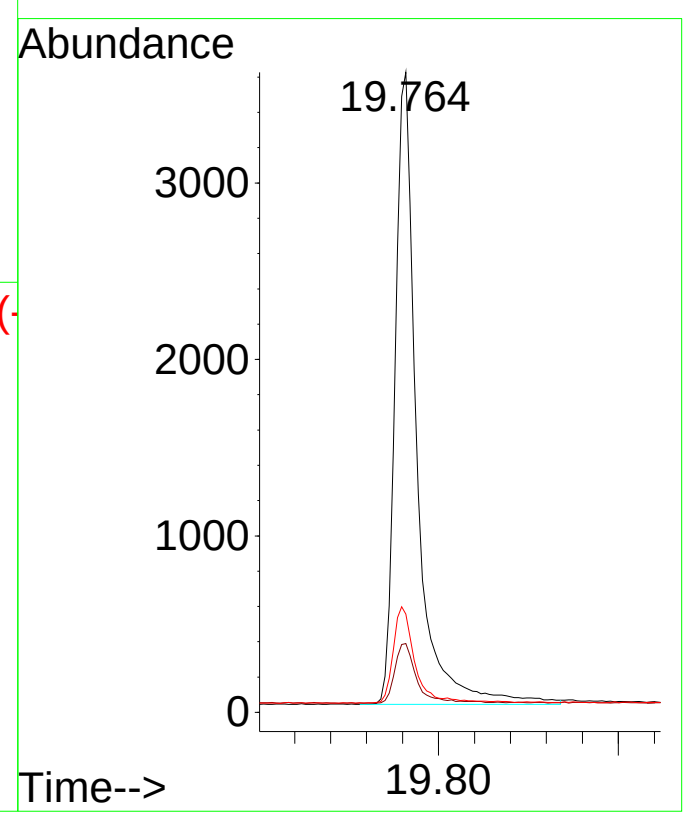

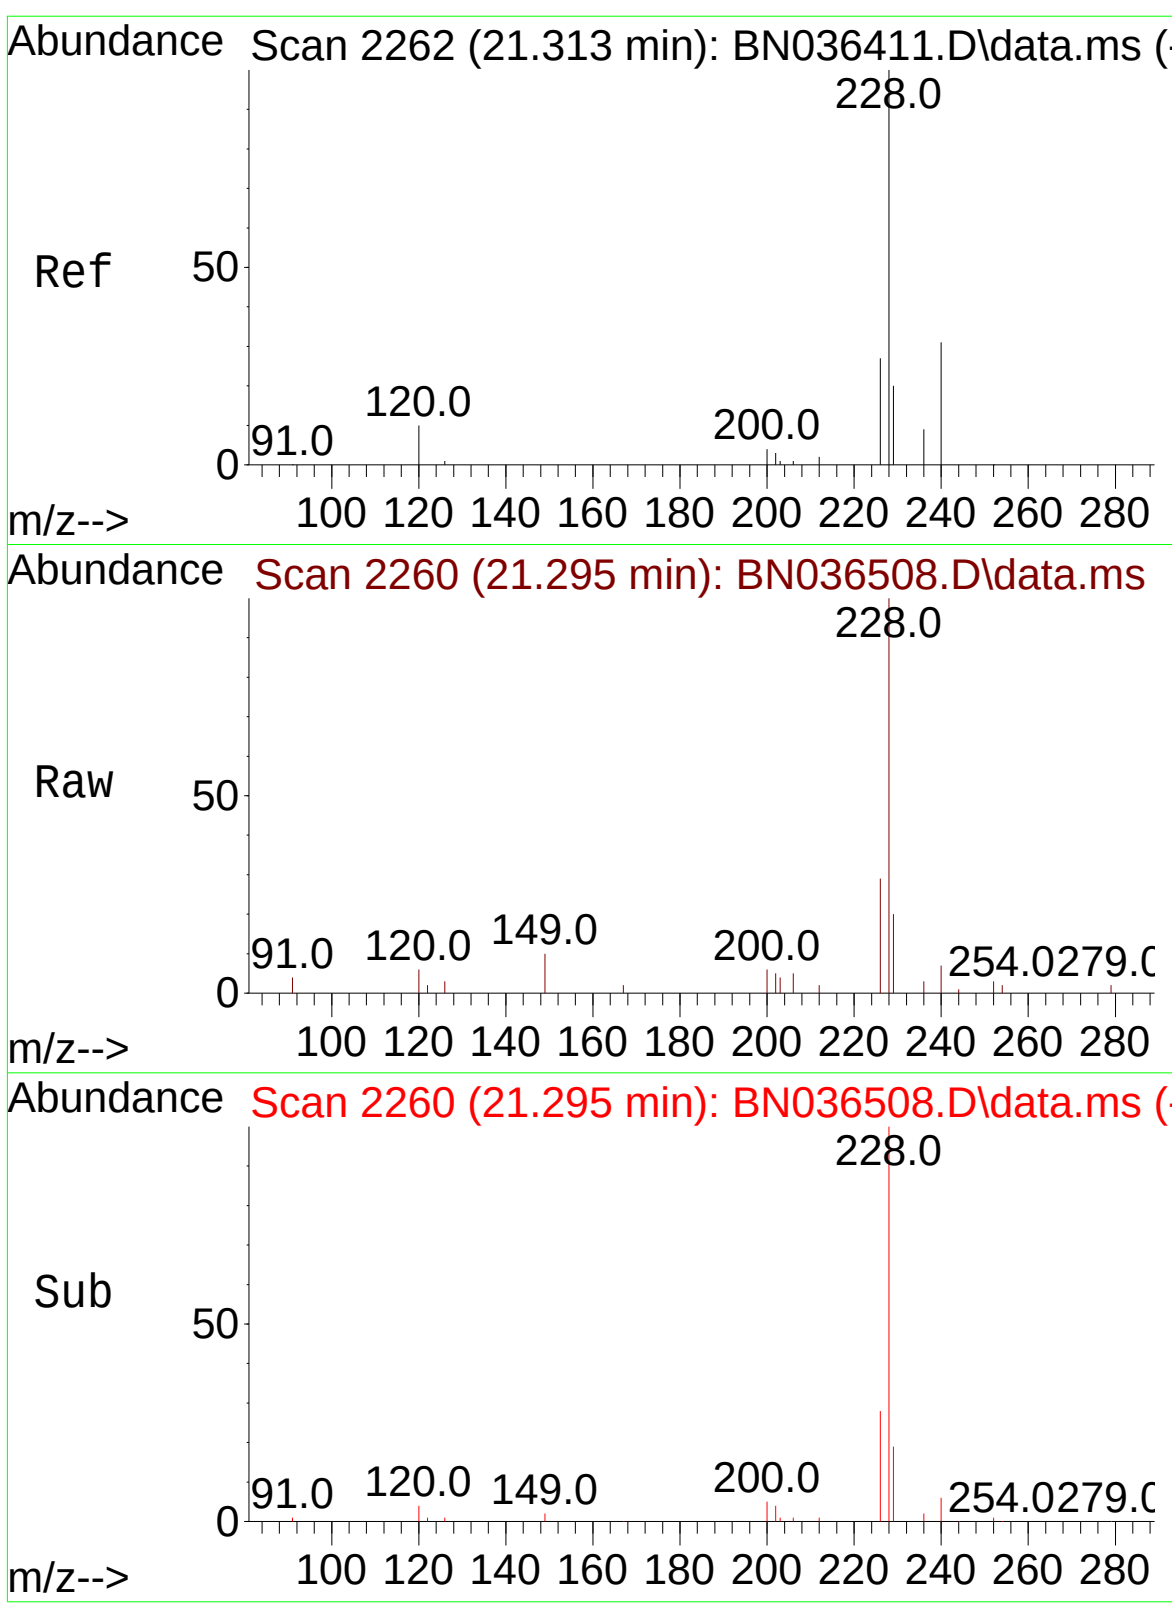

#32
Benzo(a)anthracene
Concen: 0.384 ng
RT: 21.295 min Scan# 2260
Delta R.T. -0.018 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Tgt Ion:228 Resp: 8384

Ion	Ratio	Lower	Upper
228	100		
226	28.9	22.2	33.2
229	20.3	16.5	24.7

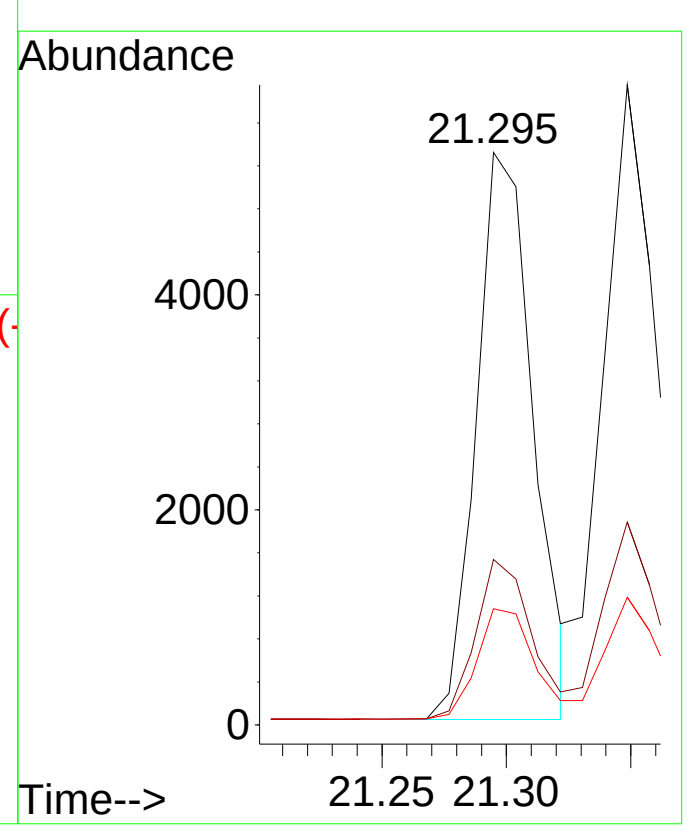

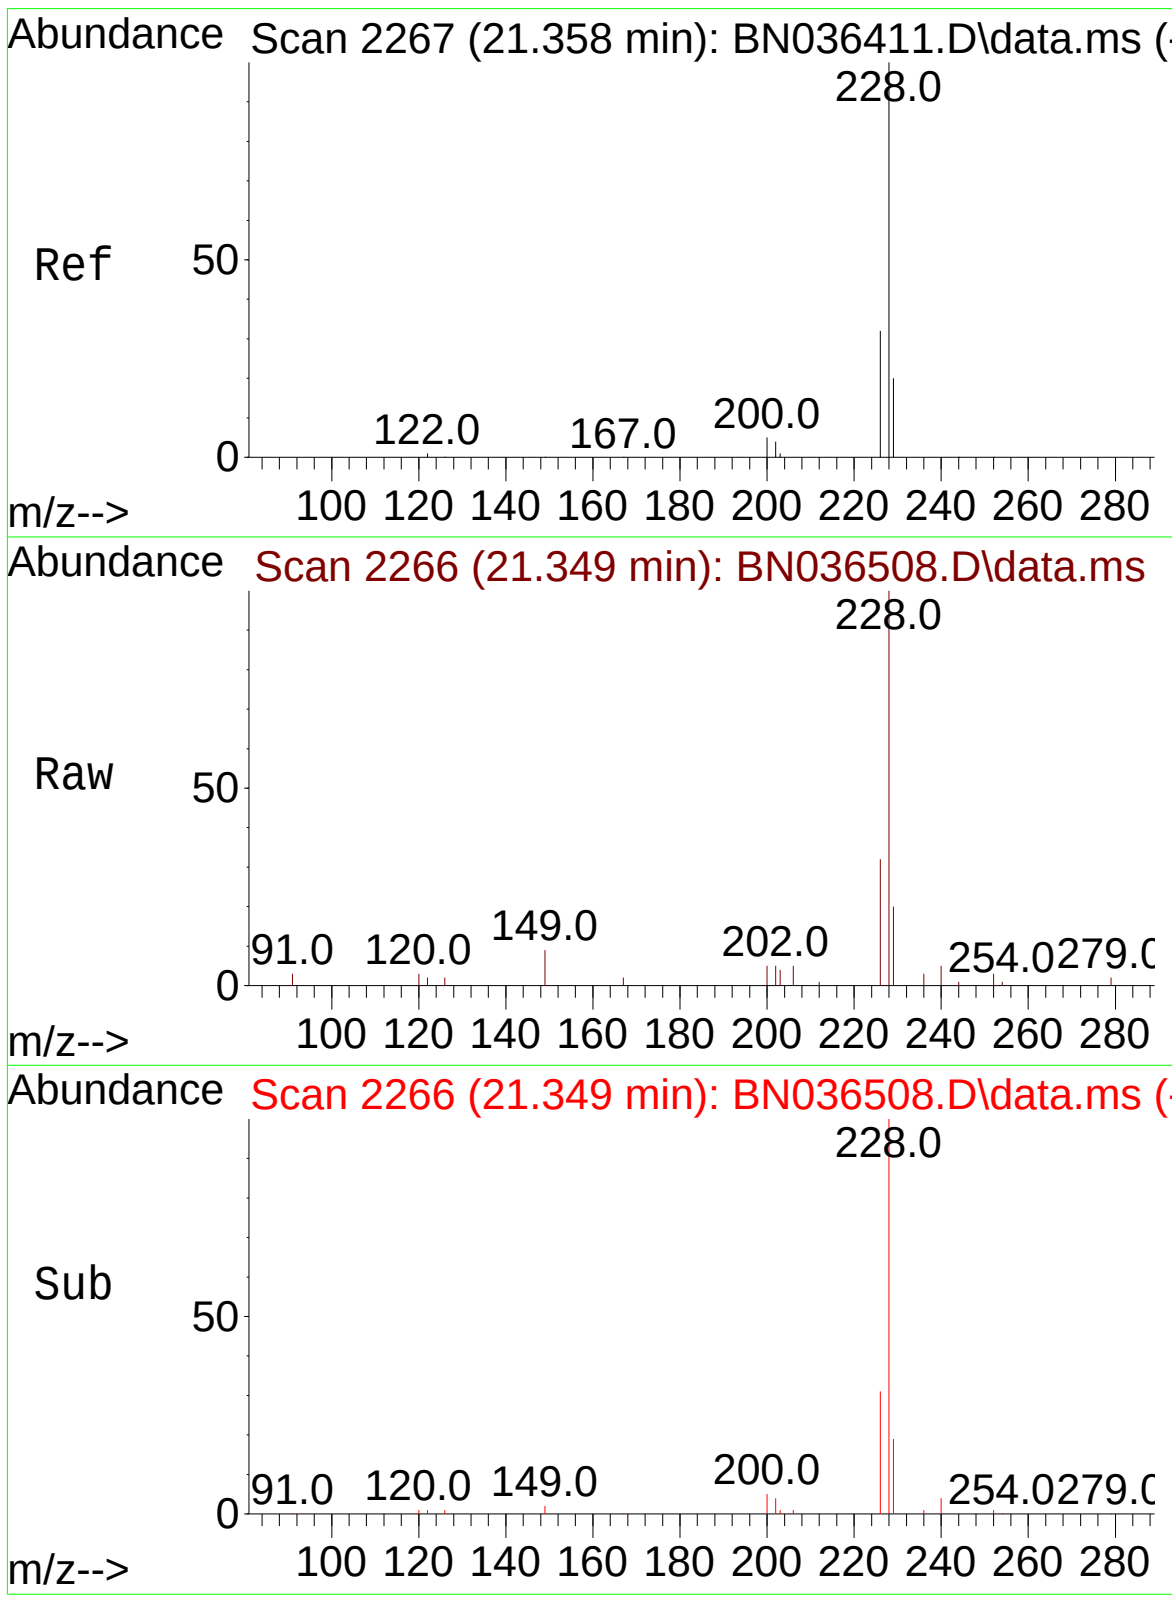

#33
Chrysene
Concen: 0.420 ng
RT: 21.349 min Scan# 2
Delta R.T. -0.009 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:228 Resp: 9942

Ion	Ratio	Lower	Upper
228	100		
226	31.7	25.5	38.3
229	19.9	16.4	24.6

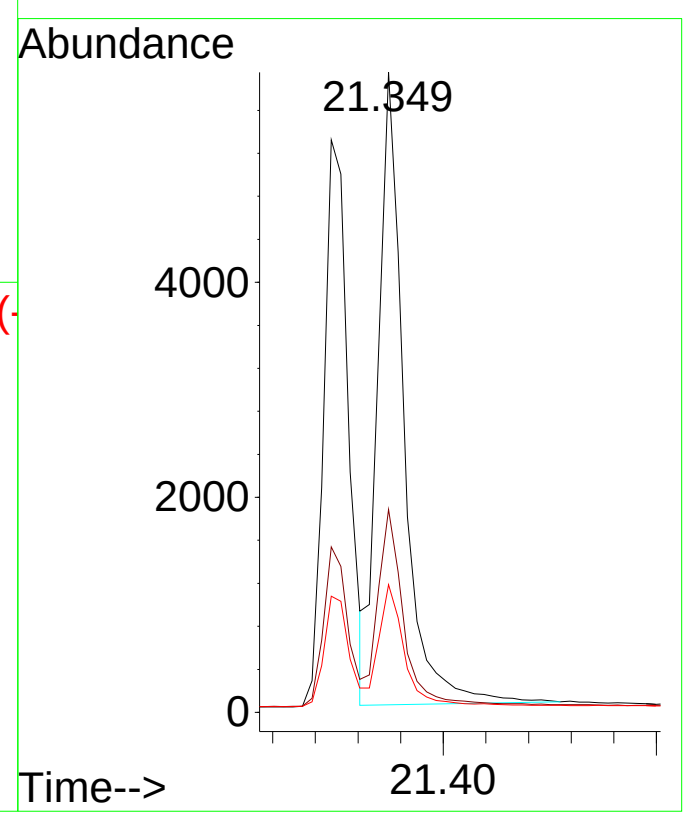

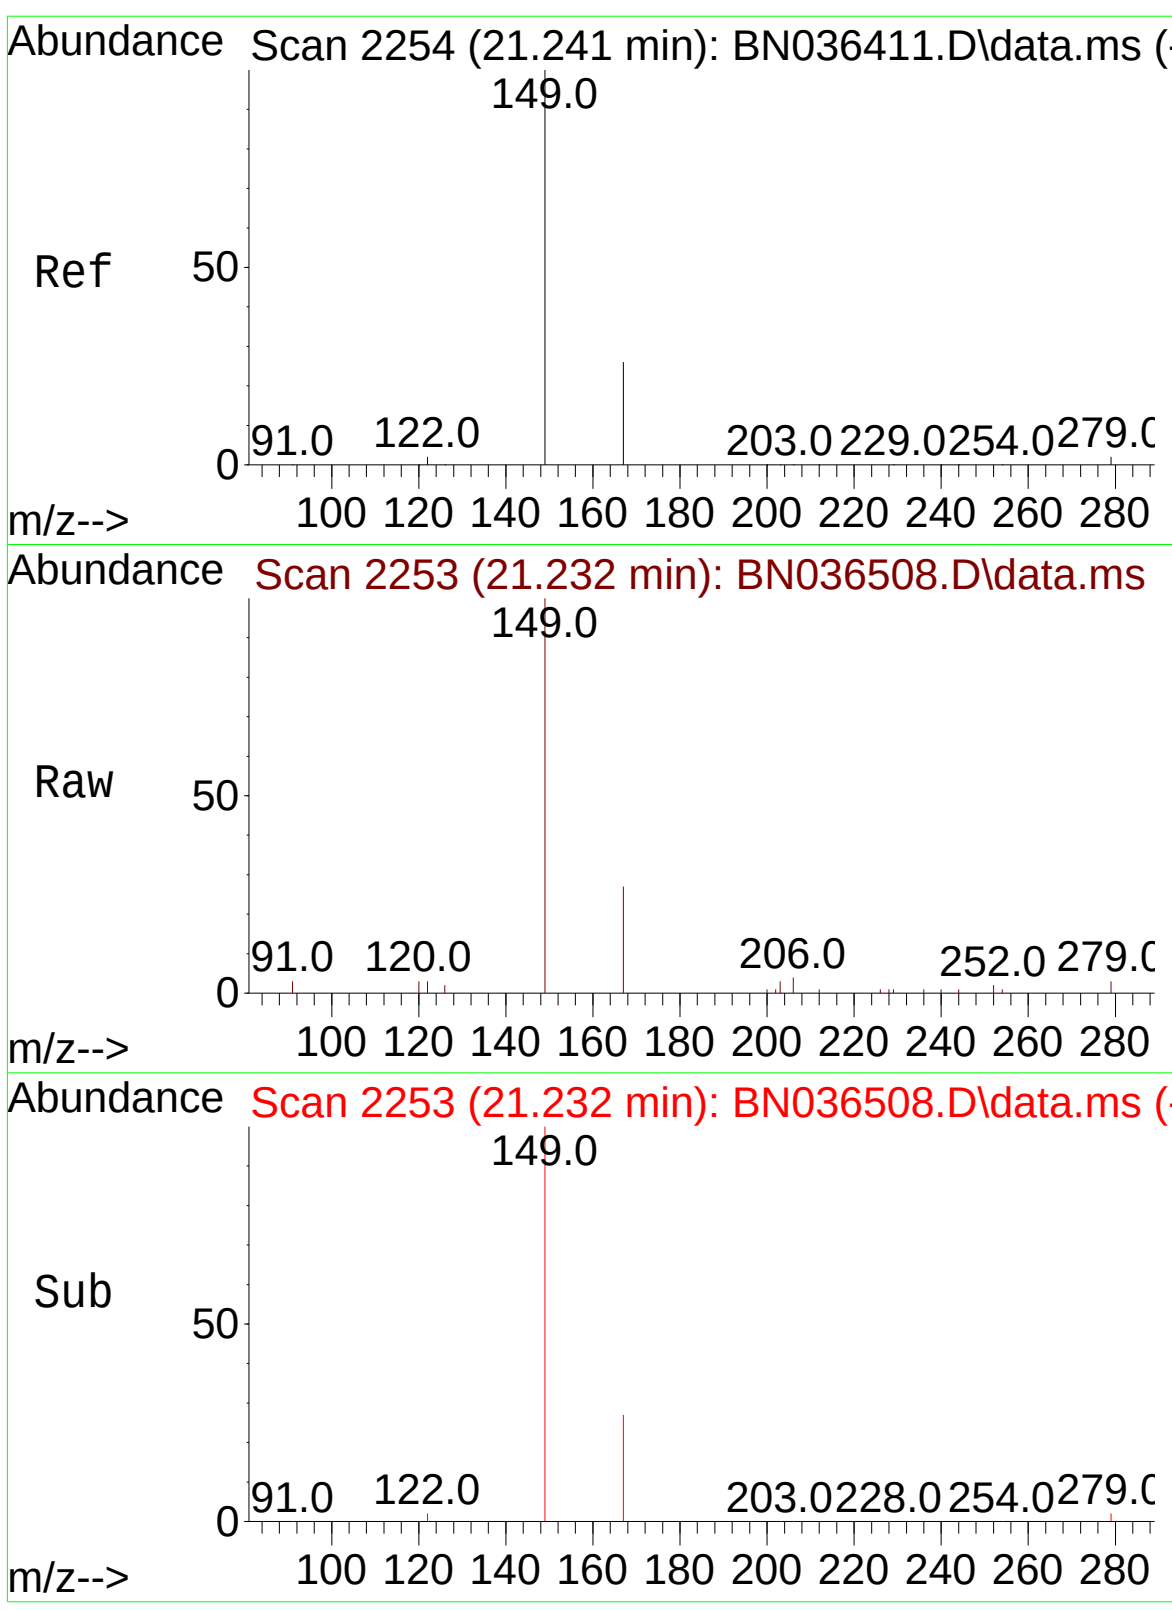

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.479 ng
RT: 21.232 min Scan# 2253
Delta R.T. -0.009 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Tgt Ion:149 Resp: 6526

Ion	Ratio	Lower	Upper
149	100		
167	26.6	21.2	31.8
279	2.7	2.7	4.1

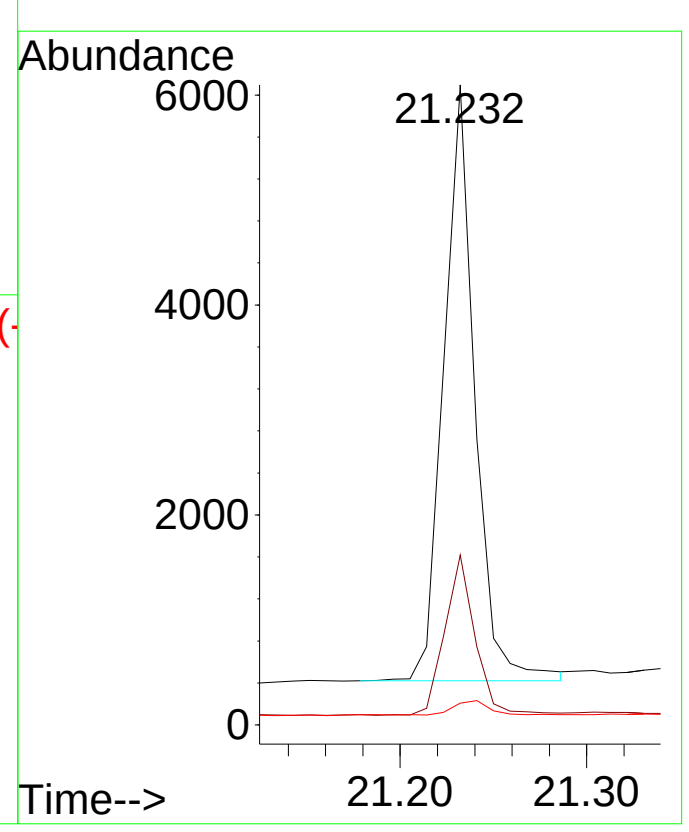

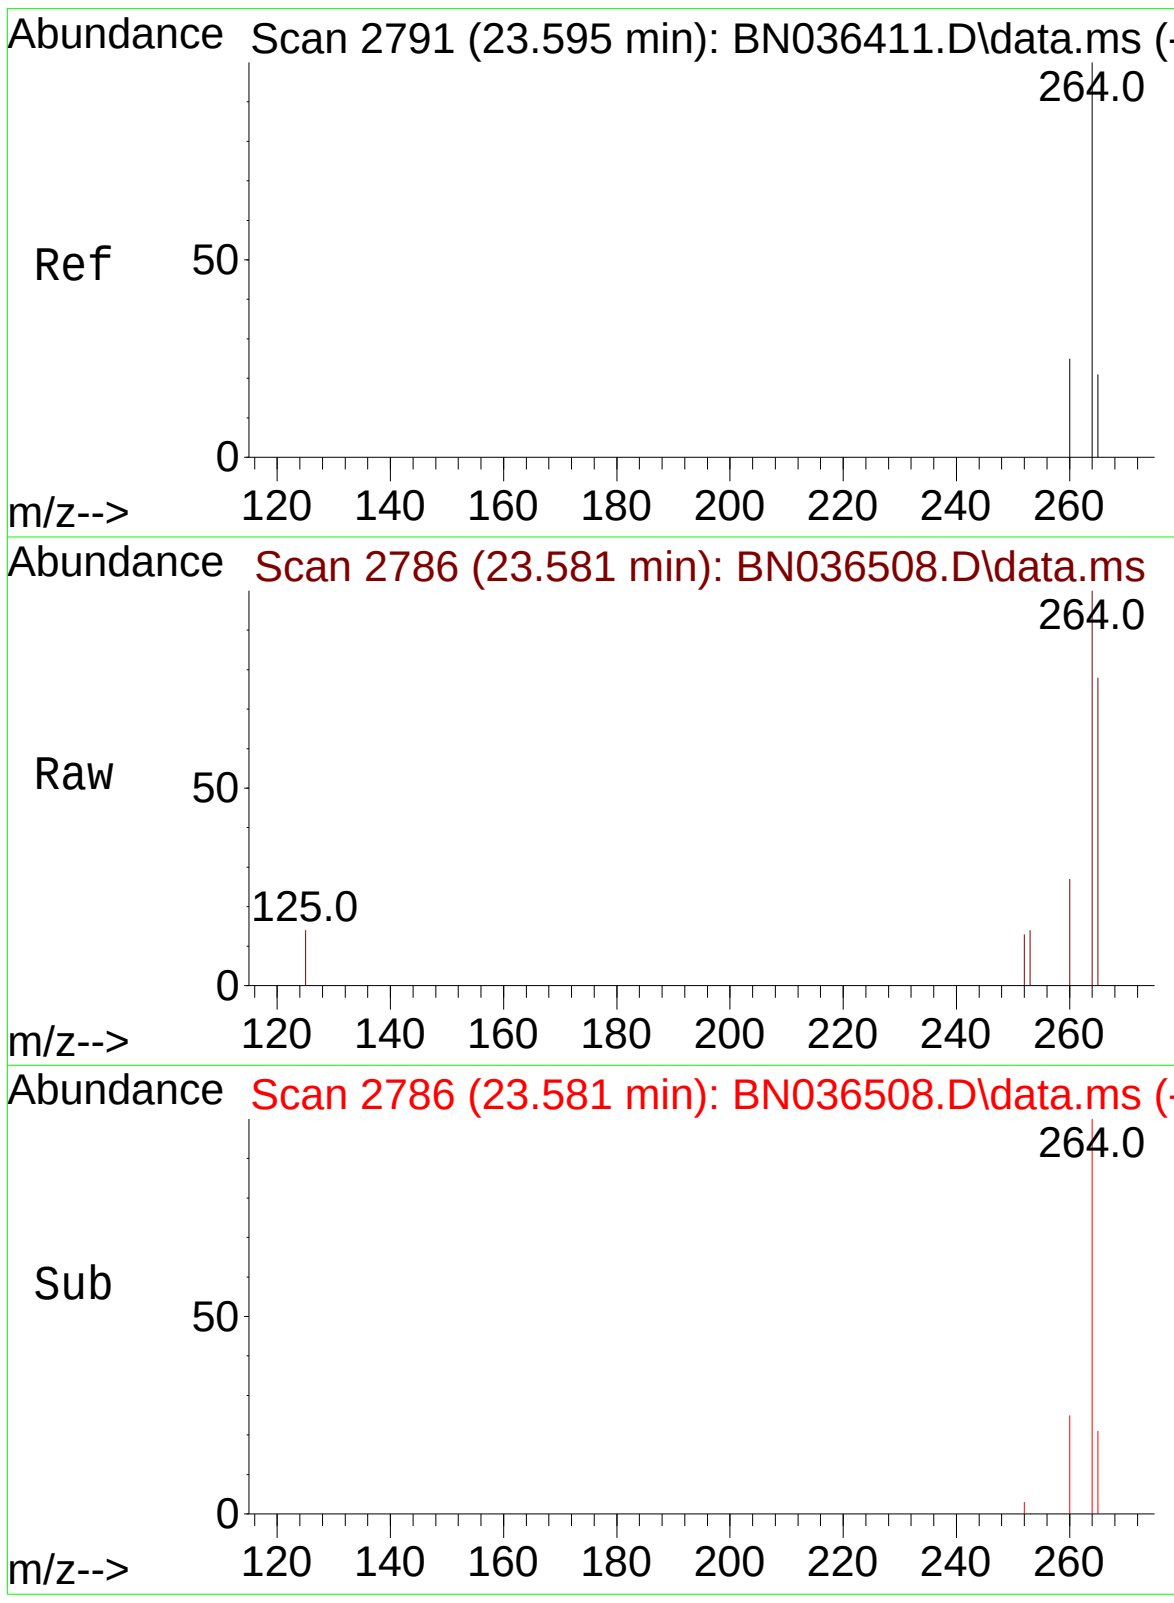

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.581 min Scan# 2
Delta R.T. -0.015 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:264 Resp: 6000

Ion	Ratio	Lower	Upper
264	100		
260	26.6	20.9	31.3
265	78.1	60.7	91.1

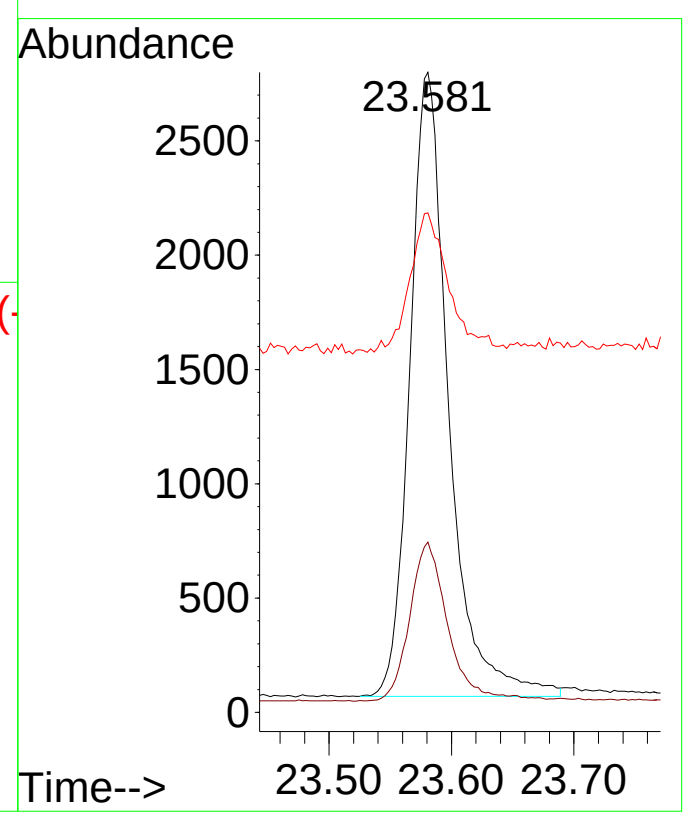

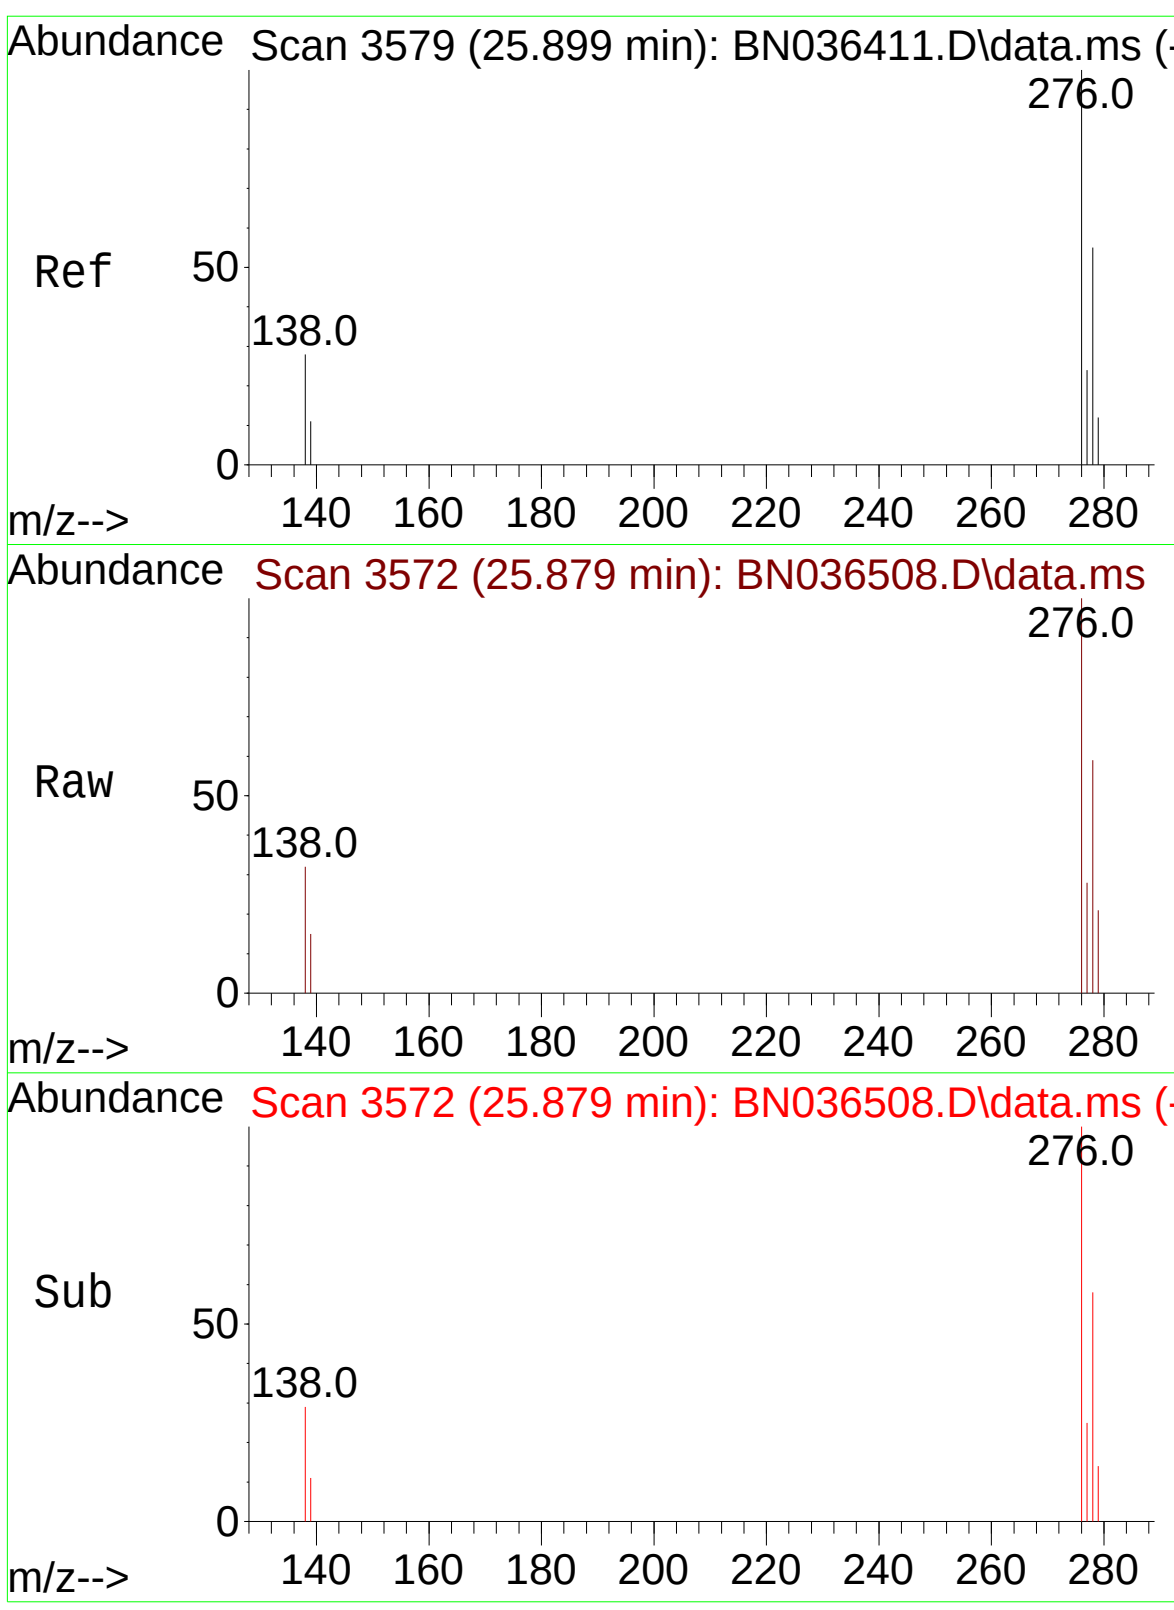

#36
Indeno(1,2,3-cd)pyrene
Concen: 0.372 ng
RT: 25.879 min Scan# 3572
Delta R.T. -0.020 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Tgt Ion:276 Resp: 7809

Ion	Ratio	Lower	Upper
276	100		
138	26.5	22.2	33.2
277	24.2	19.8	29.6

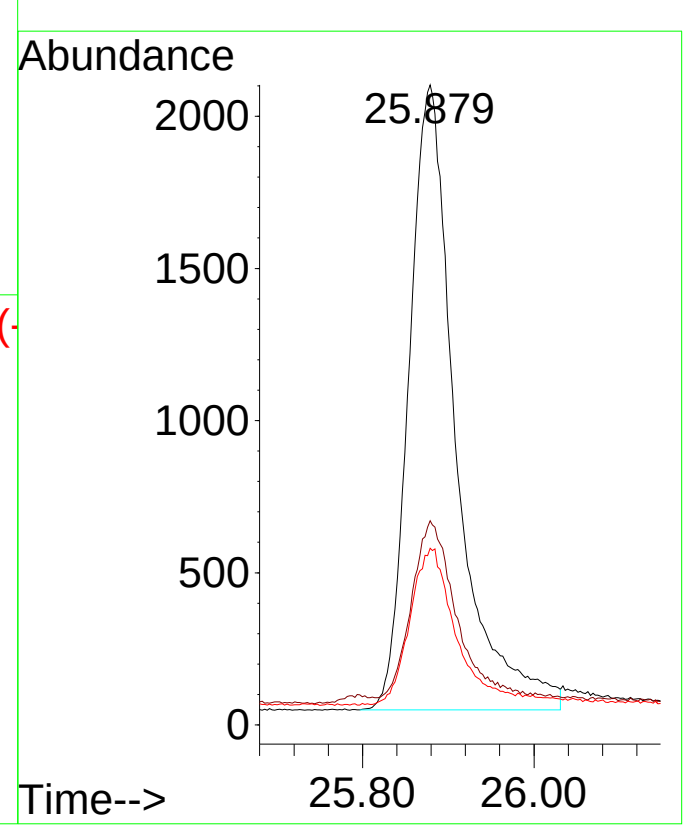

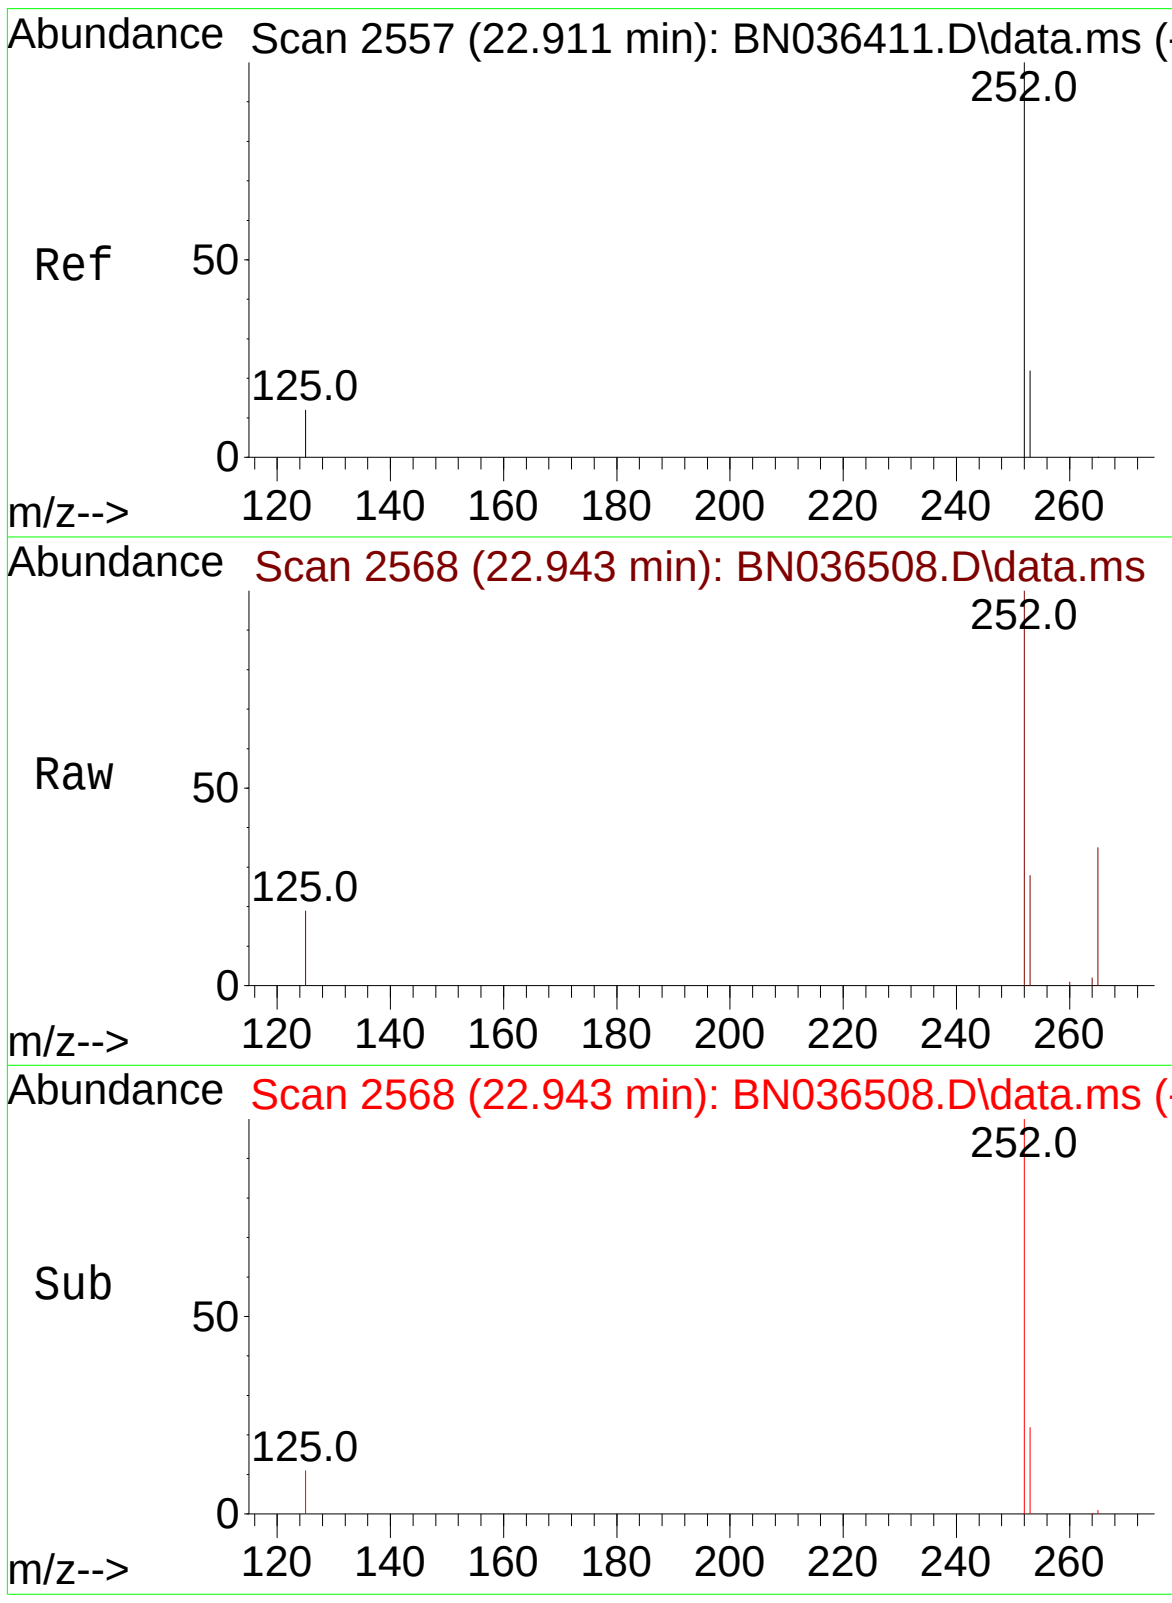

#37
Benzo(b)fluoranthene
Concen: 0.419 ng
RT: 22.943 min Scan# 2
Delta R.T. 0.032 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:252 Resp: 8277

Ion	Ratio	Lower	Upper
252	100		
253	27.9	21.9	32.9
125	19.0	15.0	22.6

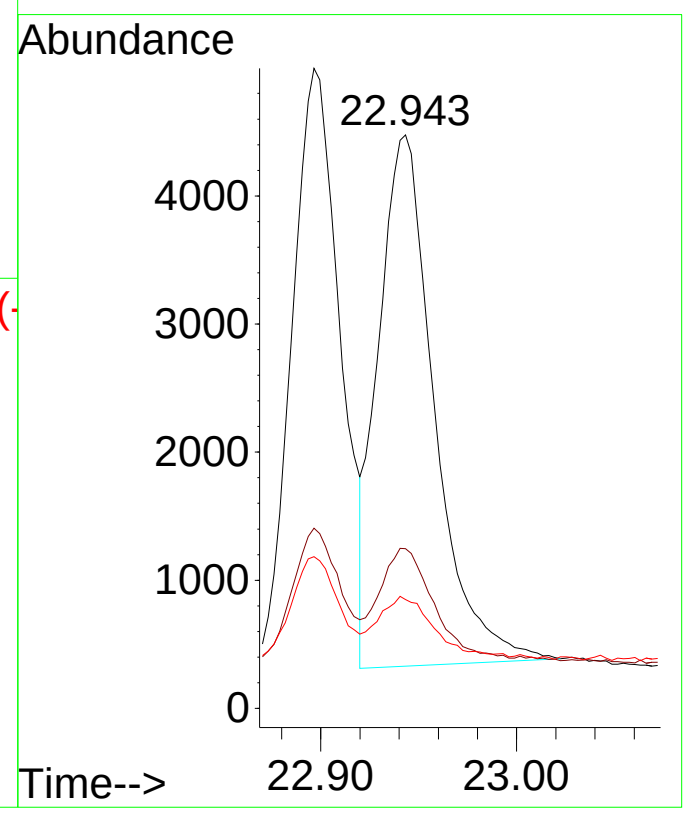

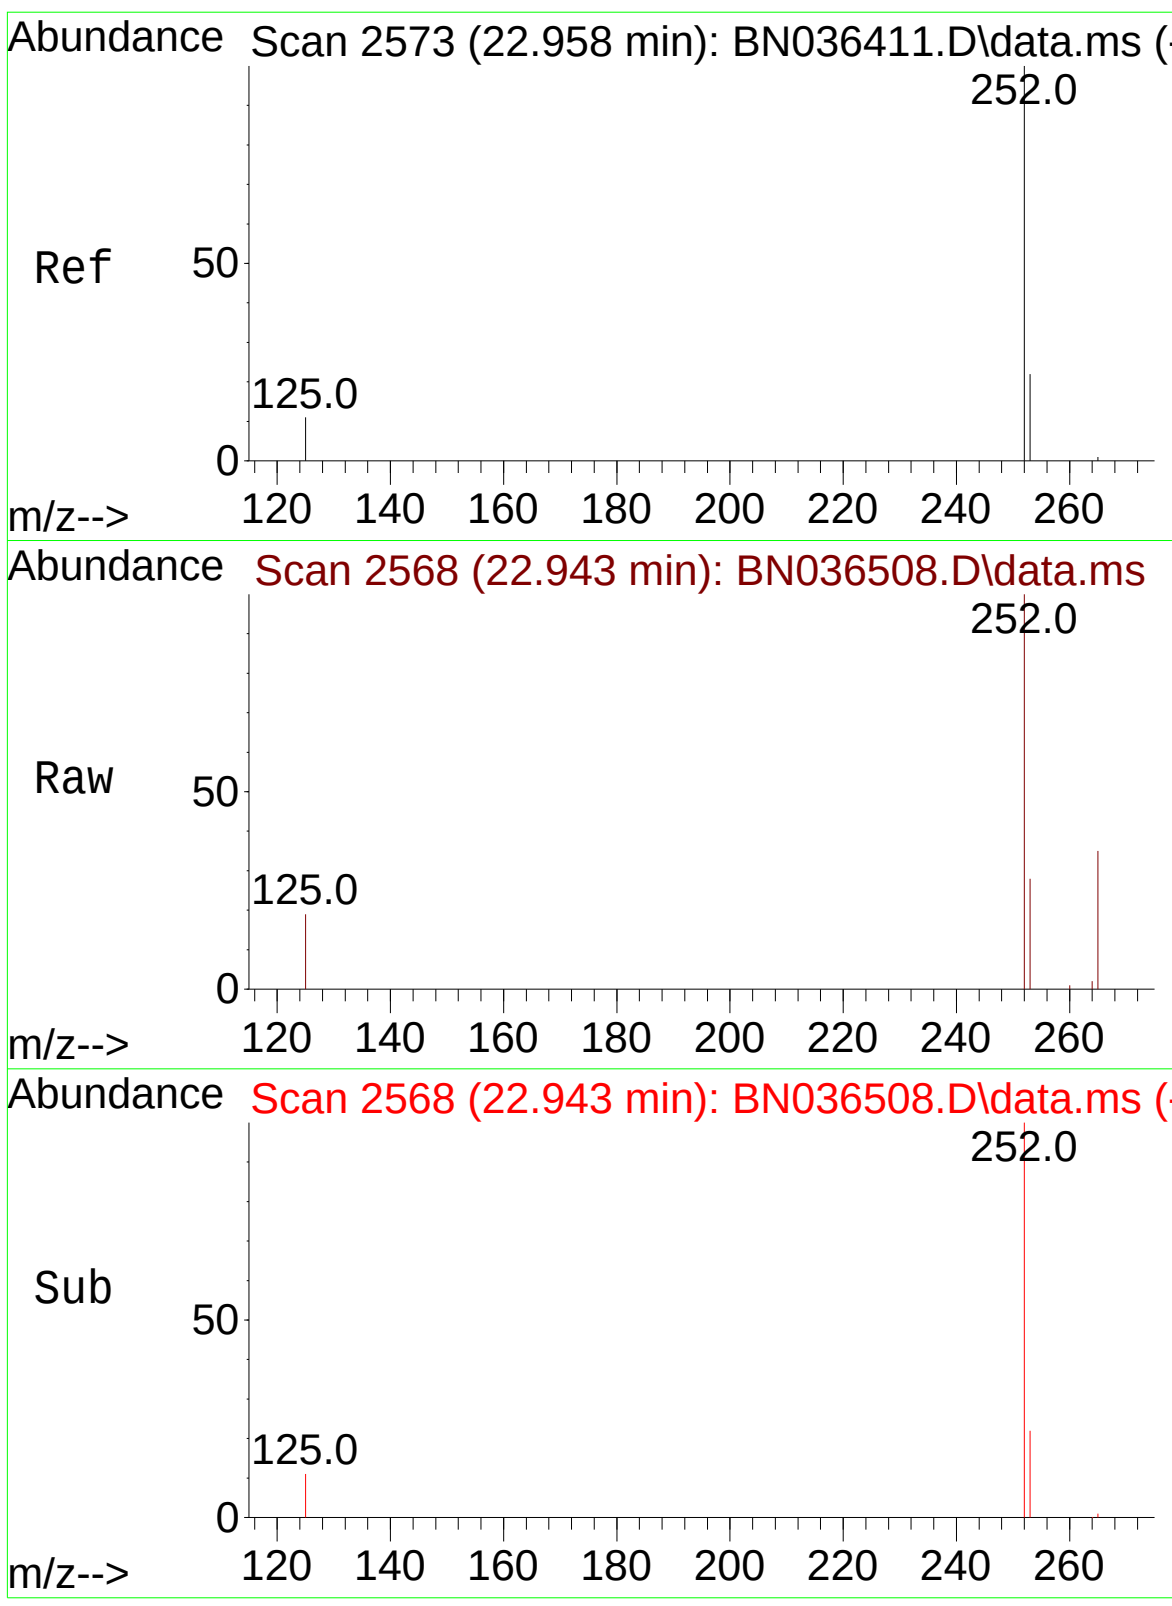

#38
Benzo(k)fluoranthene
Concen: 0.407 ng
RT: 22.943 min Scan# 2568
Delta R.T. -0.015 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Tgt Ion:252 Resp: 8277

Ion	Ratio	Lower	Upper
252	100		
253	27.9	22.2	33.4
125	19.0	15.0	22.4

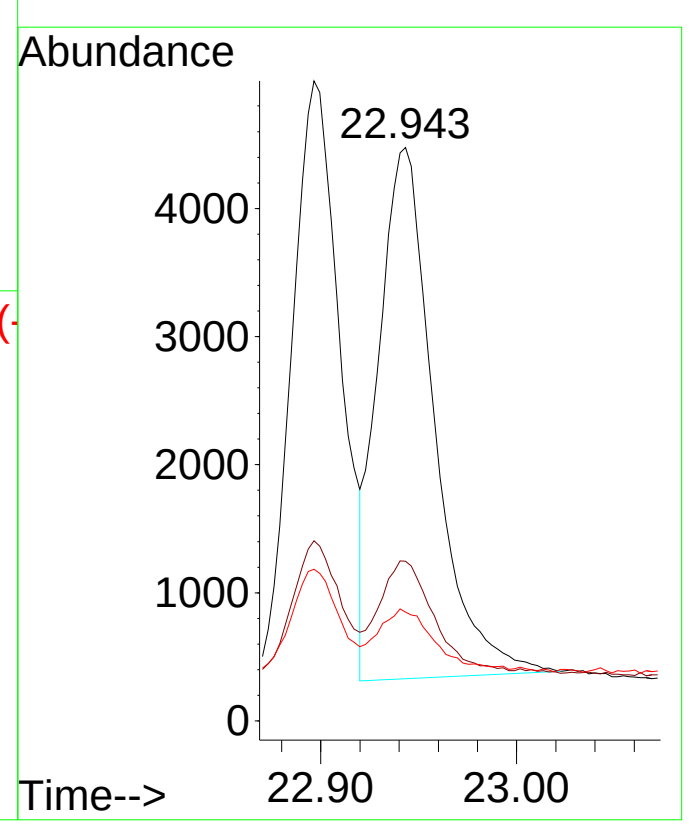

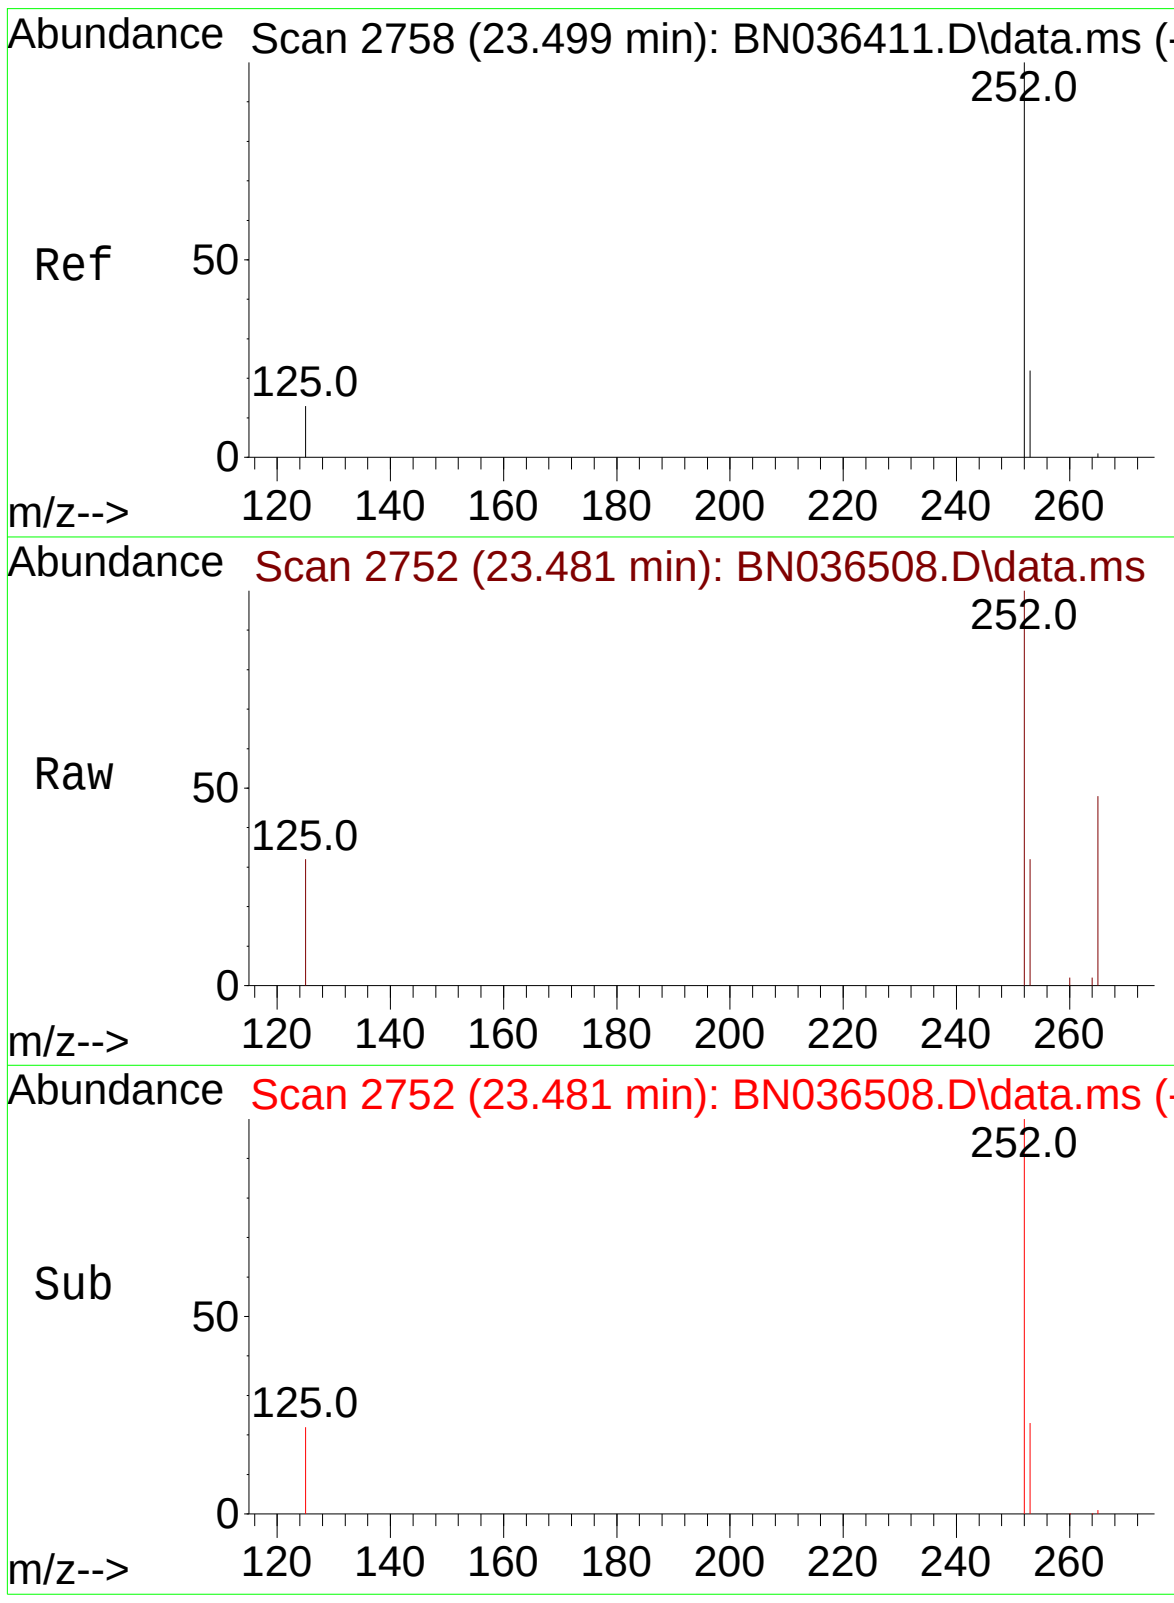

#39
Benzo(a)pyrene
Concen: 0.421 ng
RT: 23.481 min Scan# 2
Delta R.T. -0.018 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:252 Resp: 7264

Ion	Ratio	Lower	Upper
252	100		
253	32.0	24.4	36.6
125	32.1	18.2	27.2#

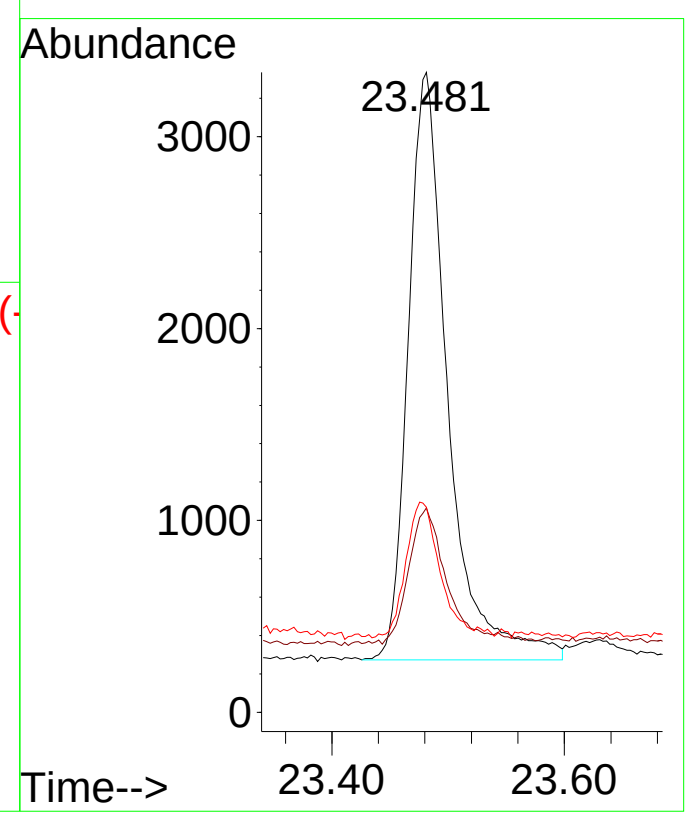

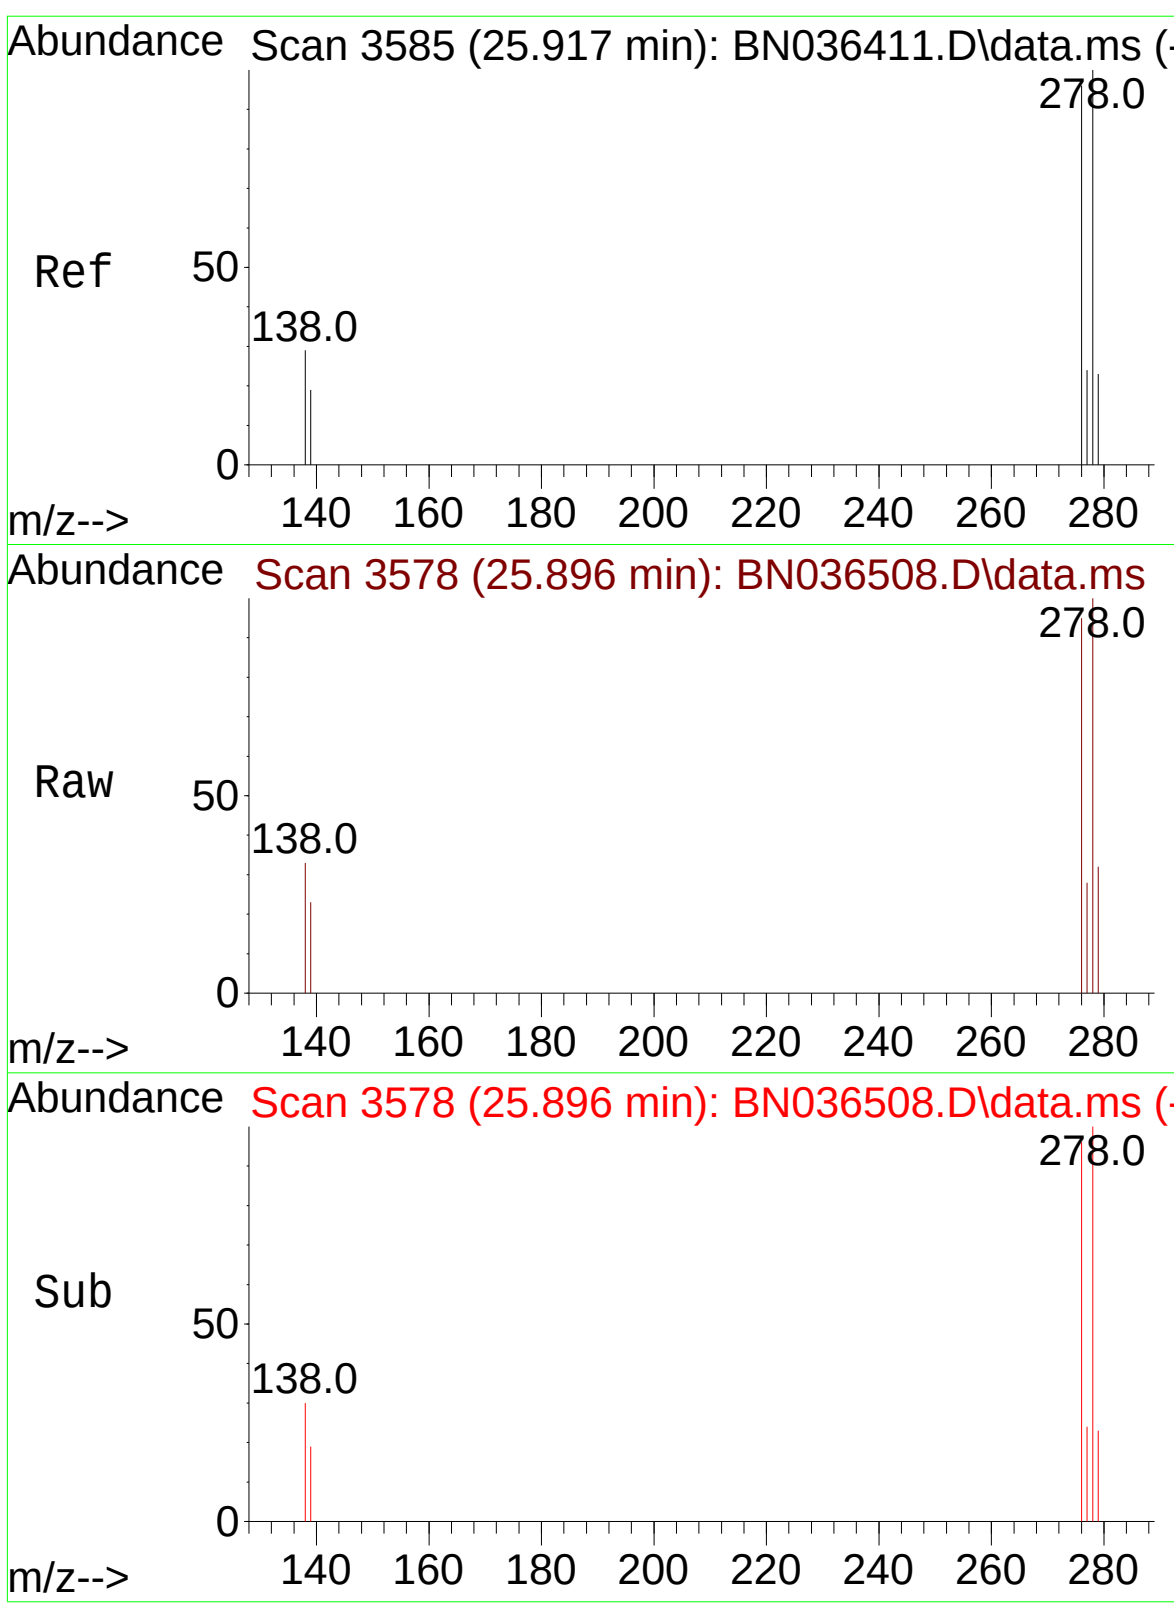

#40
Dibenzo(a,h)anthracene
Concen: 0.357 ng
RT: 25.896 min Scan# 3578
Delta R.T. -0.020 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Tgt Ion:278 Resp: 5914

Ion	Ratio	Lower	Upper
278	100		
139	23.2	18.5	27.7
279	32.3	24.8	37.2

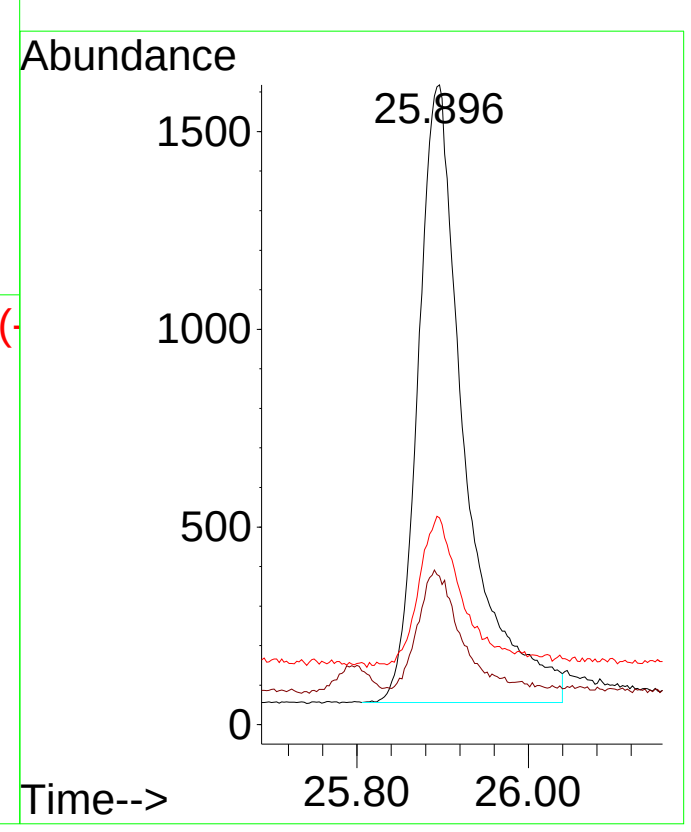

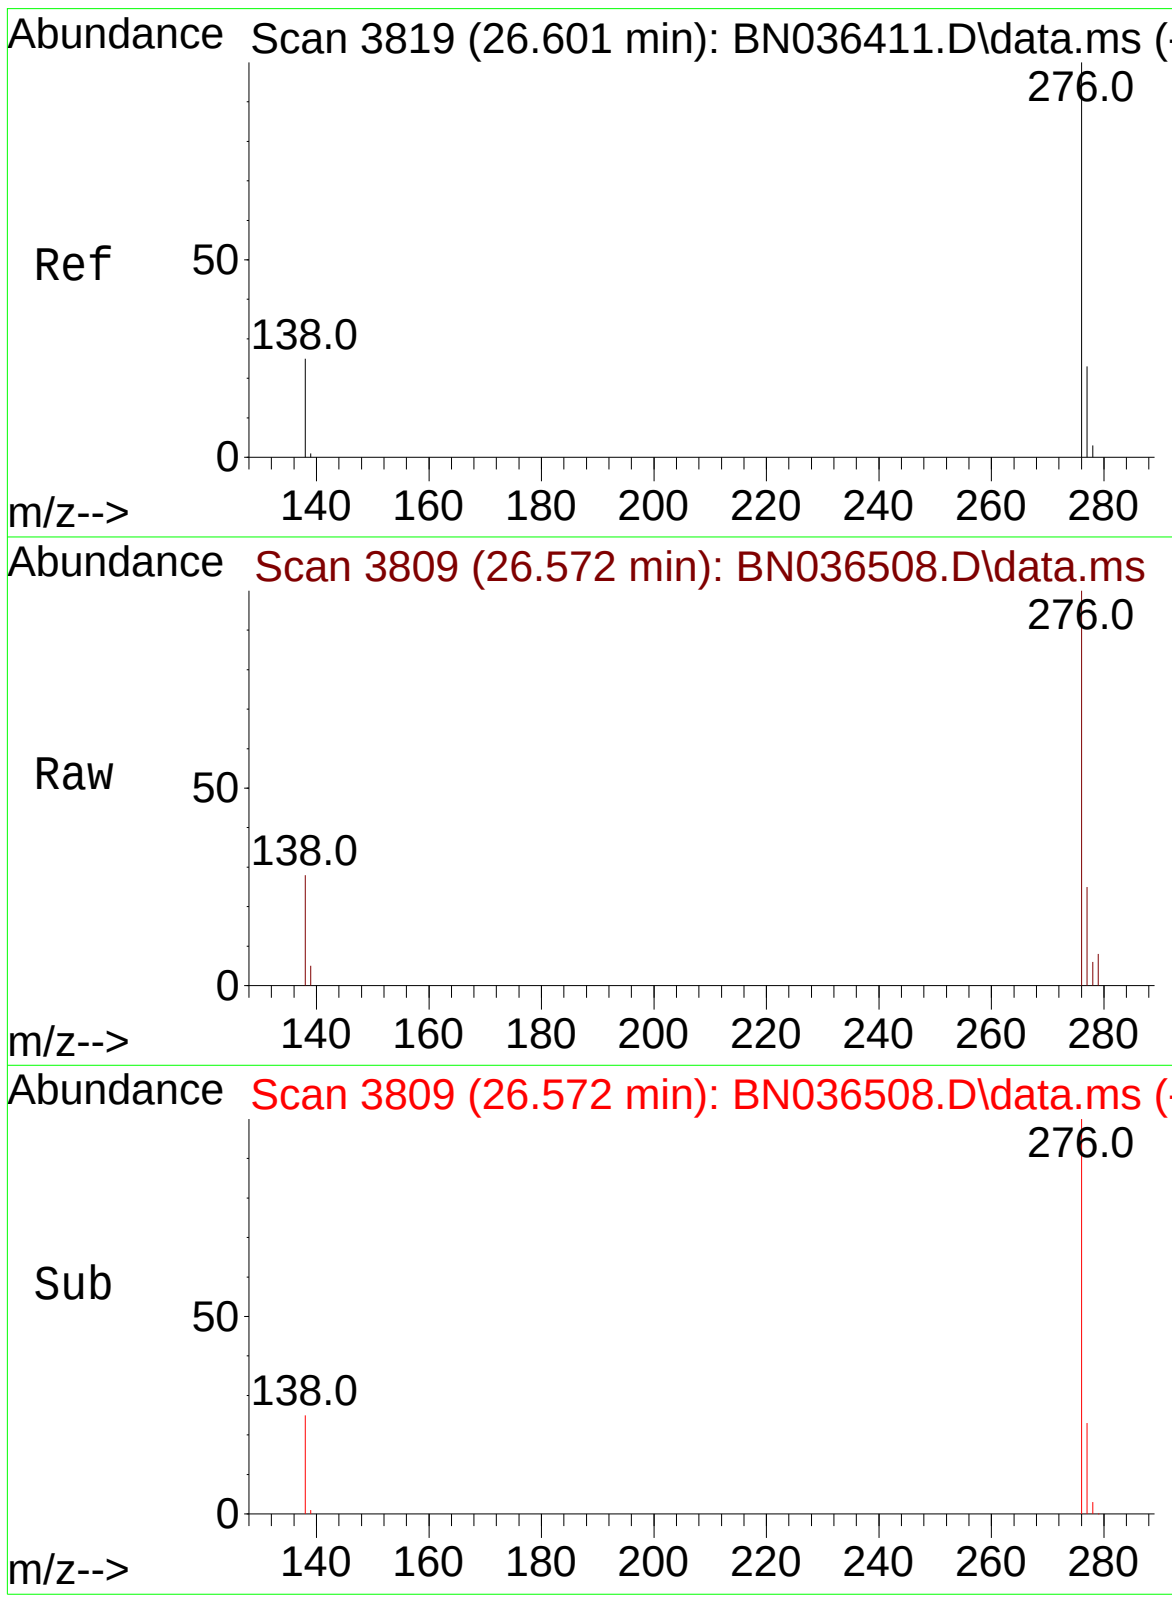

#41
Benzo(g,h,i)perylene
Concen: 0.367 ng
RT: 26.572 min Scan# 38
Delta R.T. -0.029 min
Lab File: BN036508.D
Acq: 26 Feb 2025 13:43

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:276 Resp: 6890

Ion	Ratio	Lower	Upper
276	100		
277	25.4	20.7	31.1
138	28.3	21.8	32.6