


Data Path : Z:\HPCHEM1\BNA_N\Data\BN022718\
 Data File : BN000180.D
 Acq On : 27 Feb 2018 08:42
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_N\METHODS\8270-SIM-BN022718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 27 15:07:57 2018

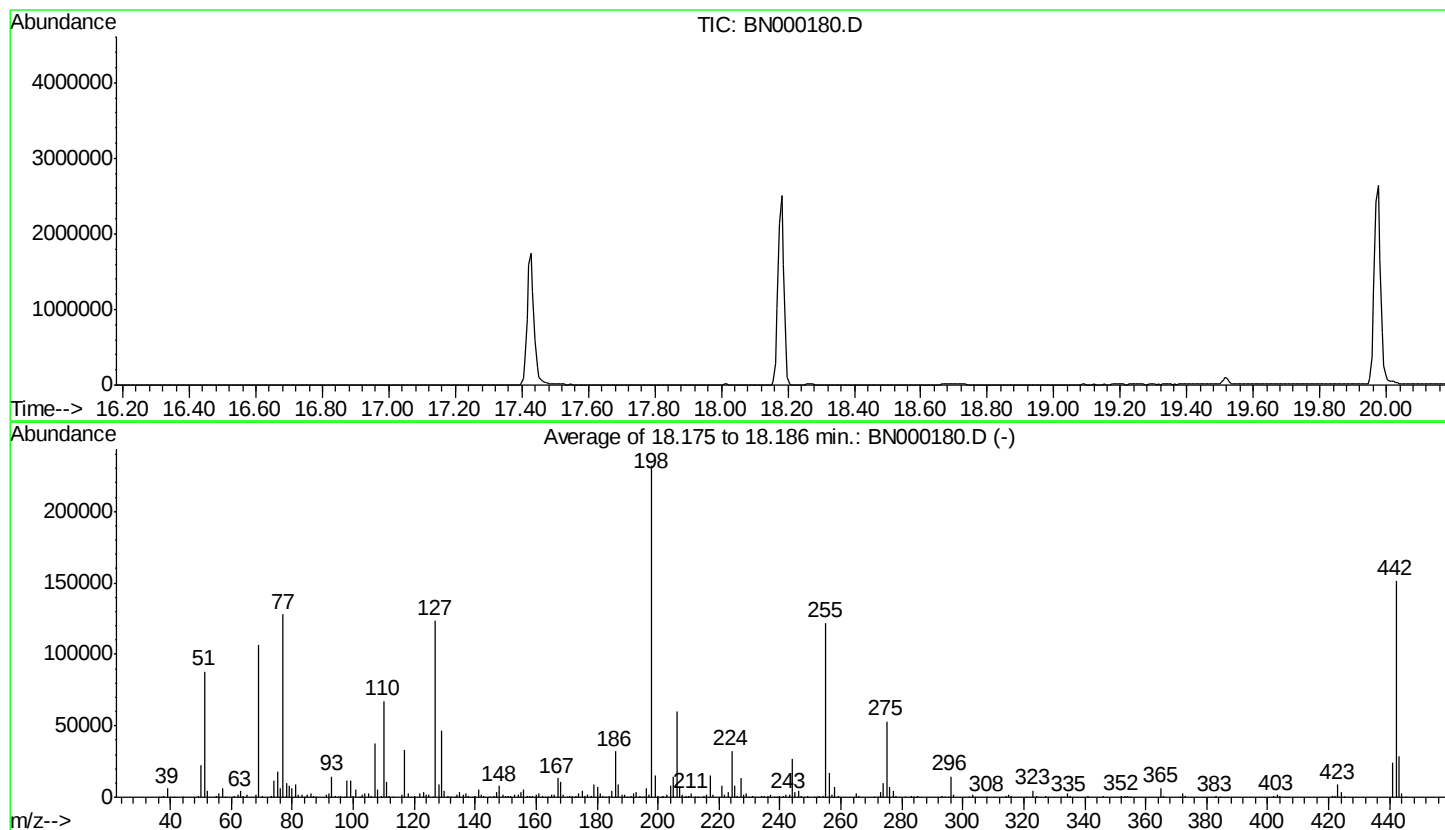

AutoFind: Scans 2582, 2583, 2584; Background Corrected with Scan 2575

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.0	88186	PASS
68	69	0.00	2	1.8	1960	PASS
69	198	0.00	100	45.9	106560	PASS
70	69	0.00	2	0.6	590	PASS
127	198	10	80	53.2	123333	PASS
197	198	0.00	2	0.6	1506	PASS
198	198	100	100	100.0	231978	PASS
199	198	5	9	6.7	15653	PASS
275	198	10	60	22.8	52848	PASS
365	198	1	100	2.8	6539	PASS
441	442	0.01	24	15.8	23925	PASS
442	198	50	100	65.4	151637	PASS
443	442	15	24	18.8	28520	PASS