
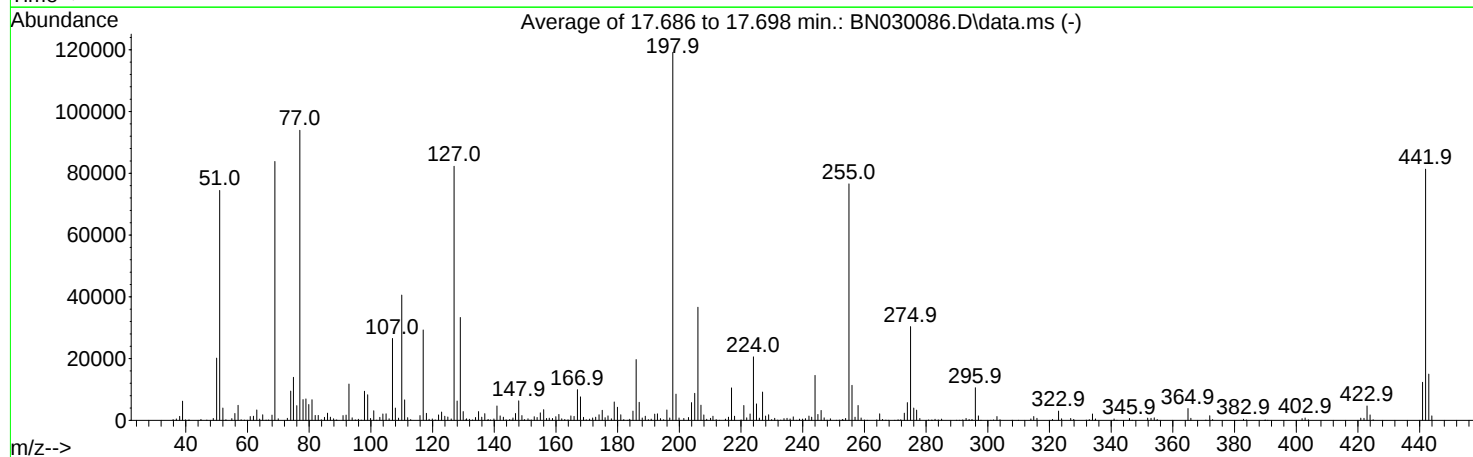


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022724\
Data File : BN030086.D
Acq On : 27 Feb 2024 09:15
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Feb 26 02:39:45 2024

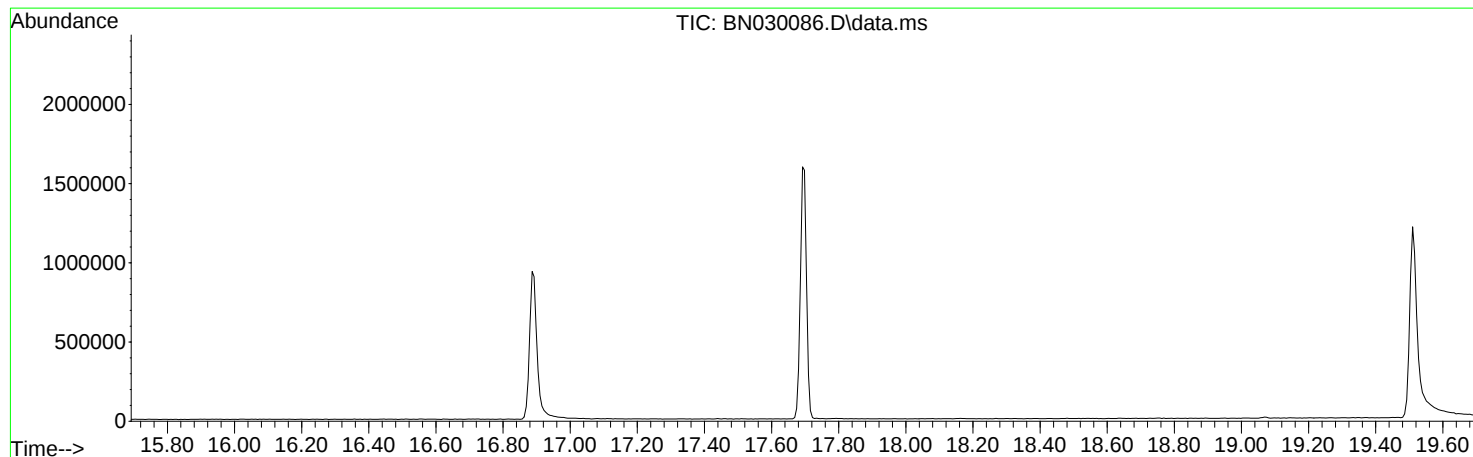




AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2476

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	62.5	74469	PASS
68	69	0.00	2	2.0	1709	PASS
69	198	0.00	100	70.4	83853	PASS
70	69	0.00	2	0.6	505	PASS
127	198	10	80	69.1	82277	PASS
197	198	0.00	2	0.7	775	PASS
198	198	100	100	100.0	119112	PASS
199	198	5	9	7.1	8491	PASS
275	198	10	60	25.5	30368	PASS
365	198	1	100	3.2	3860	PASS
441	198	0.01	100	10.3	12325	PASS
442	442	50	100	100.0	81344	PASS
443	442	15	24	18.4	14952	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022724\
Data File : BN030086.D
Acq On : 27 Feb 2024 09:15
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTTP

Quant Time: Feb 28 00:45:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 28 00:45:00 2024
Response via : Initial Calibration

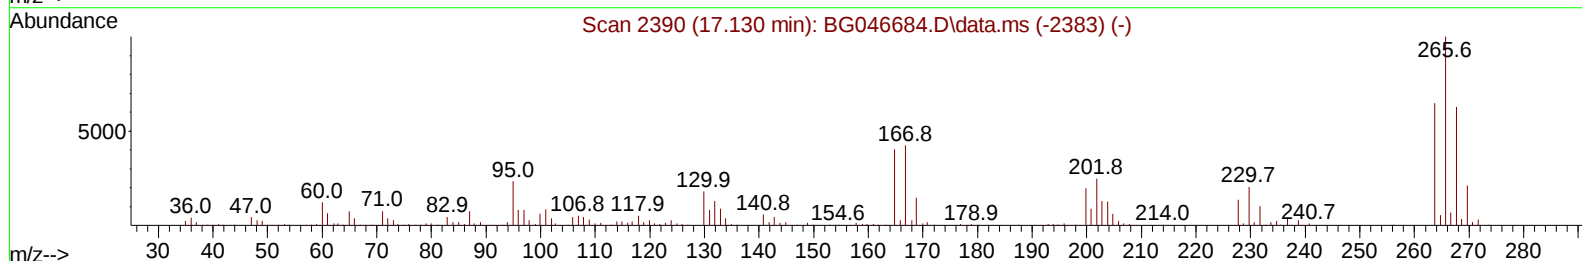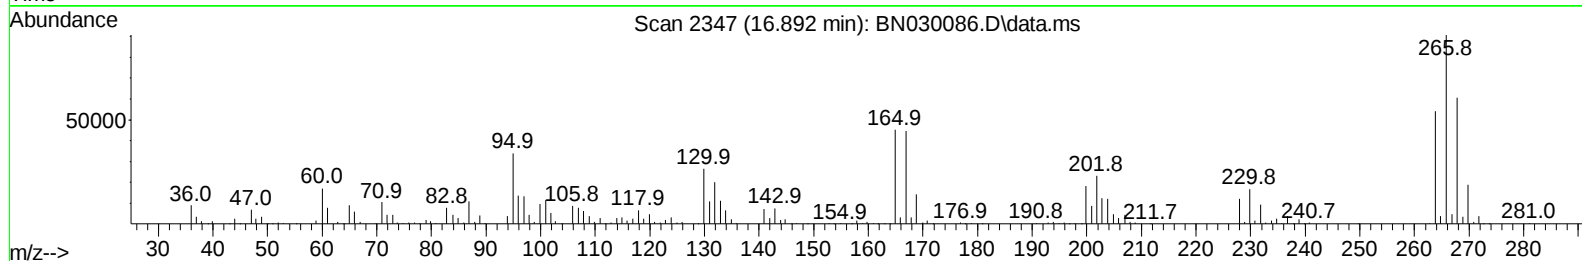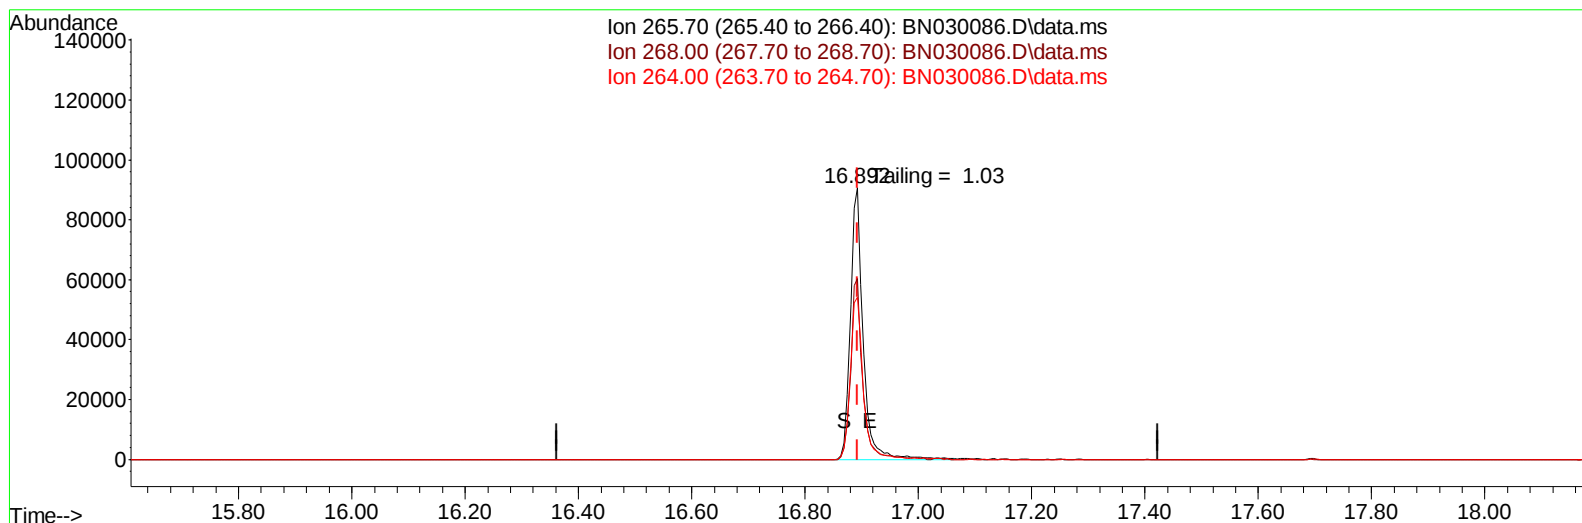

TIC: BN030086.D\data.ms

(70) Pentachlorophenol (C)

16.892min (0.000) 17108.14 ng




response 142316

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.73
264.00	61.60	59.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022724\
Data File : BN030086.D
Acq On : 27 Feb 2024 09:15
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 28 00:45:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 28 00:45:00 2024
Response via : Initial Calibration

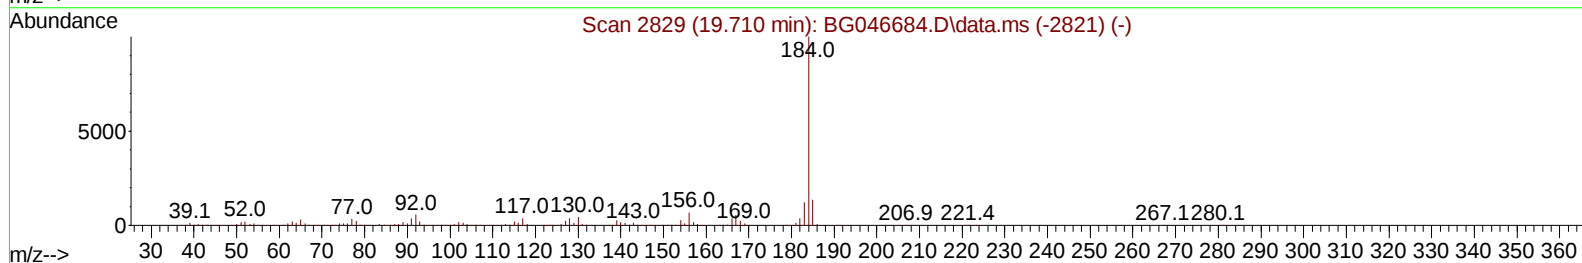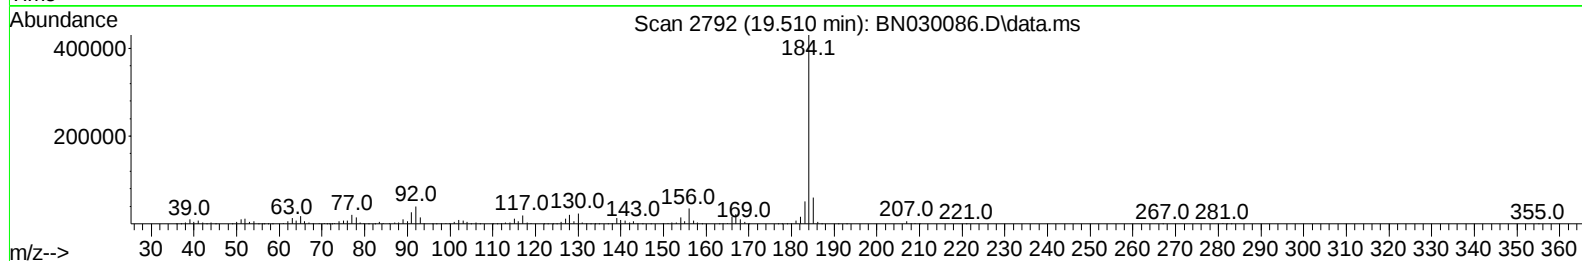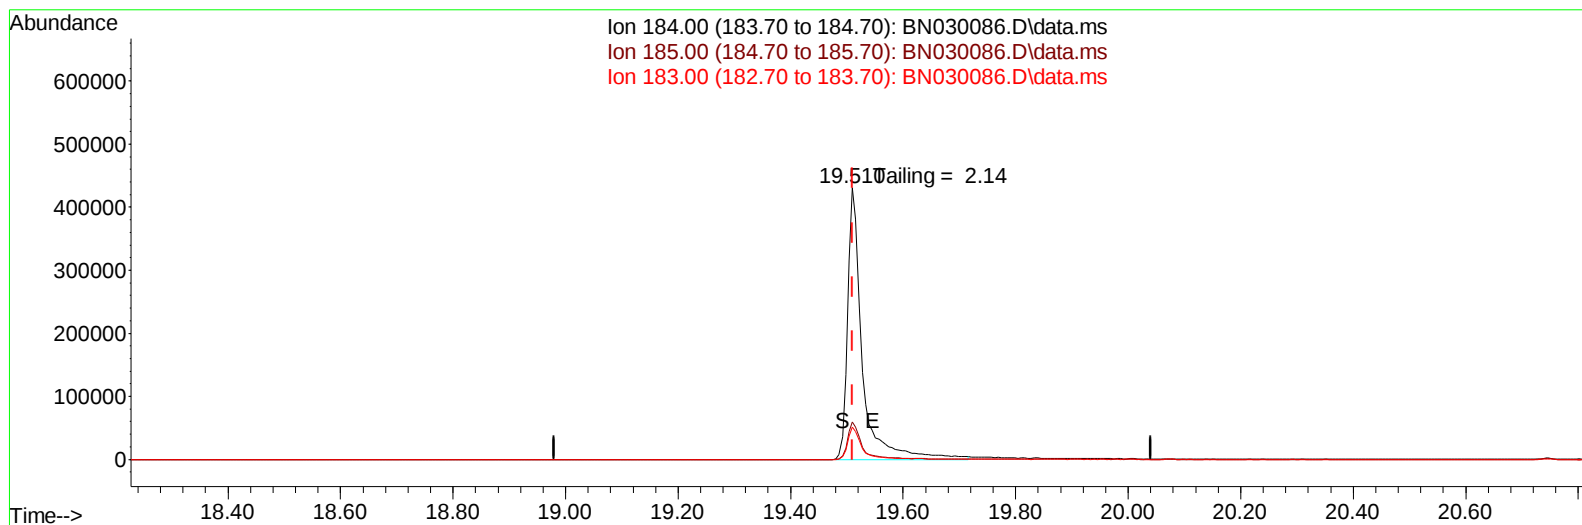

TIC: BN030086.D\data.ms

(77) Benzidine

19.510min (0.000) 0.00 ng

response 801183

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.82
183.00	13.20	11.85
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/27/2024	BNA_N	<u>BN030086.D</u>
Compound Name	Response	Retention Time
DDT	427225	20.745
DDD	12684	20.304
DDE	857	19.792
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13541	440766	3.07

Instrument :
BNA_N
ClientSampleId :
DFTPP