


Data Path : Z:\HPCHEM1\BNA_N\DATA\BN022818\
 Data File : BN000197.D
 Acq On : 28 Feb 2018 08:29
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_N\METHODS\8270-SIM-BN022718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 27 15:07:57 2018

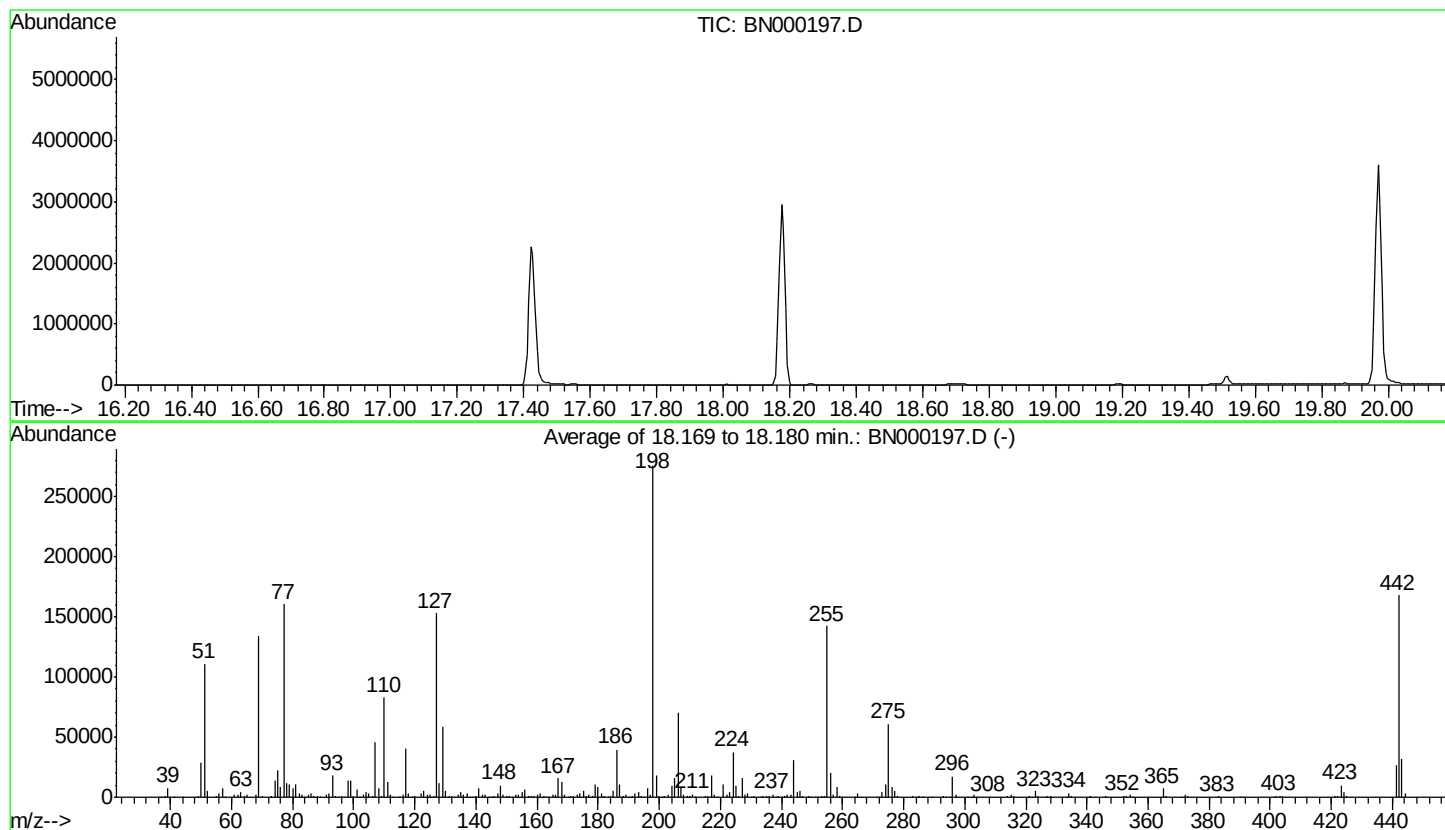

AutoFind: Scans 2581, 2582, 2583; Background Corrected with Scan 2575

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.2	110776	PASS
68	69	0.00	2	1.8	2455	PASS
69	198	0.00	100	48.6	133874	PASS
70	69	0.00	2	0.6	820	PASS
127	198	10	80	55.4	152762	PASS
197	198	0.00	2	0.7	1933	PASS
198	198	100	100	100.0	275690	PASS
199	198	5	9	6.7	18413	PASS
275	198	10	60	22.2	61197	PASS
365	198	1	100	2.7	7310	PASS
441	442	0.01	24	16.1	27038	PASS
442	198	50	100	61.0	168056	PASS
443	442	15	24	19.2	32253	PASS