

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022819\
 Data File : BN004563.D
 Acq On : 28 Feb 2019 20:41
 Operator : JU/SJ
 Sample : K1625-13
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF868

Quant Time: Mar 01 03:32:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 01 02:57:41 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	21717	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.52	136	79989	20.00	ng/ul	-0.02
36) Acenaphthene-d10	14.37	164	50644	20.00	ng/ul	-0.02
62) Phenanthrene-d10	17.12	188	131655	20.00	ng/ul	-0.01
78) Chrysene-d12	21.32	240	243213	20.00	ng/ul	-0.01
86) Perylene-d12	23.58	264	199709	20.00	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.23	96	2396	6.63	ng/uL	-0.01
5) Phenol-d5	6.89	99	14097	7.28	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	7.07	67	33330	34.32	ng/ul	-0.02
9) 2-Chlorophenol-d4	7.26	132	44455	28.32	ng/ul	-0.01
13) 4-Methylphenol-d8	8.43	113	36420	21.89	ng/ul	-0.01
19) Nitrobenzene-d5	8.89	128	22848	43.15	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.60	143	33475	60.56	ng/ul	-0.02
26) 2,4-Dichlorophenol-d3	10.13	165	51190	40.85	ng/ul	-0.02
29) 4-Chloroaniline-d4	10.66	131	2893	2.09	ng/ul	-0.02
44) Dimethylphthalate-d6	13.78	166	136241	31.72	ng/ul	-0.02
47) Acenaphthylene-d8	14.06	160	156769	30.81	ng/ul	-0.02
52) 4-Nitrophenol-d4	14.57	143	6025	7.33	ng/ul	-0.01
58) Fluorene-d10	15.36	176	164484	43.50	ng/ul	-0.02
63) 4,6-Dinitro-2-methylphenol	15.49	200	34482	44.91	ng/ul	-0.01
71) Anthracene-d10	17.22	188	221644	35.13	ng/ul	-0.02
79) Pyrene-d10	19.52	212	264081	24.23	ng/ul	-0.01
90) Benzo(a)pyrene-d12	23.44	264	349167	33.31	ng/ul	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
84) Bis(2-ethylhexyl)phthalate	21.22	149	7928	1.144	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022819\
Data File : BN004563.D
Acq On : 28 Feb 2019 20:41
Operator : JU/SJ
Sample : K1625-13
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF868

Quant Time: Mar 01 03:32:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 01 02:57:41 2019
Response via : Initial Calibration

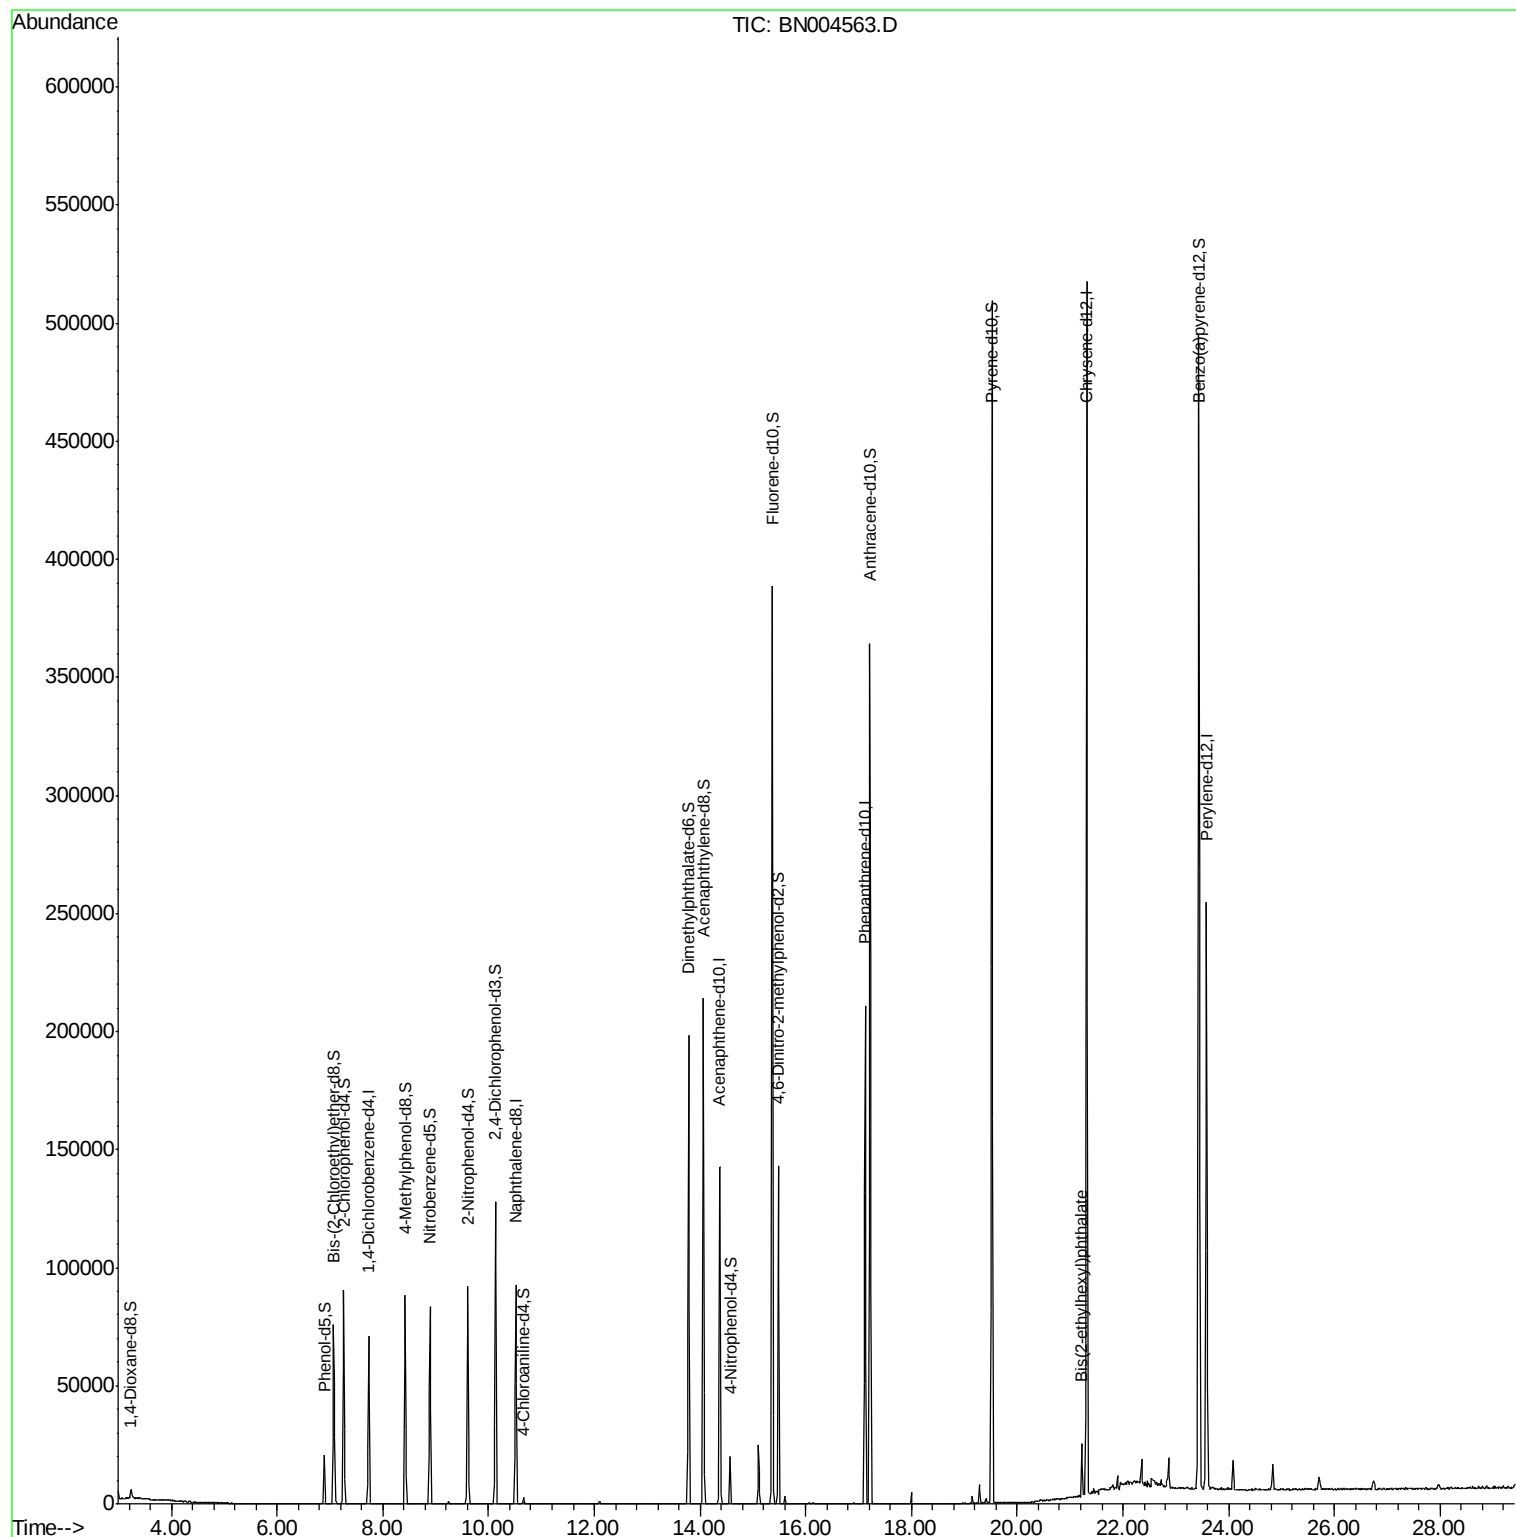

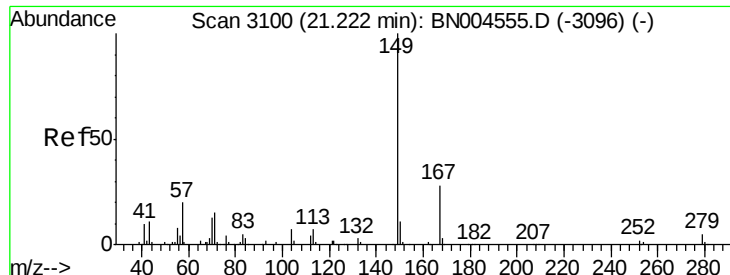

#84

Bis(2-ethylhexyl)phthalate

Concen: 1.144 ng/ul

RT: 21.22 min Scan# 3100

Delta R.T. -0.02 min

Lab File: BN004563.D

Acq: 28 Feb 2019 20:41

Instrument :

BNA_N

ClientSampleId :

BF868


Tot Ion:149 Resp: 7928

Ion Ratio Lower Upper

149 100

167 27.3 22.7 34.1

279 4.8 4.3 6.5

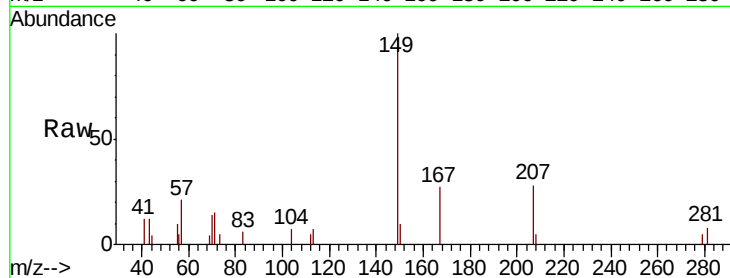

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

