
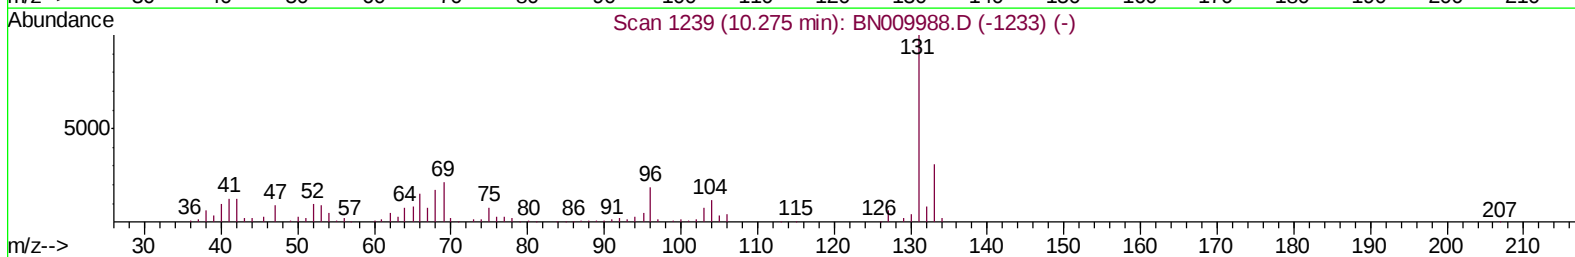
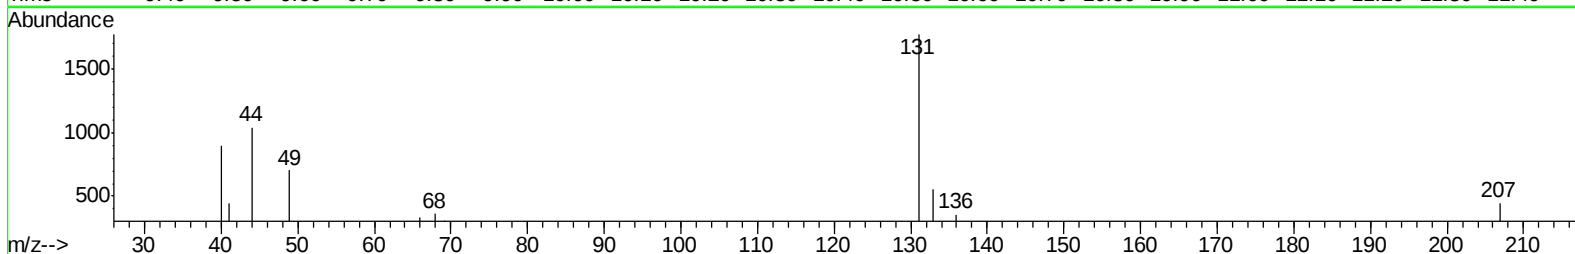


Data File : BN009997.D
Acq On : 28 Feb 2020 21:57
Operator : CG/JU
Sample : L1507-07RX
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Feb 29 01:40:08 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 29 01:38:10 2020
Response via : Initial Calibration

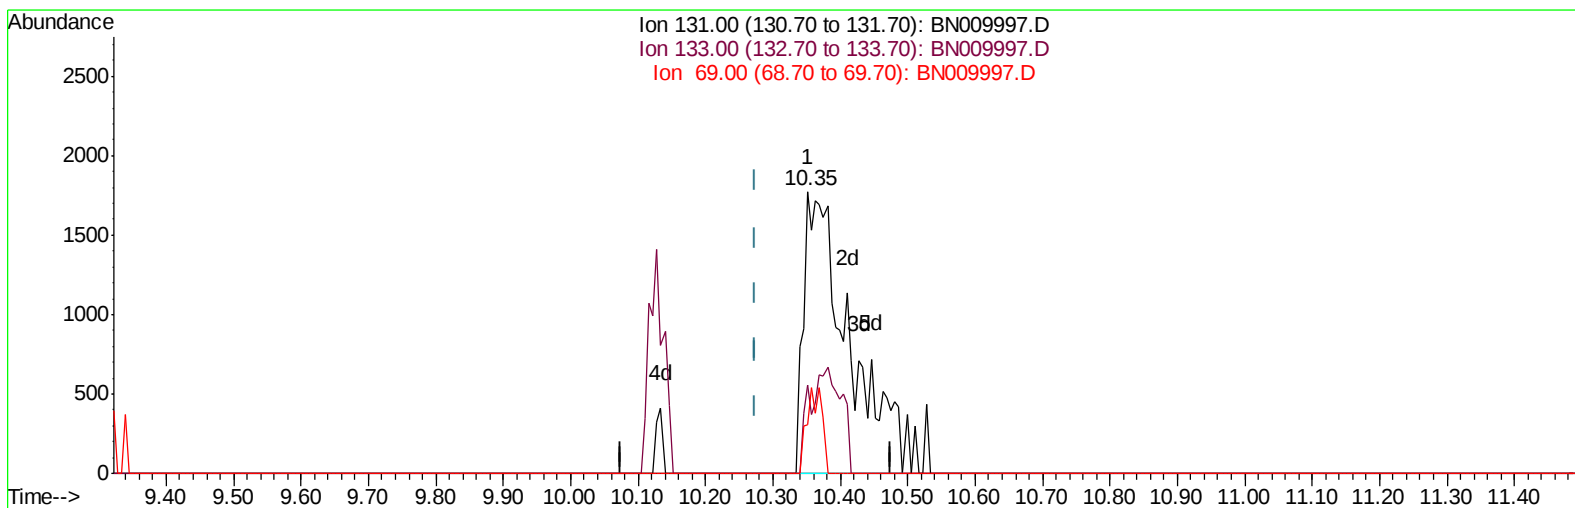

TIC: BN009997.D

(29) 4-Chloroaniline-d4 (S)

10.352min (+0.077) 1.52ng/ul m

response 8136

Ion	Exp%	Act%
131.00	100	100
133.00	33.00	31.42
69.00	22.10	17.09#
0.00	0.00	0.00