
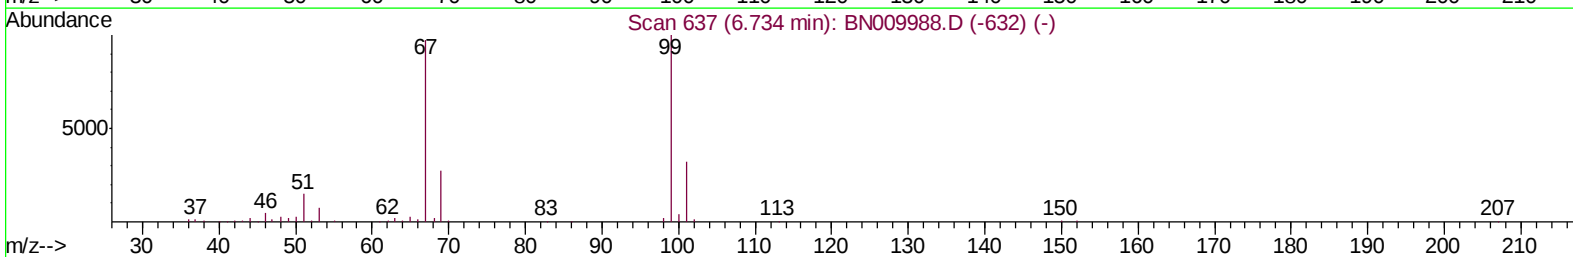
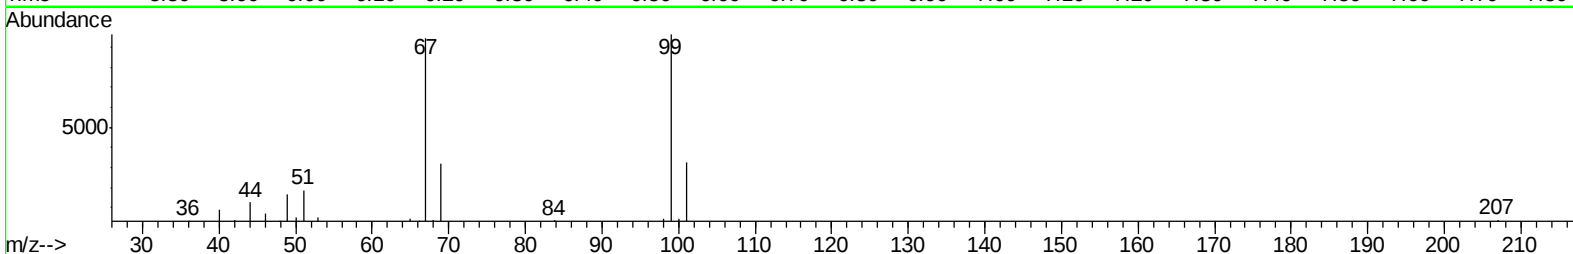


Data File : BN009998.D
Acq On : 28 Feb 2020 22:33
Operator : CG/JU
Sample : L1507-10RX
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Feb 29 01:40:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 29 01:38:10 2020
Response via : Initial Calibration

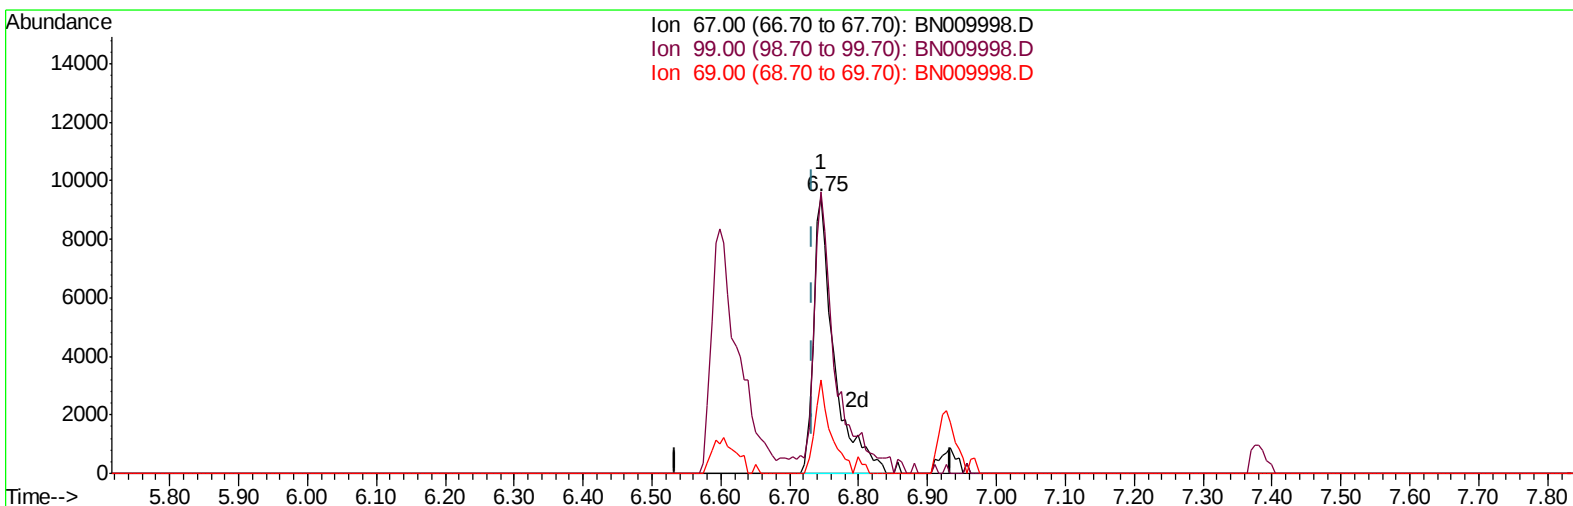

TIC: BN009998.D

(7) Bis-(2-Chloroethyl)ether-d8 (S)

6.745min (+0.011) 4.65ng/ul m

response 19724

Ion	Exp%	Act%
67.00	100	100
99.00	106.90	101.78
69.00	28.30	33.78
0.00	0.00	0.00