
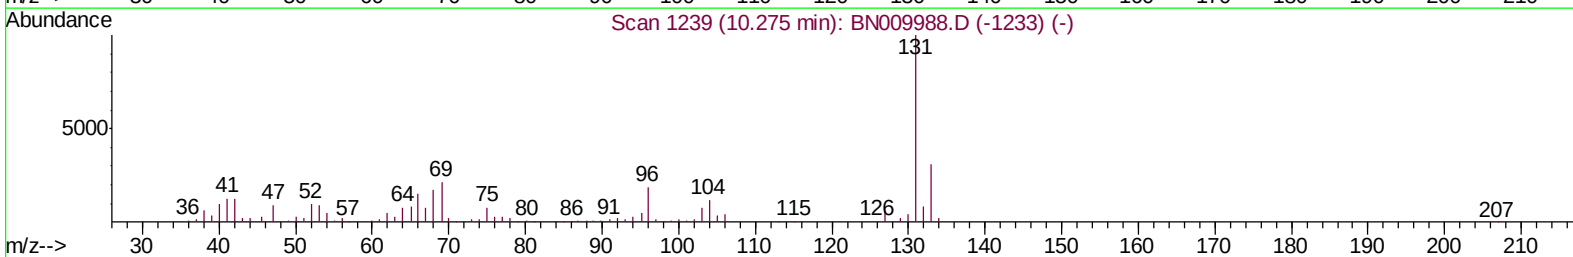
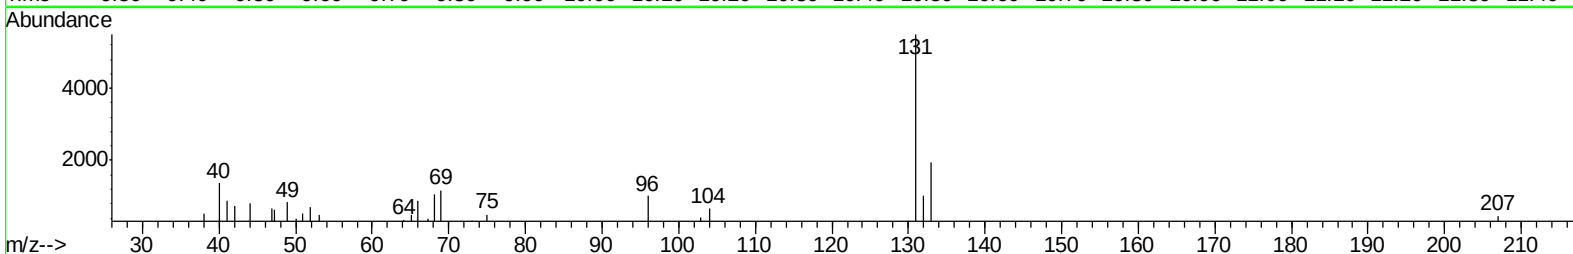


Data File : BN009998.D
Acq On : 28 Feb 2020 22:33
Operator : CG/JU
Sample : L1507-10RX
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Feb 29 01:40:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 29 01:38:10 2020
Response via : Initial Calibration

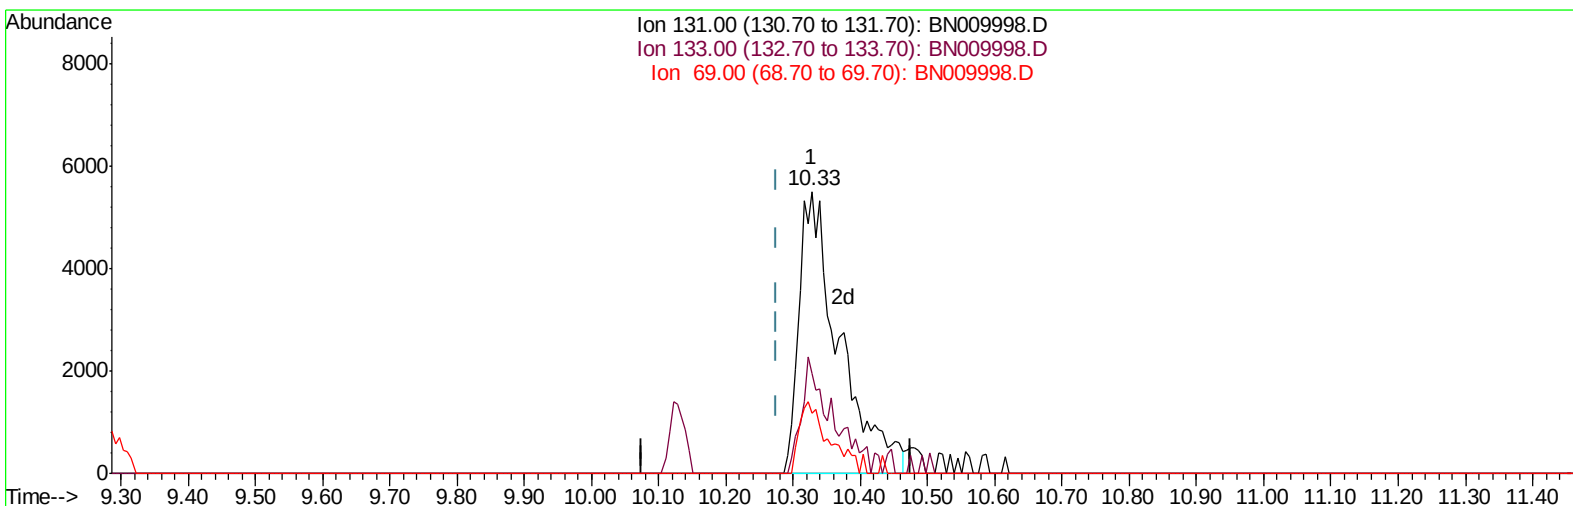

TIC: BN009998.D

(29) 4-Chloroaniline-d4 (S)
10.328min (+0.053) 4.33ng/ul m
response 22758

Ion	Exp%	Act%
131.00	100	100
133.00	33.00	35.43
69.00	22.10	21.23
0.00	0.00	0.00