
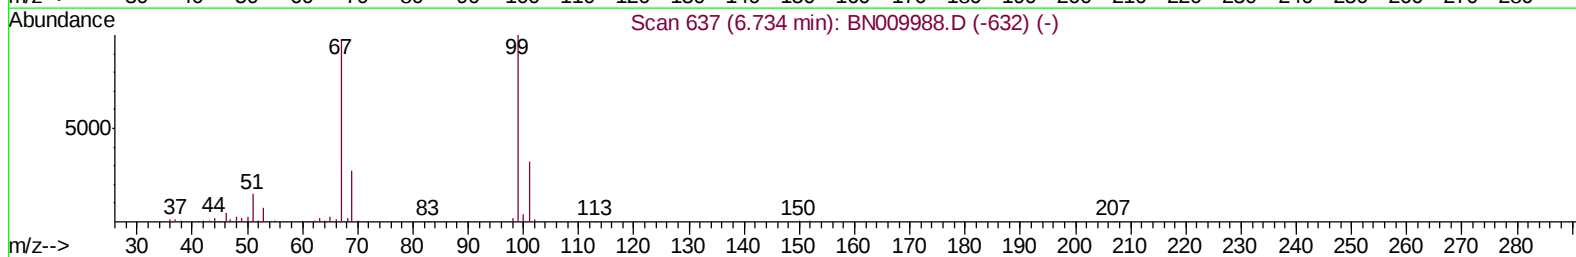
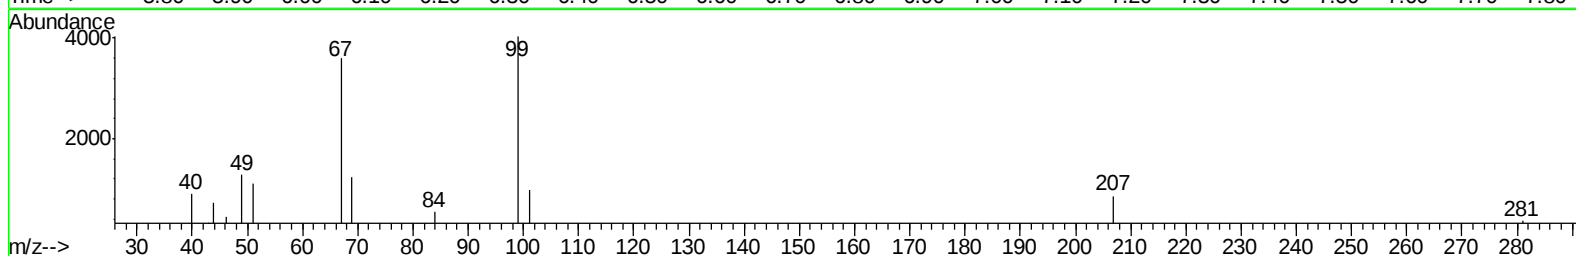


Data File : BN009999.D
Acq On : 28 Feb 2020 23:09
Operator : CG/JU
Sample : L1507-13RX
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Feb 29 01:40:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 29 01:38:10 2020
Response via : Initial Calibration

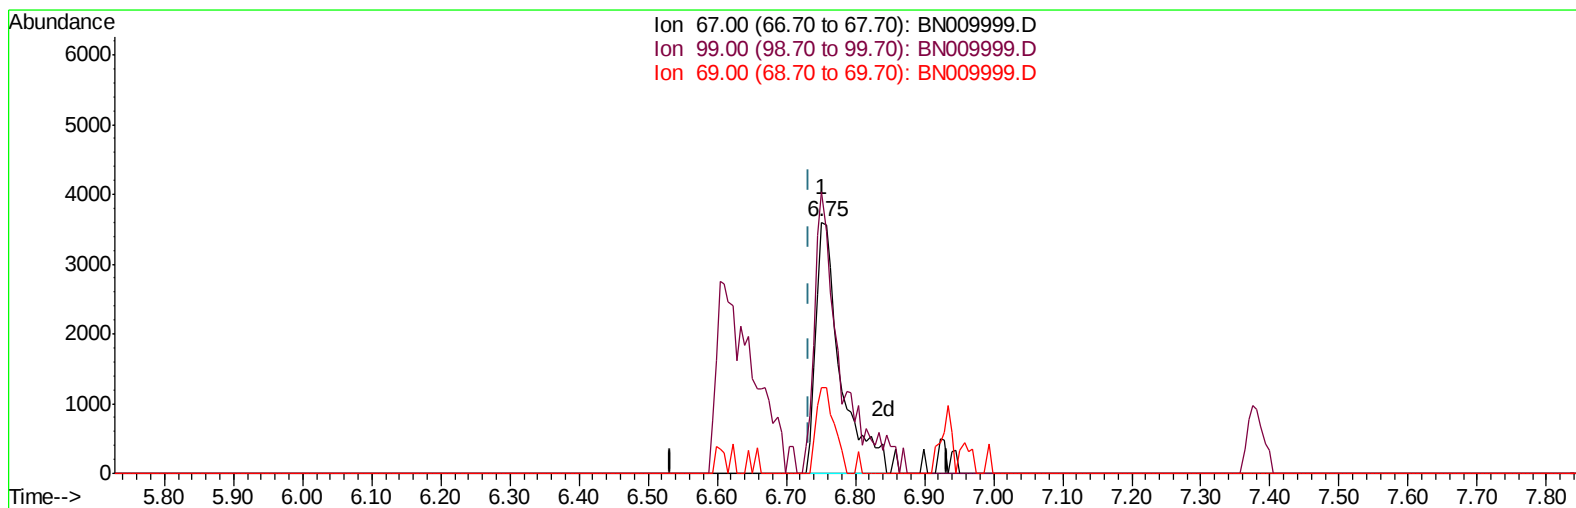

TIC: BN009999.D

(7) Bis-(2-Chloroethyl)ether-d8 (S)

6.752min (+0.018) 1.96ng/ul m

response 8893

Ion	Exp%	Act%
67.00	100	100
99.00	106.90	112.11
69.00	28.30	34.07#
0.00	0.00	0.00