
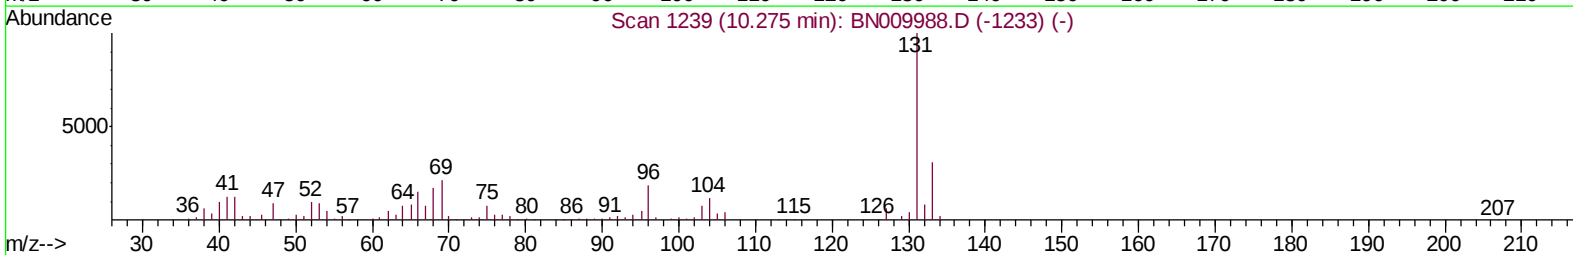
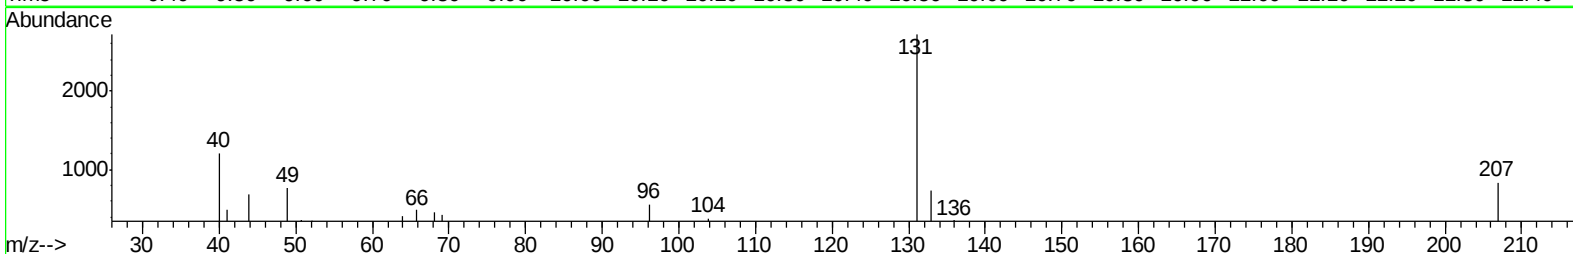


Data File : BN009999.D
Acq On : 28 Feb 2020 23:09
Operator : CG/JU
Sample : L1507-13RX
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Feb 29 01:40:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 29 01:38:10 2020
Response via : Initial Calibration

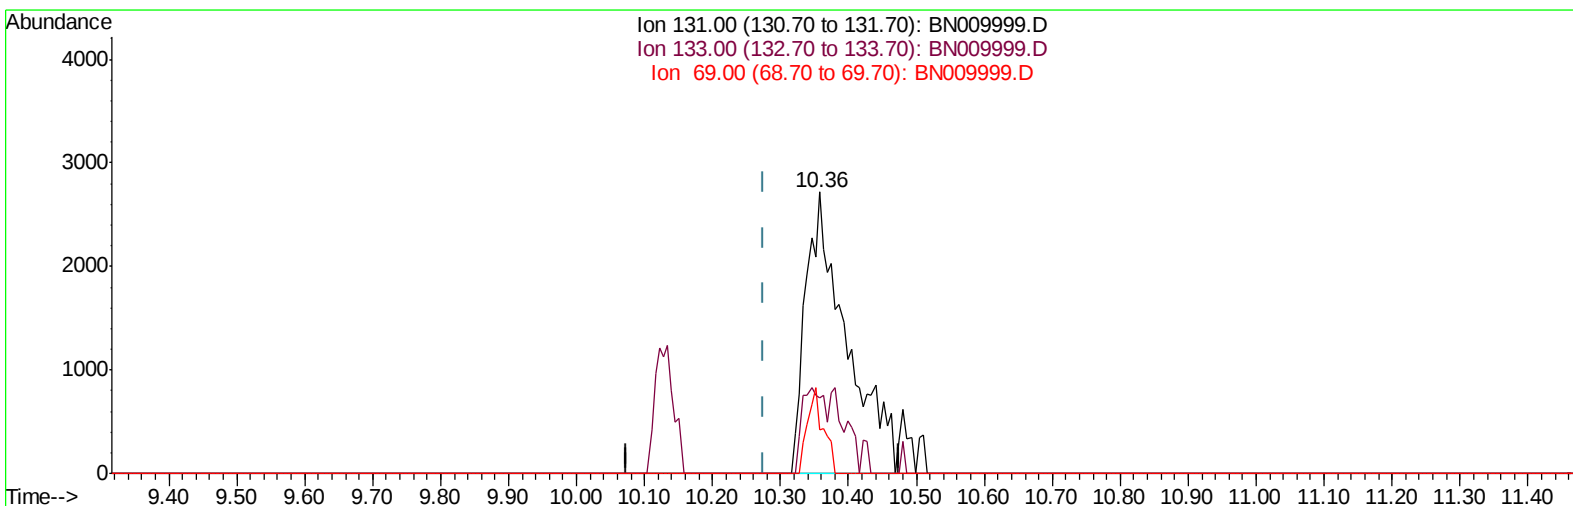

TIC: BN009999.D

(29) 4-Chloroaniline-d4 (S)
10.357min (+0.082) 1.97ng/ul m
response 11219

Ion	Exp%	Act%
131.00	100	100
133.00	33.00	26.98
69.00	22.10	15.47#
0.00	0.00	0.00