
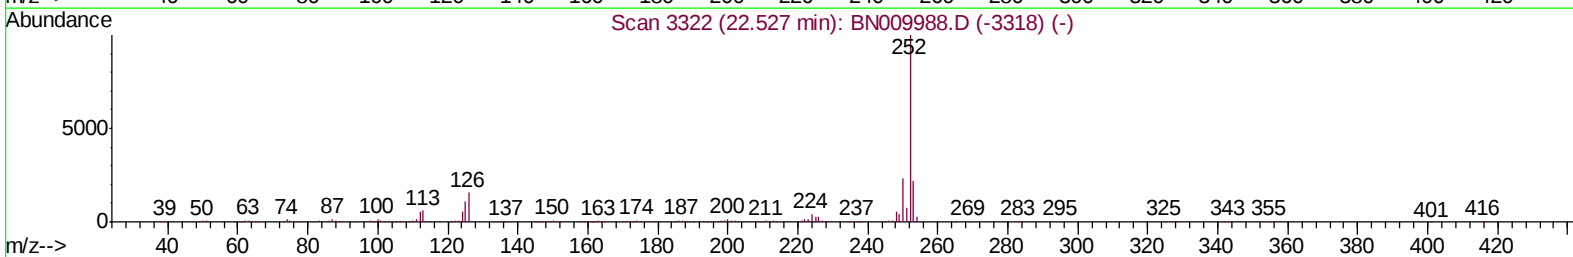
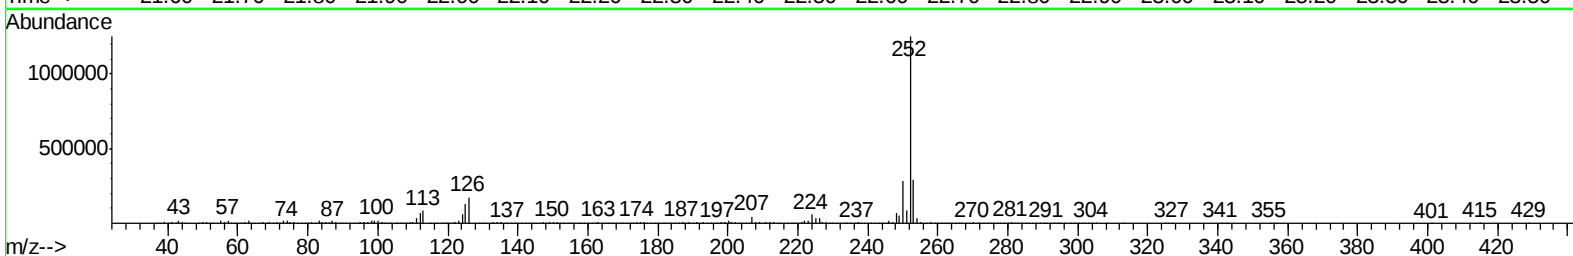


Data File : BN010000.D
Acq On : 28 Feb 2020 23:44
Operator : CG/JU
Sample : L1507-14RX
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Feb 29 01:40:26 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 29 01:38:10 2020
Response via : Initial Calibration

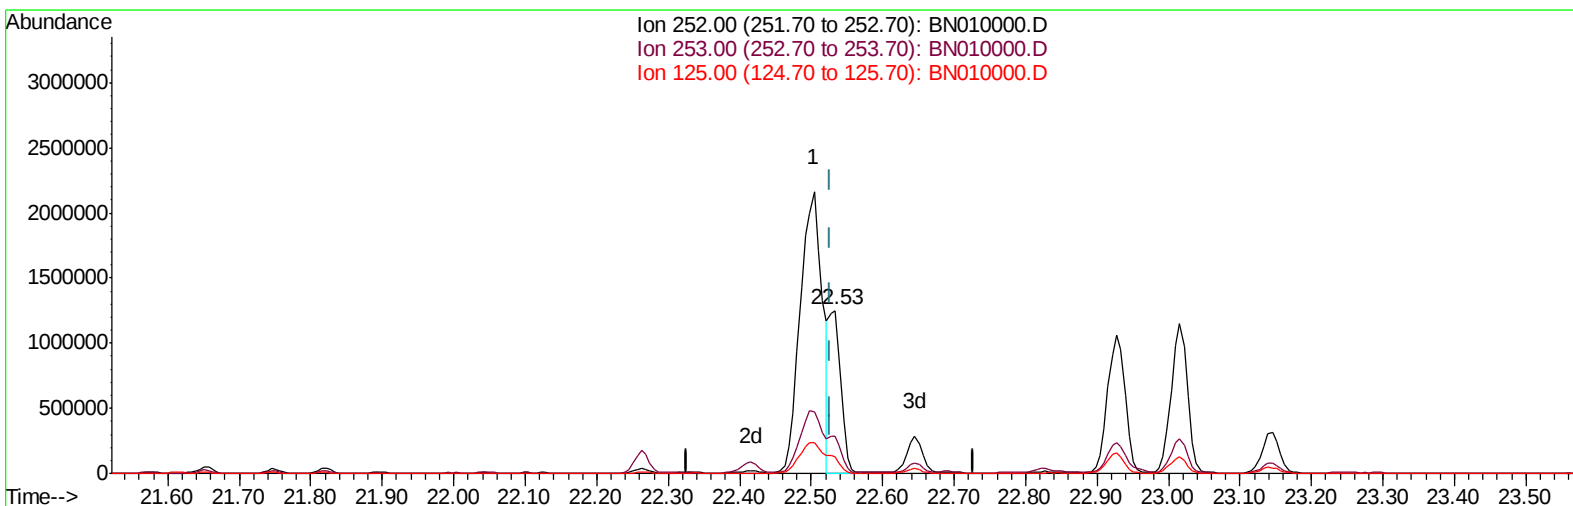

TIC: BN010000.D

(89) Benzo(k)fluoranthene

22.533min (+0.006) 44.77ng/ul m

response 1388276

Ion	Exp%	Act%
252.00	100	100
253.00	22.50	22.99
125.00	10.20	10.21
0.00	0.00	0.00