
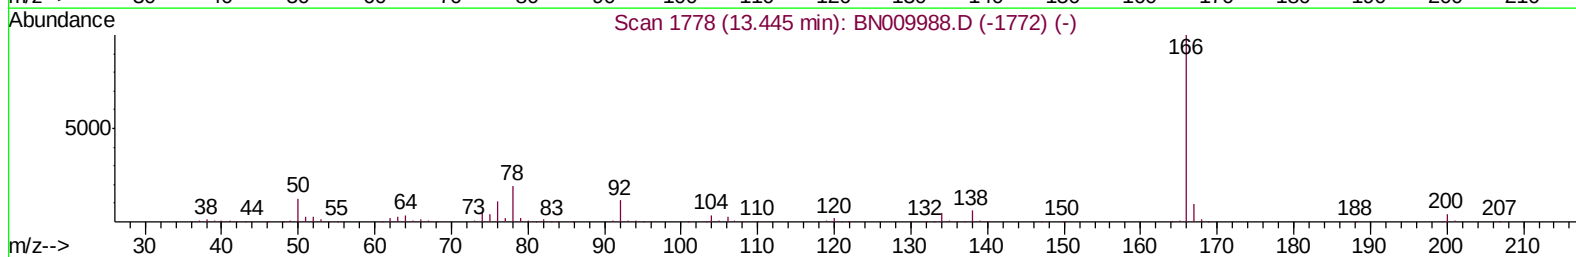
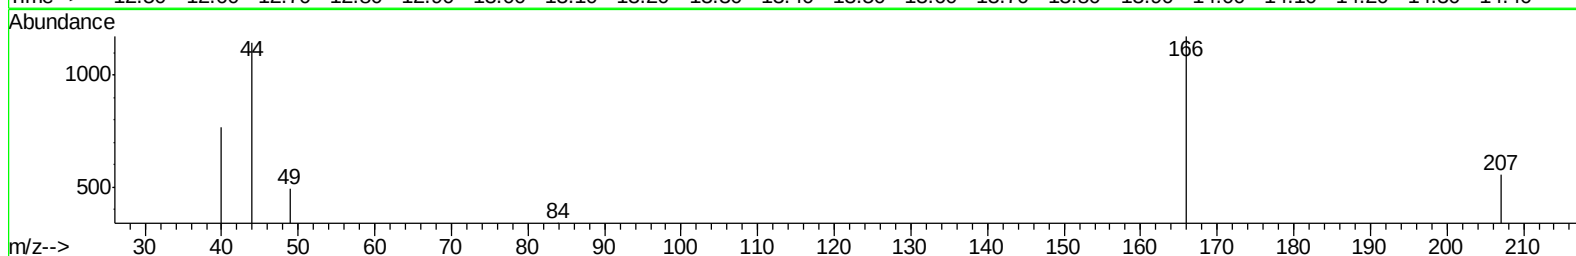


Data File : BN010001.D  
Acq On : 29 Feb 2020 00:20  
Operator : CG/JU  
Sample : L1582-07DL3 300X  
Misc :  
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Feb 29 01:40:45 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SOM-EPA-BN021220MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Sat Feb 29 01:38:10 2020  
Response via : Initial Calibration

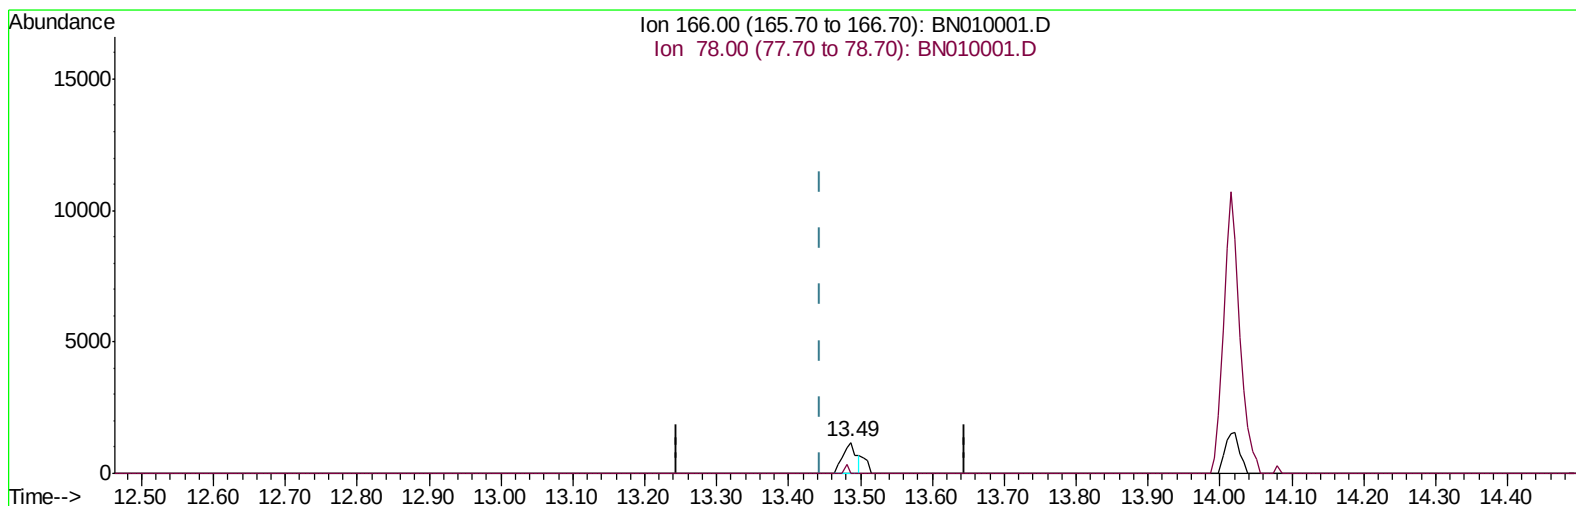

TIC: BN010001.D

(44) Dimethylphthalate-d6 (S)

13.486min (+0.041) 0.08ng/ul

response 1574

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 166.00 | 100   | 100   |
| 78.00  | 17.40 | 0.00# |
| 0.00   | 0.00  | 0.00  |
| 0.00   | 0.00  | 0.00  |