
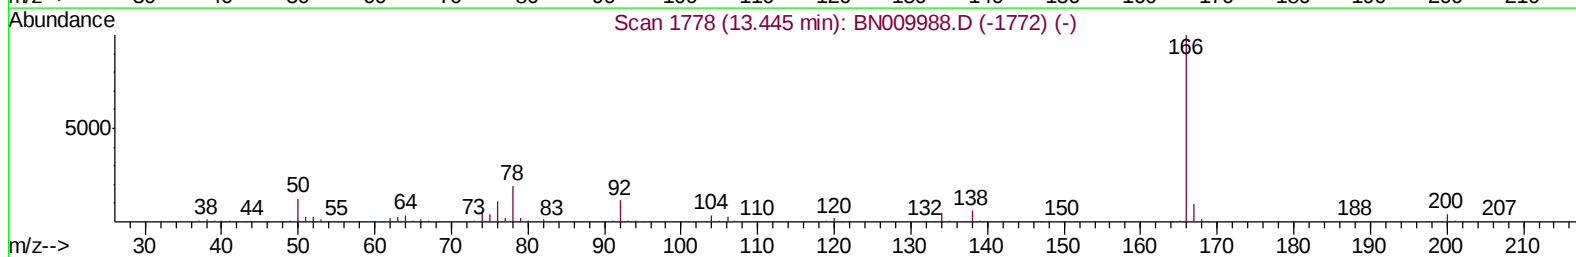
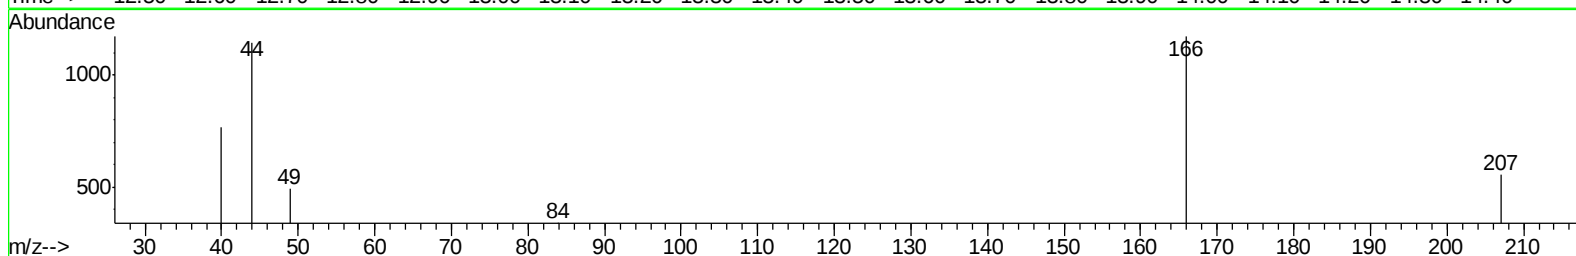


Data File : BN010001.D
Acq On : 29 Feb 2020 00:20
Operator : CG/JU
Sample : L1582-07DL3 300X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Feb 29 01:40:45 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 29 01:38:10 2020
Response via : Initial Calibration

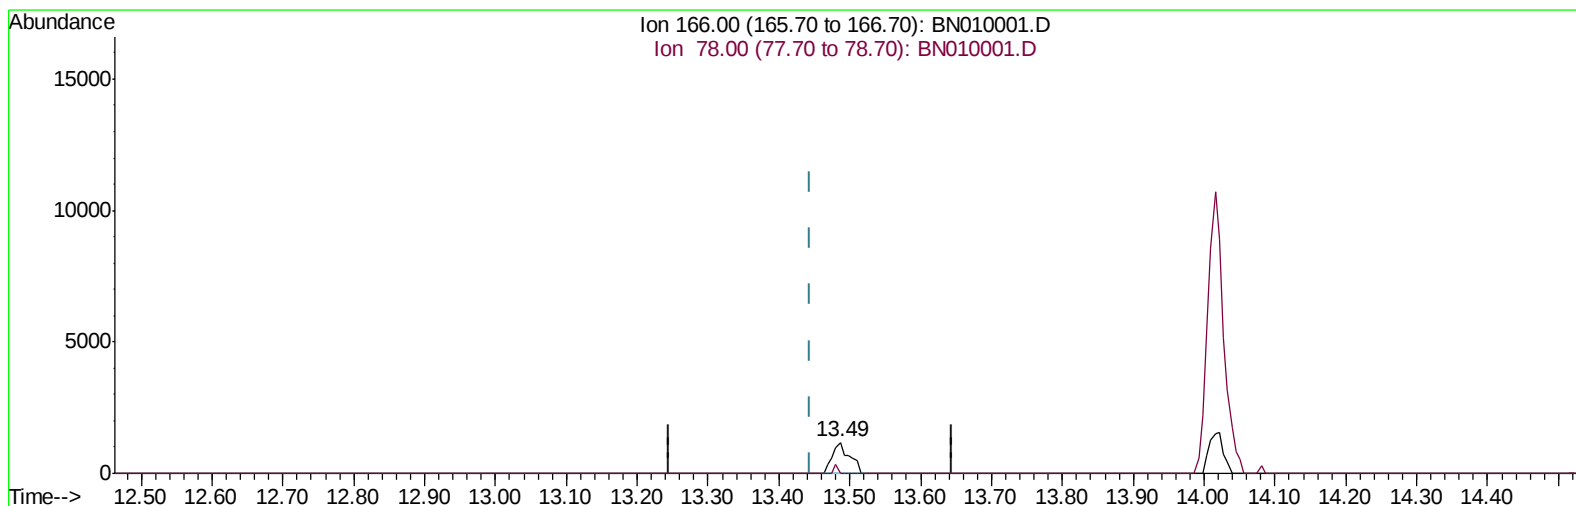

TIC: BN010001.D

(44) Dimethylphthalate-d6 (S)

13.486min (+0.041) 0.09ng/ul m

response 1955

Ion	Exp%	Act%
166.00	100	100
78.00	17.40	0.00#
0.00	0.00	0.00
0.00	0.00	0.00