
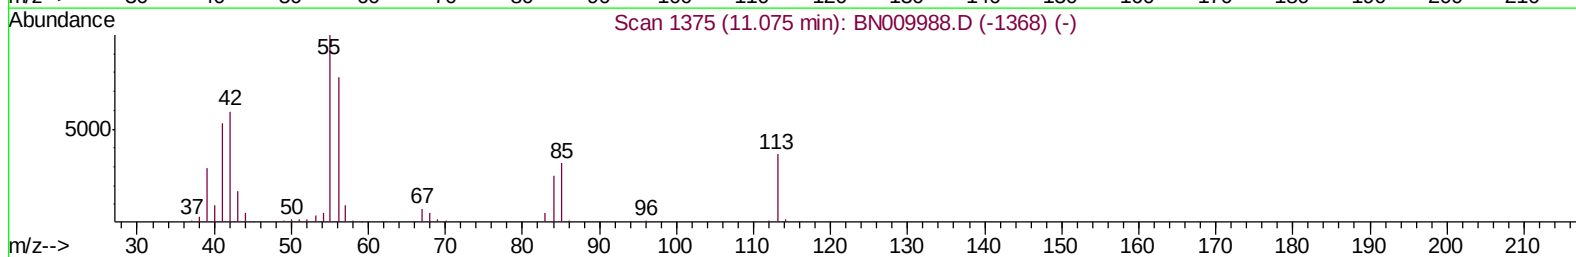
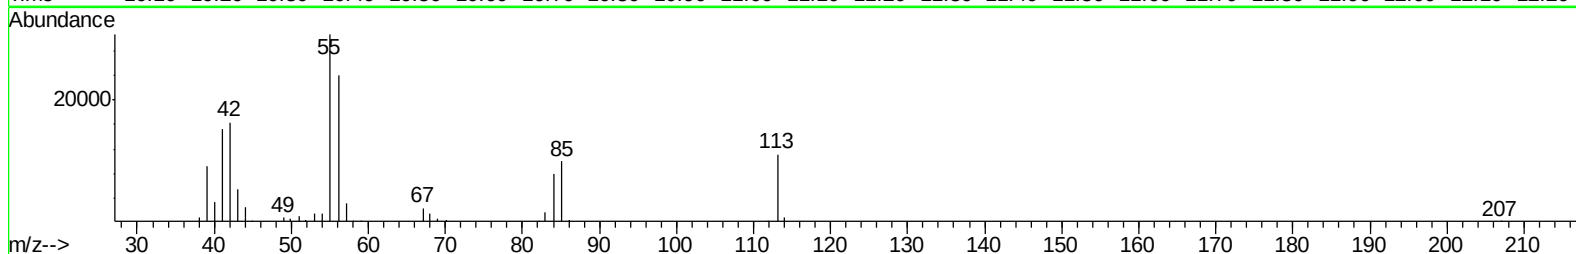


Data File : BN010002.D
Acq On : 29 Feb 2020 00:56
Operator : CG/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Feb 29 01:40:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 29 01:38:10 2020
Response via : Initial Calibration

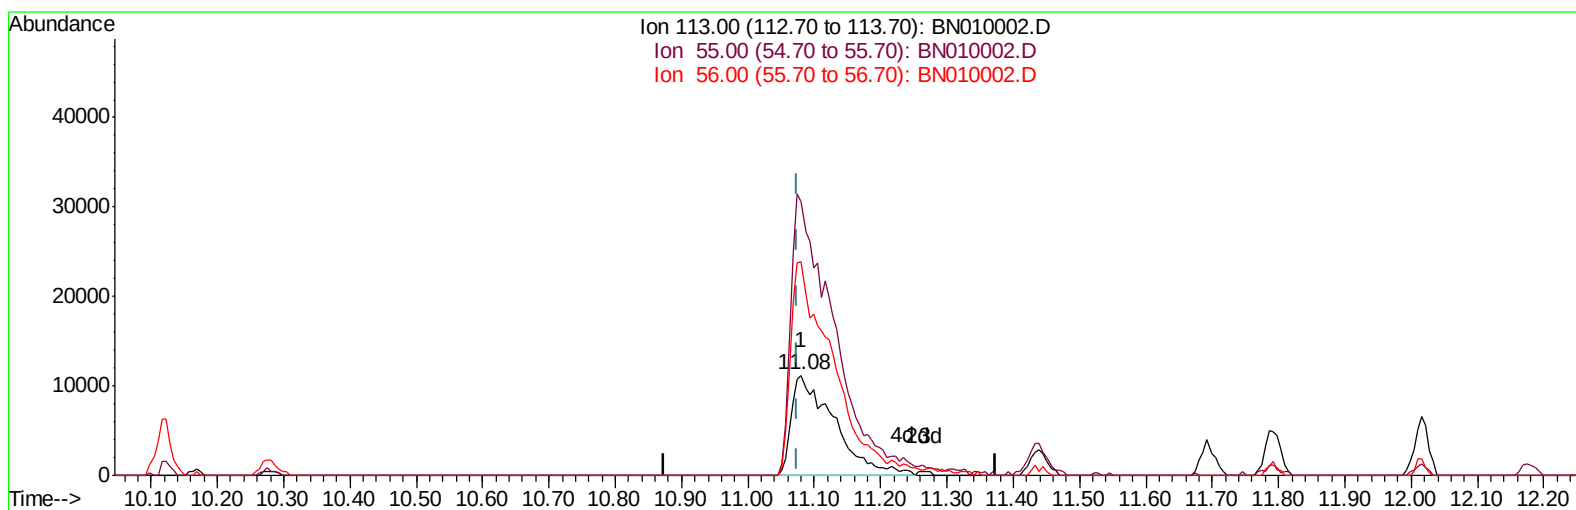

TIC: BN010002.D

(32) Caprolactam

11.081min (+0.006) 21.68ng/ul m

response 49542

Ion	Exp%	Act%
113.00	100	100
55.00	261.40	273.70
56.00	202.00	213.84
0.00	0.00	0.00