
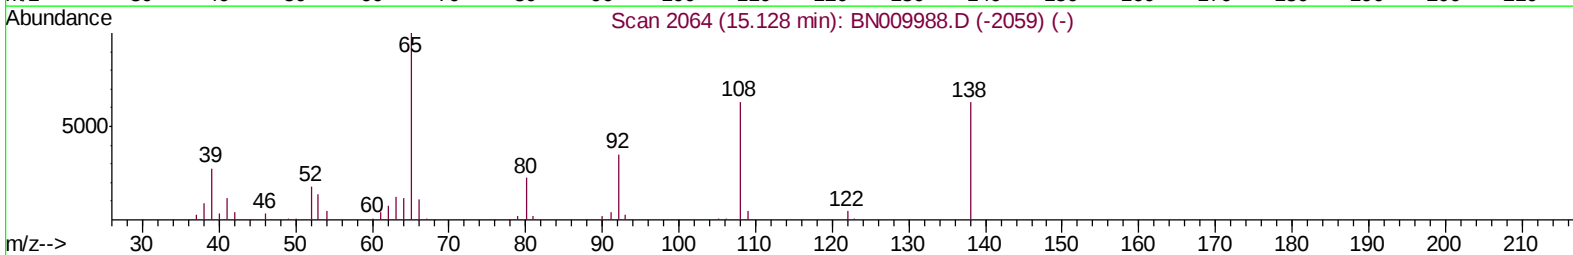
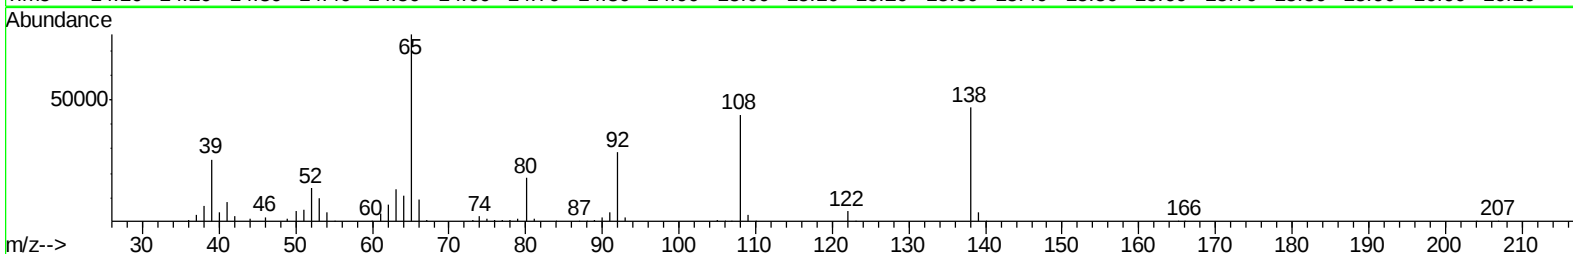


Data File : BN010002.D
Acq On : 29 Feb 2020 00:56
Operator : CG/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Feb 29 01:40:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 29 01:38:10 2020
Response via : Initial Calibration

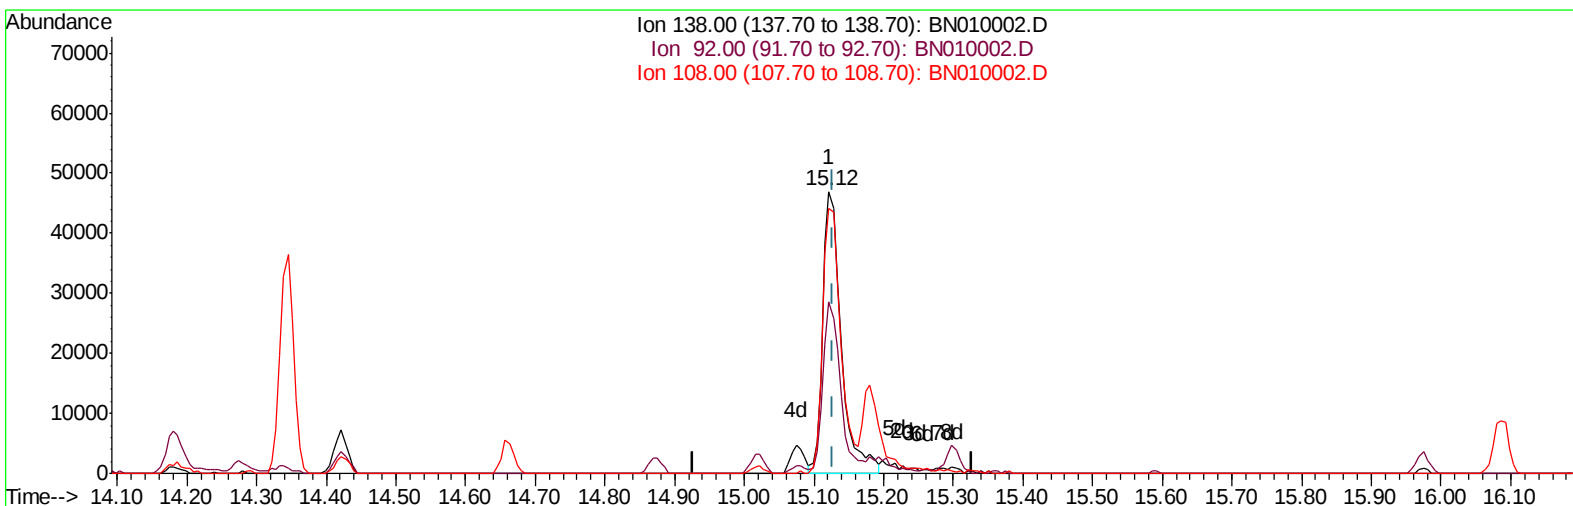

TIC: BN010002.D

(61) 4-Nitroaniline

15.122min (-0.006) 17.48ng/ul m

response 86267

Ion	Exp%	Act%
138.00	100	100
92.00	59.70	60.70
108.00	90.40	94.08
0.00	0.00	0.00