

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022820\
 Data File : BN009991.D
 Acq On : 28 Feb 2020 18:20
 Operator : CG/JU
 Sample : PB127177BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Feb 28 21:58:32 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 26 07:56:07 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	101439	20.00	ng/ul	0.00
18) Naphthalene-d8	10.12	136	454423	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.02	164	297898	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.77	188	638499	20.00	ng/ul	0.00
78) Chrysene-d12	21.00	240	603050	20.00	ng/ul	0.00
86) Perylene-d12	23.10	264	629657	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.02	96	16031	6.50	ng/uL	0.00
5) Phenol-d5	6.58	99	269023	31.18	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.73	67	205185	34.46	ng/ul	-0.01
9) 2-Chlorophenol-d4	6.92	132	217230	33.44	ng/ul	-0.01
13) 4-Methylphenol-d8	8.09	113	224136	32.66	ng/ul	0.00
19) Nitrobenzene-d5	8.52	128	109450	32.92	ng/ul	0.00
22) 2-Nitrophenol-d4	9.23	143	117808	32.39	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.76	165	207214	29.64	ng/ul	0.00
29) 4-Chloroaniline-d4	10.28	131	306404	39.01	ng/ul	0.00
44) Dimethylphthalate-d6	13.45	166	721429	32.42	ng/ul	0.00
47) Acenaphthylene-d8	13.70	160	848461	32.38	ng/ul	0.00
52) 4-Nitrophenol-d4	14.27	143	93483	23.00	ng/ul	0.00
58) Fluorene-d10	15.03	176	631667	32.88	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.19	200	84720	21.36	ng/ul	0.00
71) Anthracene-d10	16.87	188	932944	31.88	ng/ul	0.00
79) Pyrene-d10	19.19	212	1065172	33.79	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.97	264	1049079	33.36	ng/ul	0.00

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	8.09	70	6224	1.065 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022820\
Data File : BN009991.D
Acq On : 28 Feb 2020 18:20
Operator : CG/JU
Sample : PB127177BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Feb 28 21:58:32 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 26 07:56:07 2020
Response via : Initial Calibration

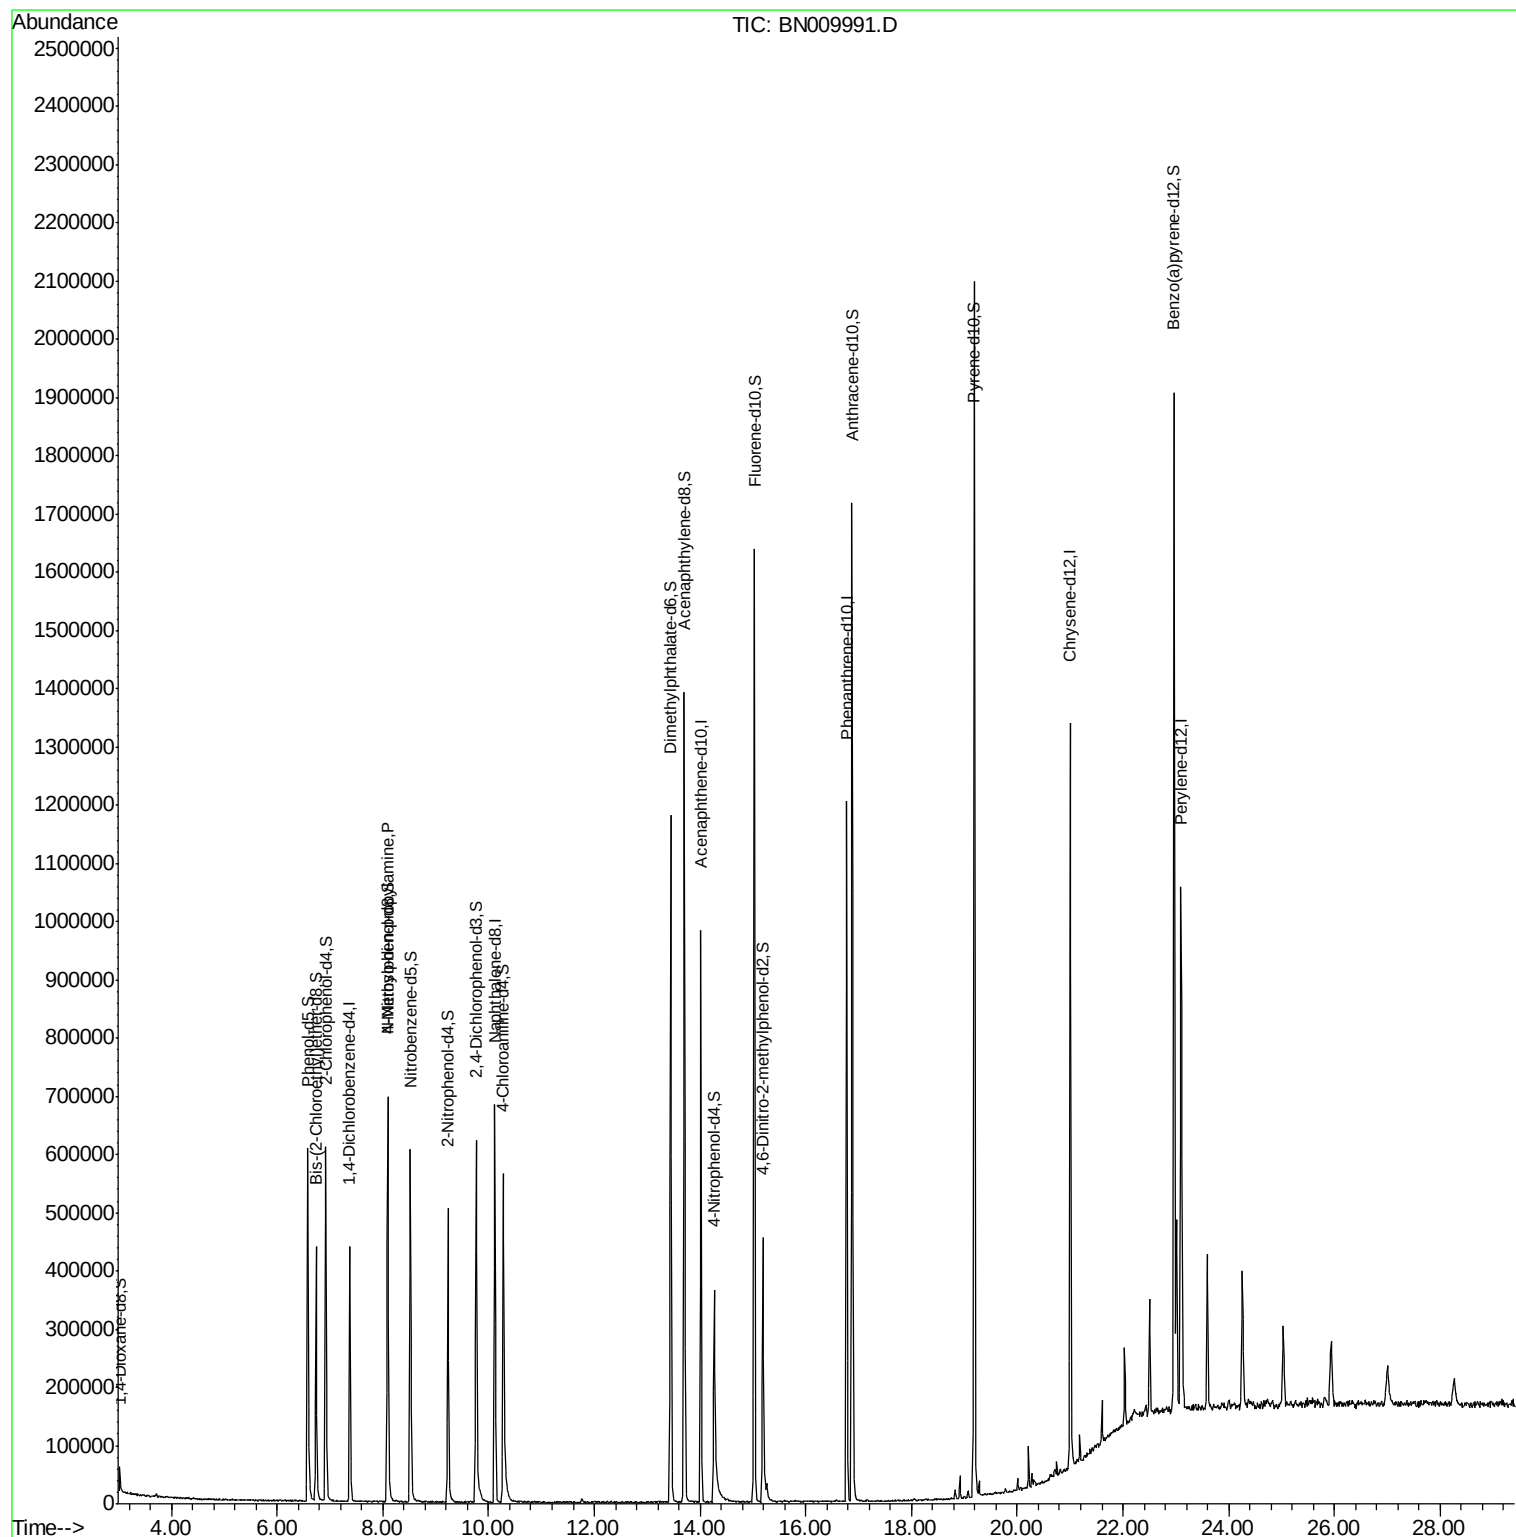

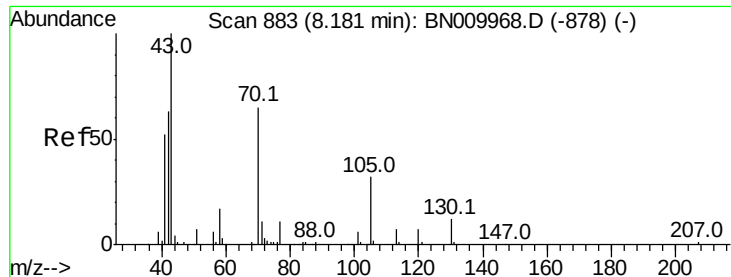

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.065 ng/ul
 RT: 8.09 min Scan# 868
 Delta R.T. -0.09 min
 Lab File: BN009991.D
 Acq: 28 Feb 2020 18:20

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion: 70 Resp: 6224
 Ion Ratio Lower Upper
 70 100
 42 646.6 72.6 108.8#
 101 0.0 7.7 11.5#
 130 0.0 14.7 22.1#

