

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022820\
 Data File : BN009993.D
 Acq On : 28 Feb 2020 19:33
 Operator : CG/JU
 Sample : L1568-04RX
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Feb 28 21:58:46 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 26 07:56:07 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	88409	20.00	ng/ul	0.00
18) Naphthalene-d8	10.12	136	370406	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.02	164	234552	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.77	188	504126	20.00	ng/ul	0.00
78) Chrysene-d12	21.00	240	456013	20.00	ng/ul	0.00
86) Perylene-d12	23.10	264	498362	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.02	96	8567	3.99	ng/uL	0.00
5) Phenol-d5	6.58	99	157845	20.99	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.73	67	125924	24.27	ng/ul	-0.01
9) 2-Chlorophenol-d4	6.92	132	135803	23.99	ng/ul	-0.01
13) 4-Methylphenol-d8	8.09	113	130220	21.77	ng/ul	0.00
19) Nitrobenzene-d5	8.52	128	67608	24.95	ng/ul	0.00
22) 2-Nitrophenol-d4	9.23	143	72546	24.47	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.77	165	123896	21.74	ng/ul	0.00
29) 4-Chloroaniline-d4	10.29	131	169769	26.51	ng/ul	0.00
44) Dimethylphthalate-d6	13.45	166	451788	25.79	ng/ul	0.00
47) Acenaphthylene-d8	13.70	160	522867	25.34	ng/ul	0.00
52) 4-Nitrophenol-d4	14.27	143	46228	14.45	ng/ul	0.00
58) Fluorene-d10	15.02	176	397696	26.29	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.19	200	48749	15.57	ng/ul	0.00
71) Anthracene-d10	16.87	188	610763	26.43	ng/ul	0.00
79) Pyrene-d10	19.19	212	700450	29.39	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.97	264	712560	28.63	ng/ul	0.00


Target Compounds				Ovalue
45) Dimethylphthalate	13.50	163	56468	3.089 ng/ul# 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022820\
Data File : BN009993.D
Acq On : 28 Feb 2020 19:33
Operator : CG/JU
Sample : L1568-04RX
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Feb 28 21:58:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 26 07:56:07 2020
Response via : Initial Calibration

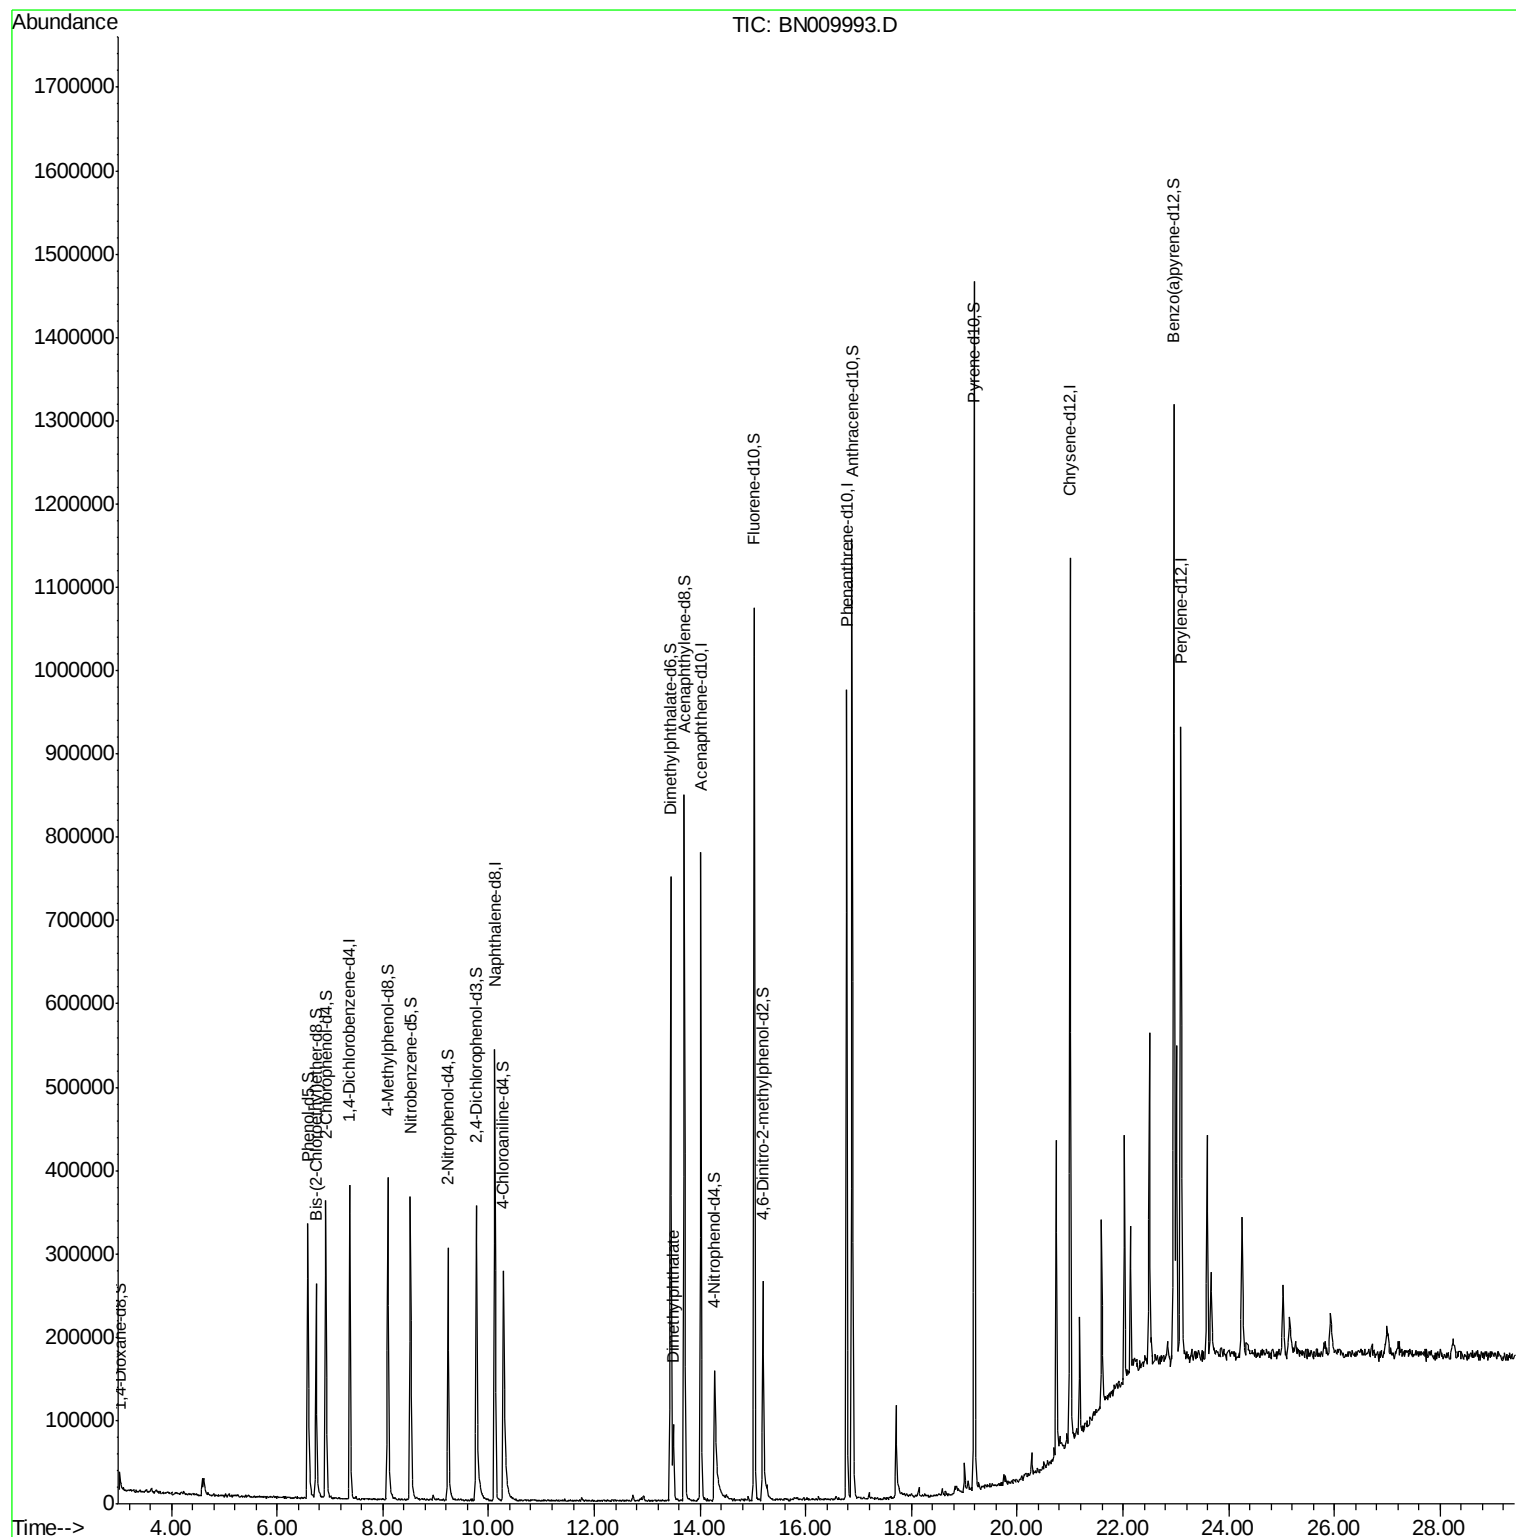

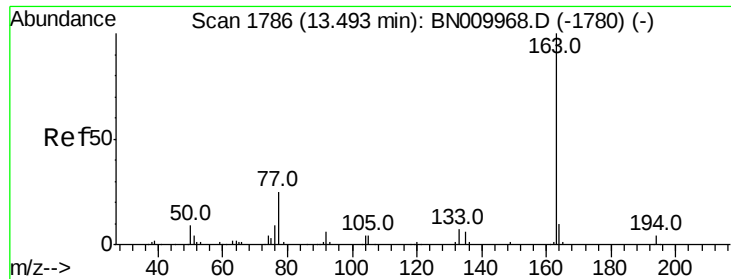

#45

Dimethylphthalate

Concen: 3.089 ng/ul

RT: 13.50 min Scan# 1787

Delta R.T. 0.00 min

Lab File: BN009993.D

Acq: 28 Feb 2020 19:33

Instrument :

BNA_N

ClientSampleId :


Tot Ion:163 Resp: 56468

Ion Ratio Lower Upper

163 100

194 5.2 3.4 5.0#

164 9.7 8.0 12.0

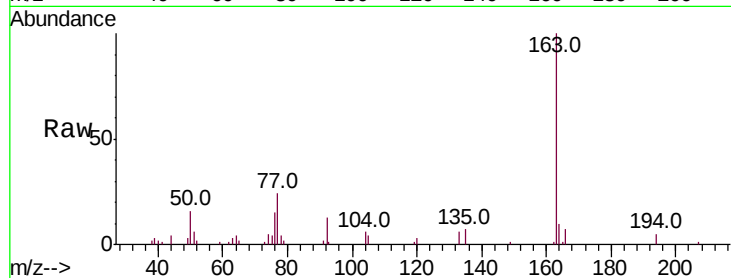

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

