

Data File : BN010001.D
Acq On : 29 Feb 2020 00:20
Operator : CG/JU
Sample : L1582-07DL3 300X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBDJ9DL3

Quant Time: Feb 29 01:40:45 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 29 01:38:10 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.37	152	96992	20.00	ng/ul	0.00
18) Naphthalene-d8	10.12	136	427811	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.02	164	280233	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.78	188	573582	20.00	ng/ul	0.00
78) Chrysene-d12	21.00	240	507649	20.00	ng/ul	0.00
86) Perylene-d12	23.09	264	534575	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	0.00	99	0	0.00	ng/ul	
7) Bis-(2-Chloroethyl)ether-d	0.00	67	0	0.00	ng/ul	
9) 2-Chlorophenol-d4	0.00	132	0	0.00	ng/ul	
13) 4-Methylphenol-d8	7.91	113	140	0.02	ng/ul	-0.18
19) Nitrobenzene-d5	0.00	128	0	0.00	ng/ul	
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul	
29) 4-Chloroaniline-d4	10.13	131	119	0.02	ng/ul	-0.14
44) Dimethylphthalate-d6	13.49	166	1574	0.08	ng/ul	0.04
47) Acenaphthylene-d8	13.70	160	2491	0.10	ng/ul	0.00
52) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
58) Fluorene-d10	15.03	176	1437	0.08	ng/ul	0.01
63) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
71) Anthracene-d10	16.89	188	7876	0.30	ng/ul	0.02
79) Pyrene-d10	19.20	212	4049	0.15	ng/ul	0.01
90) Benzo(a)pyrene-d12	22.97	264	2436	0.09	ng/ul	0.00


Target Compounds				Qvalue		
28) Naphthalene	10.17	128	602270	26.106	ng/ul	99
34) 2-Methylnaphthalene	11.81	142	46415	2.897	ng/ul	94
35) 1-Methylnaphthalene	12.03	142	24430	1.521	ng/uL#	99
50) Acenaphthene	14.09	153	27421	1.499	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN010001.D
Acq On : 29 Feb 2020 00:20
Operator : CG/JU
Sample : L1582-07DL3 300X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBDJ9DL3

Quant Time: Feb 29 01:40:45 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 29 01:38:10 2020
Response via : Initial Calibration

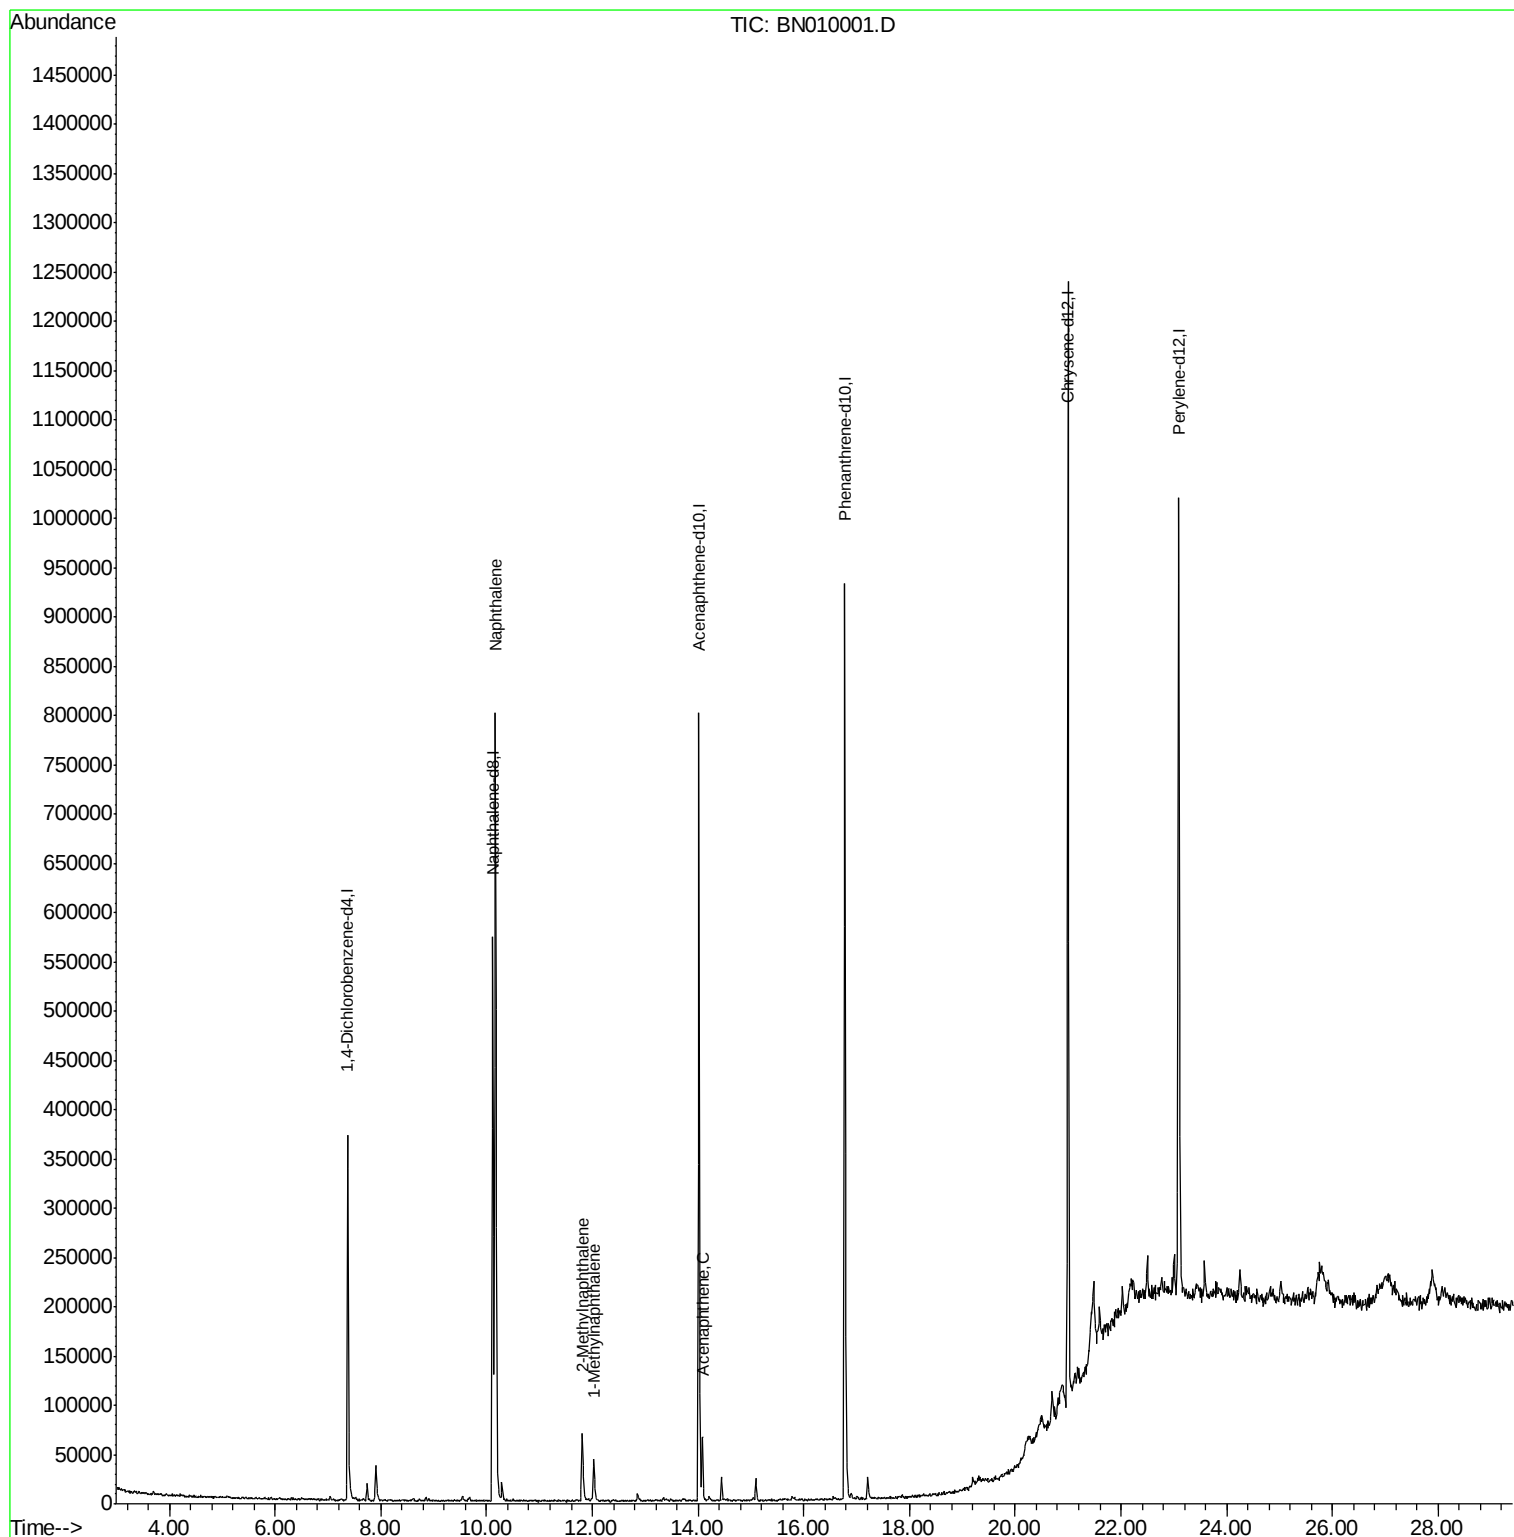

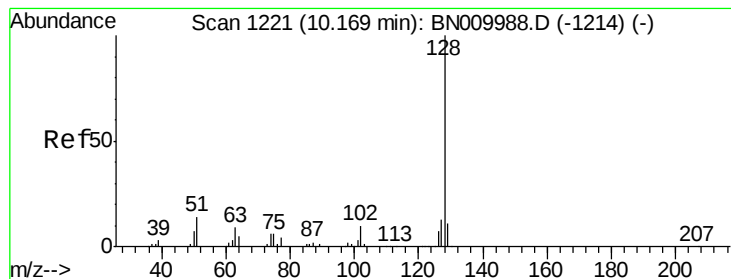

#28

Naphthalene

Concen: 26.106 ng/ul

RT: 10.17 min Scan# 1221

Delta R.T. -0.00 min

Lab File: BN010001.D

Acq: 29 Feb 2020 00:20

Instrument :

BNA_N

ClientSampleId :

DBDJ9DL3


Tgt Ion:128 Resp: 602270

Ion Ratio Lower Upper

128 100

129 10.2 8.6 13.0




127 12.5 10.3 15.5

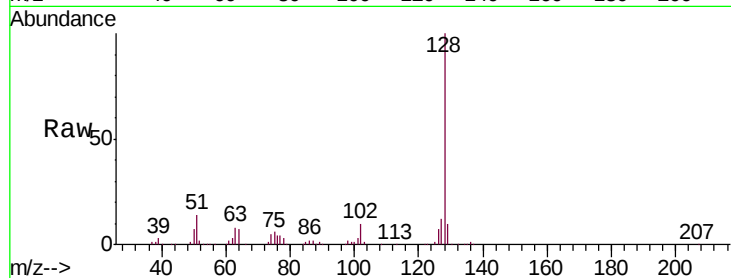

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

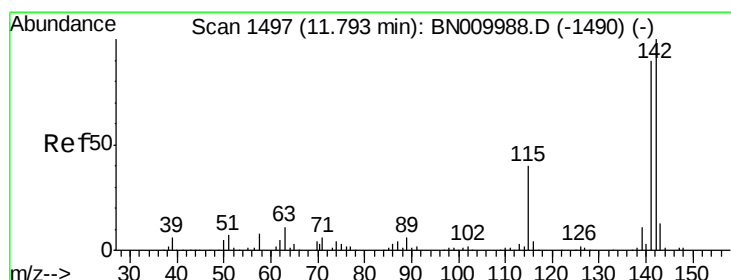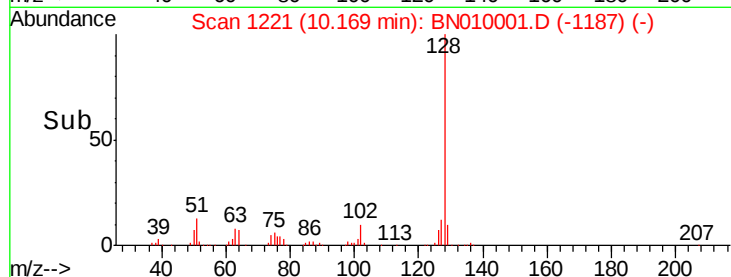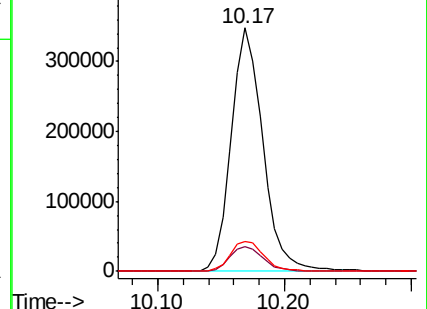

#34

2-Methylnaphthalene

Concen: 2.897 ng/ul

RT: 11.81 min Scan# 1500

Delta R.T. 0.02 min

Lab File: BN010001.D


Acq: 29 Feb 2020 00:20

Tgt Ion:142 Resp: 46415

Ion Ratio Lower Upper



142 100


141 84.7 72.1 108.1

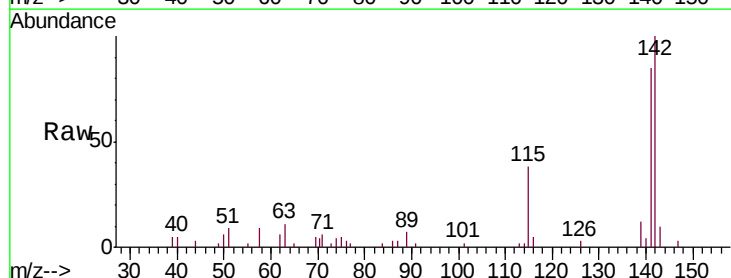

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E



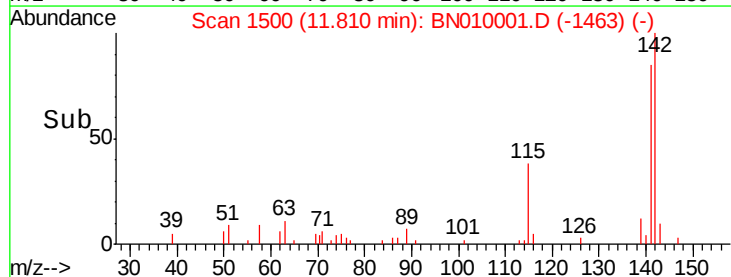
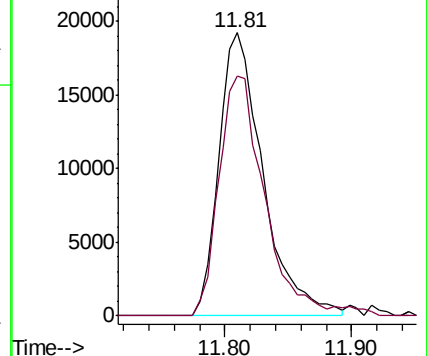


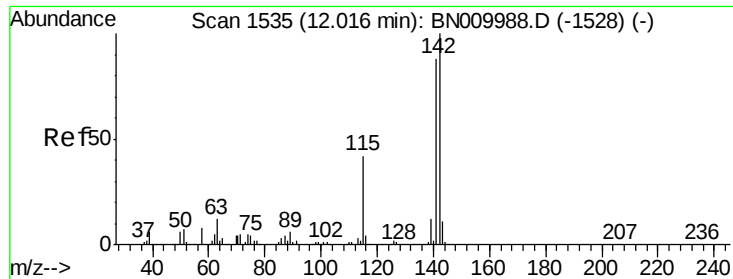

#35
 1-Methylnaphthalene
 Concen: 1.521 ng/uL
 RT: 12.03 min Scan# 1537
 Delta R.T. 0.01 min
 Lab File: BN010001.D
 Acq: 29 Feb 2020 00:20

Instrument :
 BNA_N
 ClientSampleId :
 DBDJ9DL3

Tgt Ion:142 Resp: 24430
 Ion Ratio Lower Upper
 142 100
 141 89.9 72.8 109.2
 116 1.3 3.2 4.8#

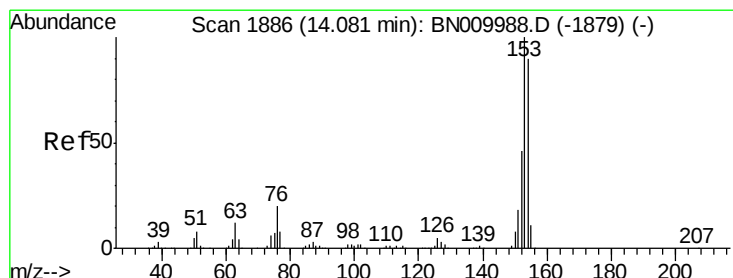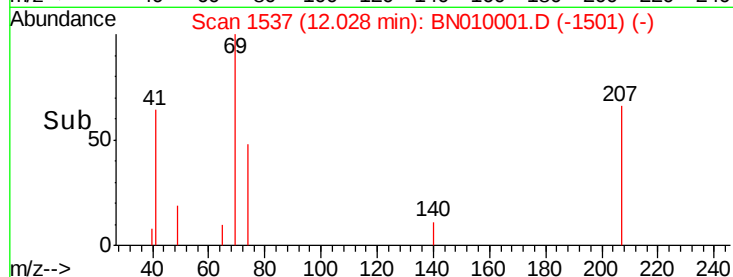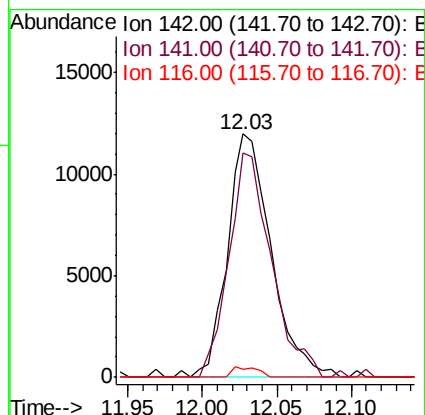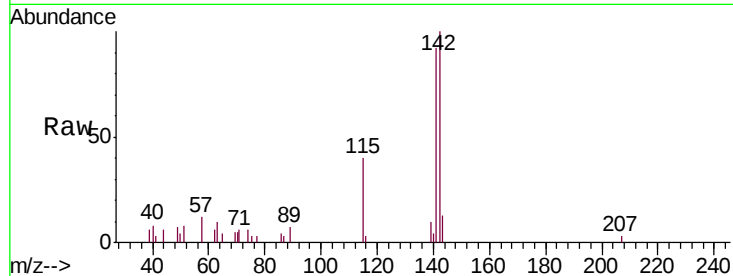

#50
 Acenaphthene
 Concen: 1.499 ng/uL
 RT: 14.09 min Scan# 1887
 Delta R.T. 0.01 min
 Lab File: BN010001.D
 Acq: 29 Feb 2020 00:20

Tgt Ion:153 Resp: 27421
 Ion Ratio Lower Upper
 153 100
 152 44.2 36.6 54.8
 154 89.6 70.6 106.0

