

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022820\
 Data File : BN010003.D
 Acq On : 29 Feb 2020 02:08
 Operator : CG/JU
 Sample : PB127111BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Mar 02 05:51:50 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Feb 29 01:38:10 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	113067	20.00	ng/ul	0.00
18) Naphthalene-d8	10.12	136	498257	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.02	164	323522	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.77	188	696349	20.00	ng/ul	0.00
78) Chrysene-d12	21.00	240	654157	20.00	ng/ul	0.00
86) Perylene-d12	23.09	264	664070	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.02	96	16295	5.93	ng/uL	0.00
5) Phenol-d5	6.58	99	306302	31.85	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.73	67	220550	33.23	ng/ul	0.00
9) 2-Chlorophenol-d4	6.92	132	245164	33.86	ng/ul	0.00
13) 4-Methylphenol-d8	8.09	113	252230	32.97	ng/ul	0.00
19) Nitrobenzene-d5	8.52	128	121290	33.27	ng/ul	0.00
22) 2-Nitrophenol-d4	9.23	143	135235	33.91	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.76	165	234428	30.58	ng/ul	0.00
29) 4-Chloroaniline-d4	10.28	131	340953	39.58	ng/ul	0.00
44) Dimethylphthalate-d6	13.45	166	783081	32.41	ng/ul	0.00
47) Acenaphthylene-d8	13.70	160	918023	32.26	ng/ul	0.00
52) 4-Nitrophenol-d4	14.27	143	100628	22.80	ng/ul	0.00
58) Fluorene-d10	15.02	176	683122	32.74	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.19	200	99680	23.04	ng/ul	0.00
71) Anthracene-d10	16.87	188	1016600	31.85	ng/ul	0.00
79) Pyrene-d10	19.19	212	1130499	33.06	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.96	264	1117601	33.70	ng/ul	0.00

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	8.09	70	7288	1.119 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022820\
Data File : BN010003.D
Acq On : 29 Feb 2020 02:08
Operator : CG/JU
Sample : PB127111BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Mar 02 05:51:50 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 29 01:38:10 2020
Response via : Initial Calibration

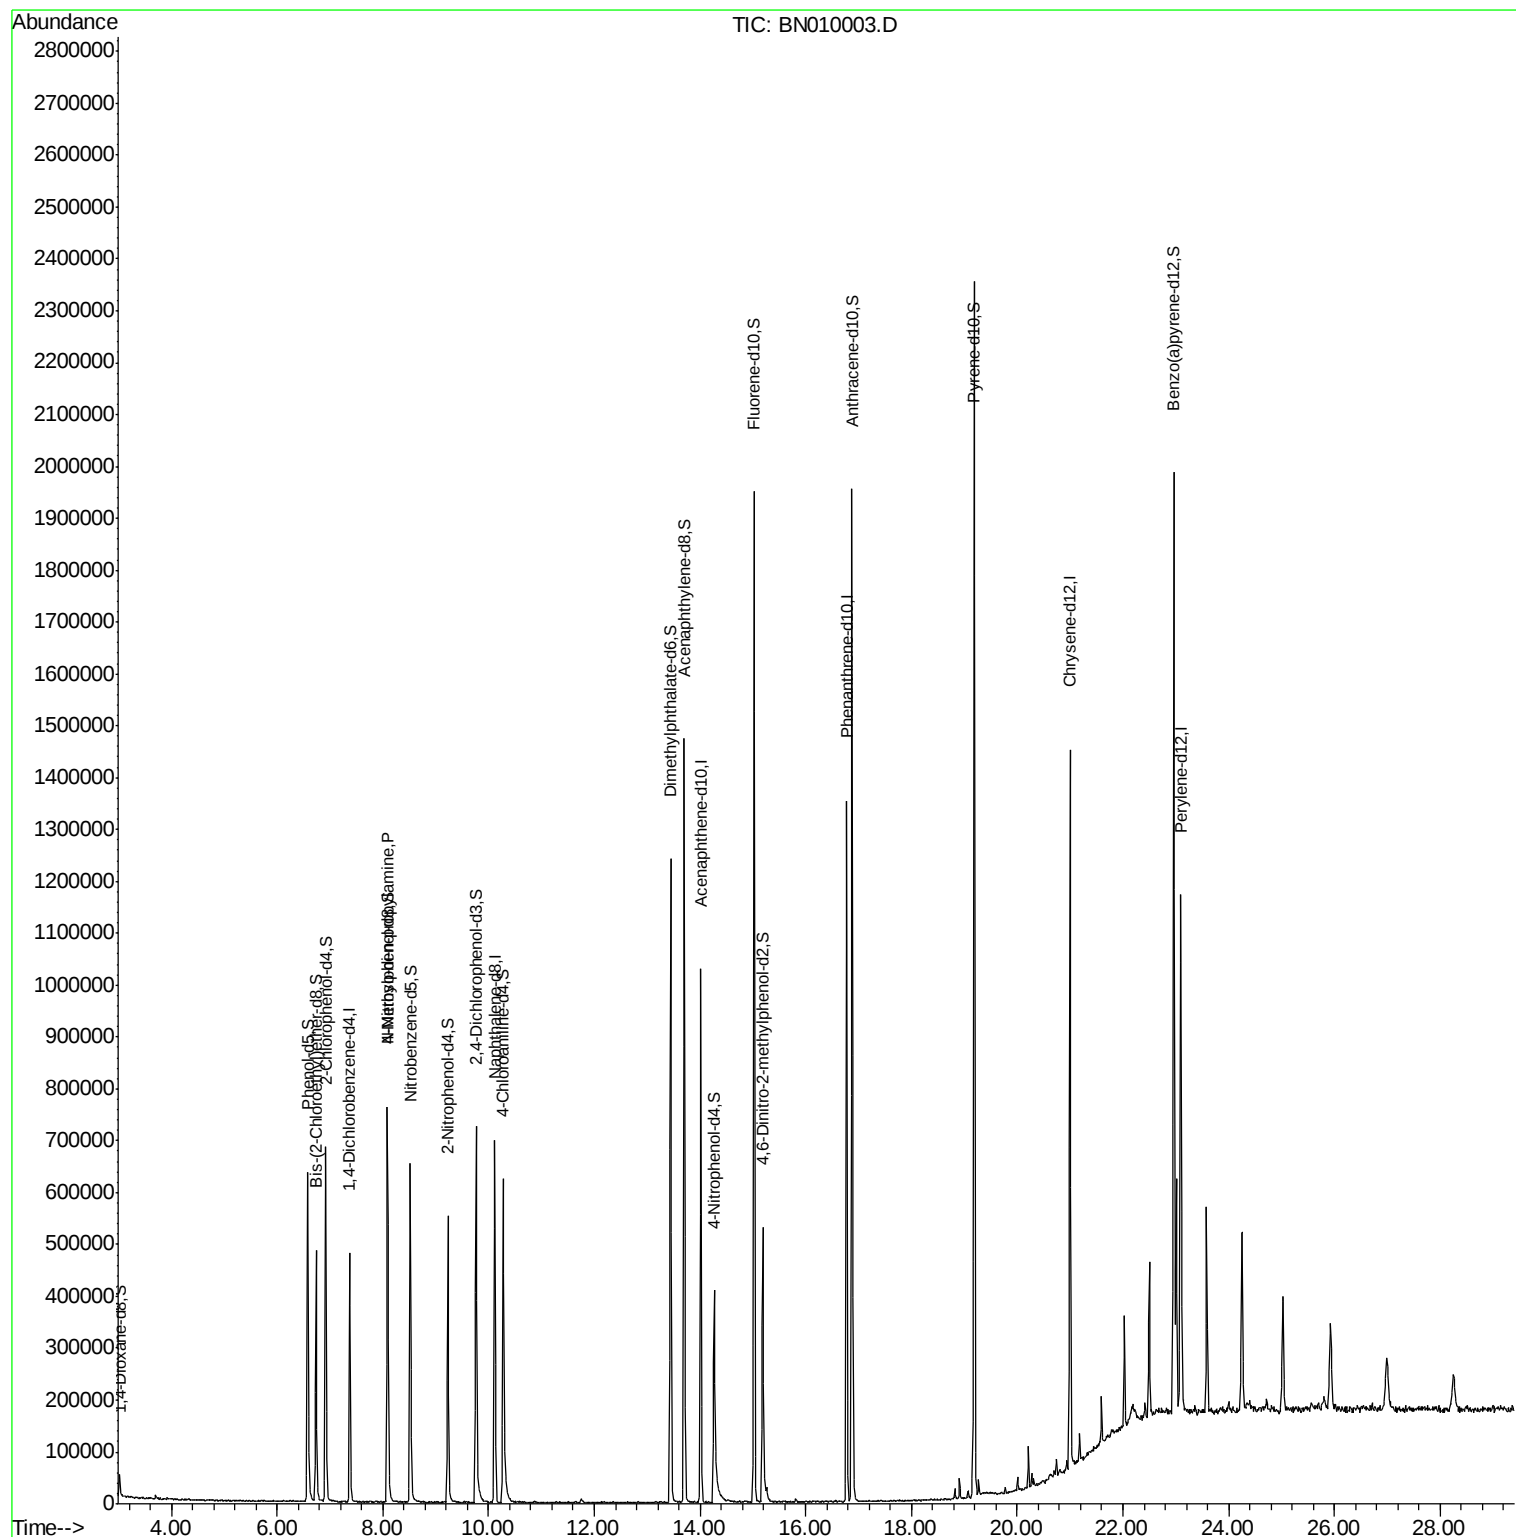

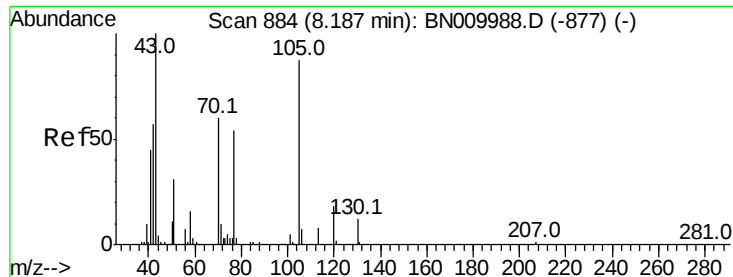

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.119 ng/ul
 RT: 8.09 min Scan# 867
 Delta R.T. -0.10 min
 Lab File: BN010003.D
 Acq: 29 Feb 2020 02:08

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion	Ion	Ratio	Lower	Upper
70	100			
42	546.5	72.6	108.8#	
101	0.0	7.7	11.5#	
130	0.0	14.7	22.1#	

