

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022820\
 Data File : BN010014.D
 Acq On : 29 Feb 2020 08:43
 Operator : CG/JU
 Sample : L1516-06
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBD24

Manual Integrations
 APPROVED

mohammad
 3/3/2020 5:00:02 PM

Quant Time: Mar 02 09:02:54 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Feb 29 01:38:10 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	104371	20.00	ng/ul	0.00
18) Naphthalene-d8	10.12	136	449407	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.02	164	274435	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.77	188	552885	20.00	ng/ul	0.00
78) Chrysene-d12	21.00	240	481357	20.00	ng/ul	0.00
86) Perylene-d12	23.09	264	497077	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.03	96	11350	4.47	ng/uL	0.00
5) Phenol-d5	6.58	99	238289	26.84	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.73	67	171454	27.99	ng/ul	0.00
9) 2-Chlorophenol-d4	6.92	132	192271	28.77	ng/ul	0.00
13) 4-Methylphenol-d8	8.09	113	192683	27.28	ng/ul	0.00
19) Nitrobenzene-d5	8.52	128	95939	29.18	ng/ul	0.00
22) 2-Nitrophenol-d4	9.23	143	104778	29.13	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.77	165	181918	26.31	ng/ul	0.00
29) 4-Chloroaniline-d4	10.28	131	213807	27.52	ng/ul	0.00
44) Dimethylphthalate-d6	13.45	166	550734	26.87	ng/ul	0.00
47) Acenaphthylene-d8	13.70	160	690170	28.59	ng/ul	0.00
52) 4-Nitrophenol-d4	14.28	143	67544	18.04	ng/ul	0.02
58) Fluorene-d10	15.02	176	491968	27.80	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.19	200	51619	15.03	ng/ul	0.00
71) Anthracene-d10	16.87	188	717530	28.31	ng/ul	0.00
79) Pyrene-d10	19.19	212	747022	29.69	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.96	264	717829	28.92	ng/ul	0.00

Target Compounds

					Ovalue
45) Dimethylphthalate	13.49	163	58787	2.748	ng/ul 98
70) Phenanthrene	16.82	178	132491	4.199	ng/ul 98
77) Fluoranthene	18.85	202	312979	8.468	ng/ul 99
80) Pyrene	19.22	202	215232	6.202	ng/ul 99
83) Benzo(a)anthracene	20.99	228	39062m	1.181	ng/ul
85) Chrysene	21.04	228	40002	1.228	ng/ul 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022820\
Data File : BN010014.D
Acq On : 29 Feb 2020 08:43
Operator : CG/JU
Sample : L1516-06
Misc :
ALS Vial : 34 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
DBD24

Manual Integrations
APPROVED

mohammad
3/3/2020 5:00:02 PM

Quant Time: Mar 02 09:02:54 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 29 01:38:10 2020
Response via : Initial Calibration

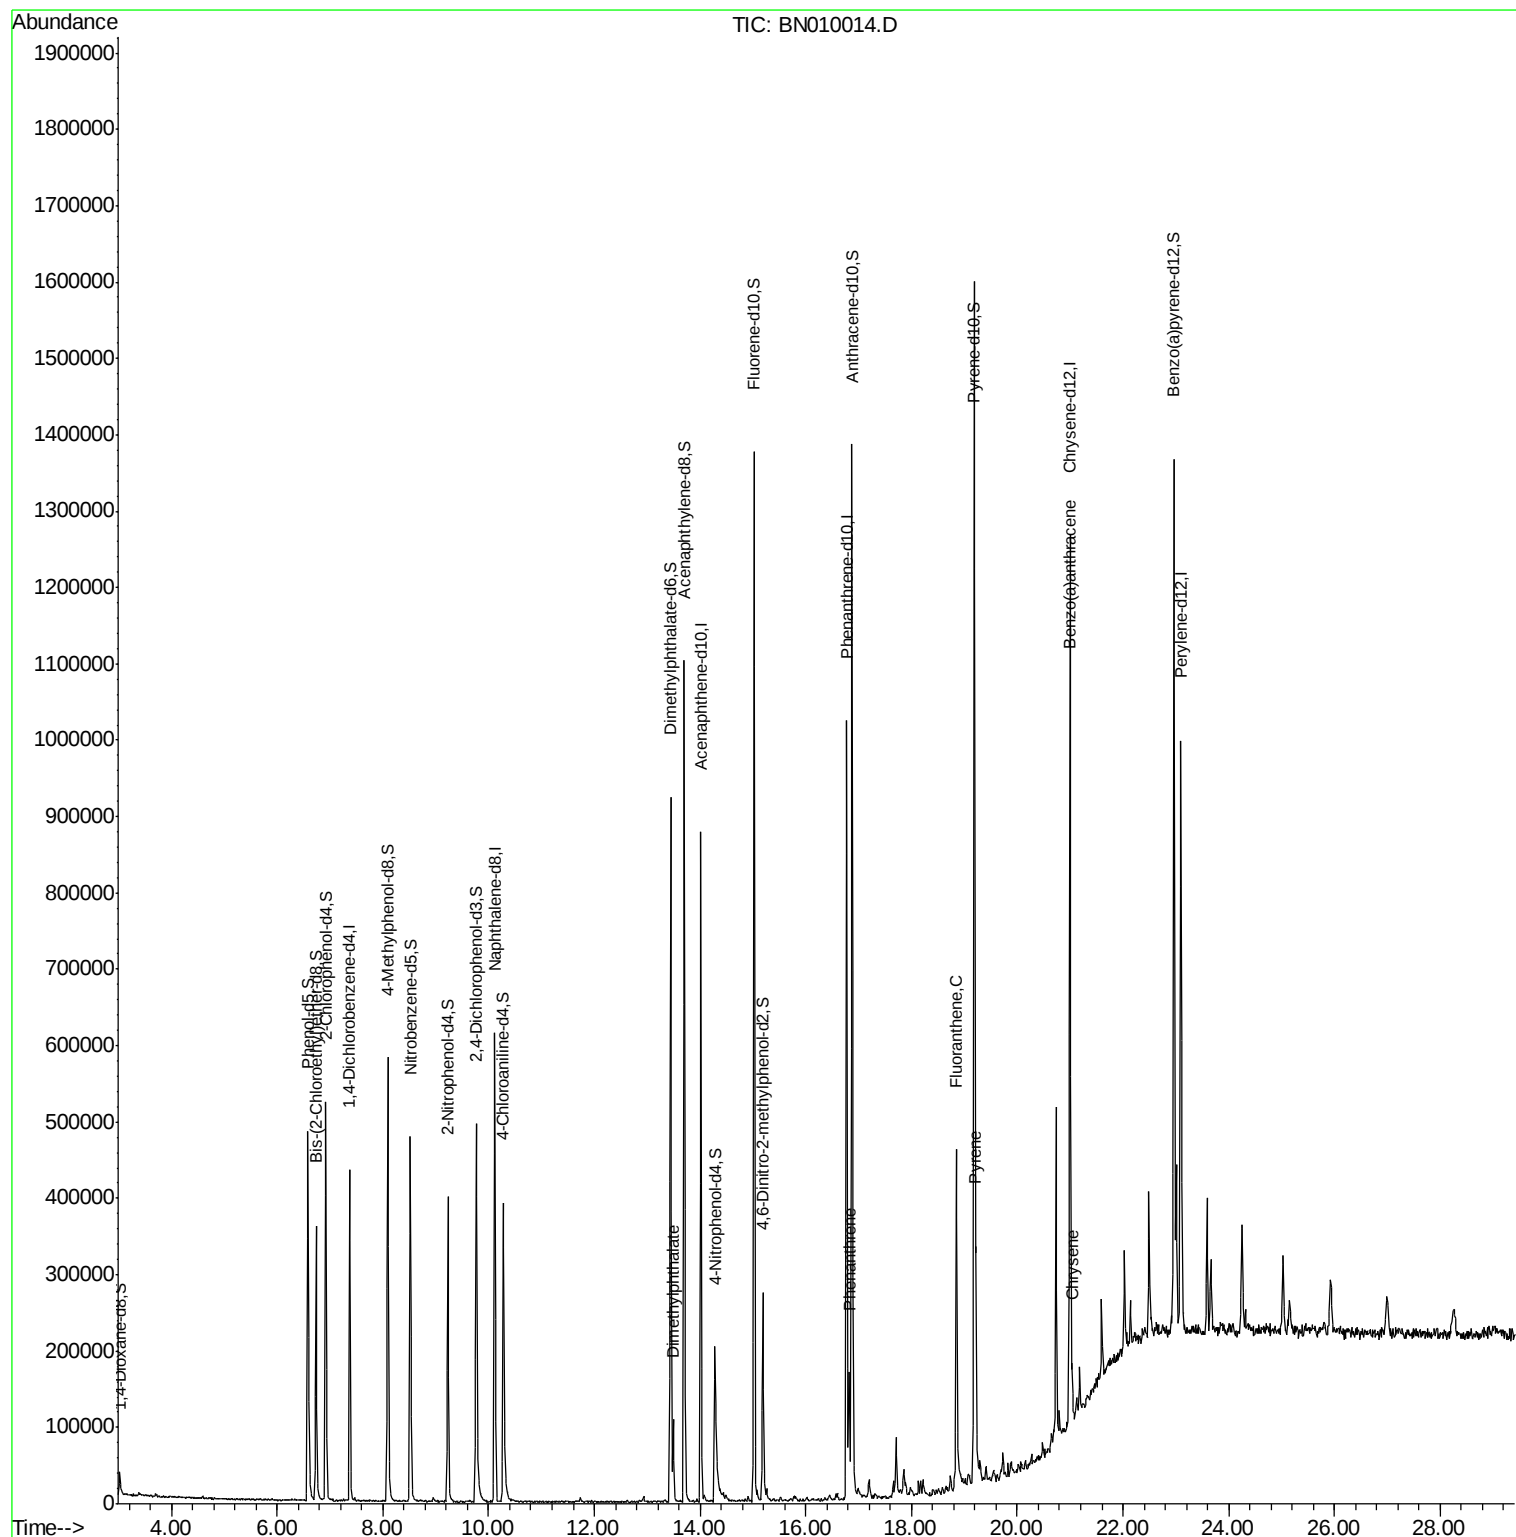

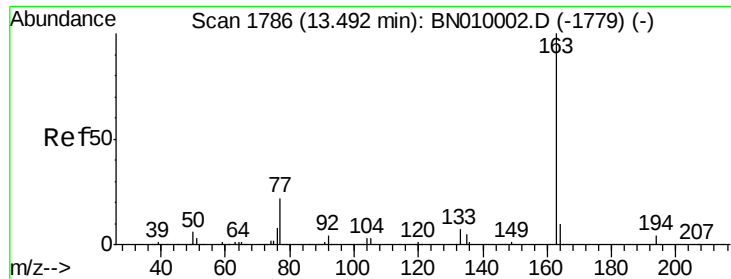





#45
Dimethylphthalate
Concen: 2.748 ng/ul
RT: 13.49 min Scan# 1786
Delta R.T. -0.00 min
Lab File: BN010014.D
Acq: 29 Feb 2020 08:43

Instrument :
BNA_N
ClientSampled :
DBD24

Tot Ion	Ratio	Lower	Upper
163	100		
194	3.9	3.4	5.0
164	9.3	8.0	12.0




Manual Integrations
APPROVED


mohammad
3/3/2020 5:00:02 PM

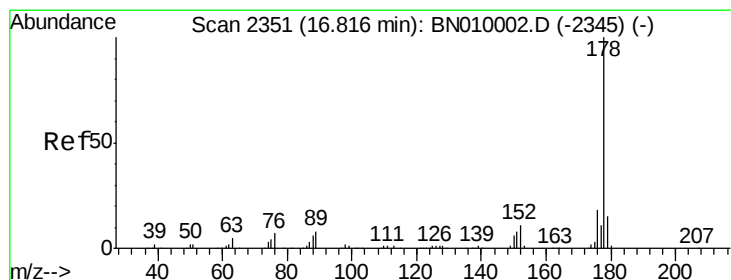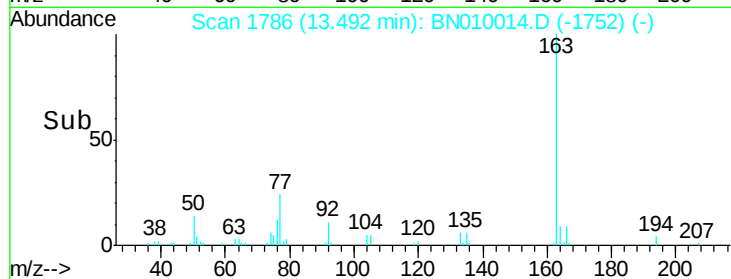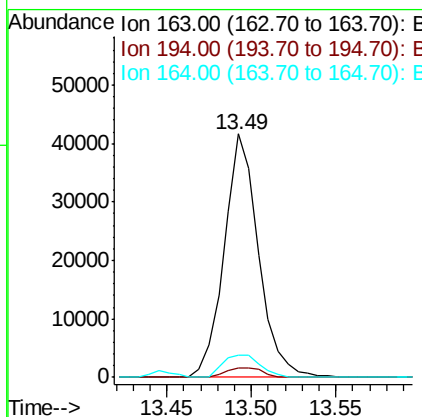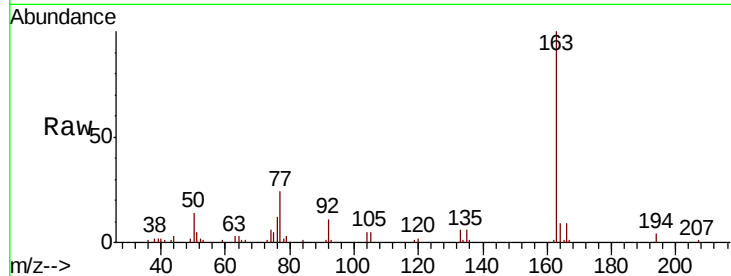

#70
Phenanthrene
Concen: 4.199 ng/ul
RT: 16.82 min Scan# 2352
Delta R.T. -0.00 min
Lab File: BN010014.D
Acq: 29 Feb 2020 08:43

Tgt Ion	Ratio	Lower	Upper
178	100		
179	16.7	12.5	18.7
176	19.1	14.6	22.0

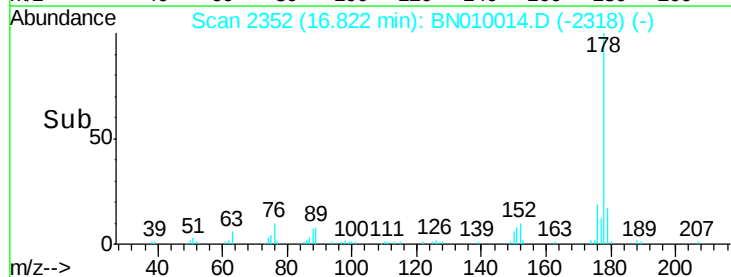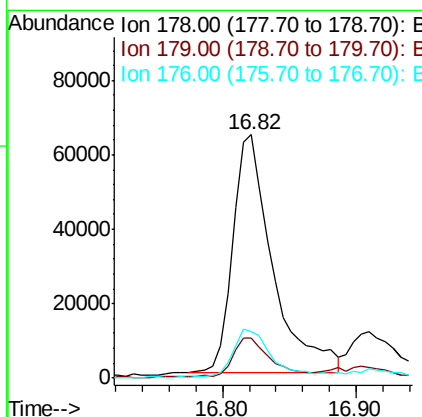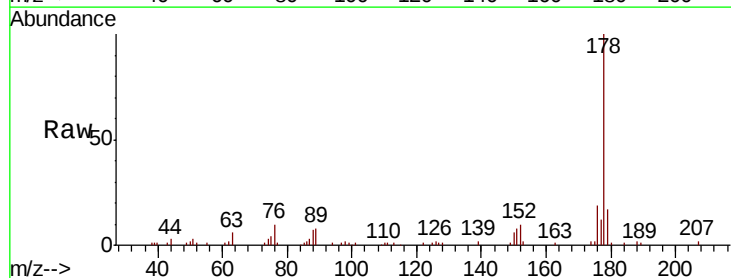

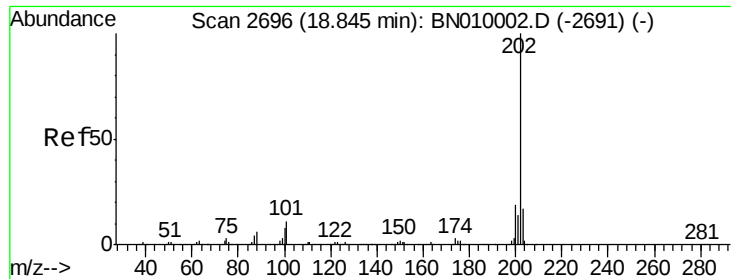

#77

Fluoranthene

Concen: 8.468 ng/ul

RT: 18.85 min Scan# 2697

Delta R.T. -0.00 min

Lab File: BN010014.D

Acq: 29 Feb 2020 08:43

Instrument :

BNA_N





ClientSampleId :

DBD24

Tot Ion:	202	Resp:	312979
Ion Ratio	Lower	Upper	
202	100		
101	11.2	9.4	14.2
100	9.2	7.2	10.8

Manual Integrations
APPROVED

mohammad
3/3/2020 5:00:02 PM

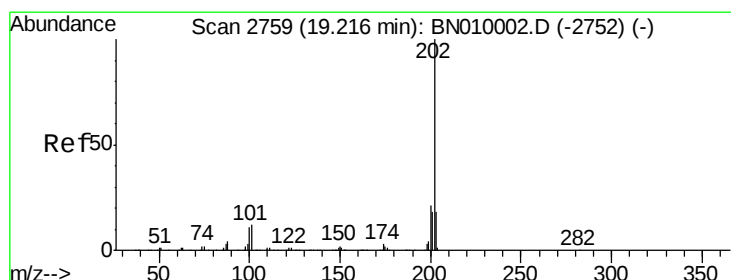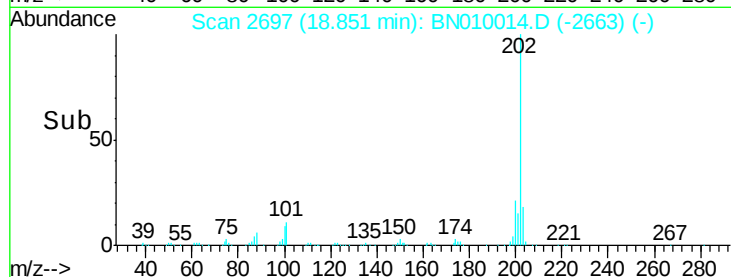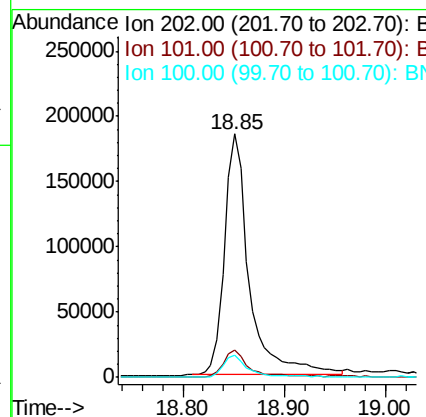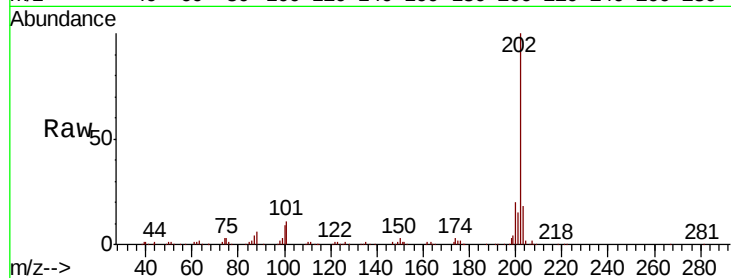

#80

Pyrene

Concen: 6.202 ng/ul




RT: 19.22 min Scan# 2759


Delta R.T. -0.00 min

Lab File: BN010014.D

Acq: 29 Feb 2020 08:43

Tgt Ion:	202	Resp:	215232
Ion Ratio	Lower	Upper	
202	100		
101	13.7	11.3	16.9
100	12.0	9.0	13.6

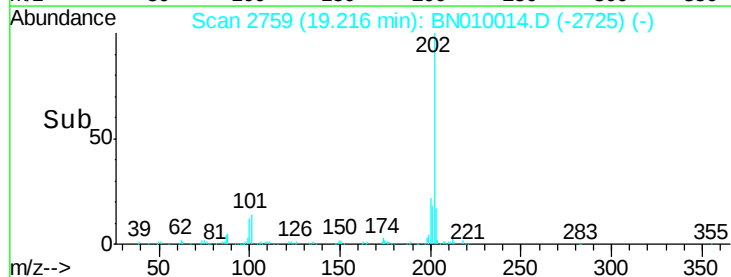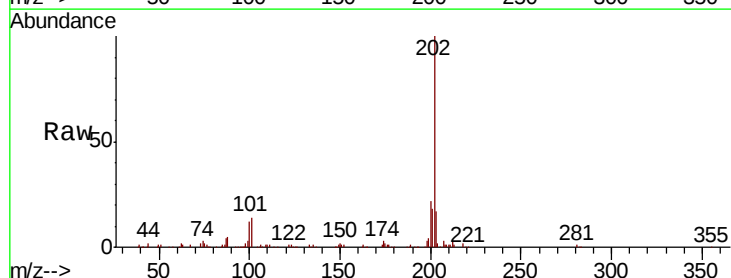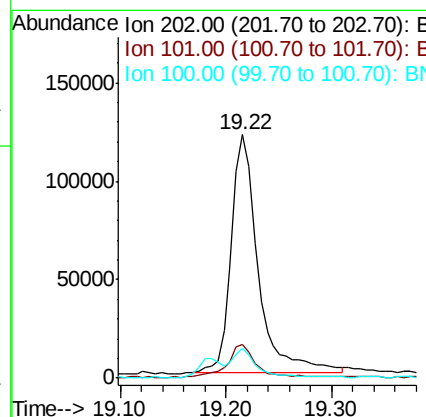

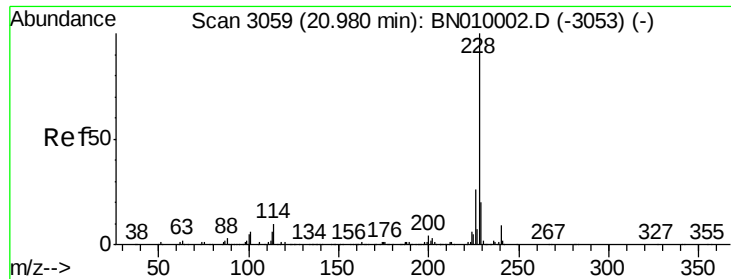





#83
Benzo(a)anthracene
Concen: 1.181 ng/ul m
RT: 20.99 min Scan# 3060
Delta R.T. -0.00 min
Lab File: BN010014.D
Acq: 29 Feb 2020 08:43

Instrument :
BNA_N
ClientSampleId :
DBD24

Tot Ion	Ratio	Lower	Upper
228	100		
229	23.1	15.0	22.4#
226	30.1	21.4	32.2

Manual Integrations
APPROVED

mohammad
3/3/2020 5:00:02 PM

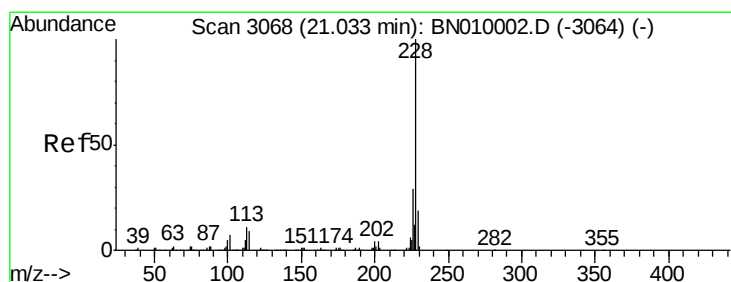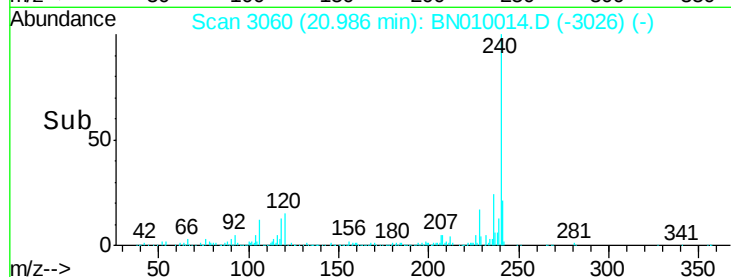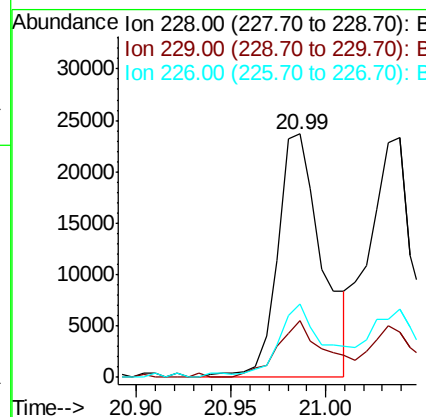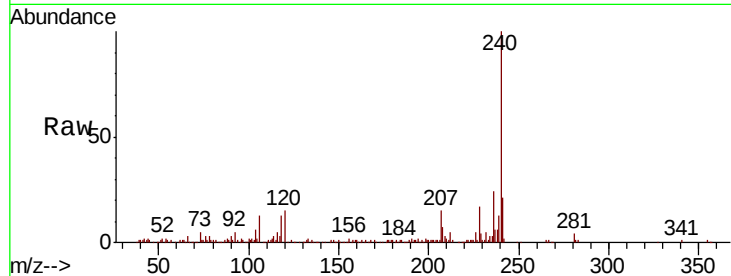

#85
Chrysene
Concen: 1.228 ng/ul
RT: 21.04 min Scan# 3069
Delta R.T. -0.00 min
Lab File: BN010014.D
Acq: 29 Feb 2020 08:43

Tgt Ion	Ratio	Lower	Upper
228	100		
226	28.3	23.4	35.2
229	18.9	15.0	22.4

