

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN022820\
 Data File : BN010020.D
 Acq On : 29 Feb 2020 12:26
 Operator : CG/JU
 Sample : L1507-14DL 10X
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleID :
 DBD12DL

Manual Integrations
 APPROVED

mohammad
 3/3/2020 5:00:08 PM

Quant Time: Mar 02 14:16:54 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Feb 29 01:38:10 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.37	152	88664	20.00	ng/ul	0.00
18) Naphthalene-d8	10.12	136	381720	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.02	164	230183	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.77	188	477967	20.00	ng/ul	0.00
78) Chrysene-d12	21.00	240	431463	20.00	ng/ul	0.00
86) Perylene-d12	23.10	264	466291	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.04	96	635	0.29	ng/uL	0.02
5) Phenol-d5	6.60	99	18461	2.45	ng/ul	0.02
7) Bis-(2-Chloroethyl)ether-d	6.74	67	13306	2.56	ng/ul	0.00
9) 2-Chlorophenol-d4	6.92	132	14985	2.64	ng/ul	0.00
13) 4-Methylphenol-d8	8.11	113	12727	2.12	ng/ul	0.02
19) Nitrobenzene-d5	8.53	128	6646	2.38	ng/ul	0.01
22) 2-Nitrophenol-d4	9.24	143	6540	2.14	ng/ul	0.01
26) 2,4-Dichlorophenol-d3	9.80	165	13812m	2.35	ng/ul	0.04
29) 4-Chloroaniline-d4	10.31	131	13801m	2.09	ng/ul	0.04
44) Dimethylphthalate-d6	13.45	166	51087	2.97	ng/ul	0.00
47) Acenaphthylene-d8	13.70	160	59698	2.95	ng/ul	0.00
52) 4-Nitrophenol-d4	14.35	143	3939m	1.25	ng/ul	0.09
58) Fluorene-d10	15.02	176	44811	3.02	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.20	200	2603m	0.88	ng/ul	0.02
71) Anthracene-d10	16.87	188	71401	3.26	ng/ul	0.00
79) Pyrene-d10	19.19	212	77312	3.43	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.96	264	78873	3.39	ng/ul	0.00

Target Compounds

					Ovalue	
28) Naphthalene	10.17	128	37508	1.822	ng/ul#	95
34) 2-Methylnaphthalene	11.80	142	25994	1.819	ng/ul	91
48) Acenaphthylene	13.73	152	42623	1.945	ng/ul	97
50) Acenaphthene	14.08	153	52412	3.488	ng/ul	96
54) Dibenzofuran	14.43	168	44349	2.103	ng/ul	97
59) Fluorene	15.08	166	43478	2.457	ng/ul	89
70) Phenanthrene	16.82	178	261780	9.597	ng/ul	97
72) Anthracene	16.91	178	195327	7.005	ng/ul	97
77) Fluoranthene	18.85	202	998965	31.265	ng/ul	98
80) Pyrene	19.22	202	1857618	59.718	ng/ul	98
83) Benzo(a)anthracene	20.98	228	331643	11.185	ng/ul	98
85) Chrysene	21.03	228	400678	13.726	ng/ul	98
88) Benzo(b)fluoranthene	22.49	252	436527	14.439	ng/ul	98
89) Benzo(k)fluoranthene	22.52	252	103856m	3.628	ng/ul	
91) Benzo(a)pyrene	23.01	252	159213	5.855	ng/ul	97
92) Indeno(1,2,3-cd)pyrene	25.13	276	100872	3.125	ng/ul	95
93) Dibenzo(a,h)anthracene	25.14	278	34866	1.262	ng/ul#	78
94) Benzo(g,h,i)perylene	25.76	276	104956	3.877	ng/ul#	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN022820\
Data File : BN010020.D
Acq On : 29 Feb 2020 12:26
Operator : CG/JU
Sample : L1507-14DL 10X
Misc :
ALS Vial : 40 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
DBD12DL

Manual Integrations
APPROVED

mohammad
3/3/2020 5:00:08 PM

Quant Time: Mar 02 14:16:54 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 29 01:38:10 2020
Response via : Initial Calibration

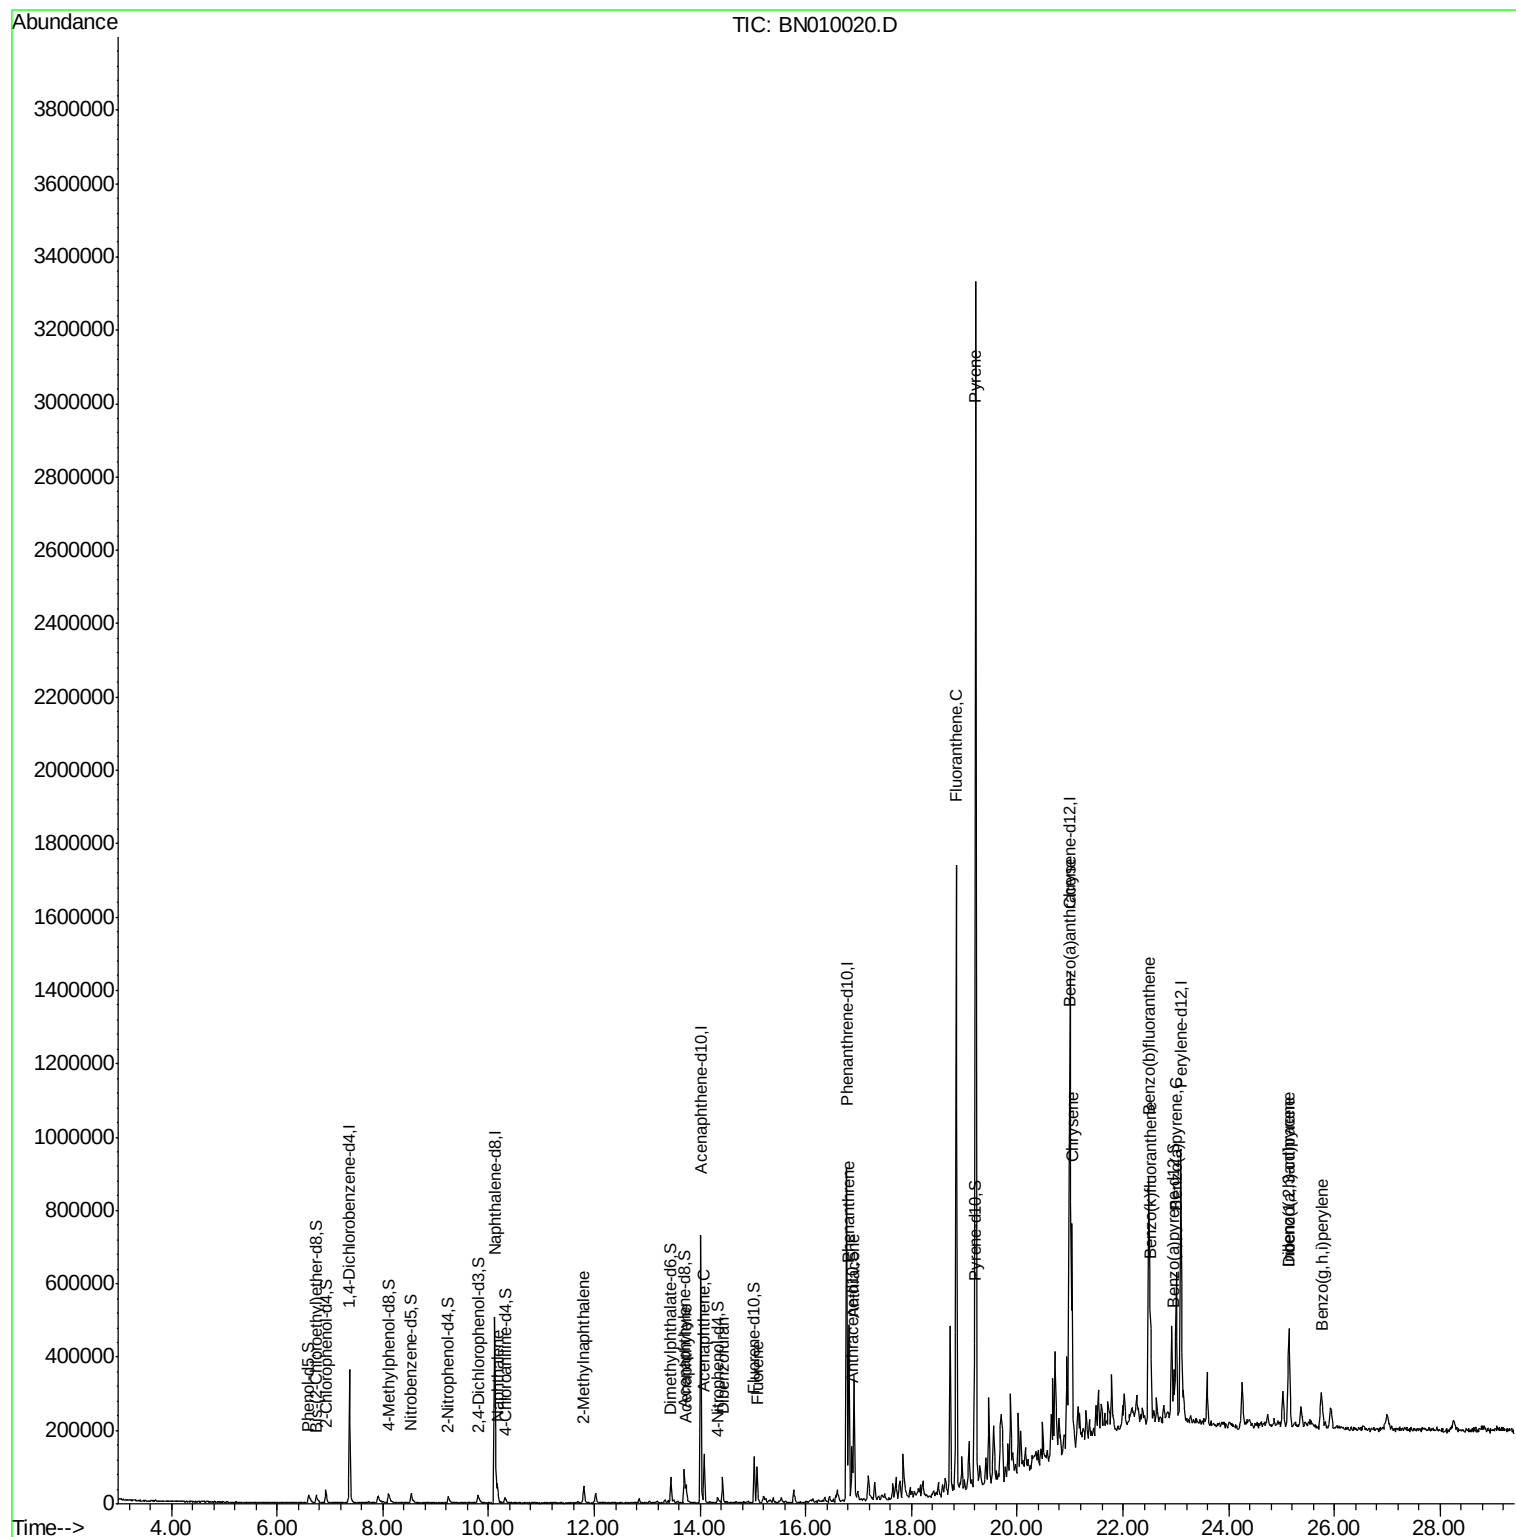

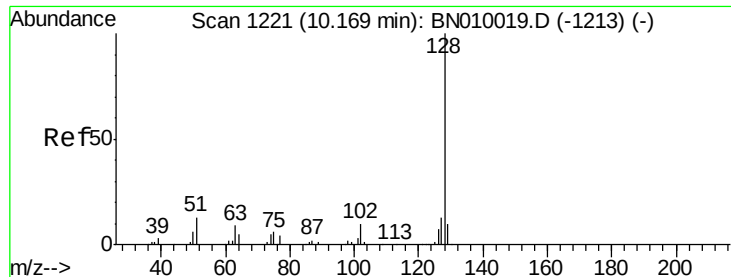





#28
Naphthalene
Concen: 1.822 ng/ul
RT: 10.17 min Scan# 1221
Delta R.T. -0.00 min
Lab File: BN010020.D
Acq: 29 Feb 2020 12:26

Instrument :
BNA_N
ClientSampled :
DBD12DL

Tot Ion	Ratio	Lower	Upper
128	100		
129	10.9	8.6	13.0
127	16.6	10.3	15.5




Manual Integrations
APPROVED


mohammad
3/3/2020 5:00:08 PM

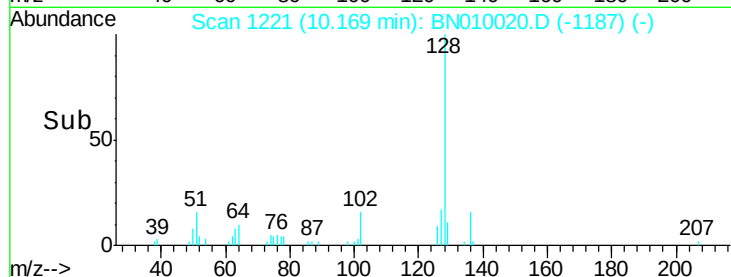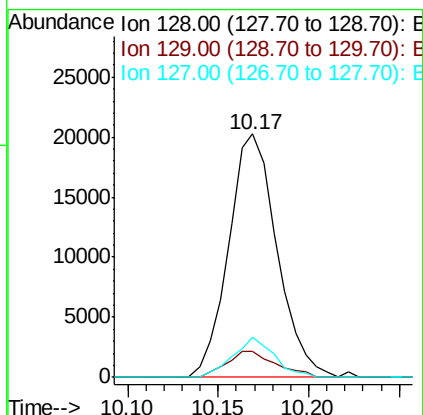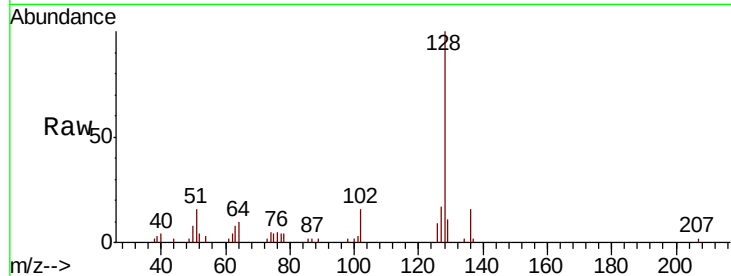

#34
2-Methylnaphthalene
Concen: 1.819 ng/ul
RT: 11.80 min Scan# 1499
Delta R.T. 0.01 min
Lab File: BN010020.D
Acq: 29 Feb 2020 12:26

Tgt Ion	Ratio	Lower	Upper
142	100		
141	81.5	72.1	108.1

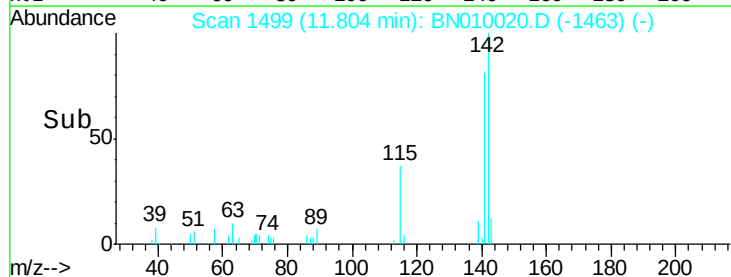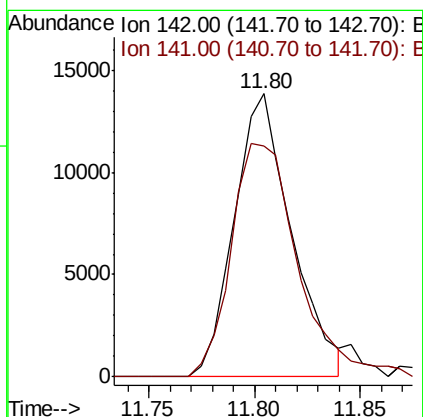



#48

Acenaphthylene

Concen: 1.945 ng/ul

RT: 13.73 min Scan# 1827

Delta R.T. -0.00 min

Lab File: BN010020.D

Acq: 29 Feb 2020 12:26

Instrument :

BNA_N





ClientSampleId :

DBD12DL

Tot Ion:	152	Resp:	42623
Ion Ratio	Lower	Upper	
152	100		
151	20.4	15.7	23.5
153	14.3	10.3	15.5

Manual Integrations
APPROVED

mohammad
3/3/2020 5:00:08 PM

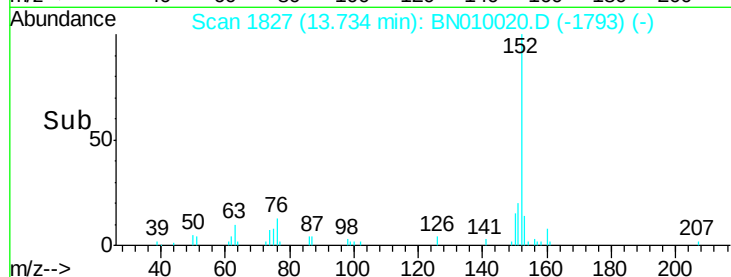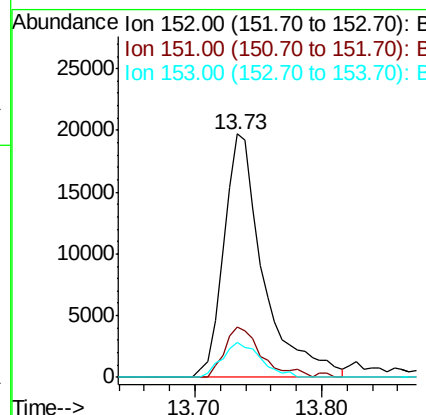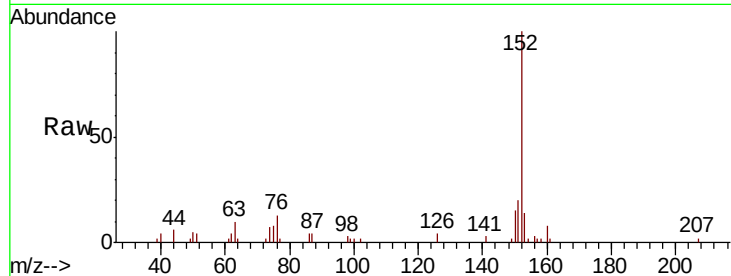

#50

Acenaphthene

Concen: 3.488 ng/ul




RT: 14.08 min Scan# 1886


Delta R.T. -0.00 min

Lab File: BN010020.D

Acq: 29 Feb 2020 12:26

Tgt Ion:	153	Resp:	52412
Ion Ratio	Lower	Upper	
153	100		
152	49.6	36.6	54.8
154	90.9	70.6	106.0

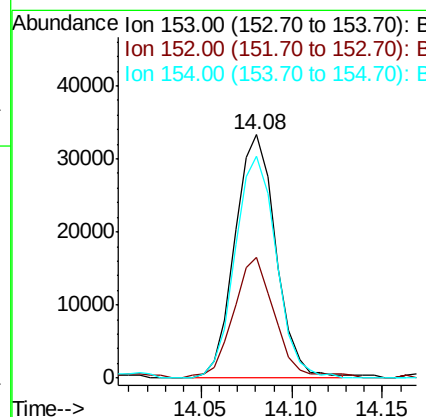



#54

Dibenzofuran

Concen: 2.103 ng/ul

RT: 14.43 min Scan# 1945

Delta R.T. 0.01 min

Lab File: BN010020.D

Acq: 29 Feb 2020 12:26

Instrument :

BNA_N

ClientSampleId :

DBD12DL

Tot Ion:168 Resp: 44349

Ion Ratio Lower Upper


168 100

139 39.0 32.7 49.1

Manual Integrations
APPROVED




mohammad

3/3/2020 5:00:08 PM



Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

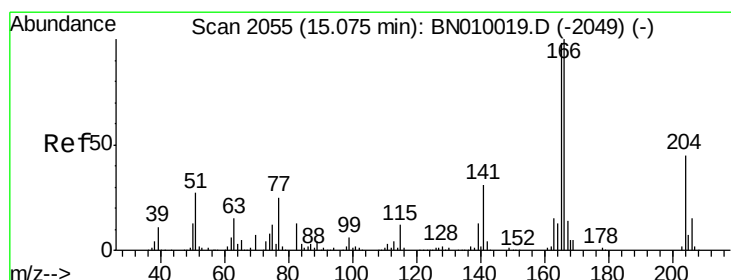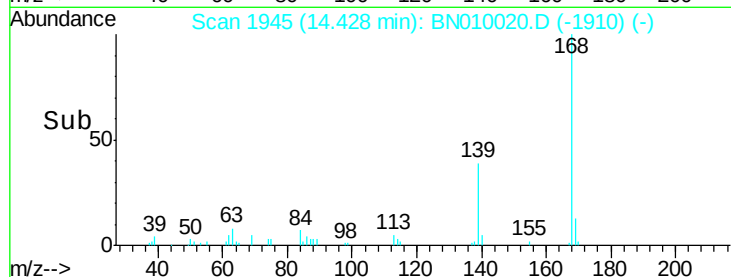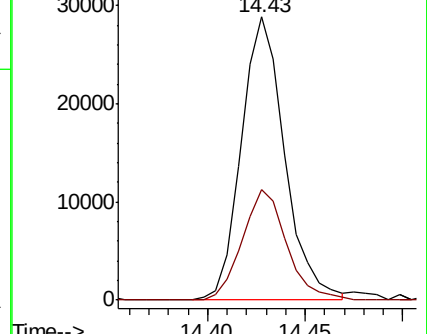

#59

Fluorene

Concen: 2.457 ng/ul

RT: 15.08 min Scan# 2056

Delta R.T. 0.01 min

Lab File: BN010020.D

Acq: 29 Feb 2020 12:26


Tgt Ion:166 Resp: 43478

Ion Ratio Lower Upper

166 100

165 88.6 79.8 119.8



167 15.7 10.7 16.1

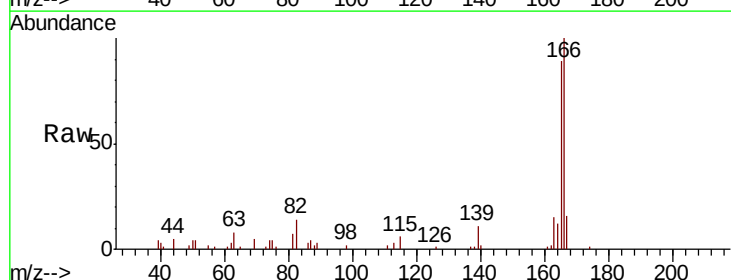


Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

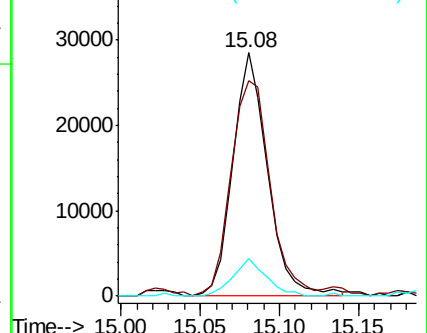

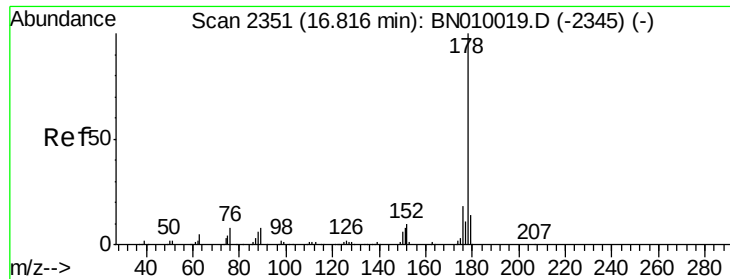





#70
Phenanthrene
Concen: 9.597 ng/ul
RT: 16.82 min Scan# 2351
Delta R.T. -0.01 min
Lab File: BN010020.D
Acq: 29 Feb 2020 12:26

Instrument :
BNA_N
ClientSampleId :
DBD12DL

Tot Ion	Ratio	Lower	Upper
178	100		
179	14.4	12.5	18.7
176	19.8	14.6	22.0




Manual Integrations
APPROVED


mohammad
3/3/2020 5:00:08 PM

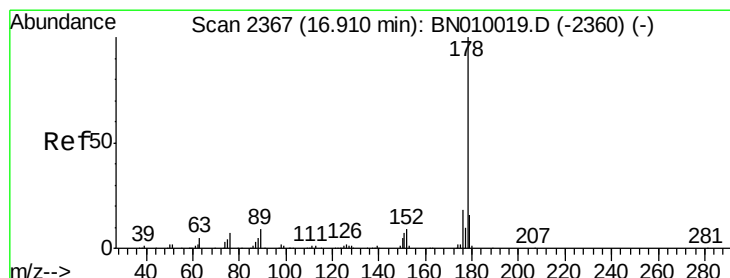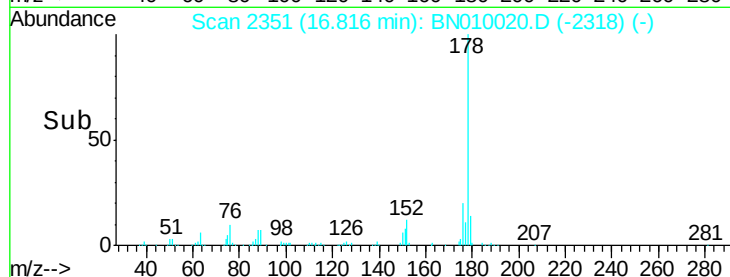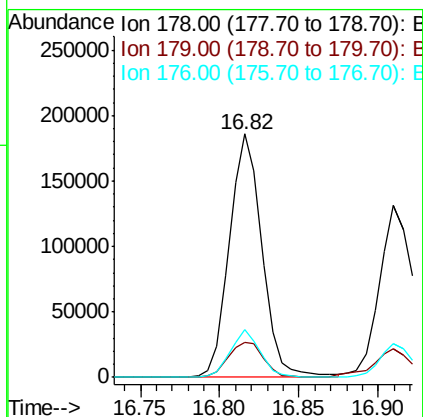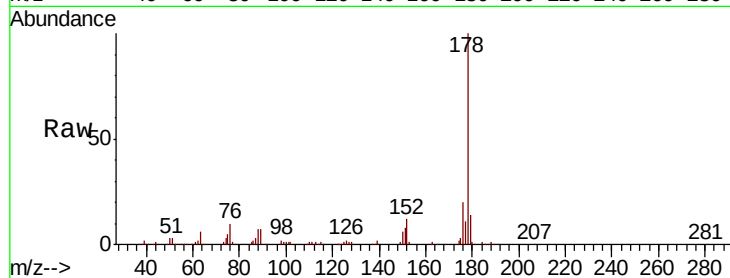

#72
Anthracene
Concen: 7.005 ng/ul
RT: 16.91 min Scan# 2367
Delta R.T. -0.00 min
Lab File: BN010020.D
Acq: 29 Feb 2020 12:26

Tgt Ion	Ratio	Lower	Upper
178	100		
179	16.5	12.2	18.2
176	19.3	14.6	21.8

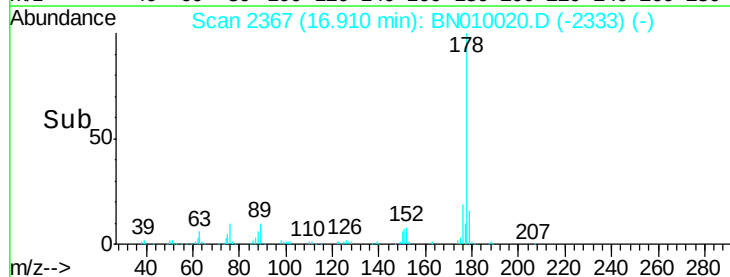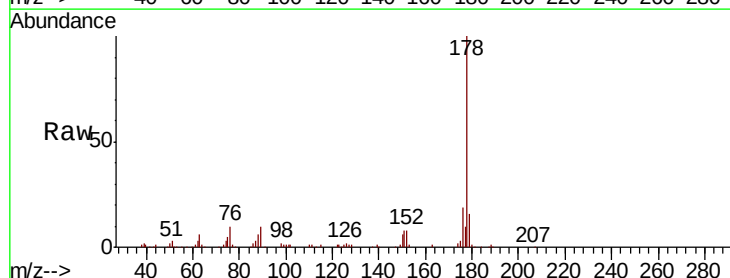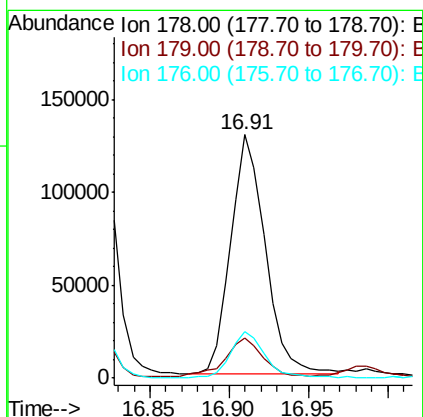







#77
Fluoranthene
Concen: 31.265 ng/ul
RT: 18.85 min Scan# 2697
Delta R.T. -0.00 min
Lab File: BN010020.D
Acq: 29 Feb 2020 12:26

Instrument :
BNA_N
ClientSampleId :
DBD12DL

Tot Ion	Ratio	Resp Lower	Upper
202	100		
101	10.9	9.4	14.2
100	8.4	7.2	10.8




Manual Integrations
APPROVED


mohammad
3/3/2020 5:00:08 PM

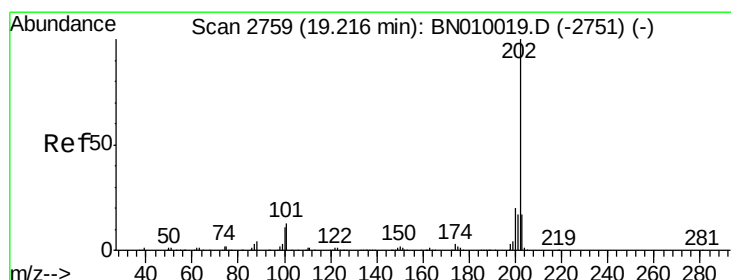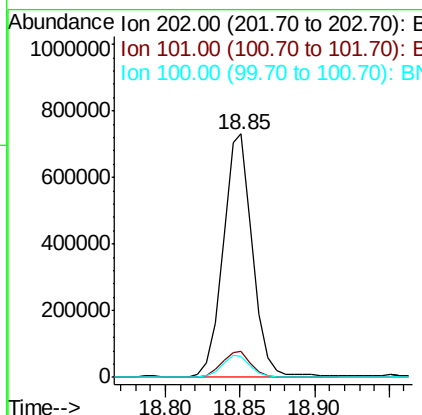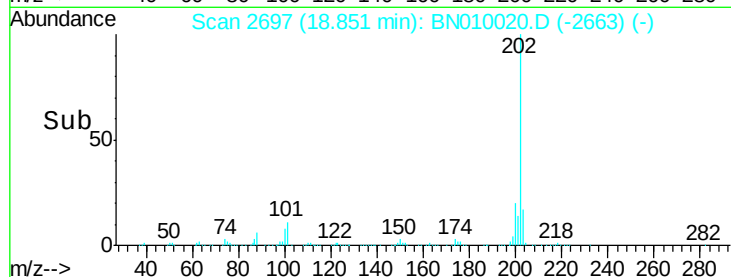

#80
Pyrene
Concen: 59.718 ng/ul
RT: 19.22 min Scan# 2759
Delta R.T. -0.00 min
Lab File: BN010020.D
Acq: 29 Feb 2020 12:26

Tgt Ion	Ratio	Resp Lower	Upper
202	100		
101	12.8	11.3	16.9
100	10.9	9.0	13.6

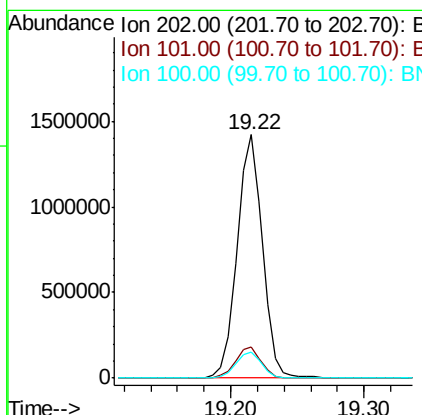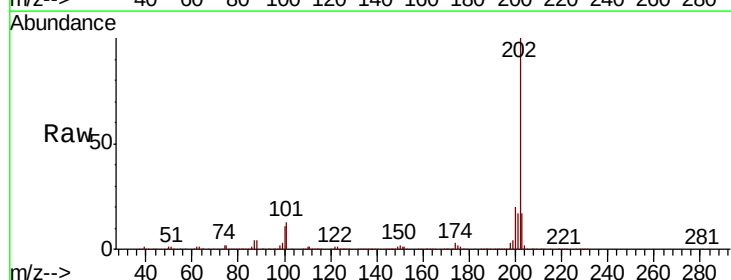







#83
Benzo(a)anthracene
Concen: 11.185 ng/ul
RT: 20.98 min Scan# 3059
Delta R.T. -0.01 min
Lab File: BN010020.D
Acq: 29 Feb 2020 12:26

Instrument :
BNA_N
ClientSampleId :
DBD12DL

Tot Ion	Ratio	Lower	Upper
228	100		
229	20.6	15.0	22.4
226	26.7	21.4	32.2




Manual Integrations
APPROVED


mohammad
3/3/2020 5:00:08 PM

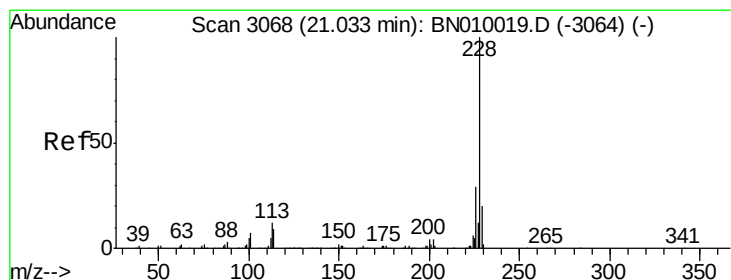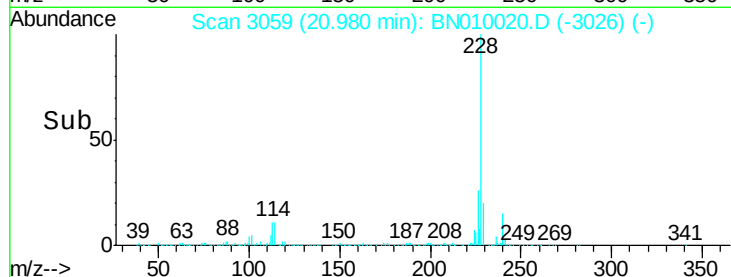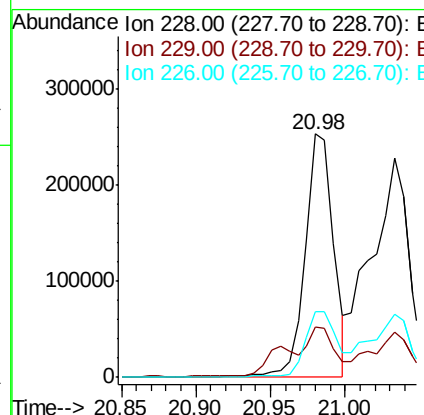

#85
Chrysene
Concen: 13.726 ng/ul
RT: 21.03 min Scan# 3068
Delta R.T. -0.01 min
Lab File: BN010020.D
Acq: 29 Feb 2020 12:26

Tgt Ion	Ratio	Lower	Upper
228	100		
226	28.9	23.4	35.2
229	20.8	15.0	22.4

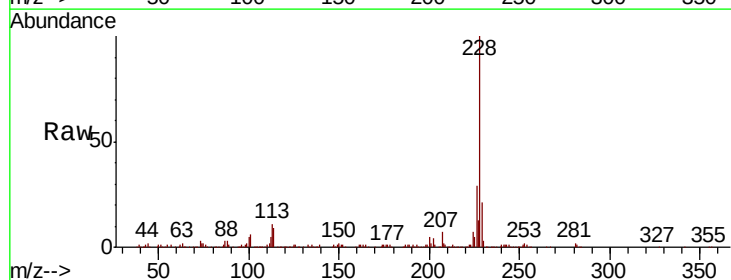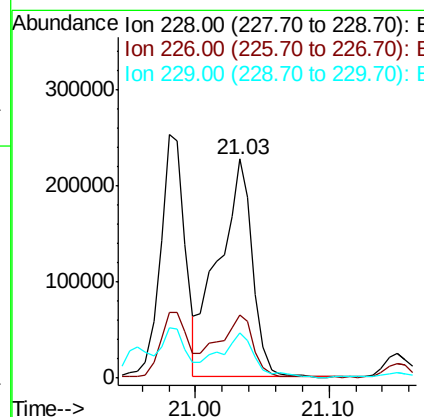







#88
Benzo(b)fluoranthene
Concen: 14.439 ng/ul
RT: 22.49 min Scan# 3315
Delta R.T. -0.00 min
Lab File: BN010020.D
Acq: 29 Feb 2020 12:26

Instrument :
BNA_N
ClientSampled :
DBD12DL

Tot Ion	Ratio	Lower	Upper
252	100		
253	22.4	17.0	25.4
125	10.8	8.0	12.0




Manual Integrations
APPROVED


mohammad
3/3/2020 5:00:08 PM

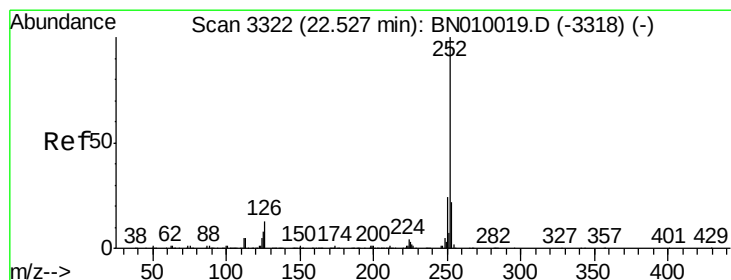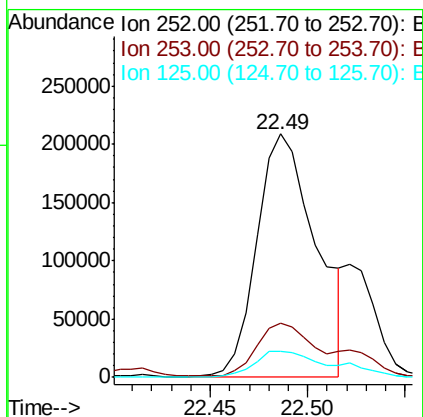

#89
Benzo(k)fluoranthene
Concen: 3.628 ng/ul m
RT: 22.52 min Scan# 3321
Delta R.T. -0.01 min
Lab File: BN010020.D
Acq: 29 Feb 2020 12:26

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.9	18.0	27.0
125	12.9	8.2	12.2#

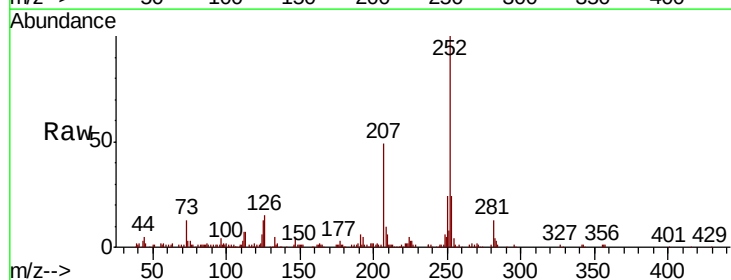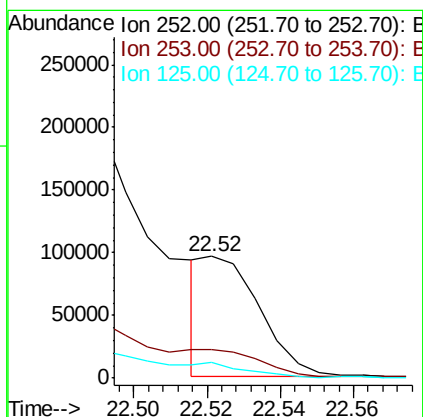



#91

Benzo(a)pyrene

Concen: 5.855 ng/ul

RT: 23.01 min Scan# 3404

Delta R.T. -0.00 min

Lab File: BN010020.D

Acq: 29 Feb 2020 12:26

Instrument :

BNA_N


ClientSampleId :

DBD12DL




Tot Ion:	252	Resp:	159213
Ion Ratio	Lower	Upper	
252	100		
253	20.8	17.4	26.0
125	10.0	9.0	13.6

Manual Integrations
APPROVED

mohammad
3/3/2020 5:00:08 PM

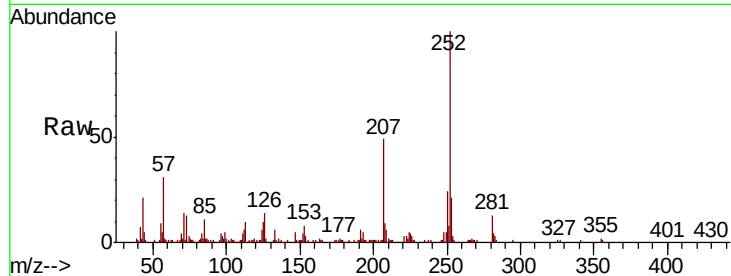

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

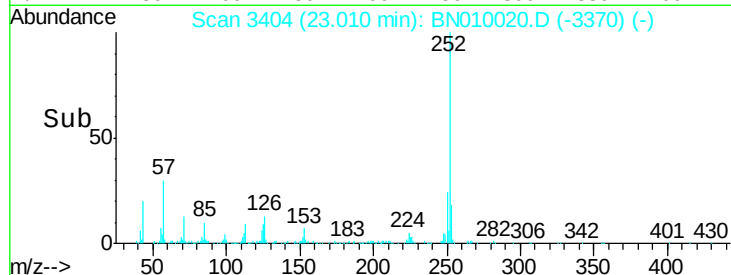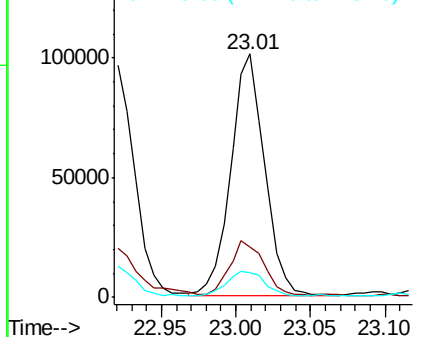

#92

Indeno(1,2,3-cd)pyrene

Concen: 3.125 ng/ul

RT: 25.13 min Scan# 3765




Delta R.T. -0.01 min


Lab File: BN010020.D

Acq: 29 Feb 2020 12:26

Tgt Ion:	276	Resp:	100872
Ion Ratio	Lower	Upper	
276	100		
138	22.2	20.9	31.3
277	23.4	18.2	27.4

Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 277.00 (276.70 to 277.70): E

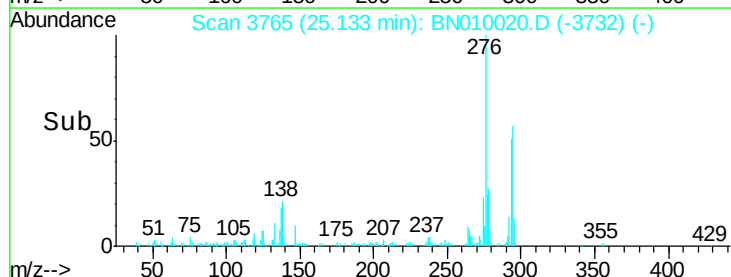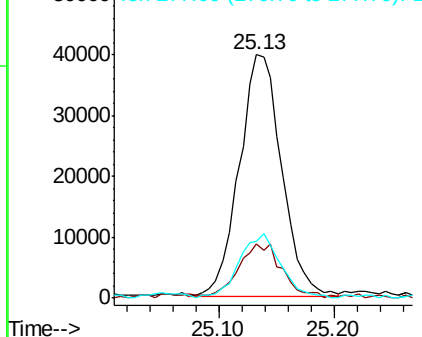







#93
Dibenzo(a,h)anthracene
Concen: 1.262 ng/ul
RT: 25.14 min Scan# 3766
Delta R.T. -0.01 min
Lab File: BN010020.D
Acq: 29 Feb 2020 12:26

Instrument :
BNA_N
ClientSampleId :
DBD12DL

Tot Ion	Ratio	Lower	Upper
278	100		
139	23.0	13.0	19.4#
279	34.4	17.5	26.3#

Manual Integrations
APPROVED

mohammad
3/3/2020 5:00:08 PM

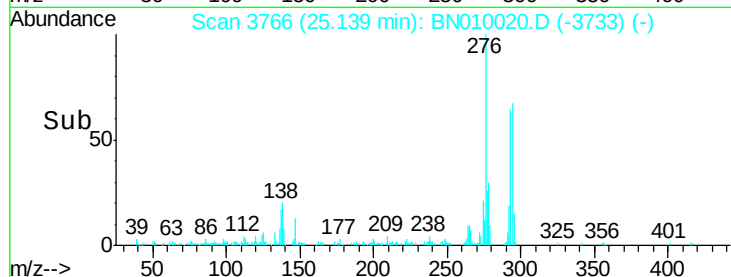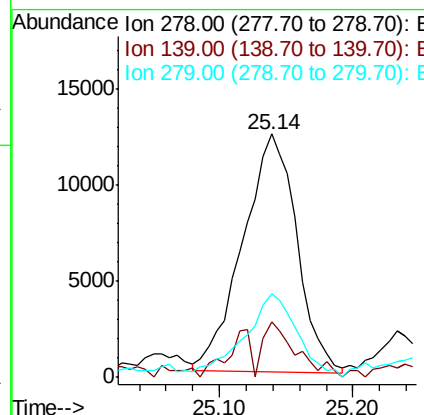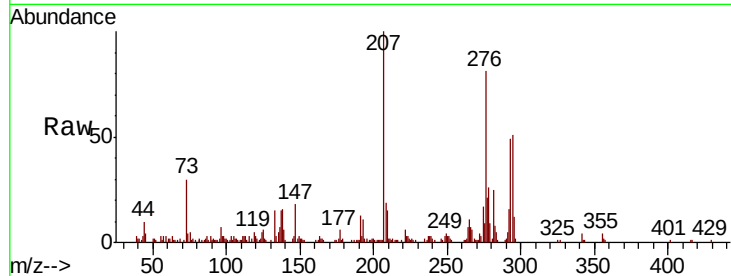

#94
Benzo(g,h,i)perylene
Concen: 3.877 ng/ul
RT: 25.76 min Scan# 3871
Delta R.T. -0.00 min
Lab File: BN010020.D
Acq: 29 Feb 2020 12:26

Tgt Ion	Ratio	Lower	Upper
276	100		
138	28.8	17.5	26.3#
277	25.9	18.1	27.1

