

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN022820\
 Data File : BN010025.D
 Acq On : 29 Feb 2020 15:25
 Operator : CG/JU
 Sample : L1615-02MS
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBDM7MS

Manual Integrations
 APPROVED

mohammad
 3/3/2020 5:00:21 PM

Quant Time: Mar 02 06:49:24 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Feb 29 01:38:10 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.37	152	101564	20.00	ng/ul	0.00
18) Naphthalene-d8	10.12	136	434050	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.02	164	270783	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.77	188	552491	20.00	ng/ul	0.00
78) Chrysene-d12	21.00	240	484522	20.00	ng/ul	0.00
86) Perylene-d12	23.10	264	493393	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.03	96	2755	1.12	ng/uL	0.01
5) Phenol-d5	6.59	99	63559	7.36	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.74	67	45871	7.69	ng/ul	0.00
9) 2-Chlorophenol-d4	6.92	132	51743	7.96	ng/ul	0.00
13) 4-Methylphenol-d8	8.10	113	46900	6.82	ng/ul	0.00
19) Nitrobenzene-d5	8.52	128	23715	7.47	ng/ul	0.00
22) 2-Nitrophenol-d4	9.24	143	25436	7.32	ng/ul	0.01
26) 2,4-Dichlorophenol-d3	9.78	165	47981	7.18	ng/ul	0.02
29) 4-Chloroaniline-d4	10.30	131	53752	7.16	ng/ul	0.02
44) Dimethylphthalate-d6	13.45	166	163186	8.07	ng/ul	0.00
47) Acenaphthylene-d8	13.70	160	185526	7.79	ng/ul	0.00
52) 4-Nitrophenol-d4	14.30	143	19117m	5.18	ng/ul	0.04
58) Fluorene-d10	15.02	176	142217	8.14	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.20	200	10317	3.01	ng/ul	0.02
71) Anthracene-d10	16.87	188	214703	8.48	ng/ul	0.00
79) Pyrene-d10	19.19	212	266552	10.53	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.96	264	258168	10.48	ng/ul	0.00

Target Compounds

					Ovalue
6) Phenol	6.61	94	69751	7.535	ng/ul 96
10) 2-Chlorophenol	6.95	128	52545	7.670	ng/ul 90
15) N-Nitroso-di-n-propylamine	8.18	70	44255	7.564	ng/ul 96
33) 4-Chloro-3-methylphenol	11.45	107	52829	6.857	ng/ul 94
50) Acenaphthene	14.08	153	167053	9.451	ng/ul 98
53) 4-Nitrophenol	14.30	109	18484m	5.545	ng/ul
54) Dibenzofuran	14.43	168	44295	1.785	ng/ul 94
55) 2,4-Dinitrotoluene	14.44	165	40061	6.542	ng/ul# 81
59) Fluorene	15.08	166	48220	2.316	ng/ul 97
69) Pentachlorophenol	16.45	266	15224	4.306	ng/ul 94
70) Phenanthrene	16.82	178	286516	9.087	ng/ul 100
72) Anthracene	16.91	178	73445	2.279	ng/ul 99
77) Fluoranthene	18.85	202	200393	5.426	ng/ul 96
80) Pyrene	19.22	202	455815	13.049	ng/ul 98
83) Benzo(a)anthracene	20.99	228	37895	1.138	ng/ul 98
85) Chrysene	21.03	228	38167	1.164	ng/ul 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN022820\
Data File : BN010025.D
Acq On : 29 Feb 2020 15:25
Operator : CG/JU
Sample : L1615-02MS
Misc :
ALS Vial : 45 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
DBDM7MS

Quant Time: Mar 02 06:49:24 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 29 01:38:10 2020
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
3/3/2020 5:00:21 PM

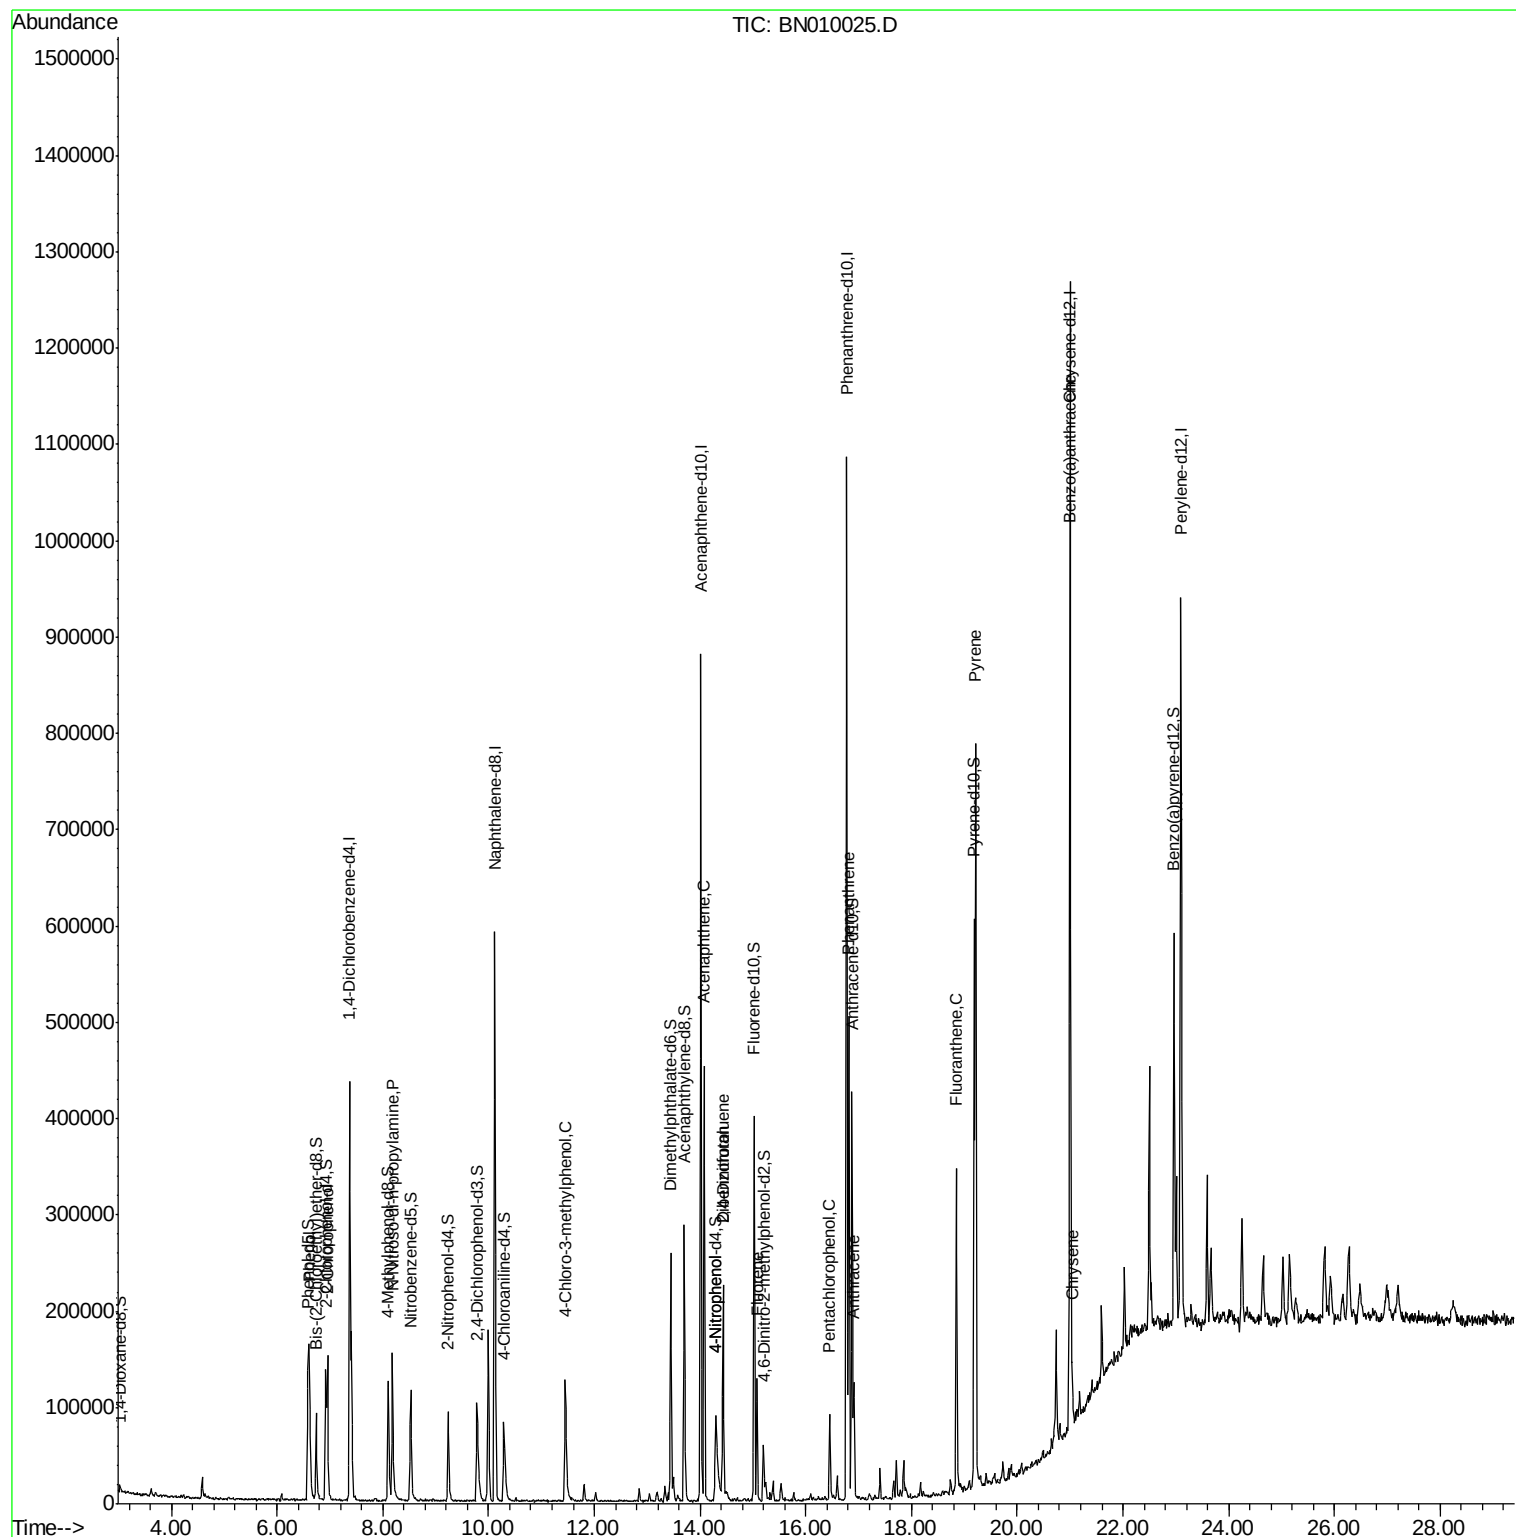

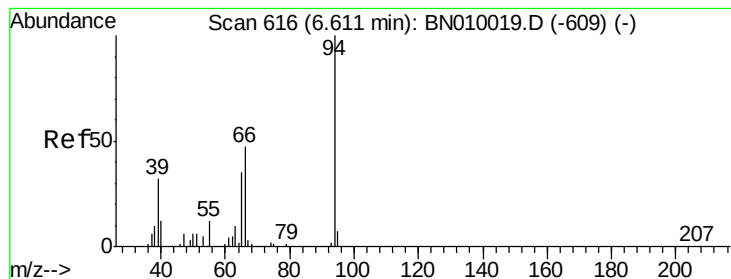

#6

Phenol

Concen: 7.535 ng/ul

RT: 6.61 min Scan# 616

Delta R.T. 0.01 min

Lab File: BN010025.D

Acq: 29 Feb 2020 15:25

Tot Ion:	94	Resp:	69751
Ion	Ratio	Lower	Upper
94	100		
65	37.7	27.6	41.4
66	50.2	38.5	57.7

Instrument :





BNA_N

ClientSampleId :

DBDM7MS

Manual Integrations
APPROVED

mohammad
3/3/2020 5:00:21 PM

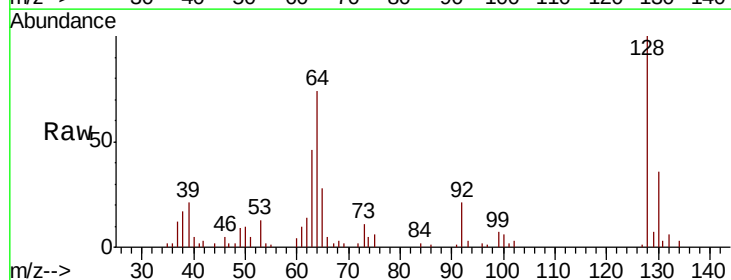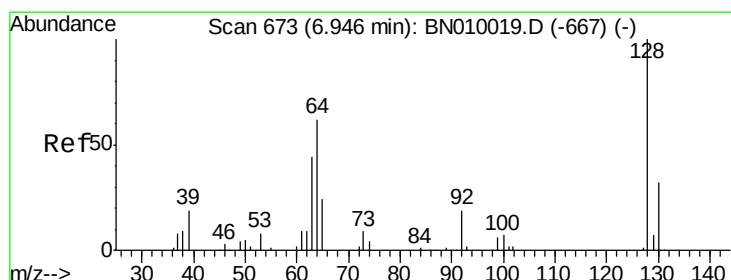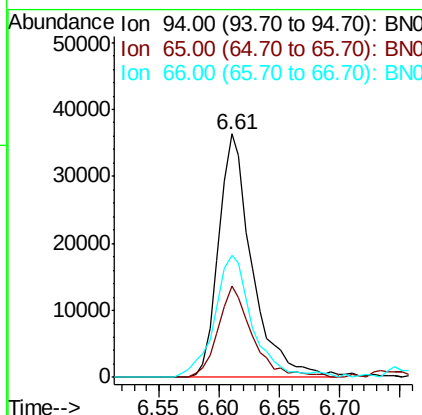

#10

2-Chlorophenol

Concen: 7.670 ng/ul


RT: 6.95 min Scan# 674




Delta R.T. -0.00 min

Lab File: BN010025.D

Acq: 29 Feb 2020 15:25

Tgt Ion:	128	Resp:	52545
Ion	Ratio	Lower	Upper
128	100		
64	73.7	52.5	78.7
130	36.2	24.4	36.6

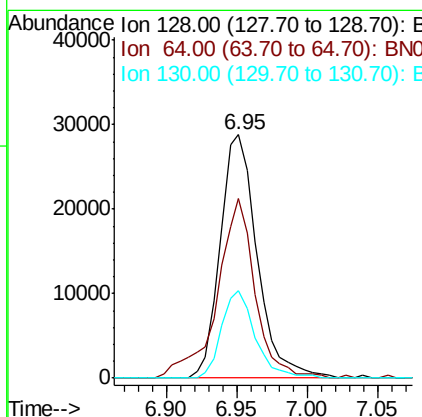

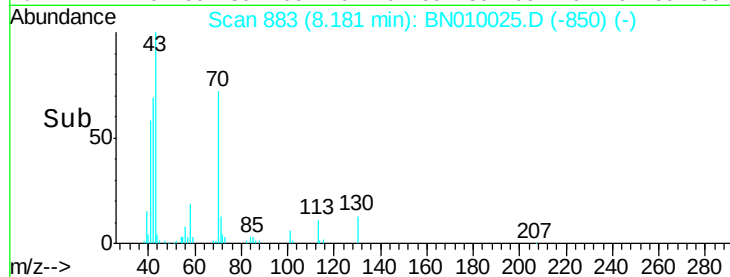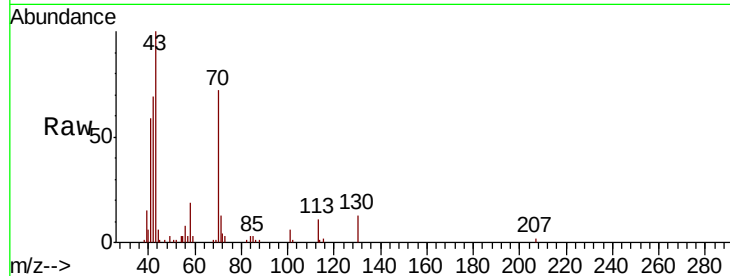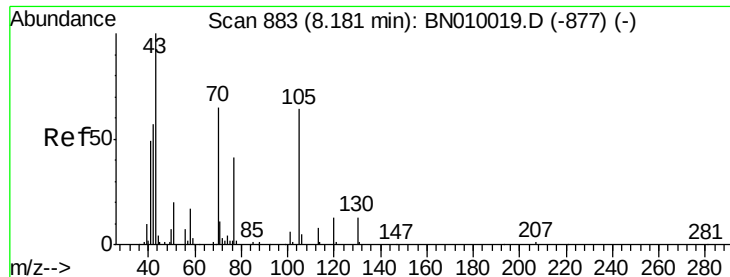

#15

N-Nitroso-di-n-propylamine

Concen: 7.564 ng/ul

RT: 8.18 min Scan# 883

Delta R.T. -0.01 min

Lab File: BN010025.D

Acq: 29 Feb 2020 15:25

Instrument :

BNA_N





ClientSampleId :

DBDM7MS

Tot Ion	Ion	Ratio	Lower	Upper
70	100			
42	95.3	72.6	108.8	
101	8.4	7.7	11.5	
130	18.4	14.7	22.1	

Manual Integrations
APPROVED

mohammad
3/3/2020 5:00:21 PM

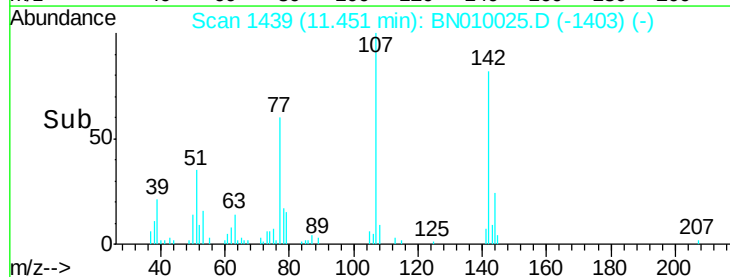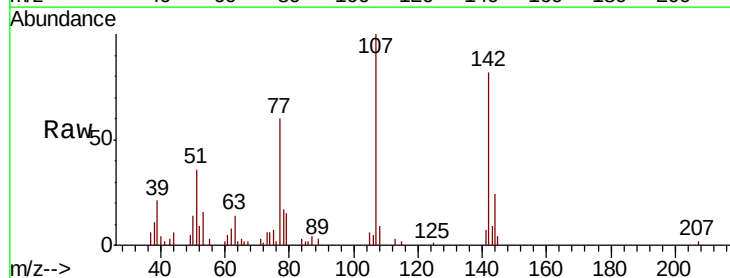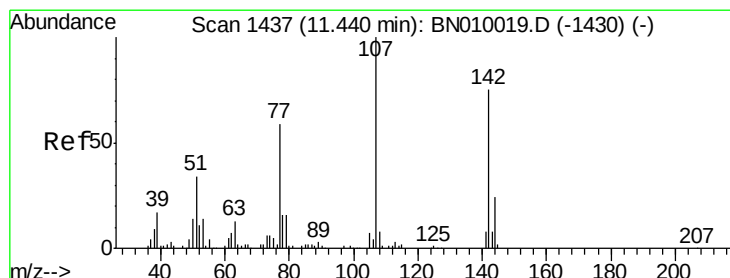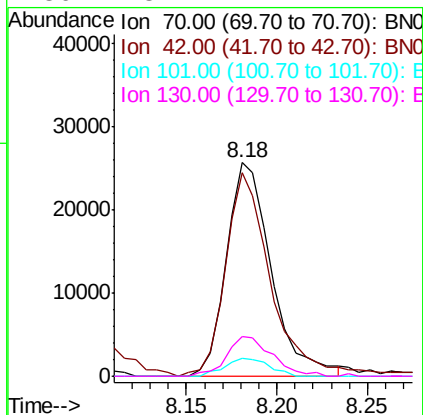

#33

4-Chloro-3-methylphenol

Concen: 6.857 ng/ul


RT: 11.45 min Scan# 1439


Delta R.T. 0.01 min

Lab File: BN010025.D

Acq: 29 Feb 2020 15:25

Tgt Ion	Ion	Ratio	Lower	Upper
107	100			
144	23.8	19.3	28.9	
142	81.5	59.5	89.3	

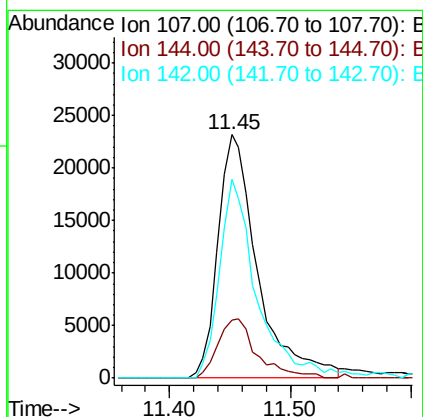

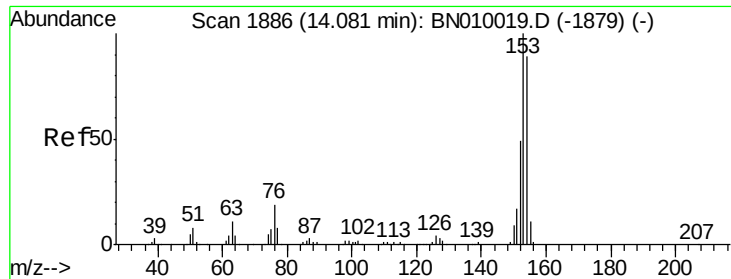

#50

Acenaphthene

Concen: 9.451 ng/ul

RT: 14.08 min Scan# 1886

Delta R.T. -0.00 min

Lab File: BN010025.D

Acq: 29 Feb 2020 15:25

Instrument :

BNA_N





ClientSampleId :

DBDM7MS

Tot Ion:	153	Resp:	167053
Ion Ratio	Lower	Upper	
153	100		
152	49.7	36.6	54.8
154	88.2	70.6	106.0

Manual Integrations
APPROVED

mohammad
3/3/2020 5:00:21 PM

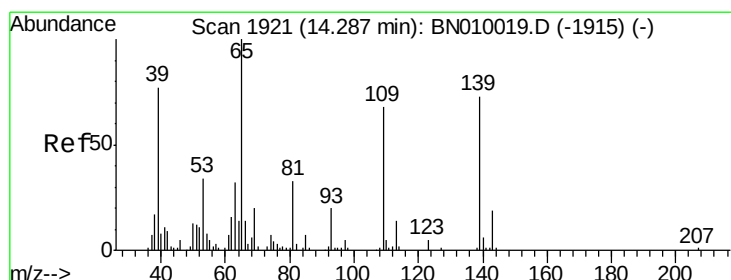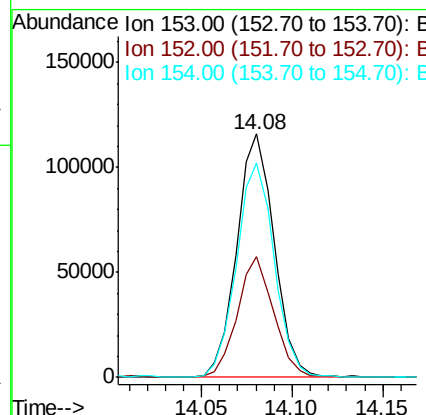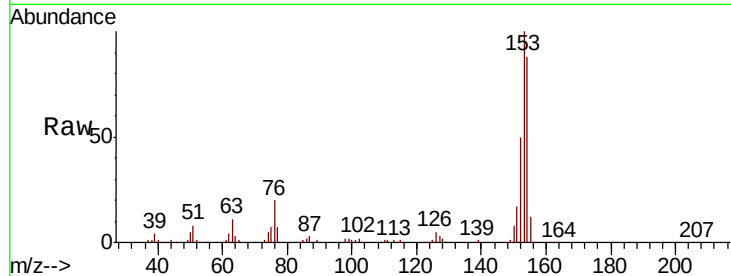

#53

4-Nitrophenol

Concen: 5.545 ng/ul m




RT: 14.30 min Scan# 1924


Delta R.T. 0.02 min

Lab File: BN010025.D

Acq: 29 Feb 2020 15:25

Tgt Ion:	109	Resp:	18484
Ion Ratio	Lower	Upper	
109	100		
139	101.2	96.3	144.5
65	132.5	129.9	194.9

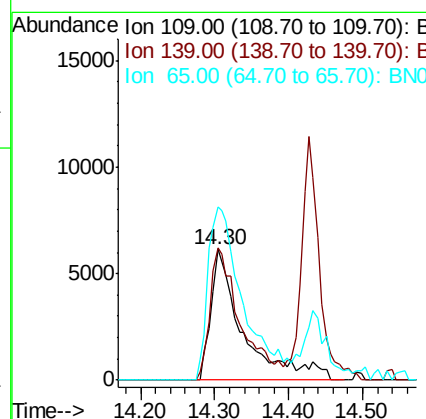

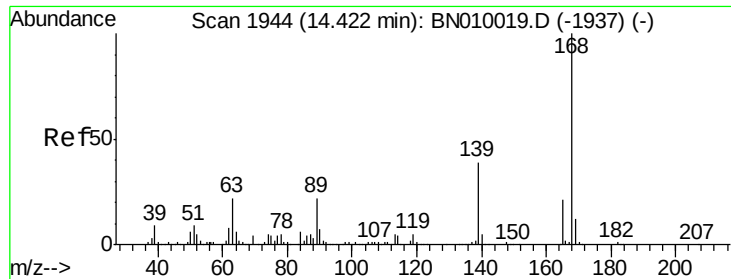

#54

Dibenzofuran

Concen: 1.785 ng/ul

RT: 14.43 min Scan# 1945

Delta R.T. 0.01 min

Lab File: BN010025.D

Acq: 29 Feb 2020 15:25

Instrument :

BNA_N

ClientSampled :

DBDM7MS

Tot Ion:168 Resp: 44295

Ion Ratio Lower Upper


168 100

139 37.0 32.7 49.1

Manual Integrations
APPROVED




mohammad

3/3/2020 5:00:21 PM



Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

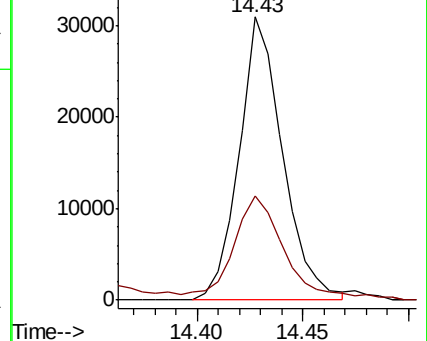

#55

2,4-Dinitrotoluene

Concen: 6.542 ng/ul

RT: 14.44 min Scan# 1947

Delta R.T. 0.01 min

Lab File: BN010025.D

Acq: 29 Feb 2020 15:25


Tgt Ion:165 Resp: 40061

Ion Ratio Lower Upper

165 100

63 67.4 68.3 102.5#



182 3.6 2.2 3.4#




Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BN0

Ion 182.00 (181.70 to 182.70): E

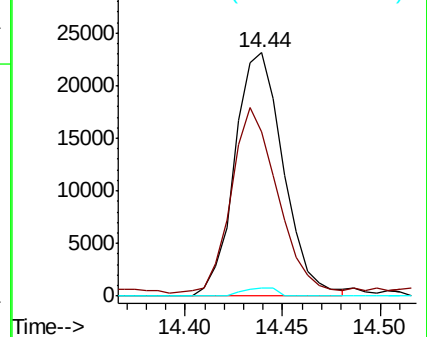

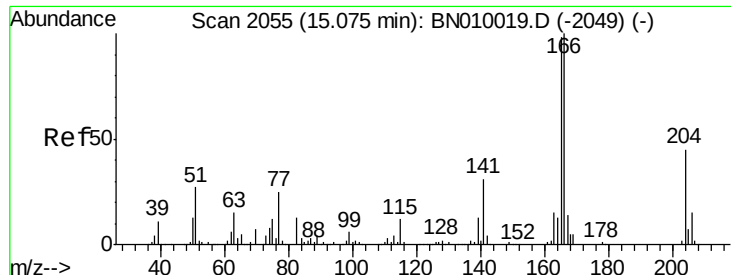

#59

Fluorene

Concen: 2.316 ng/ul

RT: 15.08 min Scan# 2056

Delta R.T. 0.01 min

Lab File: BN010025.D

Acq: 29 Feb 2020 15:25

Instrument :

BNA_N

ClientSampleId :

DBDM7MS

Tot Ion:166 Resp: 48220

Ion Ratio Lower Upper

166 100

165 102.9 79.8 119.8


167 15.3 10.7 16.1

Manual Integrations

APPROVED

mohammad




3/3/2020 5:00:21 PM

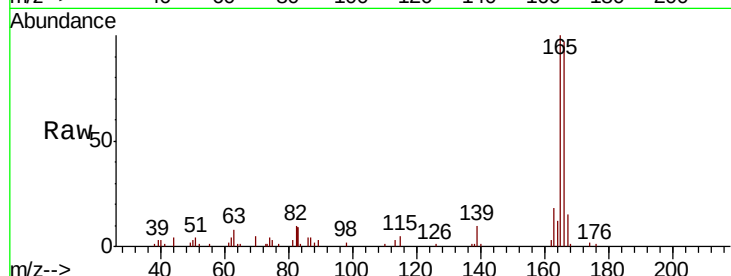

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

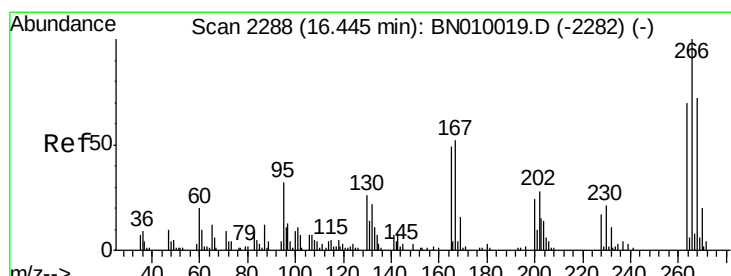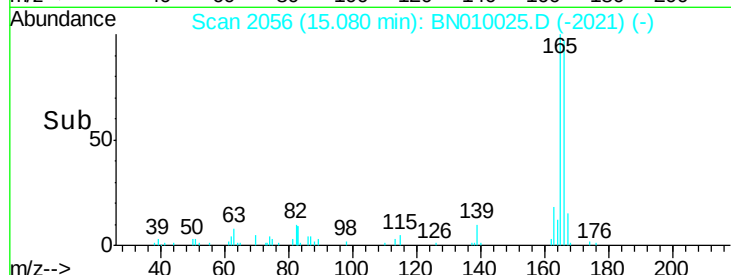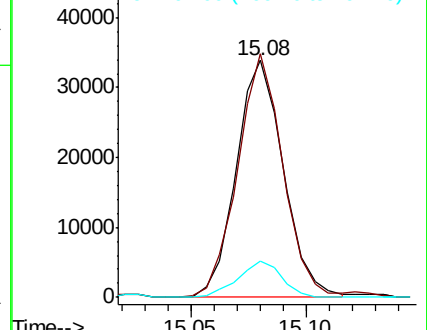

#69

Pentachlorophenol

Concen: 4.306 ng/ul

RT: 16.45 min Scan# 2289

Delta R.T. 0.01 min

Lab File: BN010025.D

Acq: 29 Feb 2020 15:25


Tgt Ion:266 Resp: 15224

Ion Ratio Lower Upper

266 100

264 64.4 52.9 79.3



268 72.7 52.5 78.7

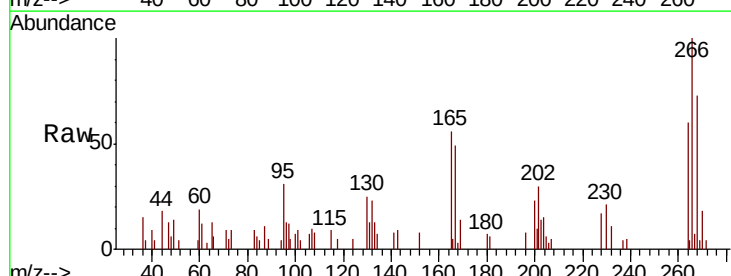


Abundance Ion 265.70 (265.40 to 266.40): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

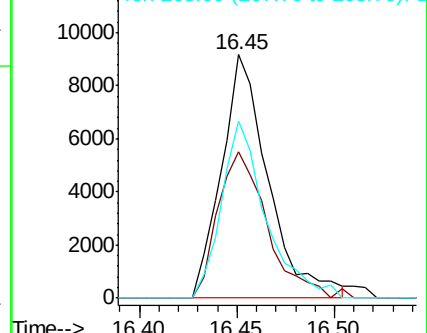







#70
Phenanthrene
Concen: 9.087 ng/ul
RT: 16.82 min Scan# 2351
Delta R.T. -0.01 min
Lab File: BN010025.D
Acq: 29 Feb 2020 15:25

Instrument :
BNA_N
ClientSampled :
DBDM7MS

Tot Ion	Ratio	Lower	Upper
178	100		
179	15.4	12.5	18.7
176	18.4	14.6	22.0




Manual Integrations
APPROVED


mohammad
3/3/2020 5:00:21 PM

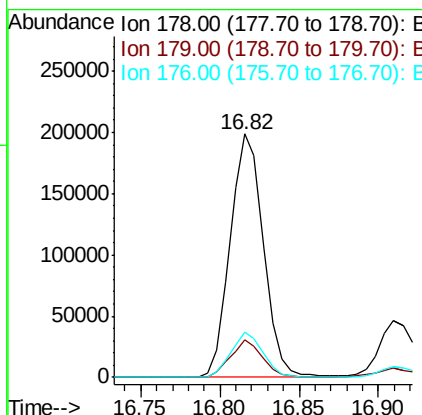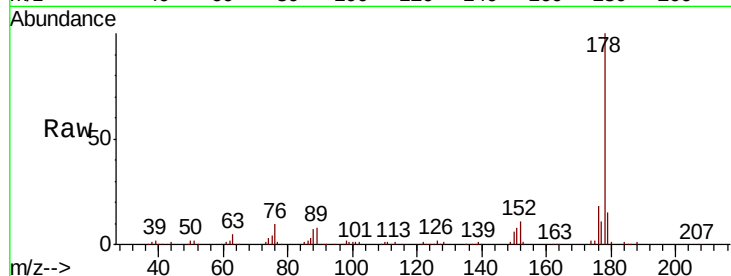

#72
Anthracene
Concen: 2.279 ng/ul
RT: 16.91 min Scan# 2367
Delta R.T. -0.00 min
Lab File: BN010025.D
Acq: 29 Feb 2020 15:25

Tgt Ion	Ratio	Lower	Upper
178	100		
179	15.8	12.2	18.2
176	18.2	14.6	21.8

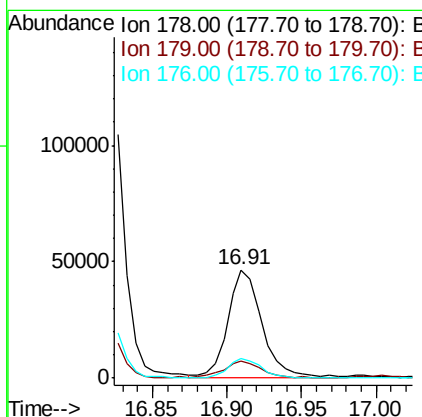

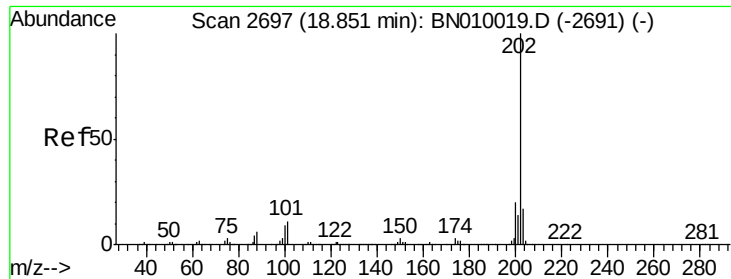





#77
Fluoranthene
Concen: 5.426 ng/ul
RT: 18.85 min Scan# 2697
Delta R.T. -0.00 min
Lab File: BN010025.D
Acq: 29 Feb 2020 15:25

Instrument :
BNA_N
ClientSampleId :
DBDM7MS

Tot Ion	Ratio	Resp Lower	Upper
202	100		
101	10.1	9.4	14.2
100	7.5	7.2	10.8




Manual Integrations
APPROVED


mohammad
3/3/2020 5:00:21 PM

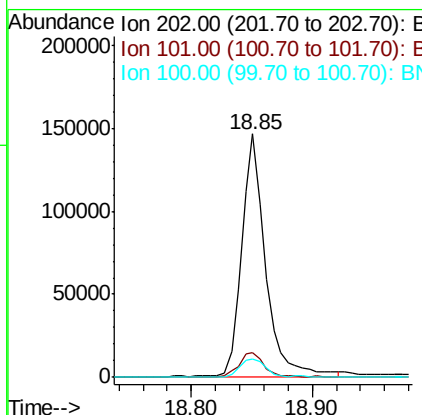

#80
Pyrene
Concen: 13.049 ng/ul
RT: 19.22 min Scan# 2759
Delta R.T. -0.00 min
Lab File: BN010025.D
Acq: 29 Feb 2020 15:25

Tgt Ion	Ratio	Resp Lower	Upper
202	100		
101	12.9	11.3	16.9
100	11.6	9.0	13.6

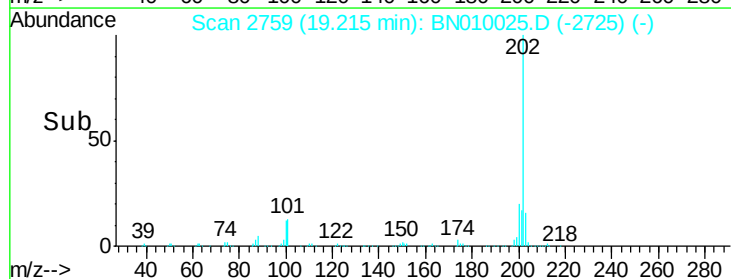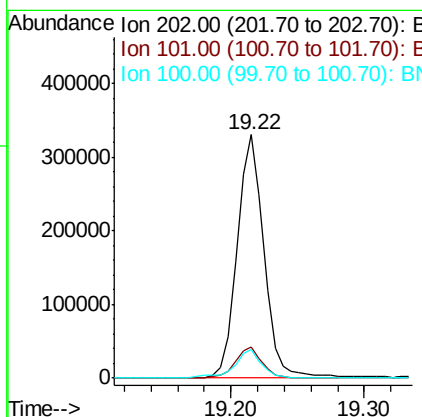

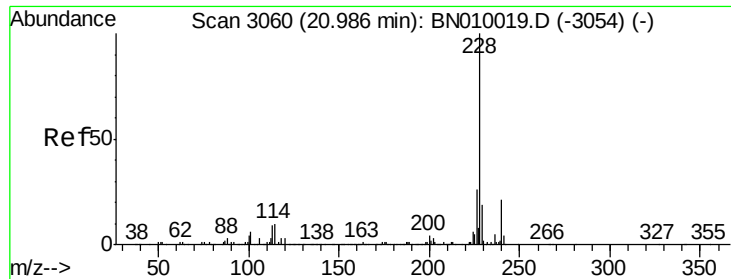





#83
Benzo(a)anthracene
Concen: 1.138 ng/ul
RT: 20.99 min Scan# 3060
Delta R.T. -0.00 min
Lab File: BN010025.D
Acq: 29 Feb 2020 15:25

Instrument :
BNA_N
ClientSampleId :
DBDM7MS

Tot Ion	Ratio	Lower	Upper
228	100		
229	19.2	15.0	22.4
226	25.8	21.4	32.2

Manual Integrations
APPROVED

mohammad
3/3/2020 5:00:21 PM

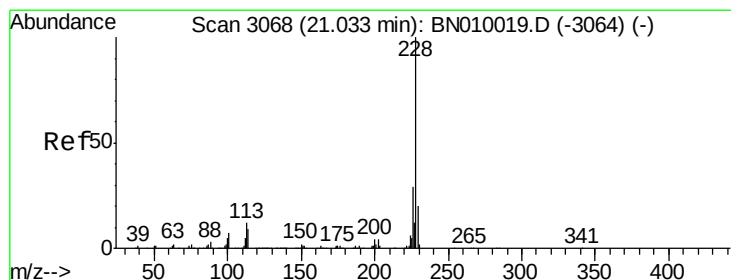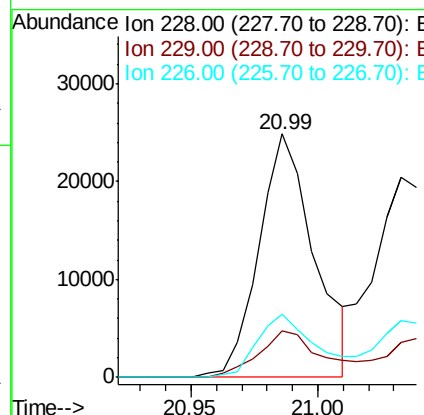

#85
Chrysene
Concen: 1.164 ng/ul
RT: 21.03 min Scan# 3068
Delta R.T. -0.01 min
Lab File: BN010025.D
Acq: 29 Feb 2020 15:25

Tgt Ion	Ratio	Lower	Upper
228	100		
226	28.5	23.4	35.2
229	17.7	15.0	22.4

