




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022822\
Data File : BN018757.D
Acq On : 28 Feb 2022 13:15
Operator : CG/JU
Sample : N1656-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGQ14

Manual IntegrationsAPPROVED

Quant Time: Feb 28 23:55:01 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN021822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 18 13:39:55 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/01/2022
Supervised By :Yogesh Patel 03/02/2022

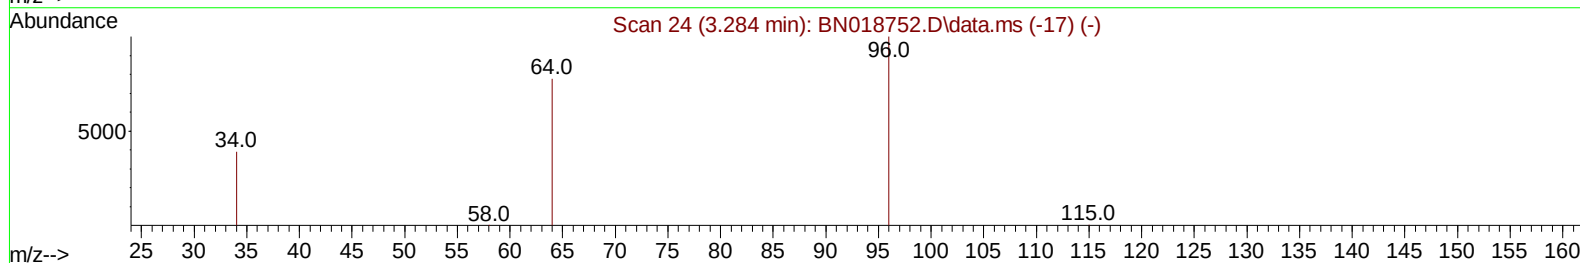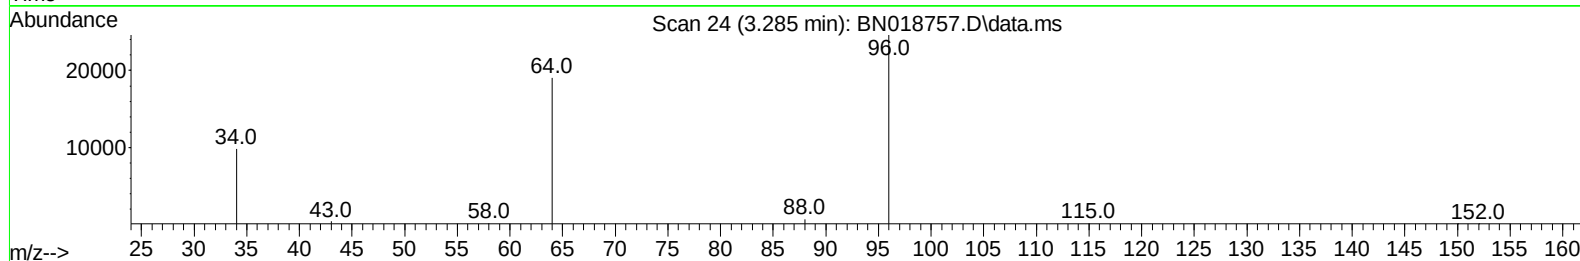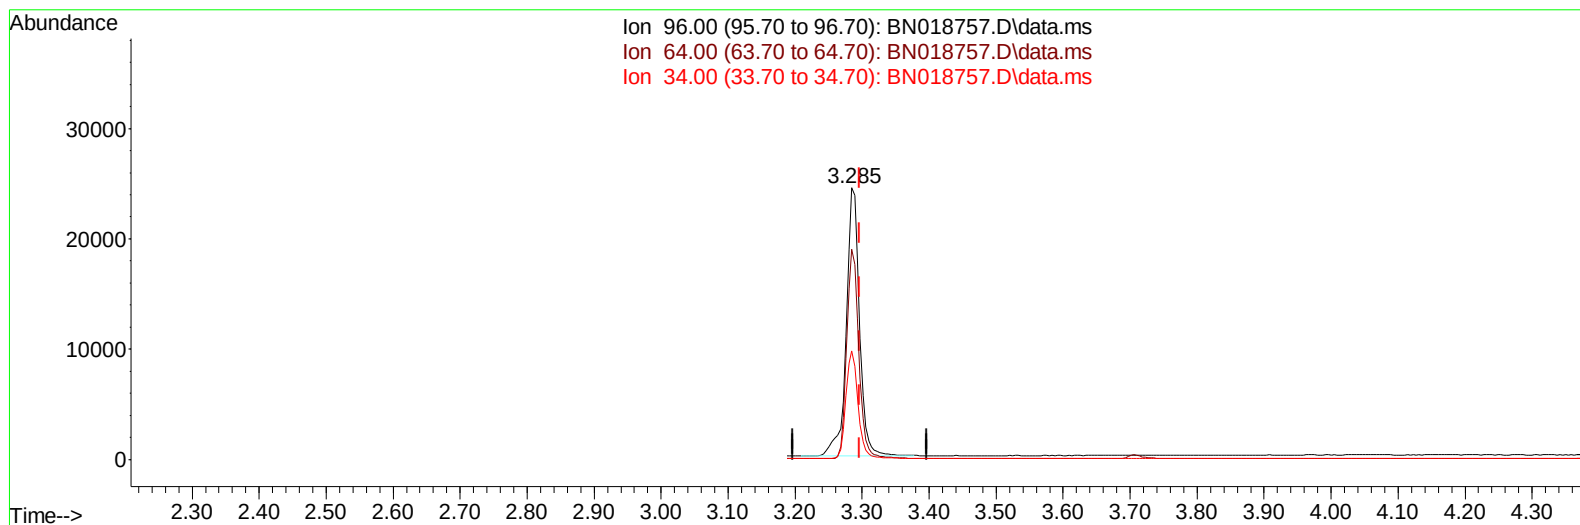

TIC: BN018757.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.285min (-0.012) 4.71 ng/u1

response 33509

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	71.10	77.51
34.00	36.30	39.86
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022822\
Data File : BN018757.D
Acq On : 28 Feb 2022 13:15
Operator : CG/JU
Sample : N1656-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGQ14

Manual IntegrationsAPPROVED

Quant Time: Feb 28 23:55:01 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN021822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 18 13:39:55 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/01/2022
Supervised By :Yogesh Patel 03/02/2022

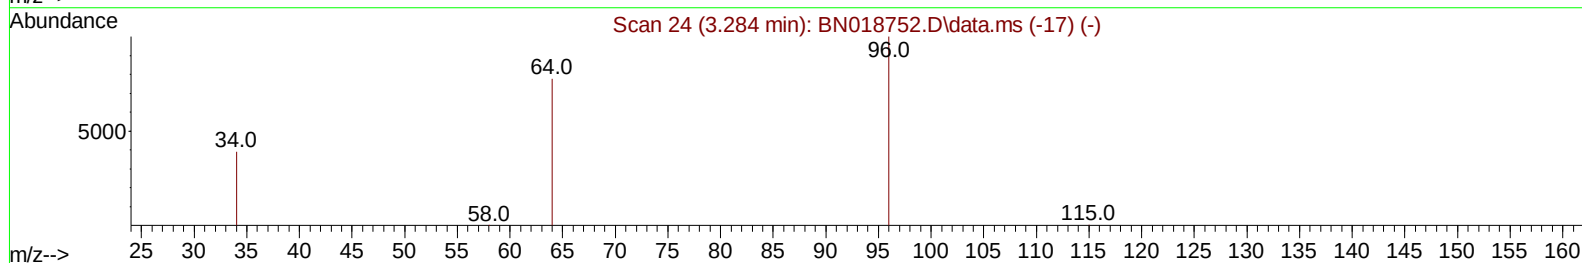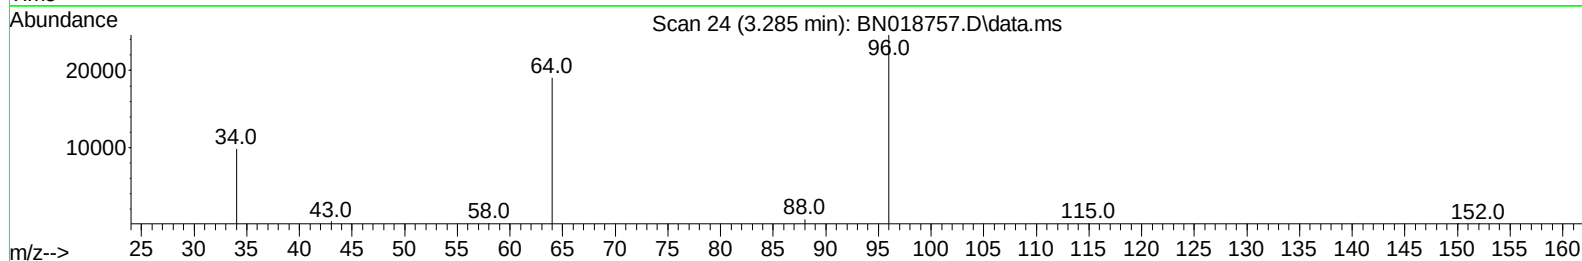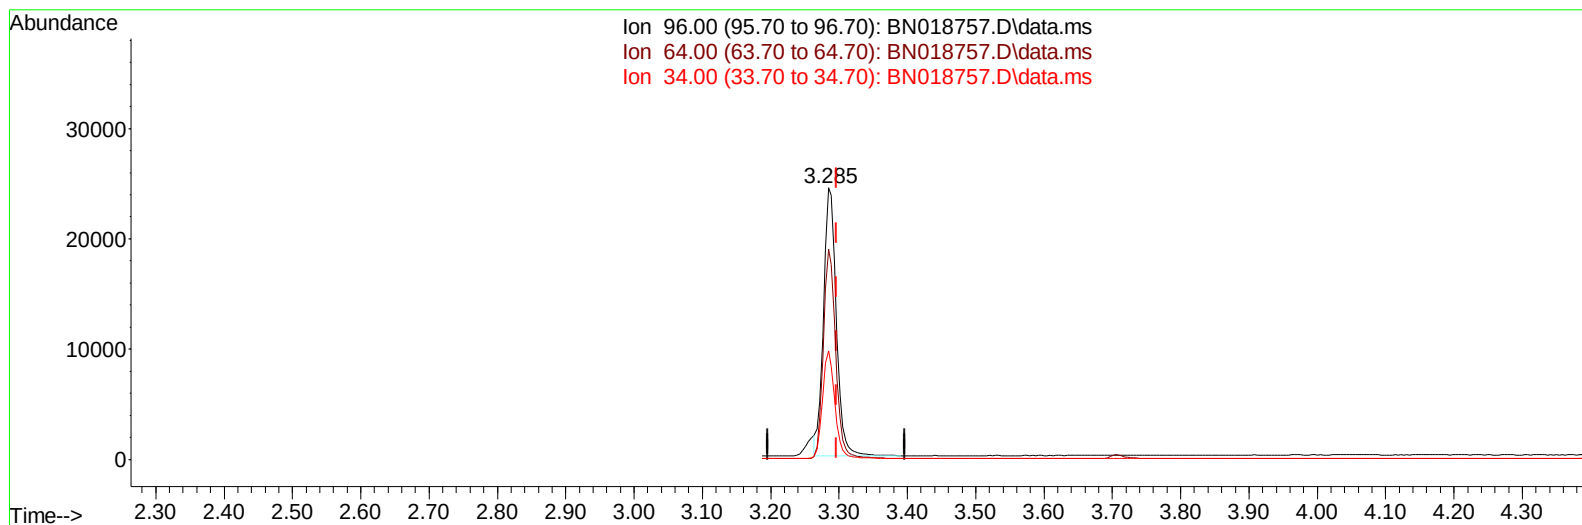

TIC: BN018757.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.285min (-0.012) 4.45 ng/ul m

response 31699

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	71.10	77.51
34.00	36.30	39.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022822\
 Data File : BN018757.D
 Acq On : 28 Feb 2022 13:15
 Operator : CG/JU
 Sample : N1656-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGQ14

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/01/2022
 Supervised By :Yogesh Patel 03/02/2022

Quant Time: Feb 28 23:55:01 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN021822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 18 13:39:55 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.917	152		6266	0.400	ng/ul	0.00
4) Naphthalene-d8	10.721	136		14981	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.547	164		7602	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.284	188		14403	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.465	240		11217	0.400	ng/ul	# 0.00
23) Perylene-d12	23.862	264		11080	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.285	96		31699m	4.454	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.310	152		7386	0.360	ng/ul	0.00
18) Fluoranthene-d10	19.312	212		16306	0.487	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.322	88		14662	2.010	ng/ul#	70
15) Phenanthrene	17.326	178		1869	0.039	ng/ul#	87
19) Fluoranthene	19.340	202		1898	0.040	ng/ul#	79

(#) = qualifier out of range (m) = manual integration (+) = signals summed

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022822\  
Data File : BN018757.D  
Acq On    : 28 Feb 2022   13:15  
Operator   : CG/JU  
Sample     : N1656-07  
Misc       :  
ALS Vial   : 7      Sample Multiplier: 1
```

Instrument :
BNA_N
ClientSampleId :
BGQ14

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/01/2022
Supervised By :Yogesh Patel 03/02/2022

Quant Time: Feb 28 23:55:01 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN021822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 18 13:39:55 2022
Response via : Initial Calibration

