




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022822\
 Data File : BN018764.D
 Acq On : 28 Feb 2022 17:28
 Operator : CG/JU
 Sample : N1656-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGQ13

Manual IntegrationsAPPROVED

Quant Time: Feb 28 23:56:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN021822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 18 13:39:55 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/01/2022
 Supervised By :Yogesh Patel 03/02/2022

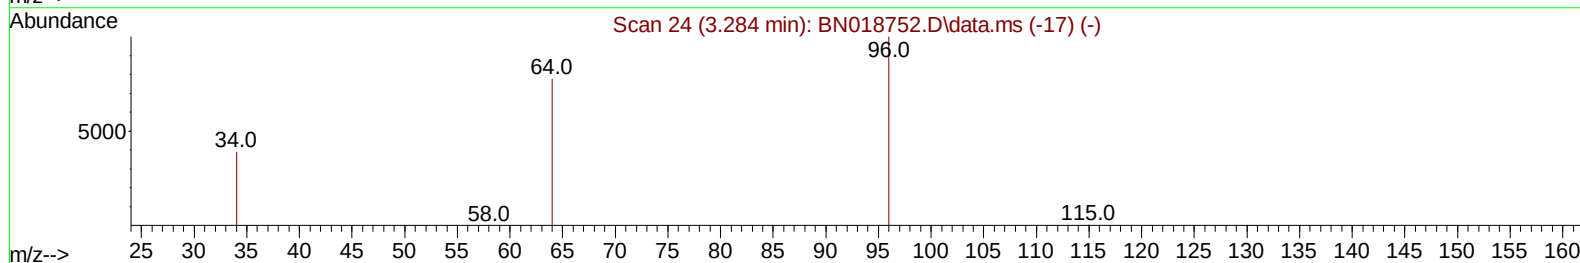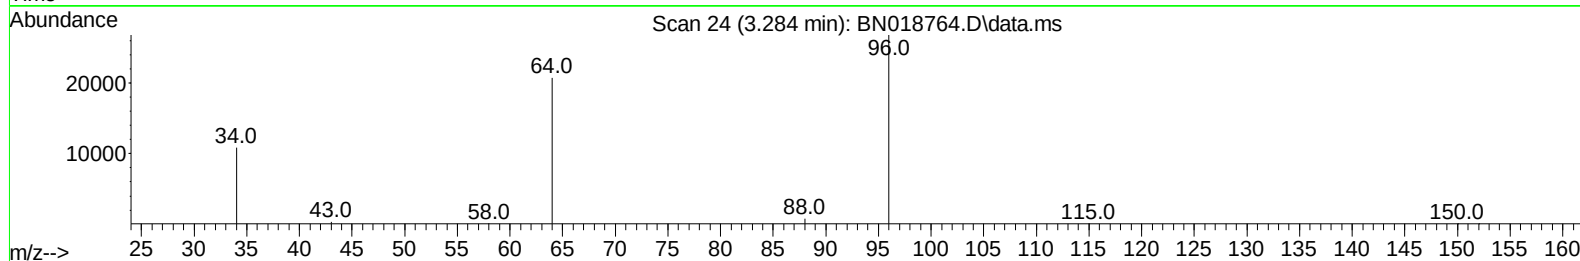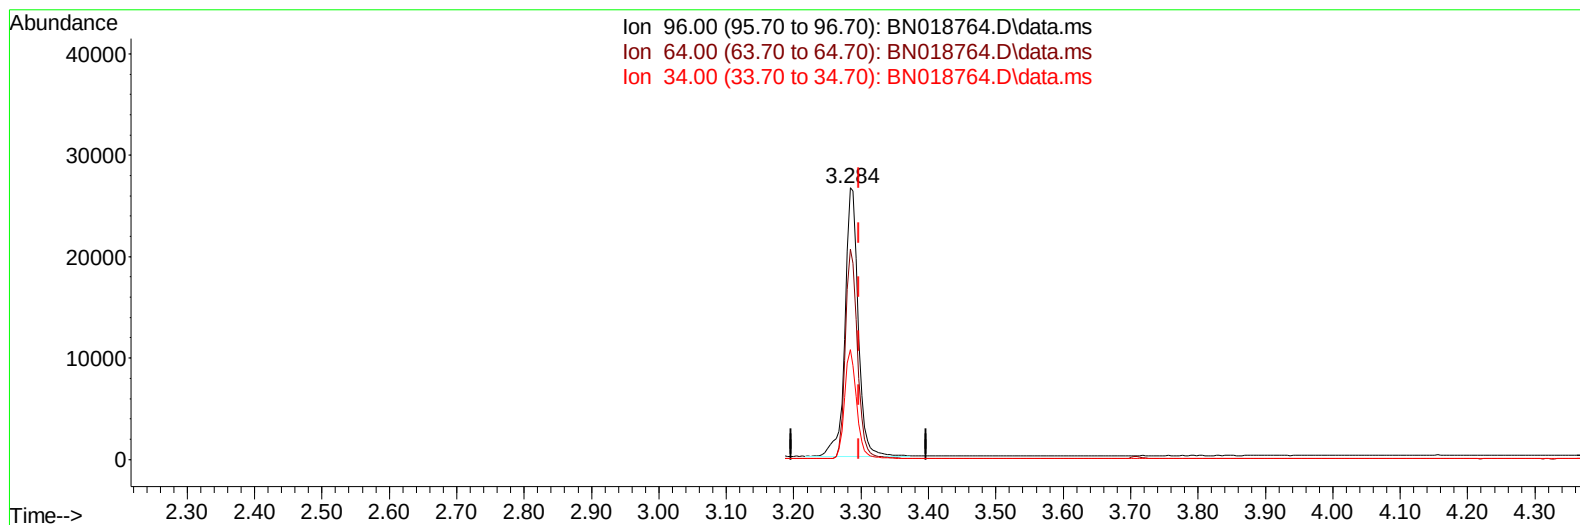

TIC: BN018764.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.284min (-0.013) 5.45 ng/u1

response 36130

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	71.10	77.38
34.00	36.30	40.34
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022822\
 Data File : BN018764.D
 Acq On : 28 Feb 2022 17:28
 Operator : CG/JU
 Sample : N1656-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGQ13

Manual IntegrationsAPPROVED

Quant Time: Feb 28 23:56:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN021822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 18 13:39:55 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/01/2022
 Supervised By :Yogesh Patel 03/02/2022

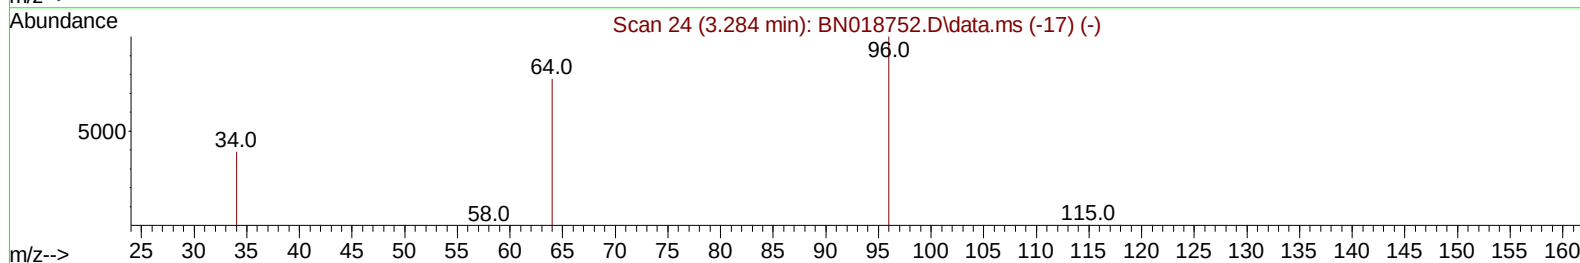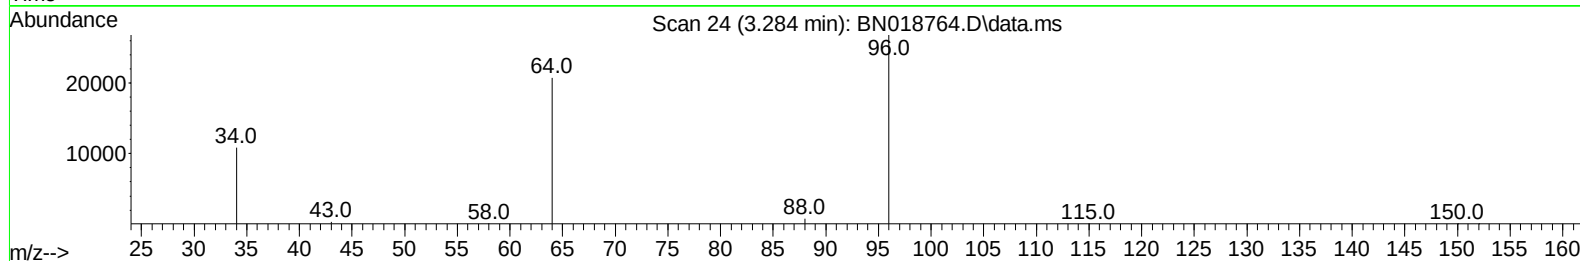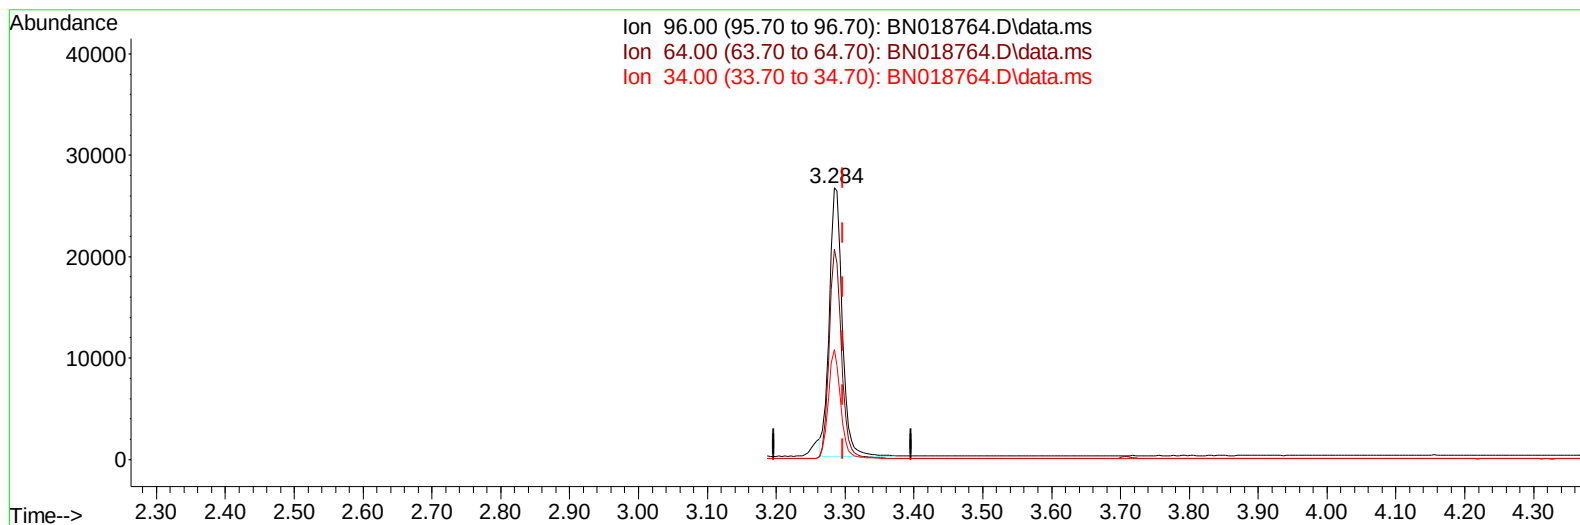

TIC: BN018764.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.284min (-0.013) 5.22 ng/ul m

response 34626

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	71.10	77.38
34.00	36.30	40.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022822\
 Data File : BN018764.D
 Acq On : 28 Feb 2022 17:28
 Operator : CG/JU
 Sample : N1656-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGQ13

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/01/2022
 Supervised By :Yogesh Patel 03/02/2022

Quant Time: Feb 28 23:56:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN021822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 18 13:39:55 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.917	152		5839	0.400	ng/ul	0.00
4) Naphthalene-d8	10.719	136		13987	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.546	164		7272	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.287	188		14118	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.466	240		11737	0.400	ng/ul	# 0.00
23) Perylene-d12	23.863	264		11559	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.284	96		34626m	5.221	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.308	152		7042	0.368	ng/ul	0.00
18) Fluoranthene-d10	19.311	212		16097	0.459	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.322	88		13655	2.009	ng/ul#	70
15) Phenanthrene	17.329	178		1634	0.035	ng/ul#	88
19) Fluoranthene	19.339	202		1711	0.035	ng/ul#	76

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022822\
Data File : BN018764.D
Acq On : 28 Feb 2022 17:28
Operator : CG/JU
Sample : N1656-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGQ13

Manual IntegrationsAPPROVED

Quant Time: Feb 28 23:56:28 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN021822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 18 13:39:55 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/01/2022
Supervised By :Yogesh Patel 03/02/2022

