




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022822\
Data File : BN018767.D
Acq On : 28 Feb 2022 19:15
Operator : CG/JU
Sample : N1656-17
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGQ24

Manual IntegrationsAPPROVED

Quant Time: Feb 28 23:56:51 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN021822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 18 13:39:55 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/01/2022
Supervised By :Yogesh Patel 03/02/2022

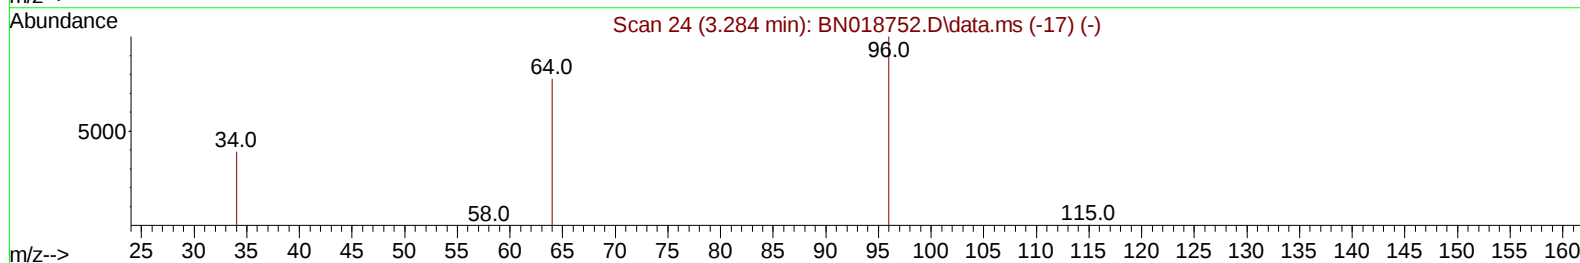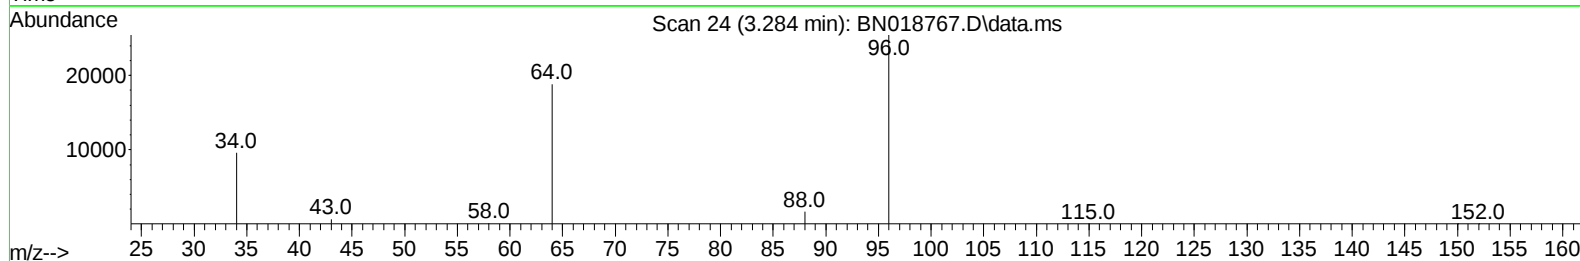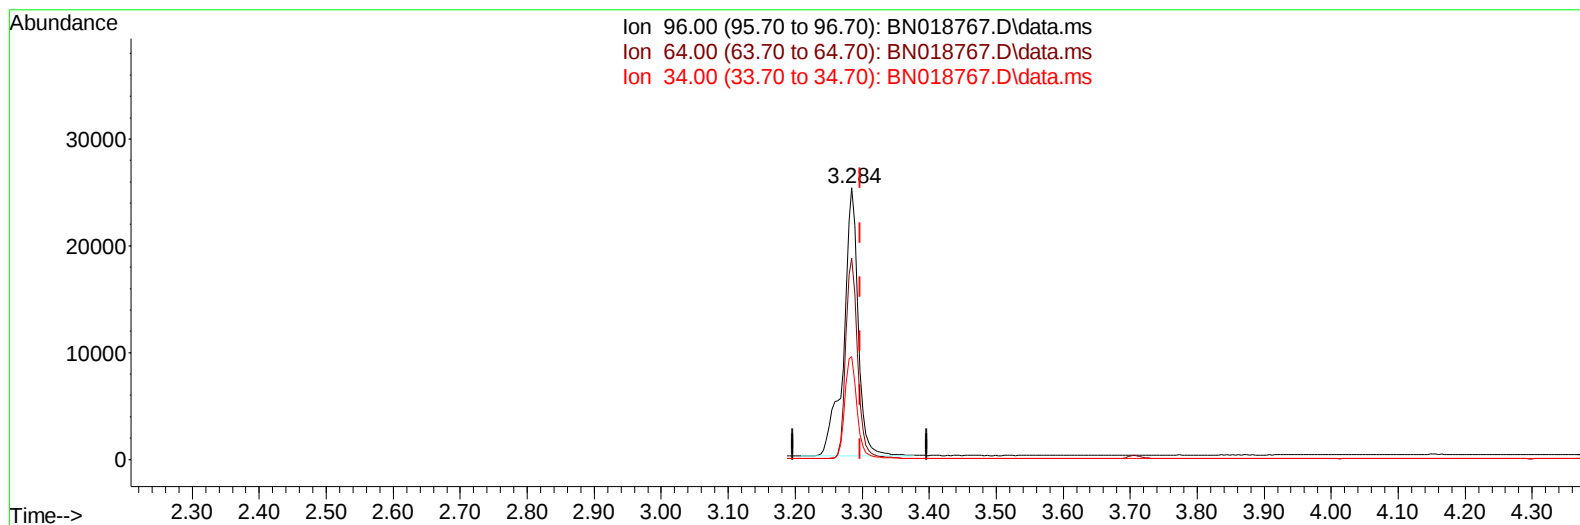

TIC: BN018767.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.284min (-0.012) 5.48 ng/u1

response 37940

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	71.10	74.13
34.00	36.30	37.76
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022822\
Data File : BN018767.D
Acq On : 28 Feb 2022 19:15
Operator : CG/JU
Sample : N1656-17
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGQ24

Manual IntegrationsAPPROVED

Quant Time: Feb 28 23:56:51 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN021822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 18 13:39:55 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/01/2022
Supervised By :Yogesh Patel 03/02/2022

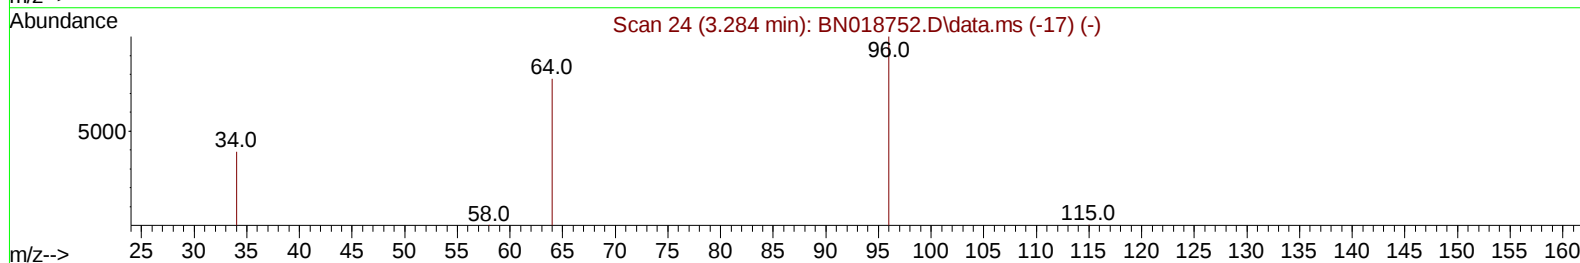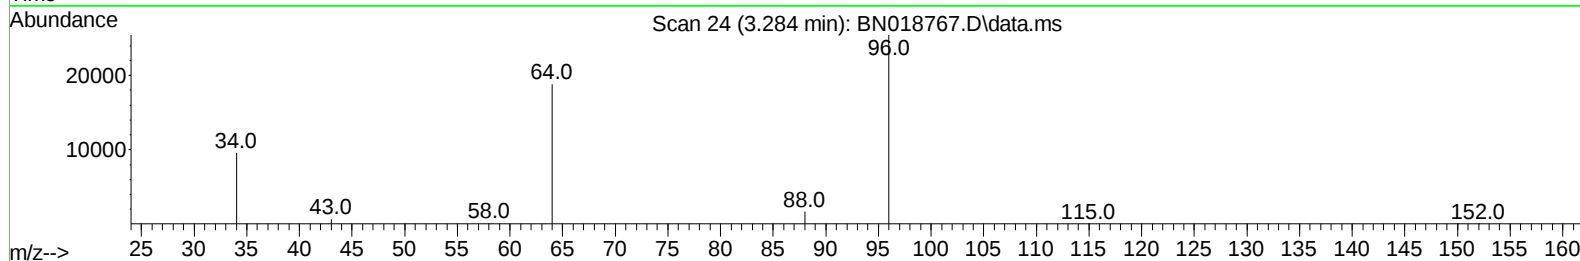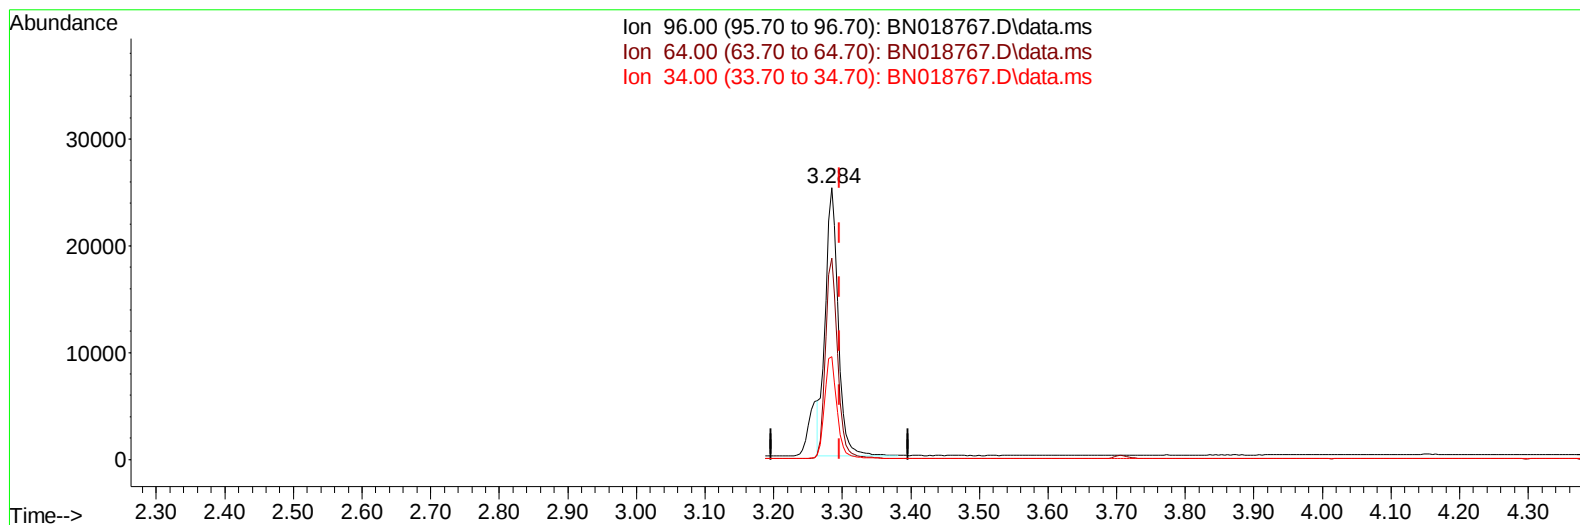

TIC: BN018767.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.284min (-0.012) 4.73 ng/ul m

response 32728

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	71.10	74.13
34.00	36.30	37.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022822\
 Data File : BN018767.D
 Acq On : 28 Feb 2022 19:15
 Operator : CG/JU
 Sample : N1656-17
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGQ24

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/01/2022
 Supervised By :Yogesh Patel 03/02/2022

Quant Time: Feb 28 23:56:51 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN021822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 18 13:39:55 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.913	152		6092	0.400	ng/ul	0.00
4) Naphthalene-d8	10.721	136		15009	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.547	164		7821	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.283	188		14929	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.467	240		11902	0.400	ng/ul	# 0.00
23) Perylene-d12	23.861	264		11820	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.284	96		32728m	4.730	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.304	152		6427	0.313	ng/ul	0.00
18) Fluoranthene-d10	19.312	212		14798	0.416	ng/ul	0.00
Target Compounds				Qvalue			
2) 1,4-Dioxane	3.322	88		4920	0.694	ng/ul#	80
8) 1-Methylnaphthalene	12.596	142		1875	0.069	ng/ul	93
12) Fluorene	15.592	166		661	0.022	ng/ul#	86
15) Phenanthrene	17.326	178		2191	0.045	ng/ul#	90
19) Fluoranthene	19.340	202		1081	0.022	ng/ul#	73

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022822\
Data File : BN018767.D
Acq On : 28 Feb 2022 19:15
Operator : CG/JU
Sample : N1656-17
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGQ24

Manual IntegrationsAPPROVED

Quant Time: Feb 28 23:56:51 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN021822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 18 13:39:55 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/01/2022
Supervised By :Yogesh Patel 03/02/2022

