

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022822\
 Data File : BN018760.D
 Acq On : 28 Feb 2022 15:03
 Operator : CG/JU
 Sample : N1656-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGQ12

Quant Time: Feb 28 23:55:29 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN021822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 18 13:39:55 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.917	152	6605	0.400	ng/ul	0.00
4) Naphthalene-d8	10.721	136	15998	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.547	164	8156	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.288	188	15322	0.400	ng/ul	0.00
17) Chrysene-d12	21.465	240	11515	0.400	ng/ul	# 0.00
23) Perylene-d12	23.861	264	11317	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.284	96	36946	4.925	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.310	152	7694	0.352	ng/ul	0.00
18) Fluoranthene-d10	19.312	212	16010	0.465	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.322	88	936	0.122	ng/ul#	79
15) Phenanthrene	17.326	178	1403	0.028	ng/ul#	84
19) Fluoranthene	19.340	202	1134	0.023	ng/ul#	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022822\
Data File : BN018760.D
Acq On : 28 Feb 2022 15:03
Operator : CG/JU
Sample : N1656-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGQ12

Quant Time: Feb 28 23:55:29 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN021822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 18 13:39:55 2022
Response via : Initial Calibration




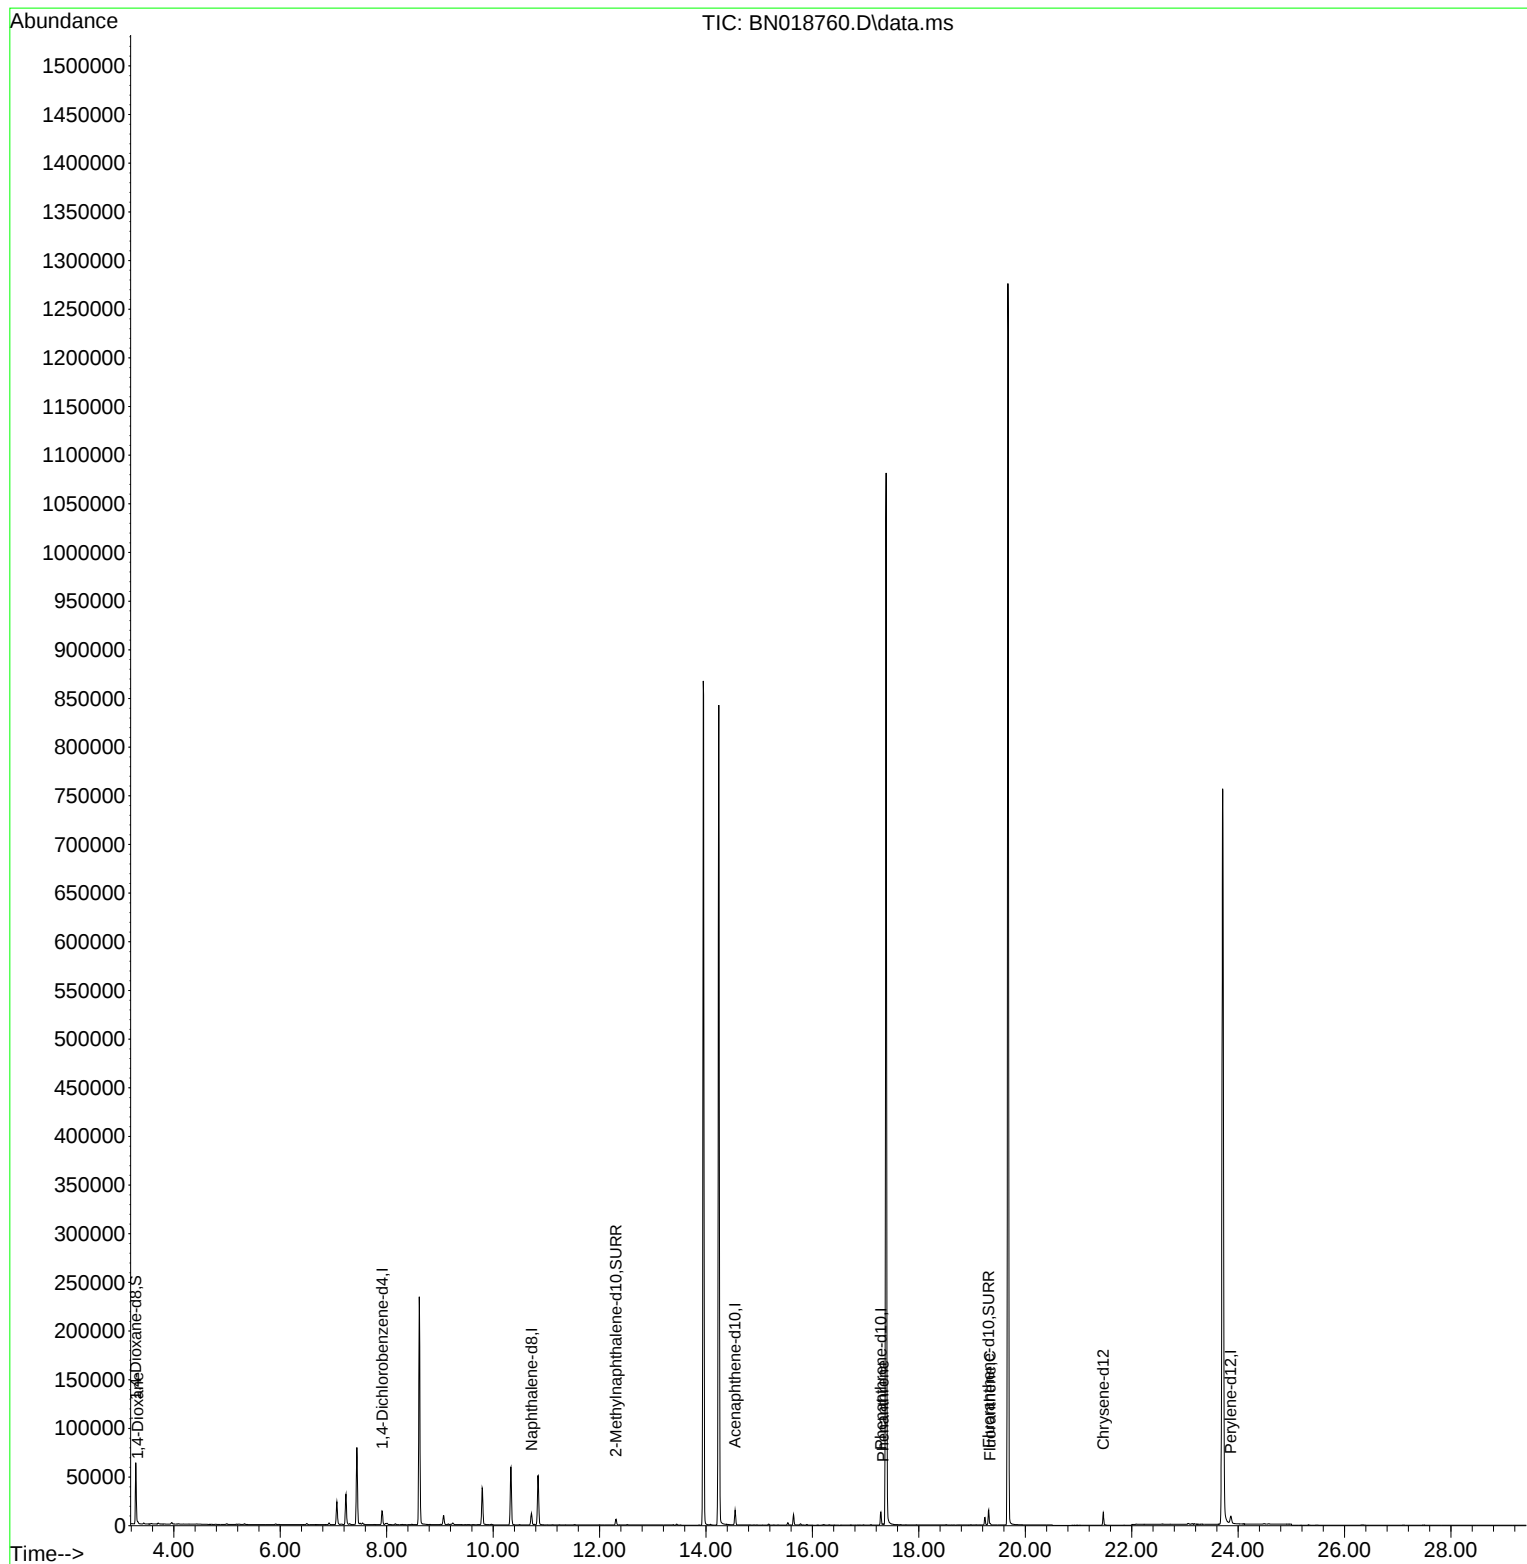


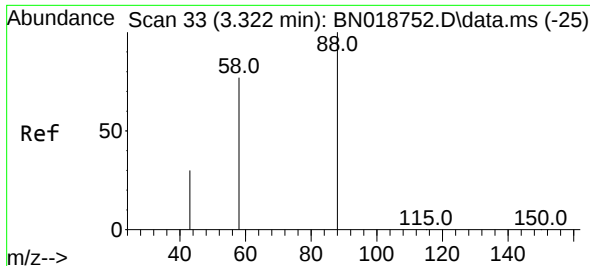

#2
 1,4-Dioxane
 Concen: 0.122 ng/ul
 RT: 3.322 min Scan# 3113
 Delta R.T. -0.012 min
 Lab File: BN018760.D
 Acq: 28 Feb 2022 15:03




Instrument :
 BNA_N
 ClientSampleId :
 BGQ12


Tgt Ion: 88 Resp: 936
 Ion Ratio Lower Upper
 88 100
 43 43.9 47.8 71.8#
 58 42.4 46.2 69.2#

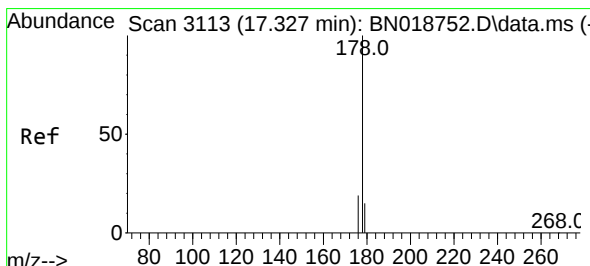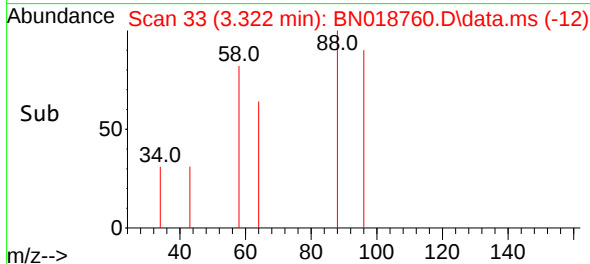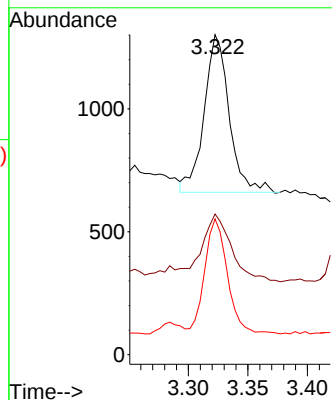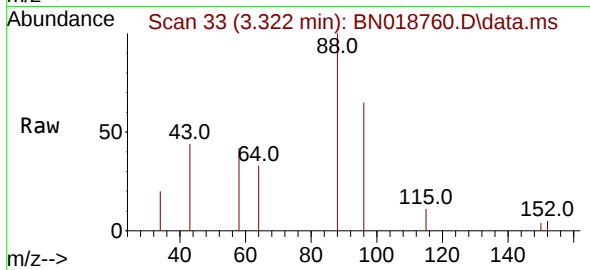

#15
 Phenanthrene
 Concen: 0.028 ng/ul
 RT: 17.326 min Scan# 3113
 Delta R.T. -0.003 min
 Lab File: BN018760.D
 Acq: 28 Feb 2022 15:03


Tgt Ion: 178 Resp: 1403
 Ion Ratio Lower Upper
 178 100
 179 23.5 12.2 18.4#
 176 25.3 15.4 23.2#

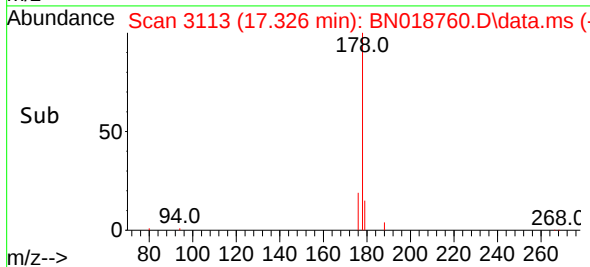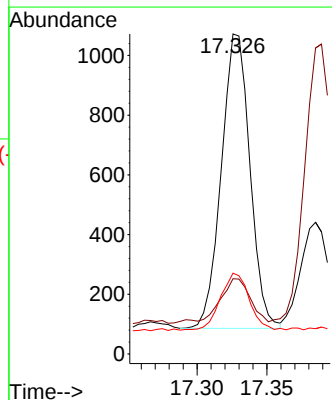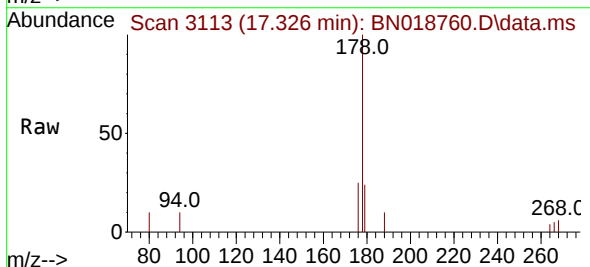

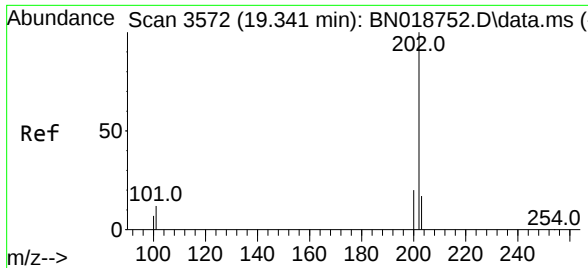

#19
 Fluoranthene
 Concen: 0.023 ng/ul
 RT: 19.340 min Scan# 31
 Delta R.T. -0.003 min
 Lab File: BN018760.D
 Acq: 28 Feb 2022 15:03

Instrument :
 BNA_N
 ClientSampleId :
 BGQ12

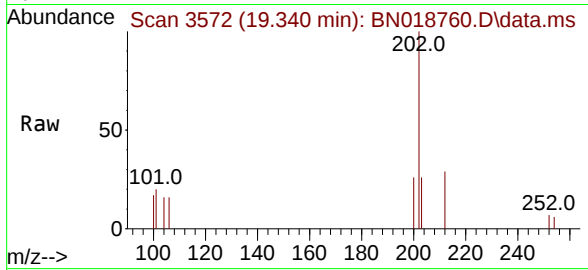

Tgt Ion:202 Resp: 1134

Ion	Ratio	Lower	Upper
202	100		
101	19.9	7.5	11.3#
100	16.7	5.4	8.2#

