

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022822\
 Data File : BN018761.D
 Acq On : 28 Feb 2022 15:39
 Operator : CG/JU
 Sample : N1656-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGQ08

Quant Time: Feb 28 23:55:37 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN021822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 18 13:39:55 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.917	152	6259	0.400	ng/ul	0.00
4) Naphthalene-d8	10.721	136	15194	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.547	164	7649	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.288	188	14178	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.464	240	11058	0.400	ng/ul	# 0.00
23) Perylene-d12	23.861	264	10563	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.289	96	33203	4.671	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.310	152	7292	0.351	ng/ul	0.00
18) Fluoranthene-d10	19.312	212	15050	0.456	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.770	128	1024	0.024	ng/ul#	83
15) Phenanthrene	17.326	178	1507	0.032	ng/ul#	85
19) Fluoranthene	19.344	202	1680	0.036	ng/ul#	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022822\
Data File : BN018761.D
Acq On : 28 Feb 2022 15:39
Operator : CG/JU
Sample : N1656-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGQ08

Quant Time: Feb 28 23:55:37 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN021822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 18 13:39:55 2022
Response via : Initial Calibration




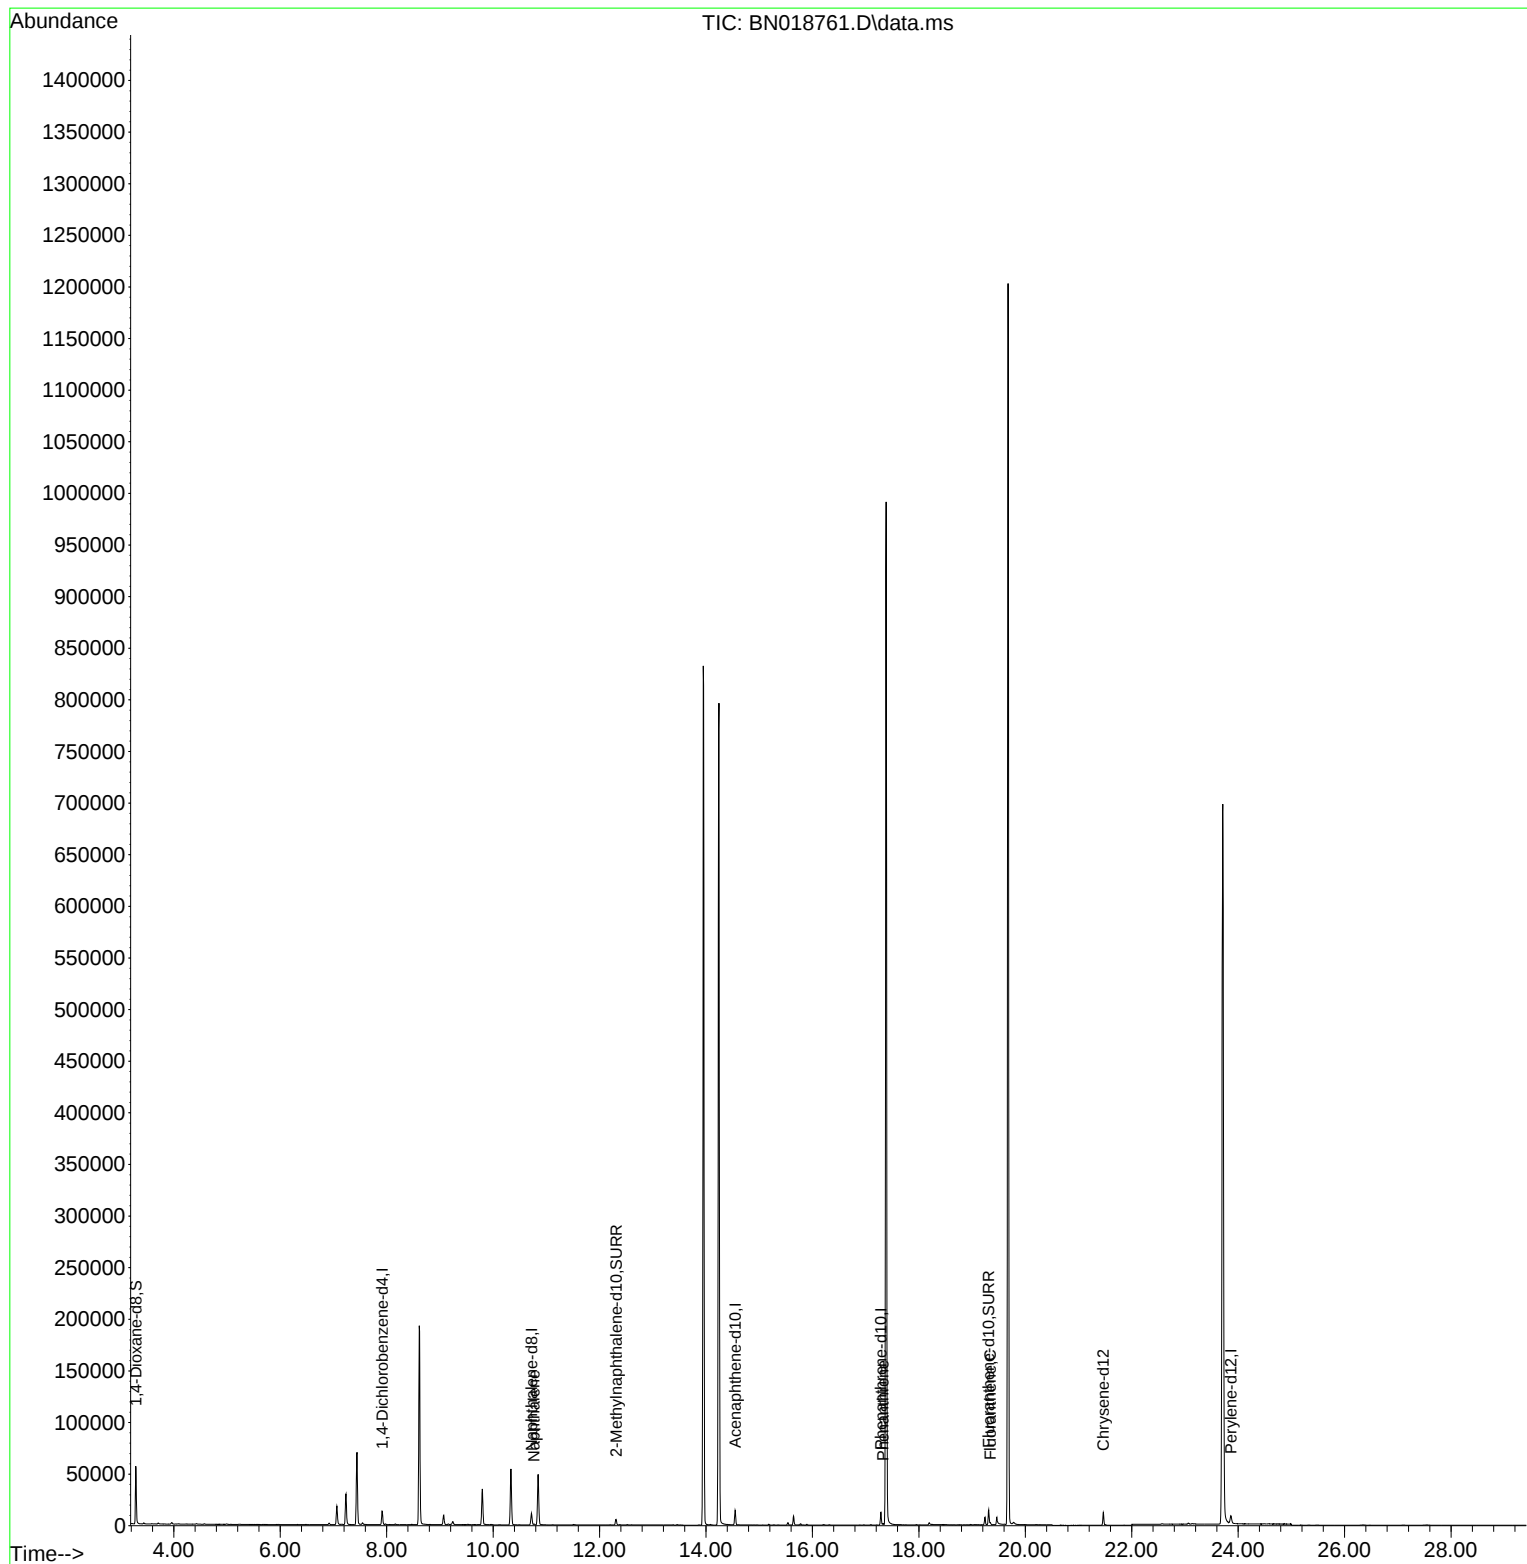


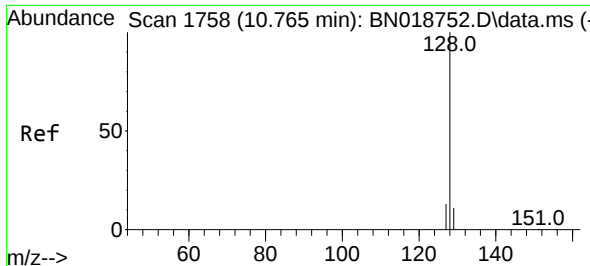

#5
Naphthalene
Concen: 0.024 ng/ul
RT: 10.770 min Scan# 1759
Delta R.T. -0.004 min
Lab File: BN018761.D
Acq: 28 Feb 2022 15:39




Instrument :
BNA_N
ClientSampleId :
BGQ08


Tgt Ion:128 Resp: 1024
Ion Ratio Lower Upper
128 100
129 20.1 9.4 14.0#
127 19.2 11.0 16.6#

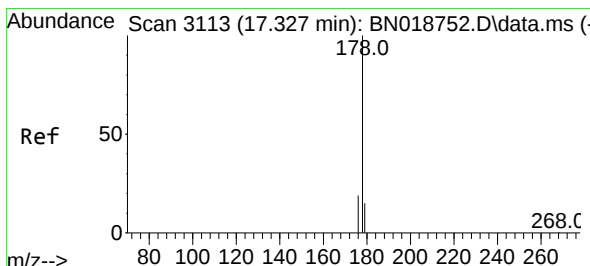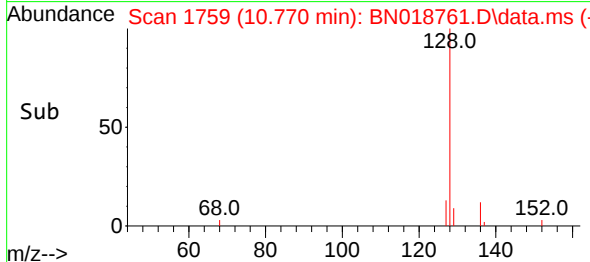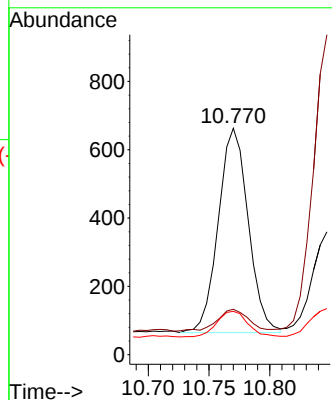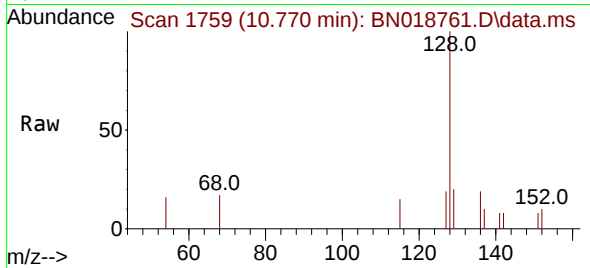

#15
Phenanthrene
Concen: 0.032 ng/ul
RT: 17.326 min Scan# 3113
Delta R.T. -0.003 min
Lab File: BN018761.D
Acq: 28 Feb 2022 15:39


Tgt Ion:178 Resp: 1507
Ion Ratio Lower Upper
178 100
179 22.5 12.2 18.4#
176 25.5 15.4 23.2#

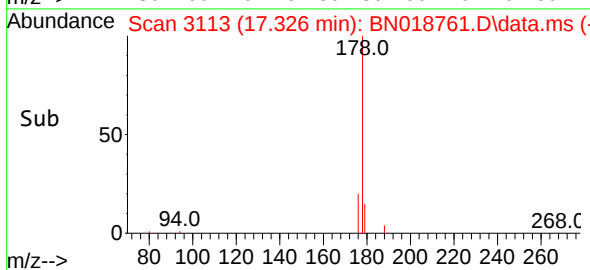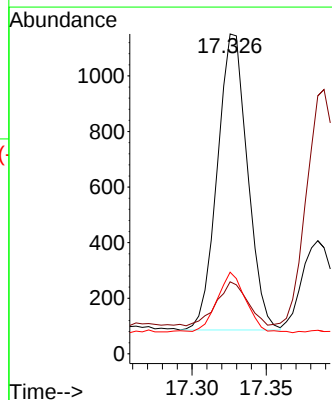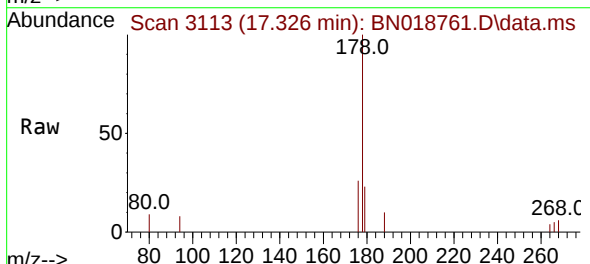

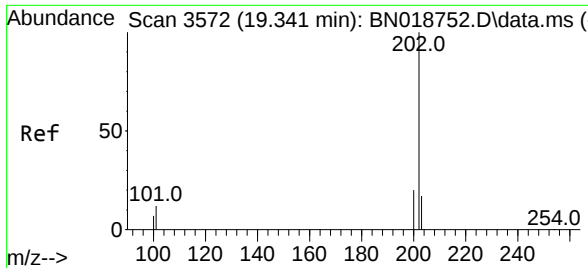

#19
 Fluoranthene
 Concen: 0.036 ng/ul
 RT: 19.344 min Scan# 31
 Delta R.T. 0.001 min
 Lab File: BN018761.D
 Acq: 28 Feb 2022 15:39

Instrument :
 BNA_N
 ClientSampleId :
 BGQ08

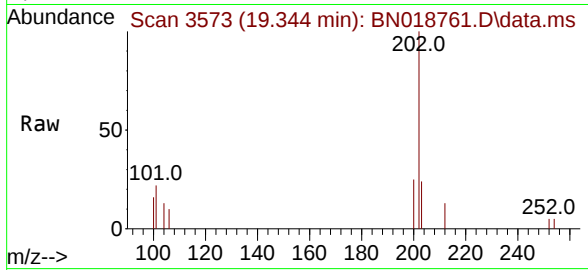

Tgt Ion:	202	Resp:	1680
Ion Ratio	Lower	Upper	
202	100		
101	21.6	7.5	11.3#
100	16.3	5.4	8.2#

