

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
 Data File : BN030136.D
 Acq On : 28 Feb 2024 19:01
 Operator : MA/JU
 Sample : PB159157BL
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK157

Quant Time: Feb 28 23:06:38 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 27 23:49:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.855	152	6092	0.400	ng/ul	0.00
4) Naphthalene-d8	10.650	136	13132	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.497	164	9948	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.251	188	19059	0.400	ng/ul	-0.01
17) Chrysene-d12	21.461	240	10291	0.400	ng/ul	0.00
23) Perylene-d12	23.814	264	13460	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.315	96	40670	5.354	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.245	152	6516	0.390	ng/ul	0.00
18) Fluoranthene-d10	19.285	212	13431	0.397	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.497	166	2635	0.068	ng/ul#	15
20) Pyrene	19.653	202	2112	0.044	ng/ul#	1
26) Benzo(a)pyrene	23.665	252	3882	0.082	ng/ul#	59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030136.D
Acq On : 28 Feb 2024 19:01
Operator : MA/JU
Sample : PB159157BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK157

Quant Time: Feb 28 23:06:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration




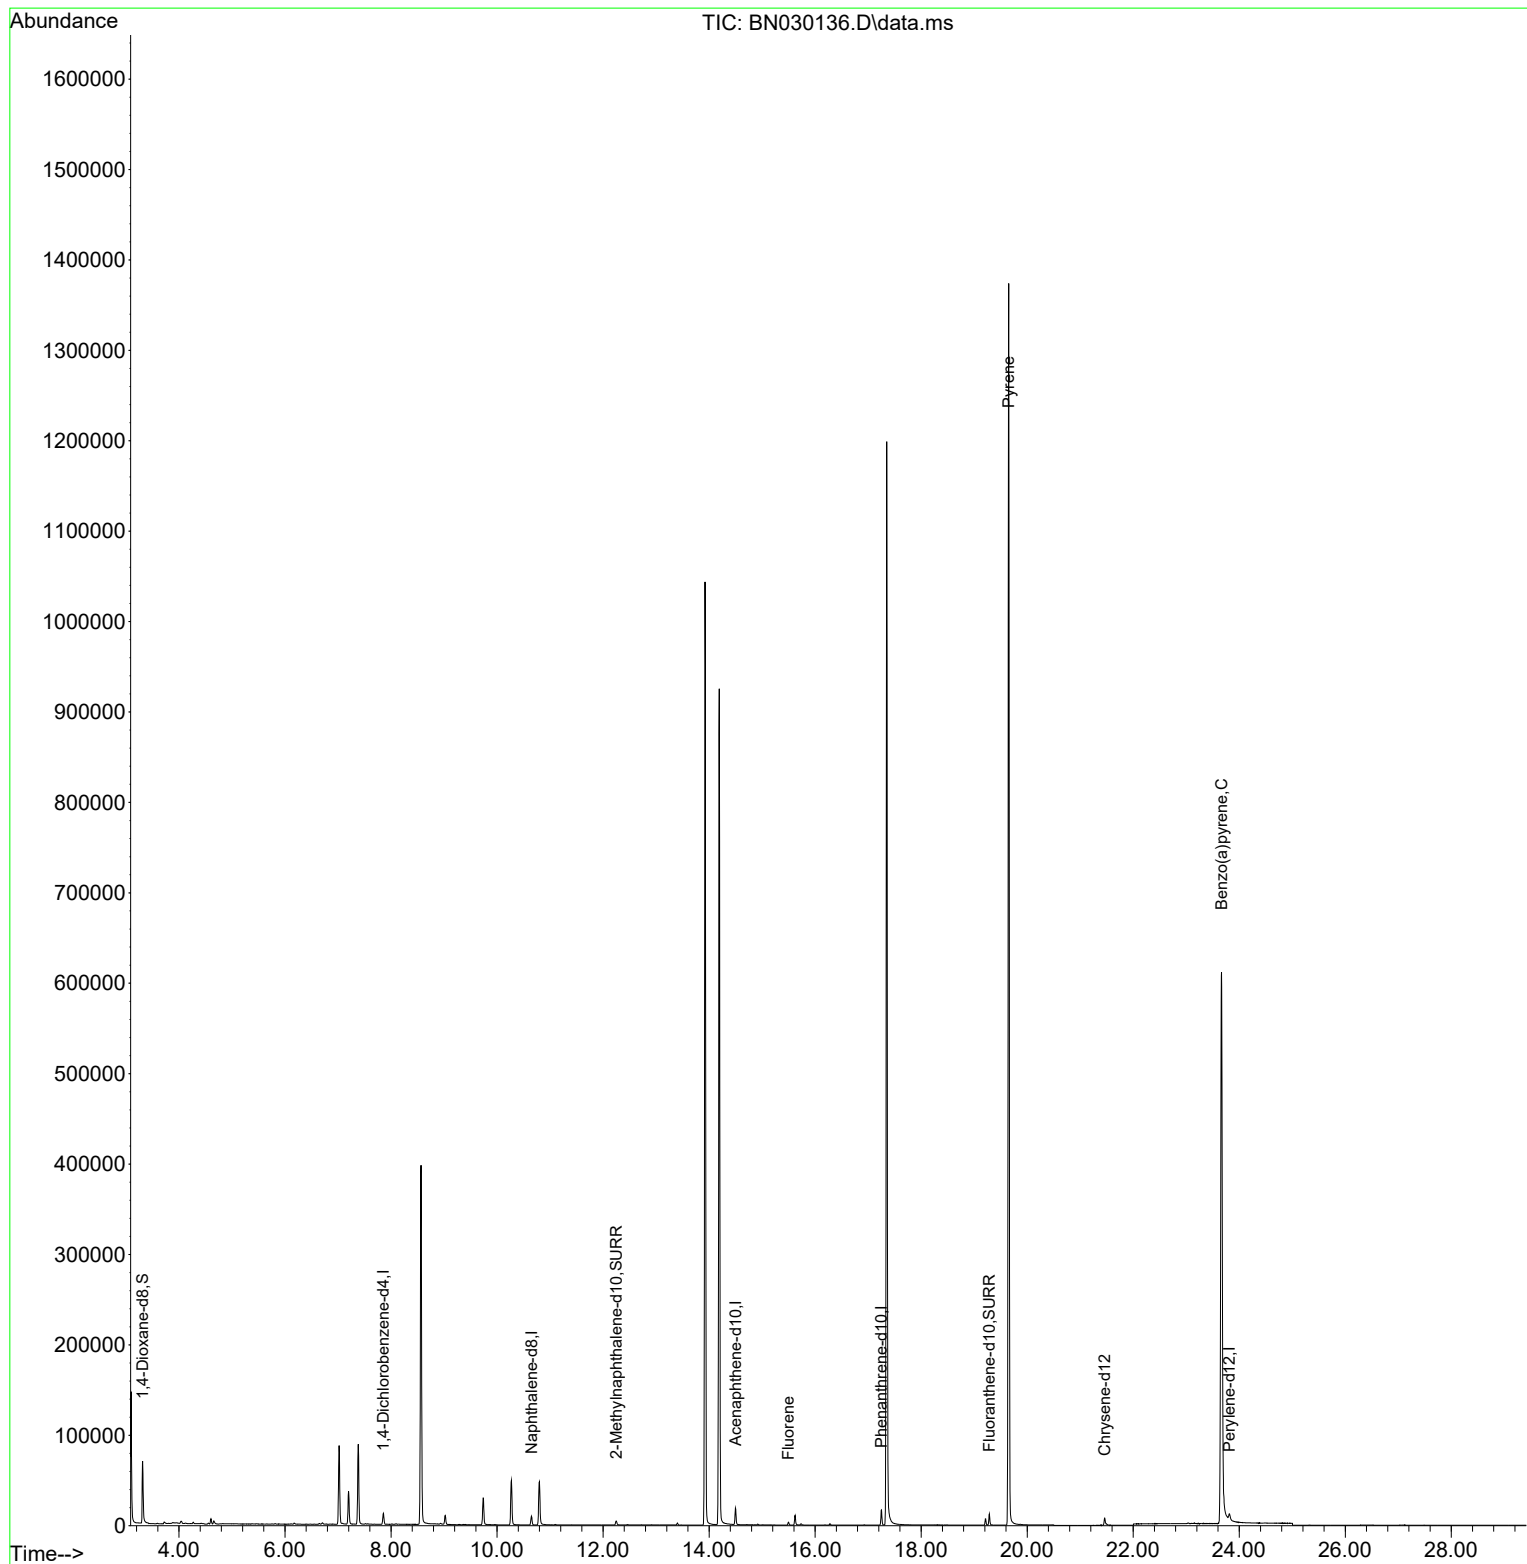


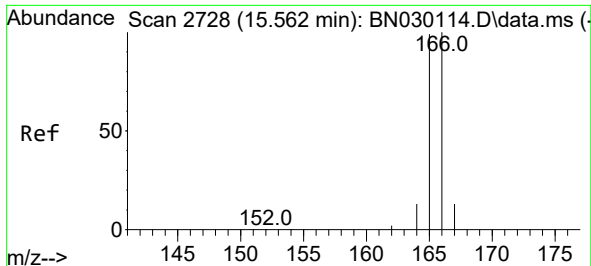

#12
Fluorene
Concen: 0.068 ng/ul
RT: 15.497 min Scan# 2714
Delta R.T. -0.064 min
Lab File: BN030136.D
Acq: 28 Feb 2024 19:01




Instrument :
BNA_N
ClientSampleId :
SBLK157


Tgt Ion:166 Resp: 2635
Ion Ratio Lower Upper
166 100
165 9.5 78.6 117.8#
167 35.7 11.5 17.3#

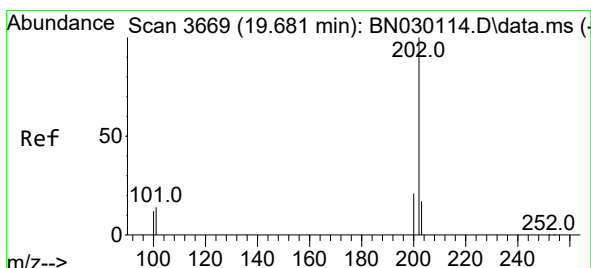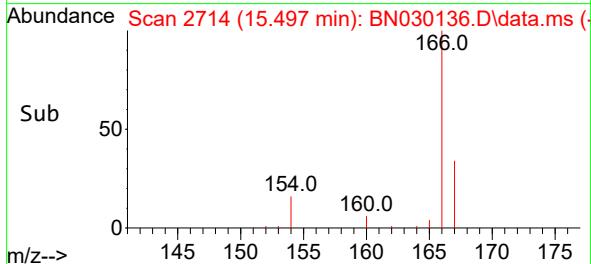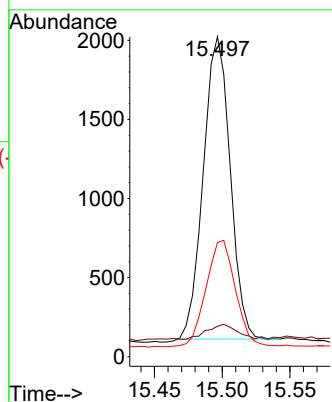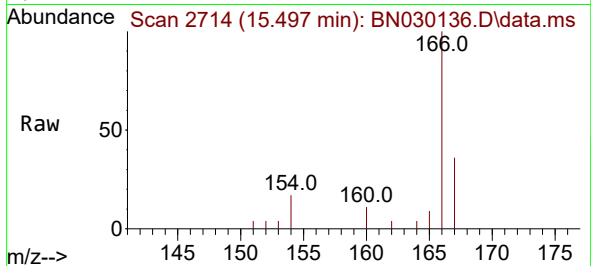

#20
Pyrene
Concen: 0.044 ng/ul
RT: 19.653 min Scan# 3663
Delta R.T. -0.032 min
Lab File: BN030136.D
Acq: 28 Feb 2024 19:01


Tgt Ion:202 Resp: 2112
Ion Ratio Lower Upper
202 100
101 201.6 12.5 18.7#
100 1498.0 10.0 15.0#

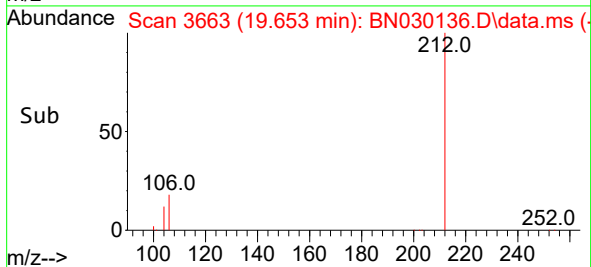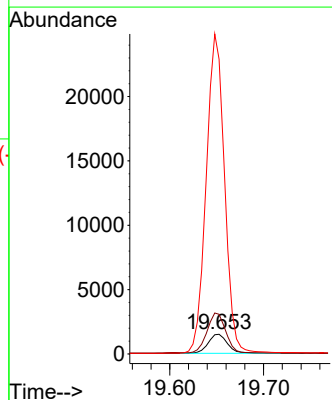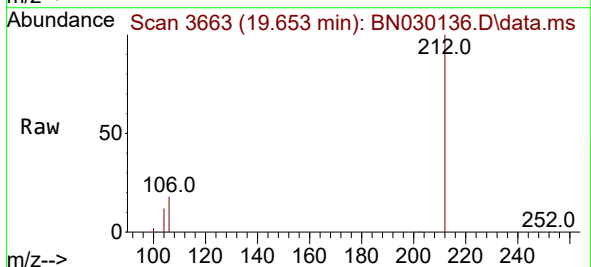

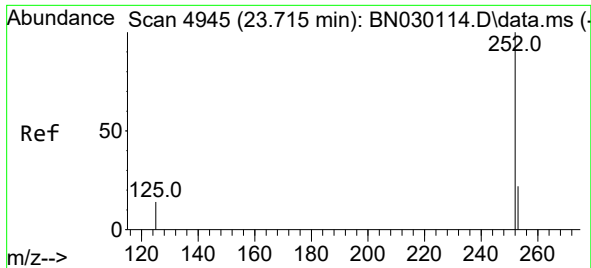

#26
Benzo(a)pyrene
Concen: 0.082 ng/ul
RT: 23.665 min Scan# 4945
Delta R.T. -0.060 min
Lab File: BN030136.D
Acq: 28 Feb 2024 19:01

Instrument :
BNA_N
ClientSampleId :
SBLK157

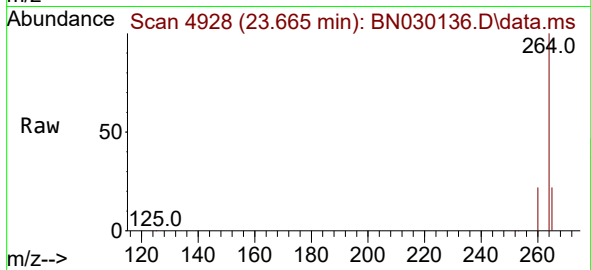

Tgt Ion:252 Resp: 3882
Ion Ratio Lower Upper
252 100
253 52.7 25.4 38.0#
125 40.7 16.0 24.0#

