




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
 Data File : BN030101.D
 Acq On : 27 Feb 2024 20:43
 Operator : MA/JU
 Sample : P1508-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH403

Manual IntegrationsAPPROVED

Quant Time: Feb 27 23:51:33 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 27 23:49:29 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/28/2024
 Supervised By :mohammad ahmed 03/01/2024

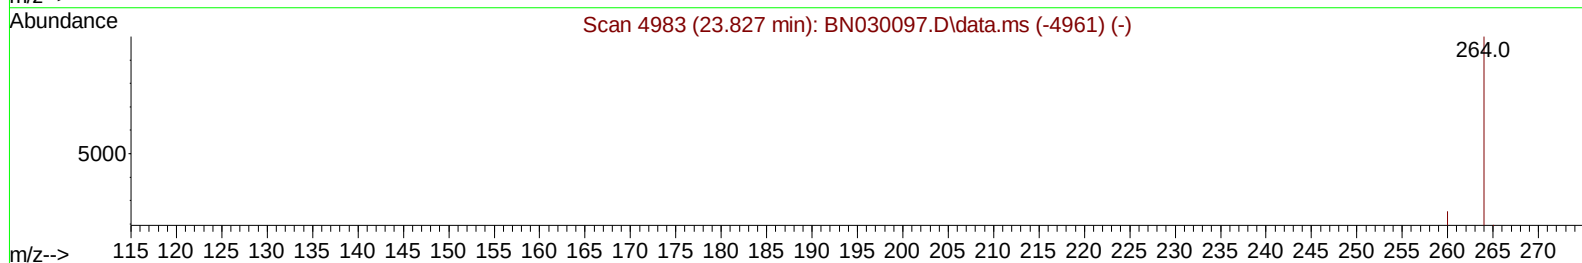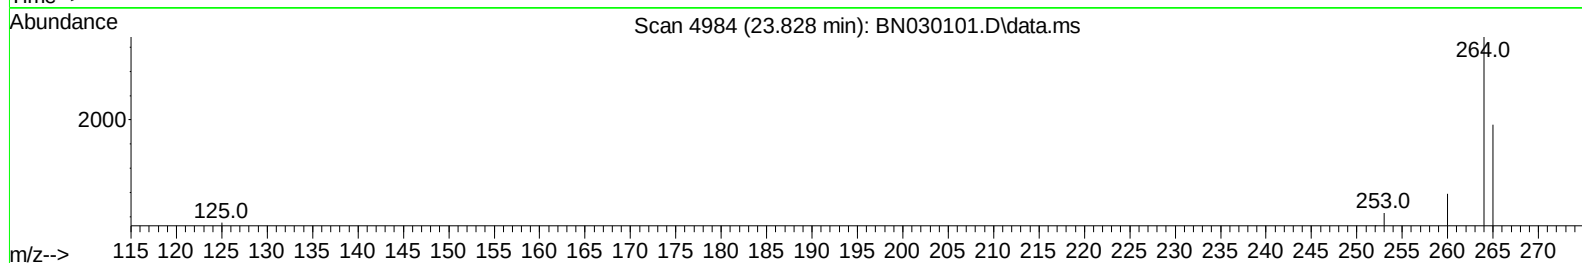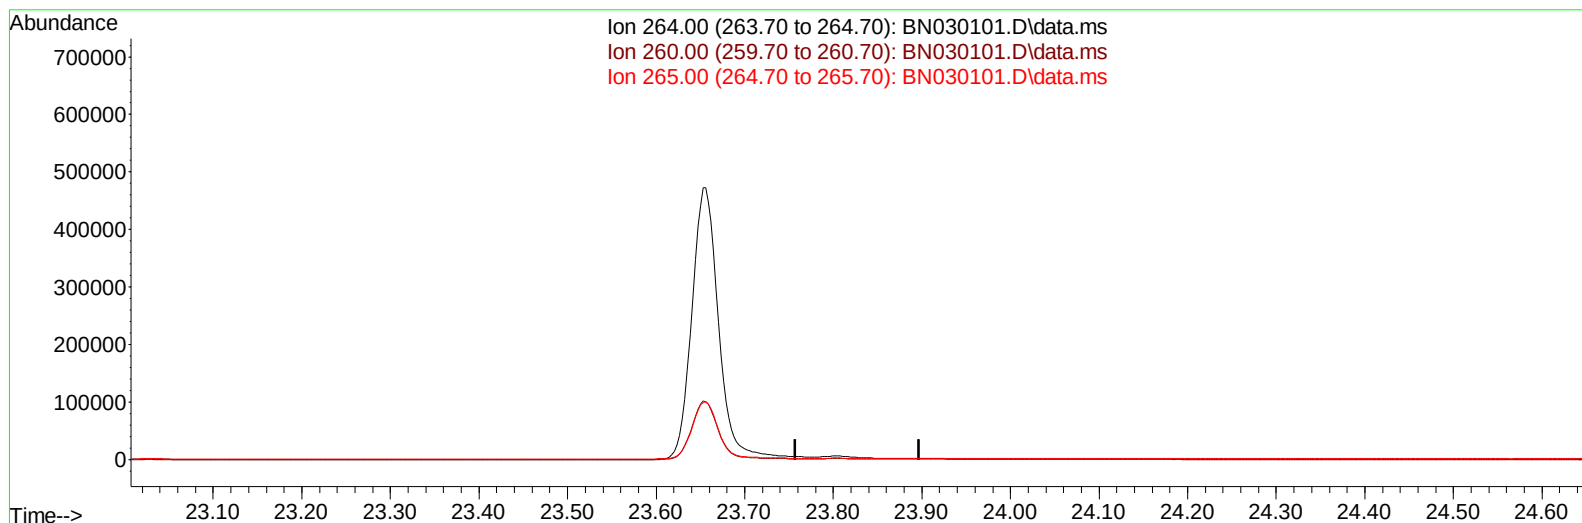

TIC: BN030101.D\data.ms

(23) Perylene-d12 (I)

23.827min (-23.827) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	25.70	0.00#
265.00	43.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030101.D
Acq On : 27 Feb 2024 20:43
Operator : MA/JU
Sample : P1508-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH403

Manual IntegrationsAPPROVED

Quant Time: Feb 27 23:51:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/28/2024
Supervised By :mohammad ahmed 03/01/2024

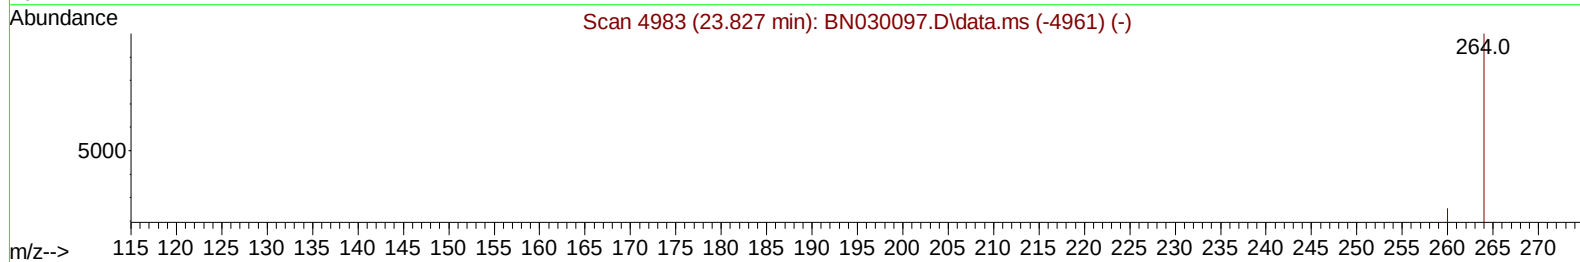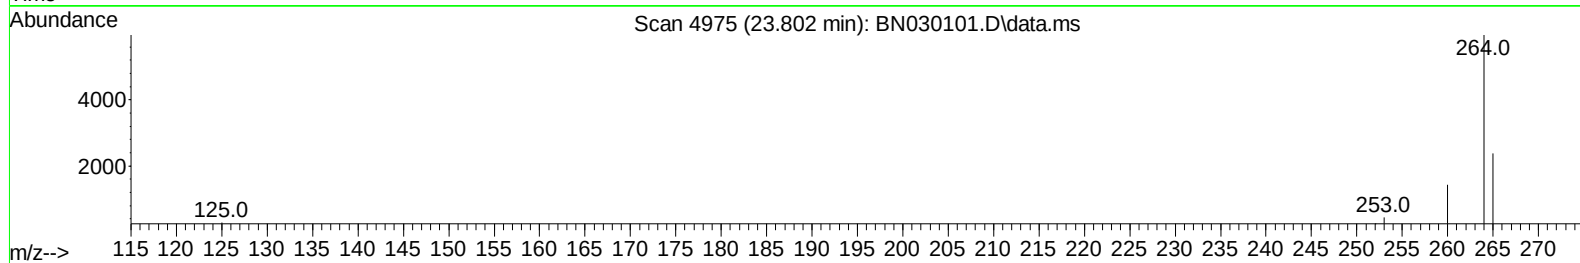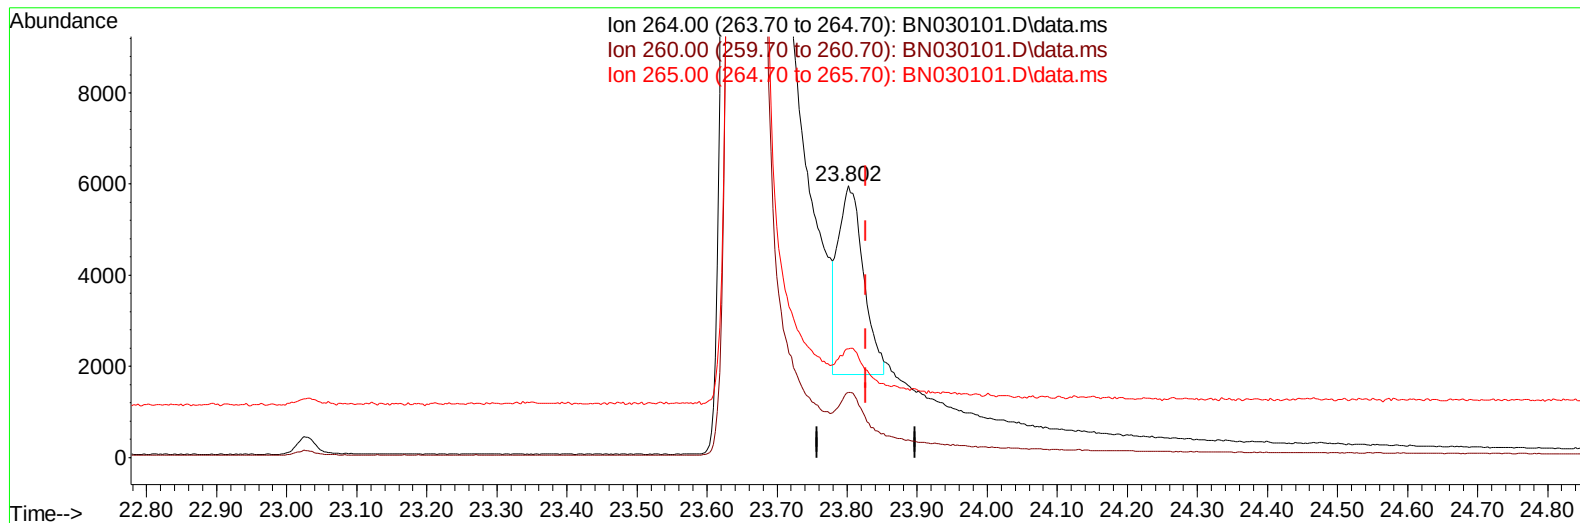

TIC: BN030101.D\data.ms

(23) Perylene-d12 (I)

23.802min (-0.025) 0.40 ng/ul m

response 10494

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.70	23.95
265.00	43.50	40.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
 Data File : BN030101.D
 Acq On : 27 Feb 2024 20:43
 Operator : MA/JU
 Sample : P1508-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH403

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/28/2024
 Supervised By :mohammad ahmed 03/01/2024

Quant Time: Feb 27 23:51:33 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 27 23:49:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.850	152	4122	0.400	ng/ul	0.00
4) Naphthalene-d8	10.643	136	12054	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.496	164	5819	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.249	188	10897	0.400	ng/ul	-0.01
17) Chrysene-d12	21.455	240	7010	0.400	ng/ul	-0.01
23) Perylene-d12	23.802	264	10494m	0.400	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.315	96	22901	4.456	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.243	152	6113	0.399	ng/ul	0.00
18) Fluoranthene-d10	19.283	212	11989	0.520	ng/ul	-0.01
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.353	88	373	0.067	ng/ul#	69

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030101.D
Acq On : 27 Feb 2024 20:43
Operator : MA/JU
Sample : P1508-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH403

Manual IntegrationsAPPROVED

Quant Time: Feb 27 23:51:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/28/2024
Supervised By :mohammad ahmed 03/01/2024

