




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030109.D
Acq On : 28 Feb 2024 01:33
Operator : MA/JU
Sample : P1526-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E10B7

Manual IntegrationsAPPROVED

Quant Time: Feb 28 01:59:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/28/2024
Supervised By :mohammad ahmed 03/01/2024

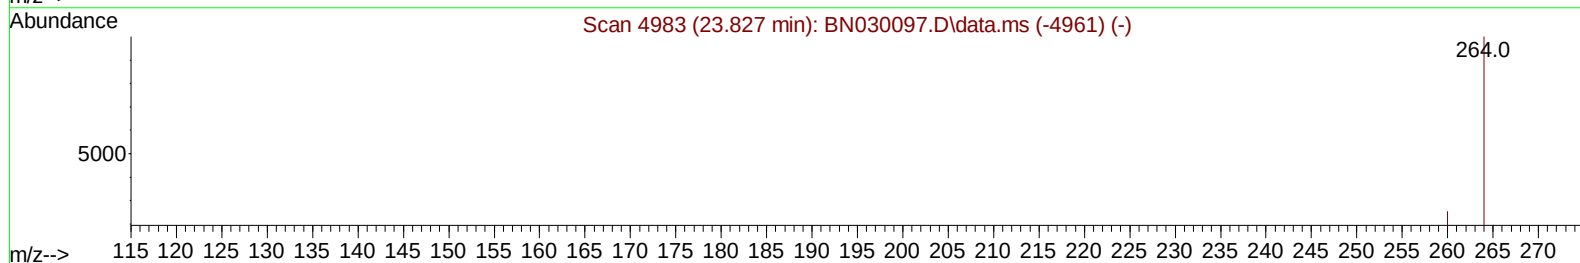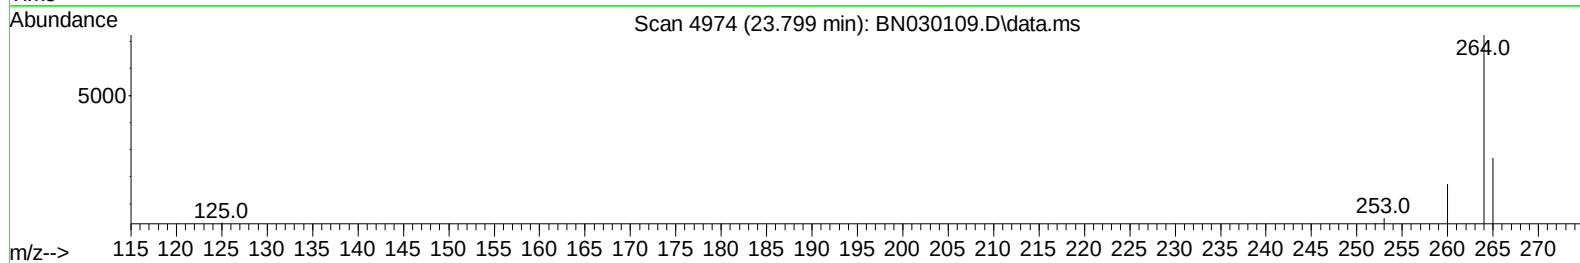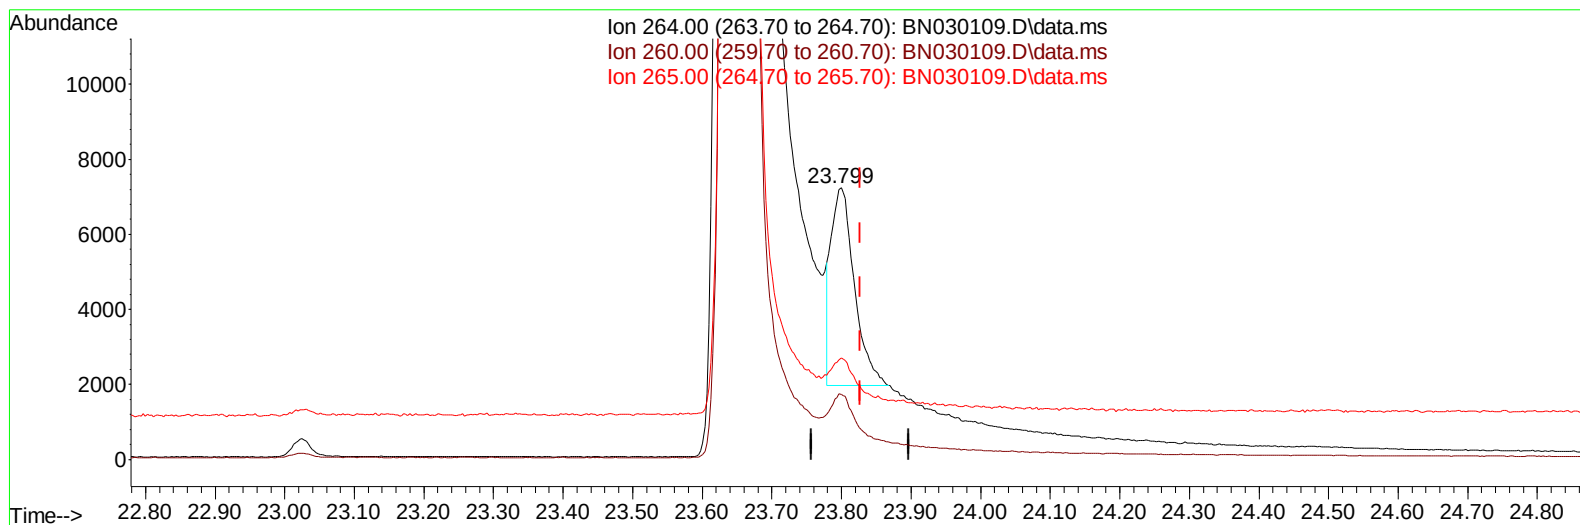

TIC: BN030109.D\data.ms

(23) Perylene-d12 (I)

23.799min (-0.028) 0.40 ng/u1

response 12252

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.70	23.93
265.00	43.50	37.27
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030109.D
Acq On : 28 Feb 2024 01:33
Operator : MA/JU
Sample : P1526-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E10B7

Manual IntegrationsAPPROVED

Quant Time: Feb 28 01:59:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/28/2024
Supervised By :mohammad ahmed 03/01/2024

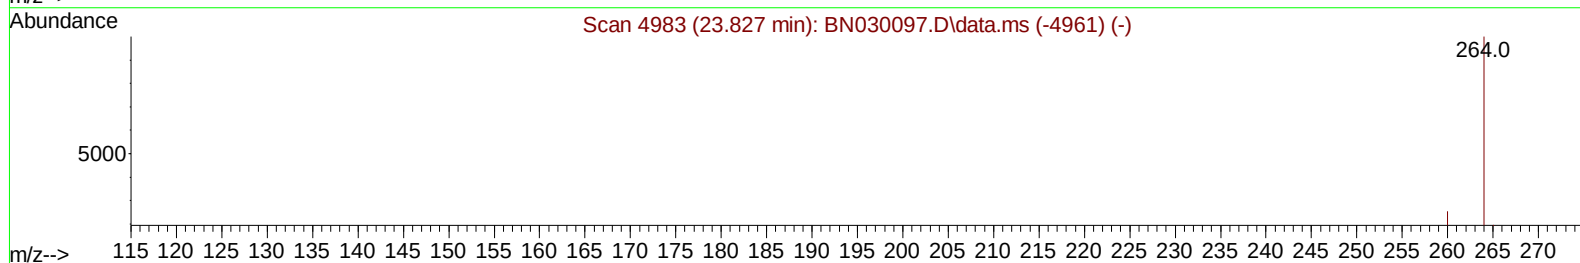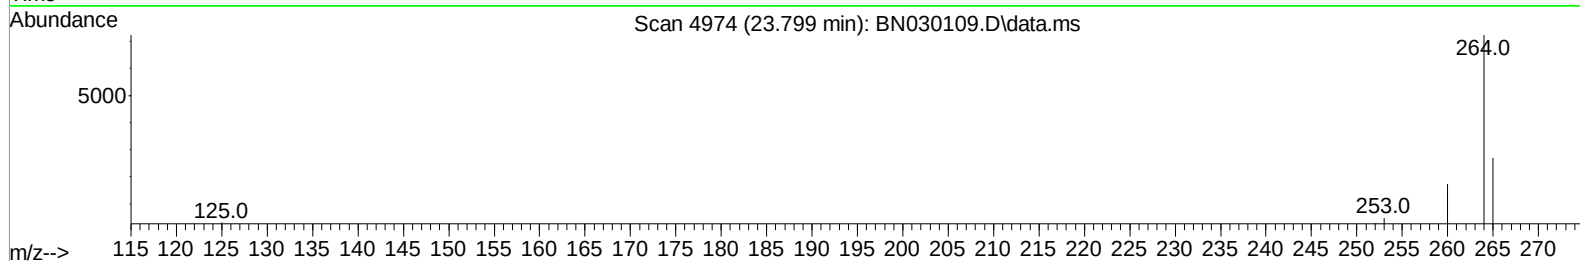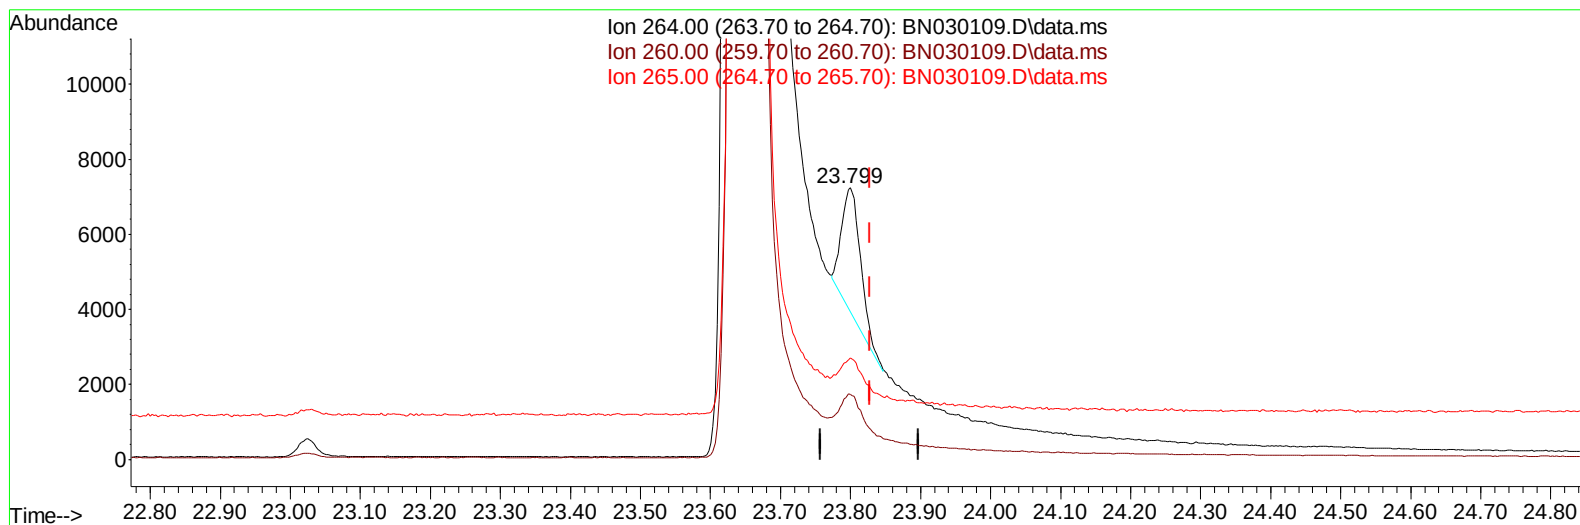

TIC: BN030109.D\data.ms

(23) Perylene-d12 (I)

23.799min (-0.028) 0.40 ng/ul m

response 5985

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.70	23.93
265.00	43.50	37.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
 Data File : BN030109.D
 Acq On : 28 Feb 2024 01:33
 Operator : MA/JU
 Sample : P1526-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E10B7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/28/2024
 Supervised By :mohammad ahmed 03/01/2024

Quant Time: Feb 28 01:59:47 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 27 23:49:29 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.851	152		3910	0.400	ng/ul	0.00
4) Naphthalene-d8	10.643	136		11194	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.496	164		5663	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.245	188		11324	0.400	ng/ul	-0.02
17) Chrysene-d12	21.452	240		8458	0.400	ng/ul	-0.01
23) Perylene-d12	23.799	264		5985m	0.400	ng/ul	-0.03
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.315	96		21374	4.384	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.244	152		5947	0.418	ng/ul	0.00
18) Fluoranthene-d10	19.279	212		13725	0.494	ng/ul	-0.02
Target Compounds							Qvalue
5) Naphthalene	10.693	128		806	0.026	ng/ul#	72

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030109.D
Acq On : 28 Feb 2024 01:33
Operator : MA/JU
Sample : P1526-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E10B7

Manual IntegrationsAPPROVED

Quant Time: Feb 28 01:59:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/28/2024
Supervised By :mohammad ahmed 03/01/2024

