




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
 Data File : BN030116.D
 Acq On : 28 Feb 2024 06:23
 Operator : MA/JU
 Sample : PB159258BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK258

Manual IntegrationsAPPROVED

Quant Time: Feb 28 06:50:55 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 27 23:49:29 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/28/2024
 Supervised By :mohammad ahmed 03/01/2024

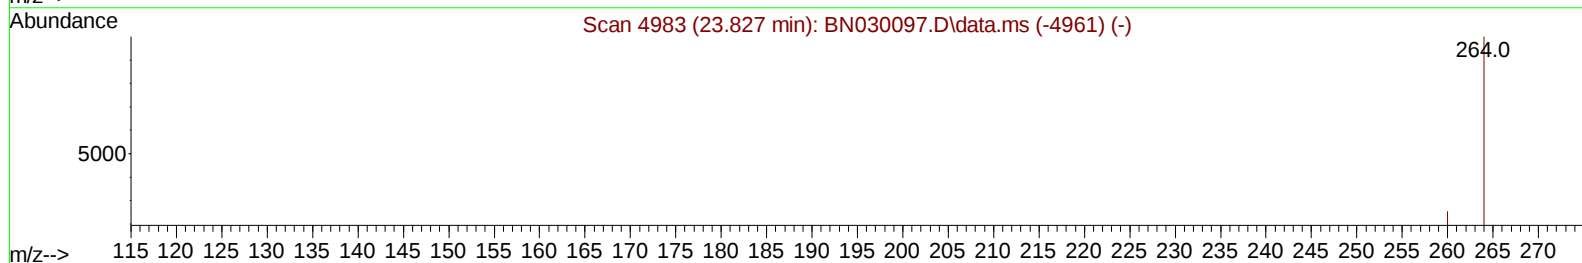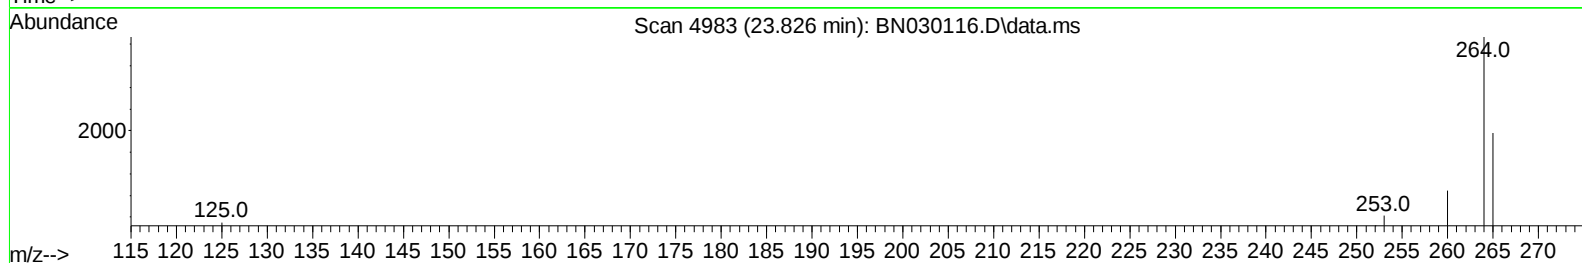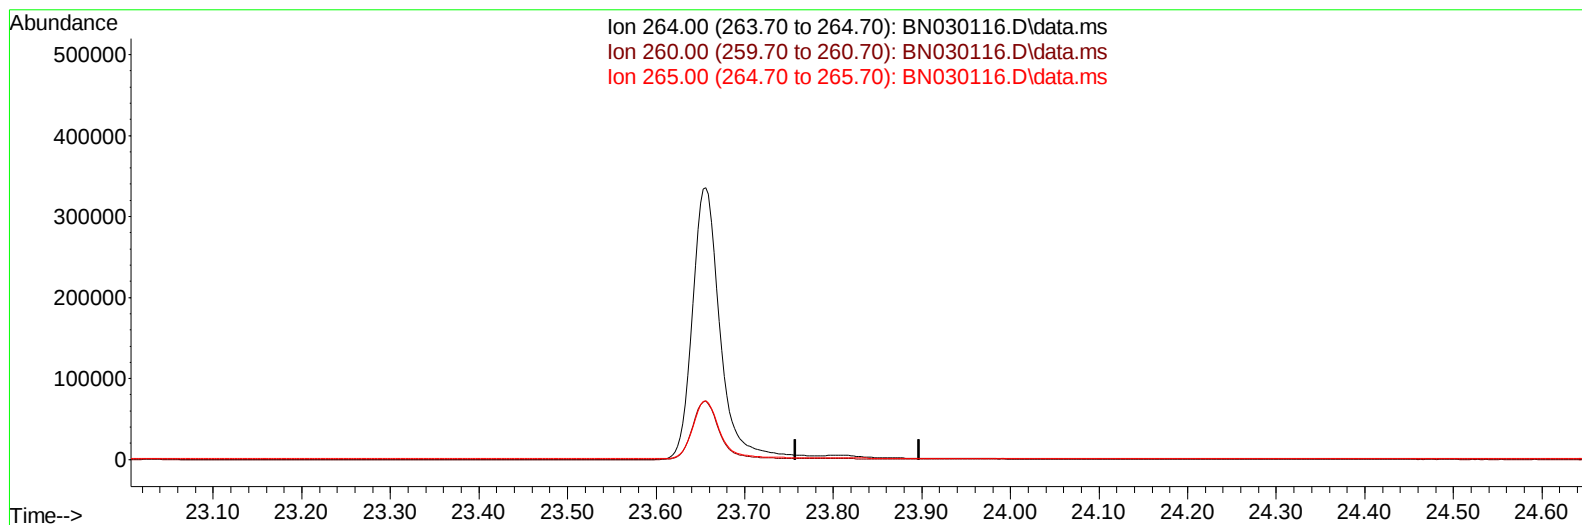

TIC: BN030116.D\data.ms

(23) Perylene-d12 (I)

23.827min (-23.827) 0.00 ng/u1

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	25.70	0.00#
265.00	43.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030116.D
Acq On : 28 Feb 2024 06:23
Operator : MA/JU
Sample : PB159258BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK258

Manual IntegrationsAPPROVED

Quant Time: Feb 28 06:50:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/28/2024
Supervised By :mohammad ahmed 03/01/2024

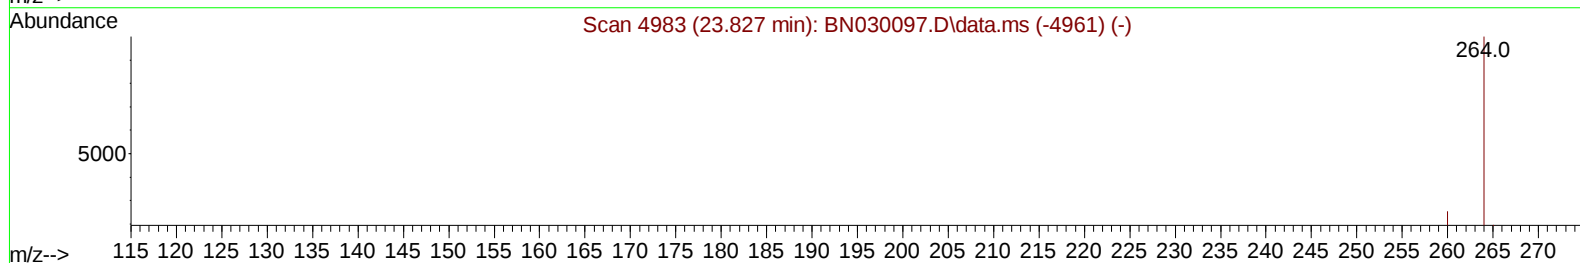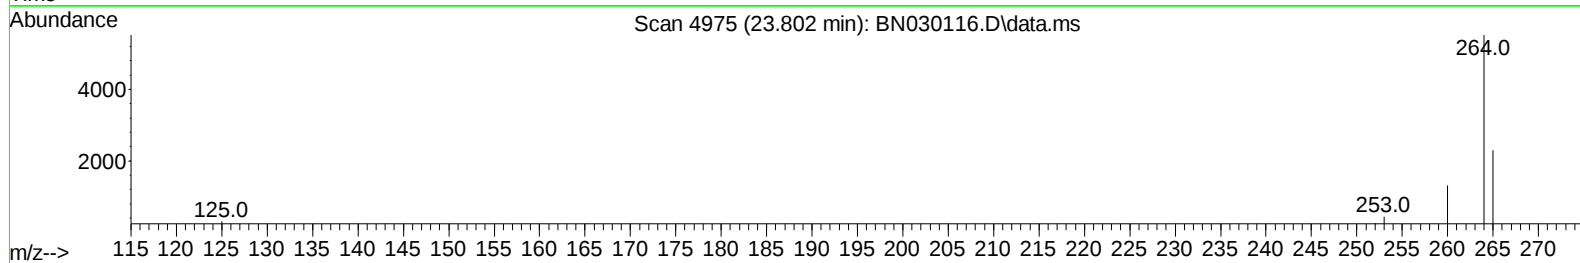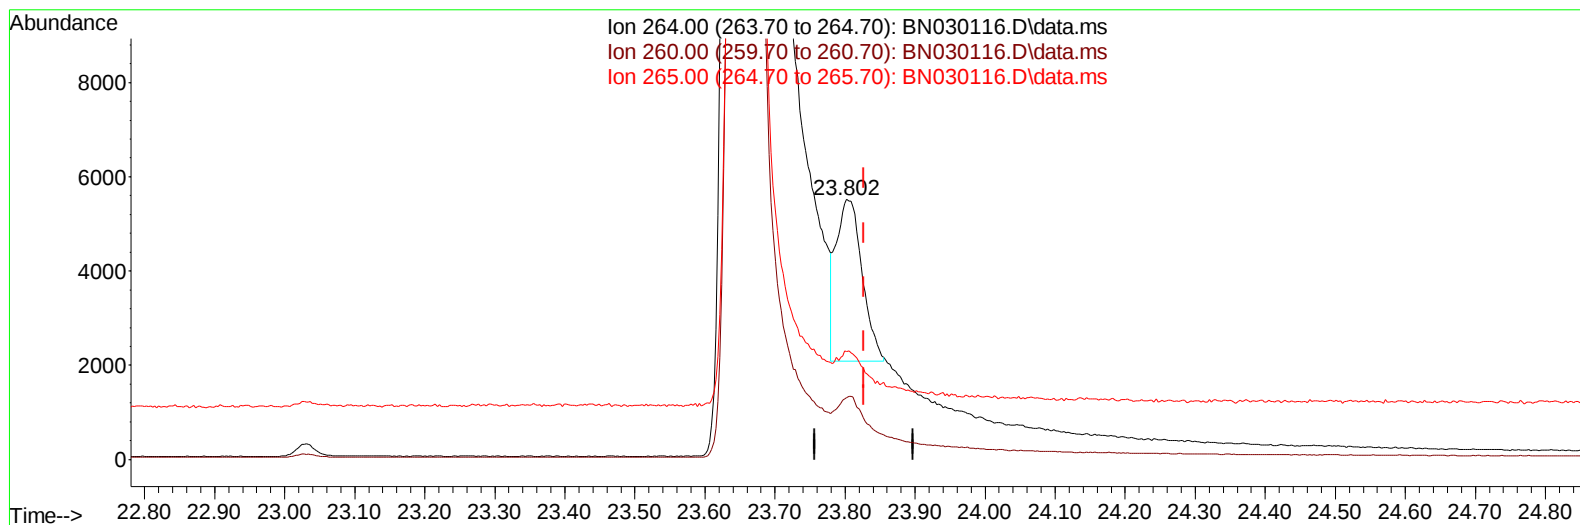

TIC: BN030116.D\data.ms

(23) Perylene-d12 (I)

23.802min (-0.025) 0.40 ng/ul m

response 8917

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.70	23.81
265.00	43.50	41.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
 Data File : BN030116.D
 Acq On : 28 Feb 2024 06:23
 Operator : MA/JU
 Sample : PB159258BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK258

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/28/2024
 Supervised By :mohammad ahmed 03/01/2024

Quant Time: Feb 28 06:50:55 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 27 23:49:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.851	152	4097	0.400	ng/ul	0.00
4) Naphthalene-d8	10.645	136	11982	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.493	164	5866	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.247	188	11156	0.400	ng/ul	-0.02
17) Chrysene-d12	21.458	240	6482	0.400	ng/ul	0.00
23) Perylene-d12	23.802	264	8917m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.311	96	35200	6.890	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.245	152	5594	0.367	ng/ul	0.00
18) Fluoranthene-d10	19.281	212	8922	0.419	ng/ul	-0.01

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030116.D
Acq On : 28 Feb 2024 06:23
Operator : MA/JU
Sample : PB159258BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK258

Manual IntegrationsAPPROVED

Quant Time: Feb 28 06:50:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/28/2024
Supervised By :mohammad ahmed 03/01/2024

