




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
 Data File : BN030123.D
 Acq On : 28 Feb 2024 10:37
 Operator : MA/JU
 Sample : P1526-02
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E10A5

Manual IntegrationsAPPROVED

Quant Time: Feb 28 11:44:23 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 27 23:49:29 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/29/2024
 Supervised By :mohammad ahmed 03/01/2024

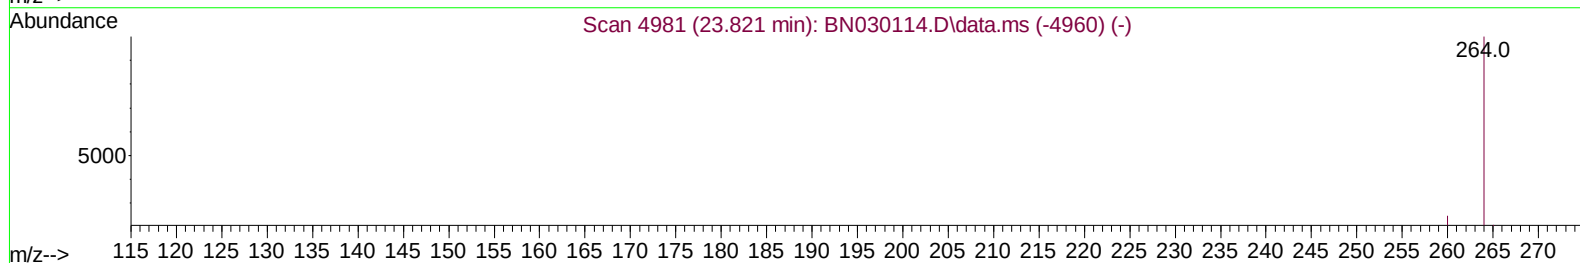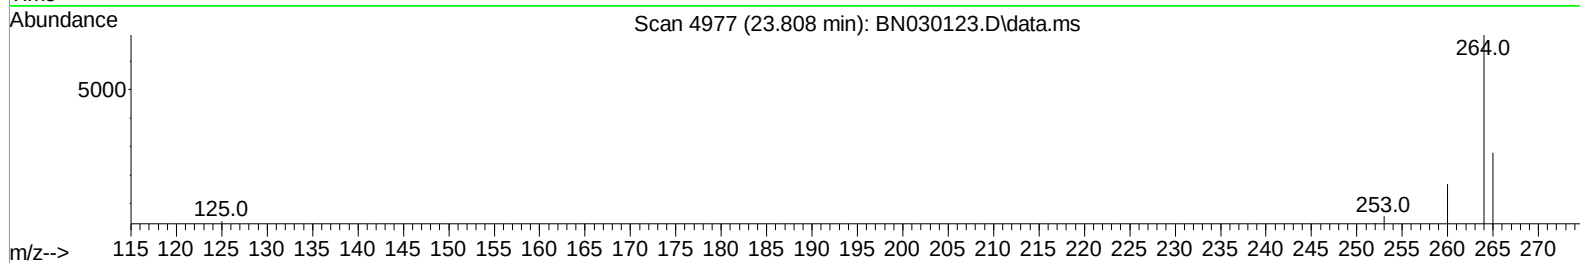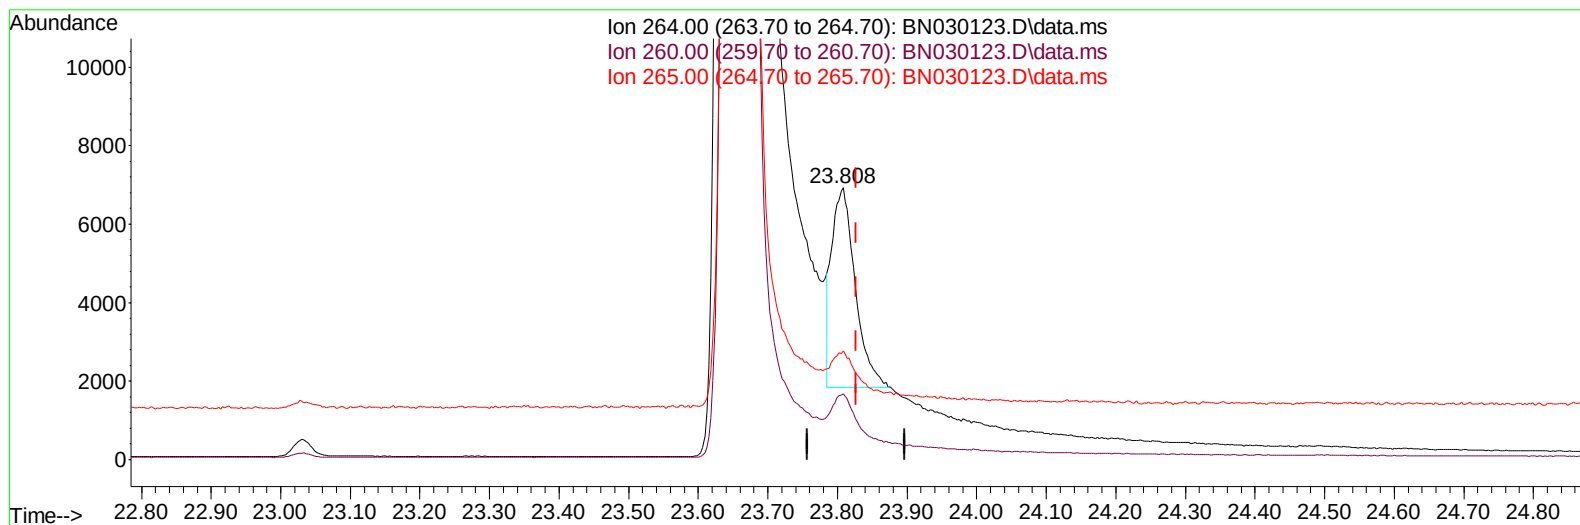

TIC: BN030123.D\data.ms

(23) Perylene-d12 (I)

23.808min (-0.019) 0.40 ng/uL

response 11911

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.70	24.19
265.00	43.50	40.02
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030123.D
Acq On : 28 Feb 2024 10:37
Operator : MA/JU
Sample : P1526-02
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E10A5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/29/2024
Supervised By :mohammad ahmed 03/01/2024

Quant Time: Feb 28 11:44:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

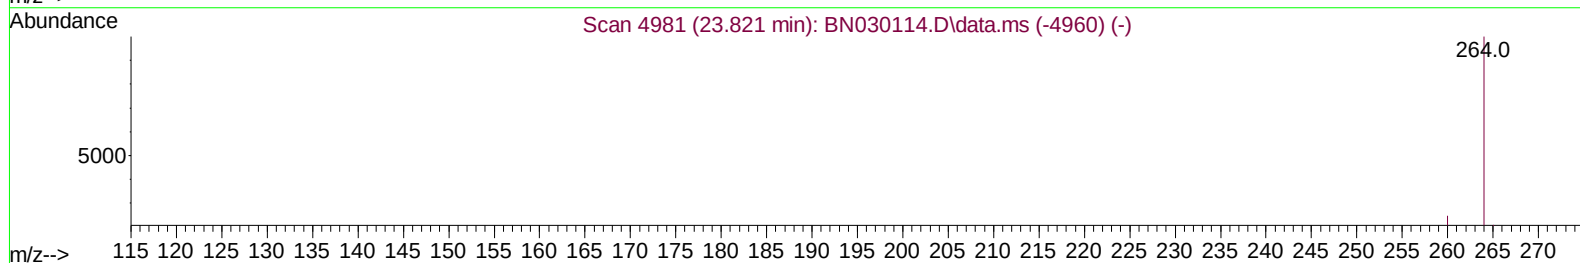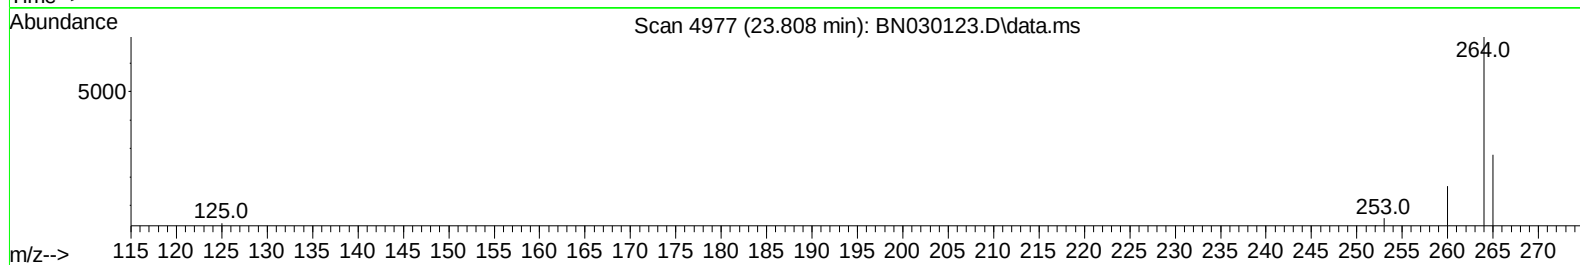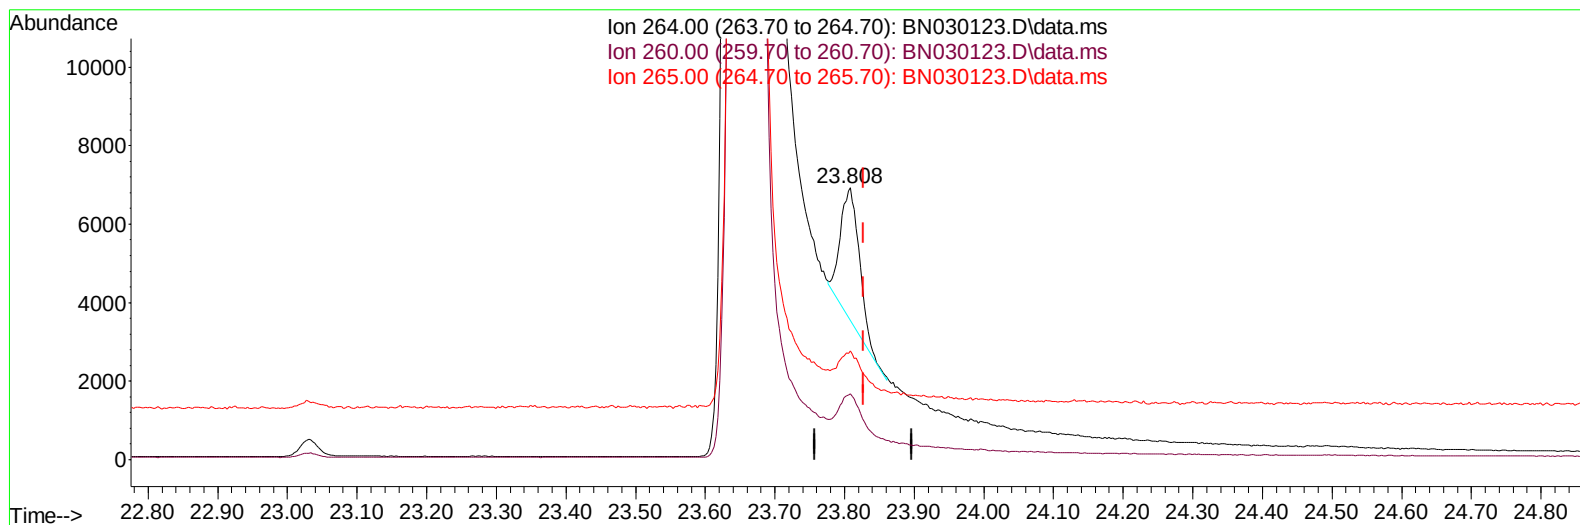

TIC: BN030123.D\data.ms

(23) Perylene-d12 (I)

23.808min (-0.019) 0.40 ng/ul m

response 6101

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.70	24.19
265.00	43.50	40.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
 Data File : BN030123.D
 Acq On : 28 Feb 2024 10:37
 Operator : MA/JU
 Sample : P1526-02
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E10A5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/29/2024
 Supervised By :mohammad ahmed 03/01/2024

Quant Time: Feb 28 11:44:23 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 27 23:49:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.851	152	4220	0.400	ng/ul	0.00
4) Naphthalene-d8	10.645	136	16061	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.497	164	7982	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.247	188	14738	0.400	ng/ul	-0.02
17) Chrysene-d12	21.455	240	8765	0.400	ng/ul	-0.01
23) Perylene-d12	23.808	264	6101m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.315	96	27173	5.164	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.245	152	7387	0.361	ng/ul	0.00
18) Fluoranthene-d10	19.281	212	14434	0.501	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030123.D
Acq On : 28 Feb 2024 10:37
Operator : MA/JU
Sample : P1526-02
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E10A5

Manual IntegrationsAPPROVED

Quant Time: Feb 28 11:44:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/29/2024
Supervised By :mohammad ahmed 03/01/2024

