




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030128.D
Acq On : 28 Feb 2024 13:37
Operator : MA/JU
Sample : P1498-13
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD2

Manual IntegrationsAPPROVED

Quant Time: Feb 28 14:05:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/29/2024
Supervised By :mohammad ahmed 03/01/2024

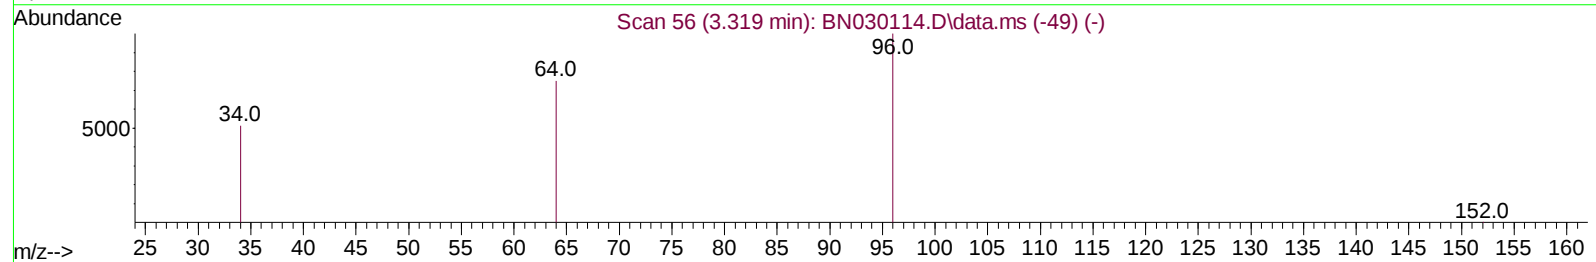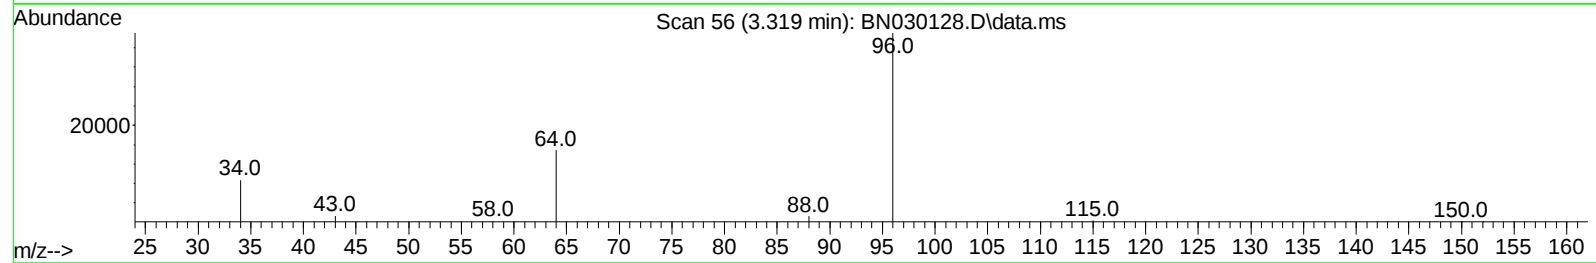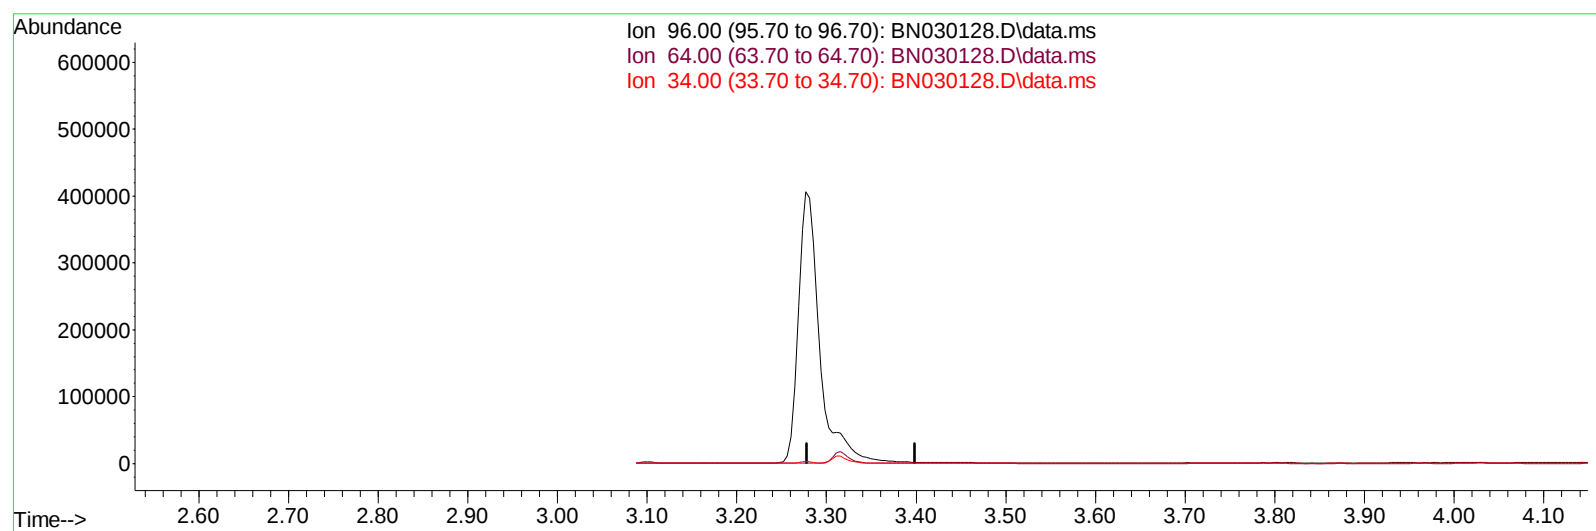

TIC: BN030128.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.319min (-3.319) 0.00 ng/u1

response 0

Ion	Exp%	Act%
96.00	100.00	0.00
64.00	69.60	0.00#
34.00	42.70	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030128.D
Acq On : 28 Feb 2024 13:37
Operator : MA/JU
Sample : P1498-13
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD2

Manual IntegrationsAPPROVED

Quant Time: Feb 28 14:05:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/29/2024
Supervised By :mohammad ahmed 03/01/2024

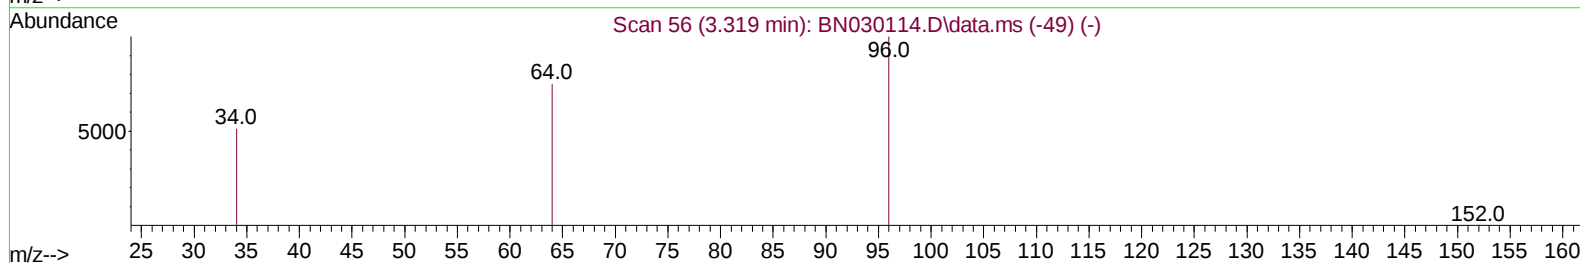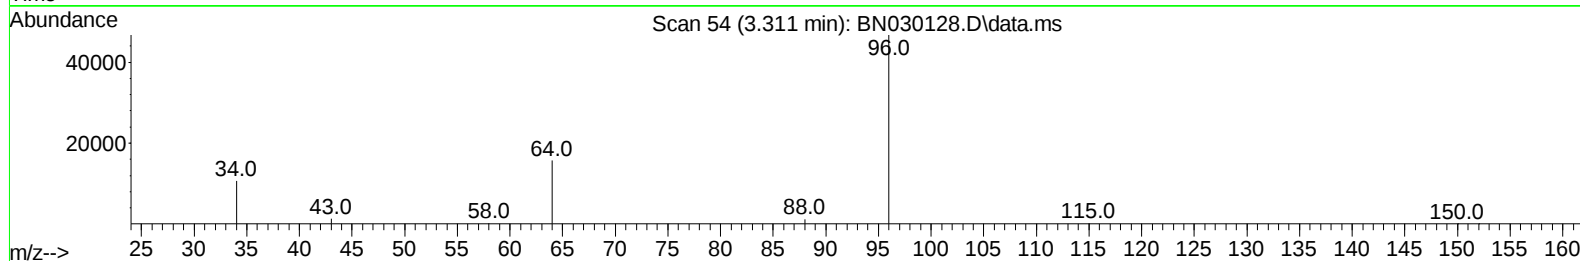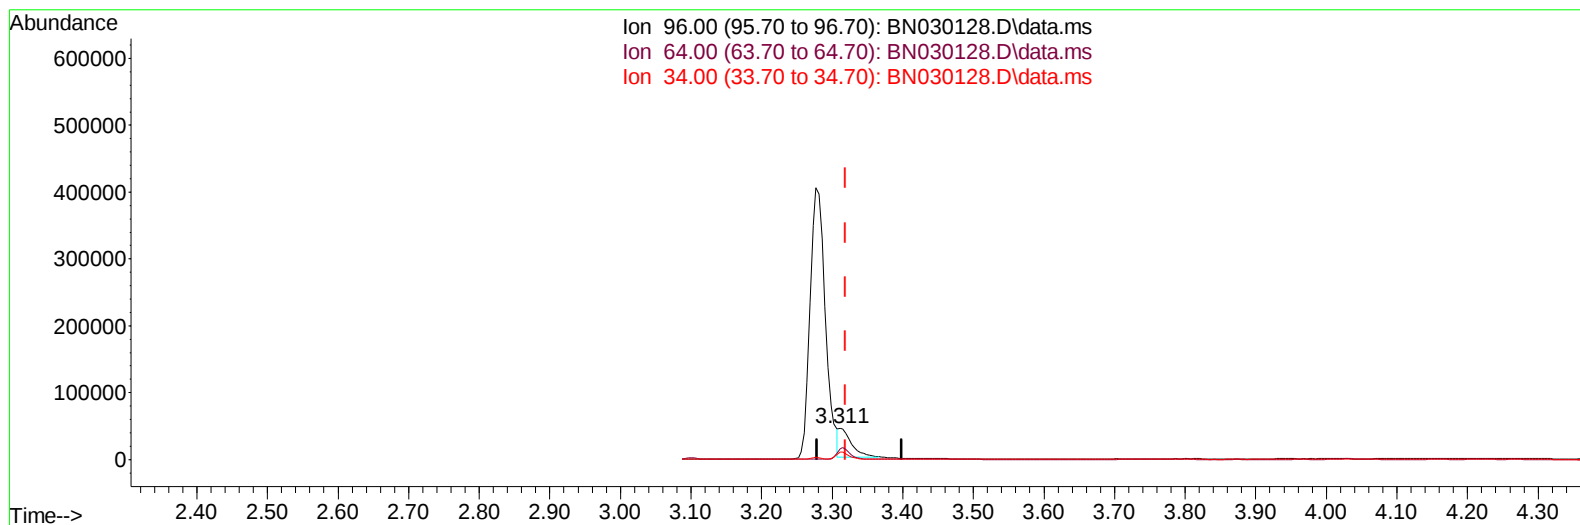

TIC: BN030128.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.311min (-0.008) 8.42 ng/ul m

response 52610

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	69.60	33.68#
34.00	42.70	23.02#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
 Data File : BN030128.D
 Acq On : 28 Feb 2024 13:37
 Operator : MA/JU
 Sample : P1498-13
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/29/2024
 Supervised By :mohammad ahmed 03/01/2024

Quant Time: Feb 28 14:05:28 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 27 23:49:29 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.855	152		5008	0.400	ng/ul	0.00
4) Naphthalene-d8	10.645	136		15192	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.497	164		7592	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.247	188		14777	0.400	ng/ul	-0.02
17) Chrysene-d12	21.449	240		10424	0.400	ng/ul	-0.02
23) Perylene-d12	23.808	264		11959	0.400	ng/ul	-0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.311	96		52610m	8.425	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.240	152		9062	0.469	ng/ul	0.00
18) Fluoranthene-d10	19.281	212		16214	0.473	ng/ul	-0.01
Target Compounds							Qvalue
2) 1,4-Dioxane	3.353	88		8740	1.286	ng/ul#	69

(#) = qualifier out of range (m) = manual integration (+) = signals summed

