




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030150.D
Acq On : 29 Feb 2024 04:03
Operator : MA/JU
Sample : PB159153BL
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK153

Manual IntegrationsAPPROVED

Quant Time: Feb 29 04:40:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/29/2024
Supervised By :mohammad ahmed 03/01/2024

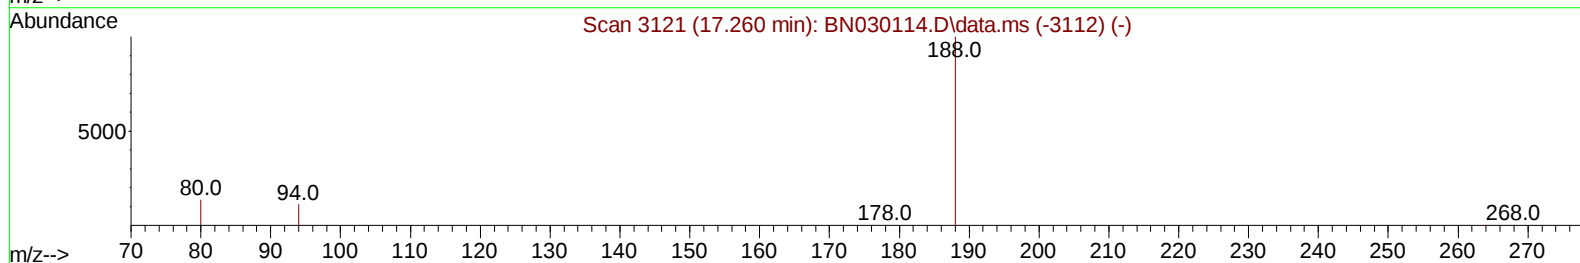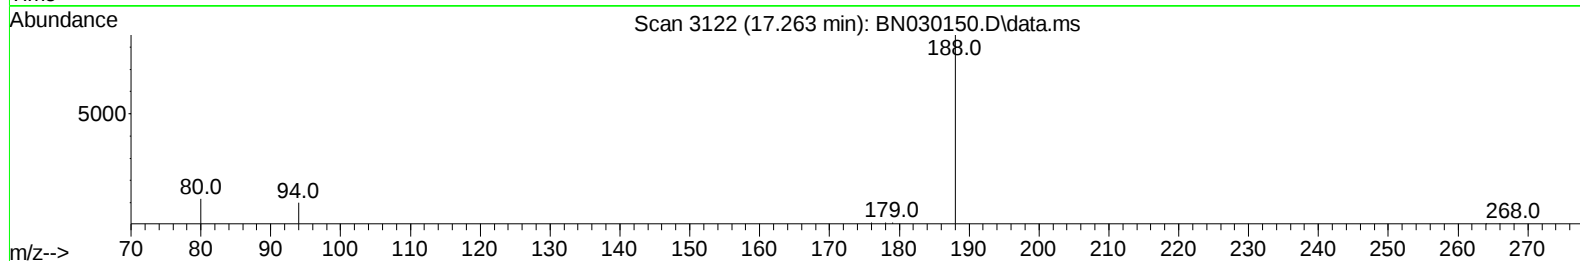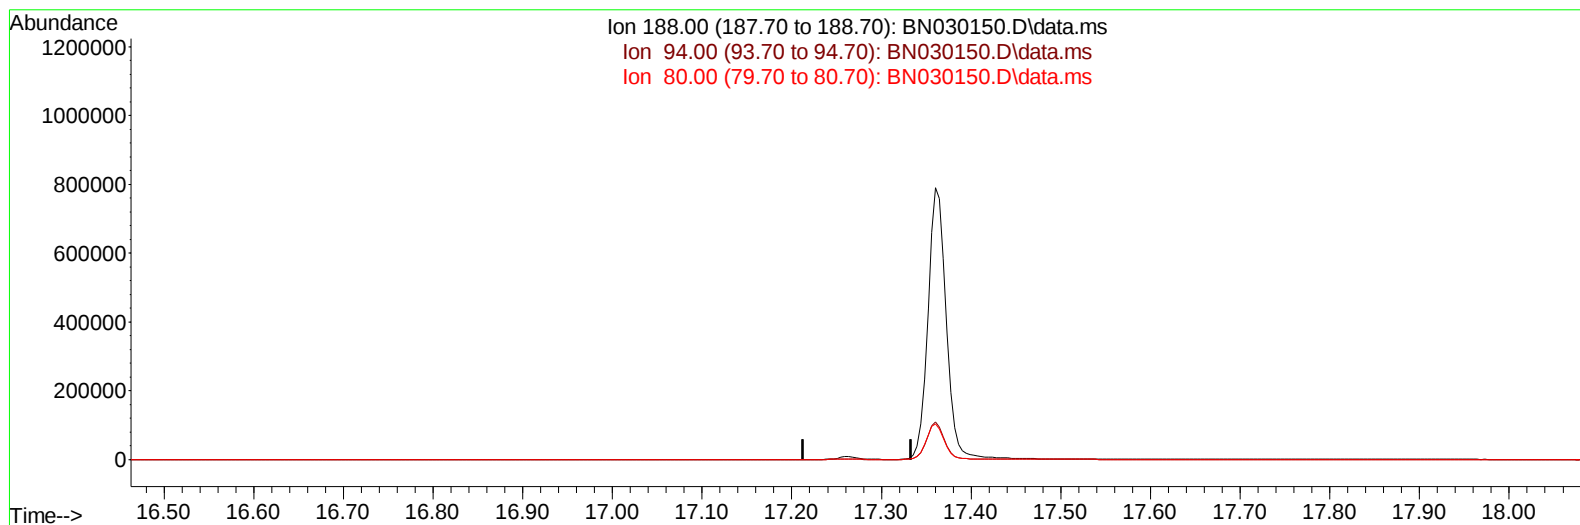

TIC: BN030150.D\data.ms

(13) Phenanthrene-d10 (I)

17.263min (-17.263) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	12.00	0.00#
80.00	13.70	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030150.D
Acq On : 29 Feb 2024 04:03
Operator : MA/JU
Sample : PB159153BL
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK153

Manual IntegrationsAPPROVED

Quant Time: Feb 29 04:40:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/29/2024
Supervised By :mohammad ahmed 03/01/2024

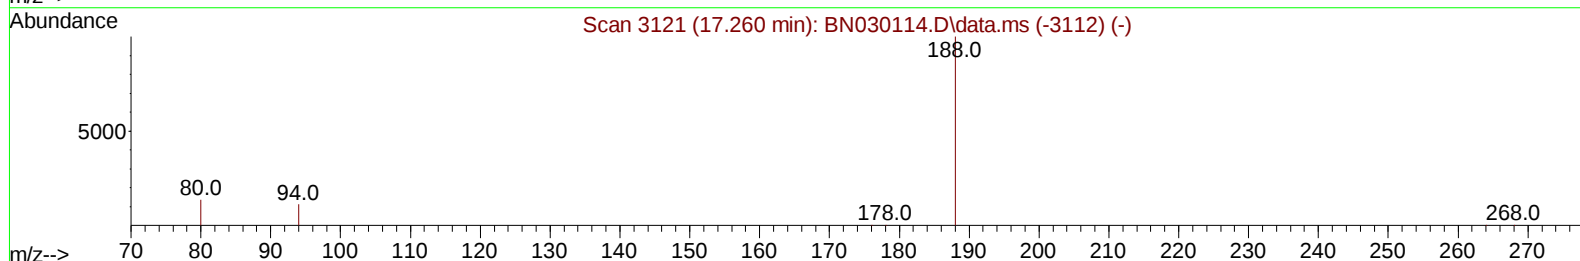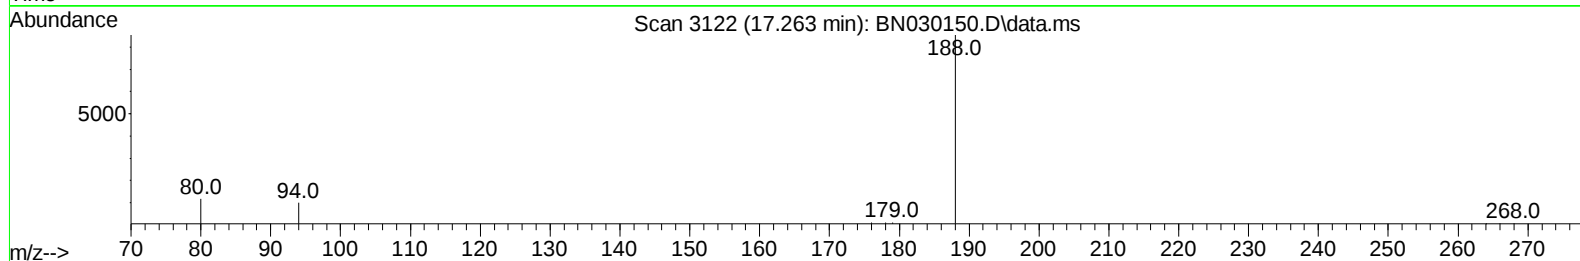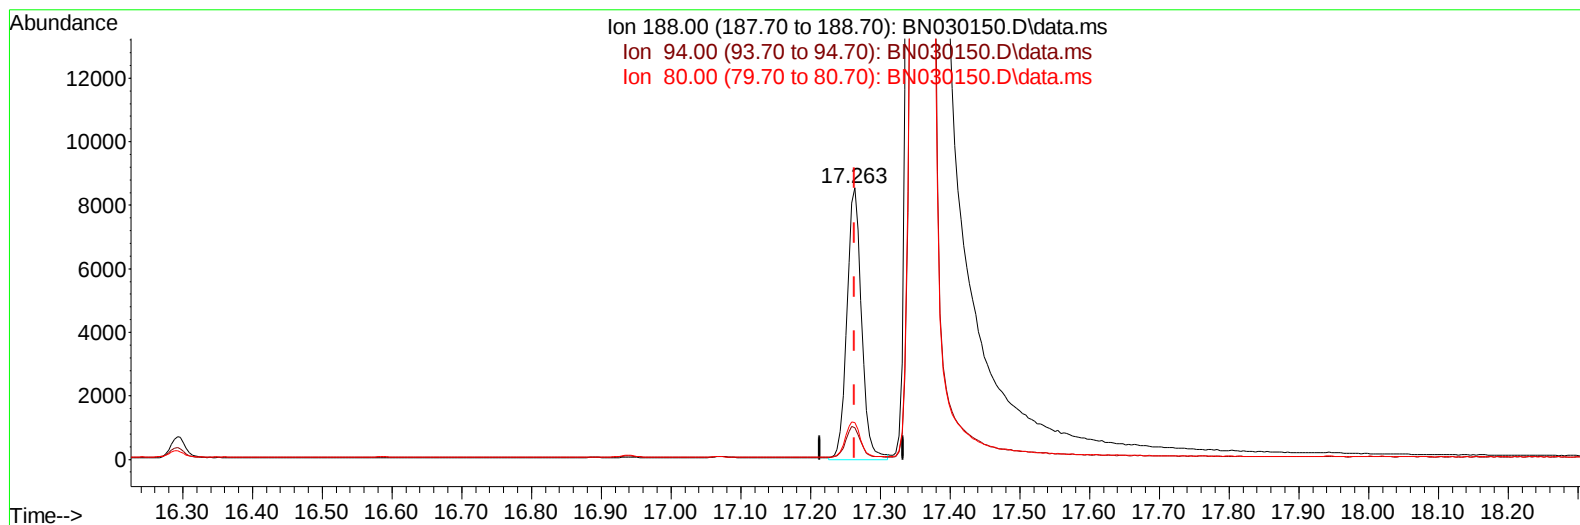

TIC: BN030150.D\data.ms

(13) Phenanthrene-d10 (I)

17.263min (+ 0.000) 0.40 ng/u1 m

response 12401

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.00	11.70
80.00	13.70	13.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
 Data File : BN030150.D
 Acq On : 29 Feb 2024 04:03
 Operator : MA/JU
 Sample : PB159153BL
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK153

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/29/2024
 Supervised By :mohammad ahmed 03/01/2024

Quant Time: Feb 29 04:40:01 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 27 23:49:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.867	152	4151	0.400	ng/ul	0.01
4) Naphthalene-d8	10.661	136	12147	0.400	ng/ul #	0.01
9) Acenaphthene-d10	14.511	164	6105	0.400	ng/ul #	0.01
13) Phenanthrene-d10	17.263	188	12401m	0.400	ng/ul	0.00
17) Chrysene-d12	21.470	240	7620	0.400	ng/ul	0.00
23) Perylene-d12	23.826	264	9798	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.319	96	39642	7.659	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.261	152	4526	0.293	ng/ul	0.02
18) Fluoranthene-d10	19.295	212	11216	0.448	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030150.D
Acq On : 29 Feb 2024 04:03
Operator : MA/JU
Sample : PB159153BL
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK153

Manual IntegrationsAPPROVED

Quant Time: Feb 29 04:40:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/29/2024
Supervised By :mohammad ahmed 03/01/2024

