




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030151.D
Acq On : 29 Feb 2024 04:39
Operator : MA/JU
Sample : P1494-14
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3W6

Manual IntegrationsAPPROVED

Quant Time: Feb 29 05:13:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/29/2024
Supervised By :mohammad ahmed 03/01/2024

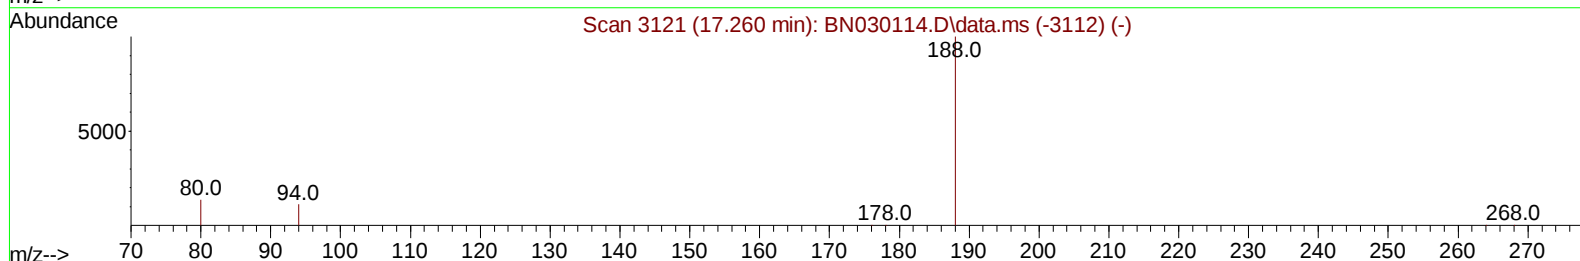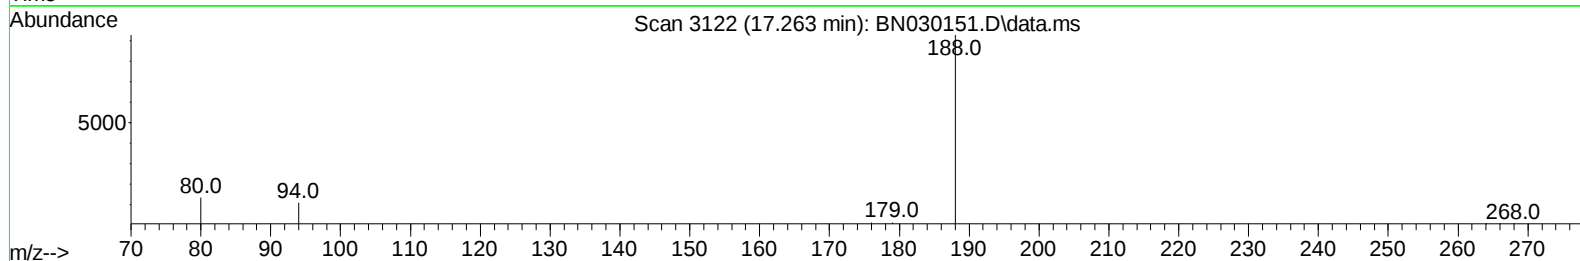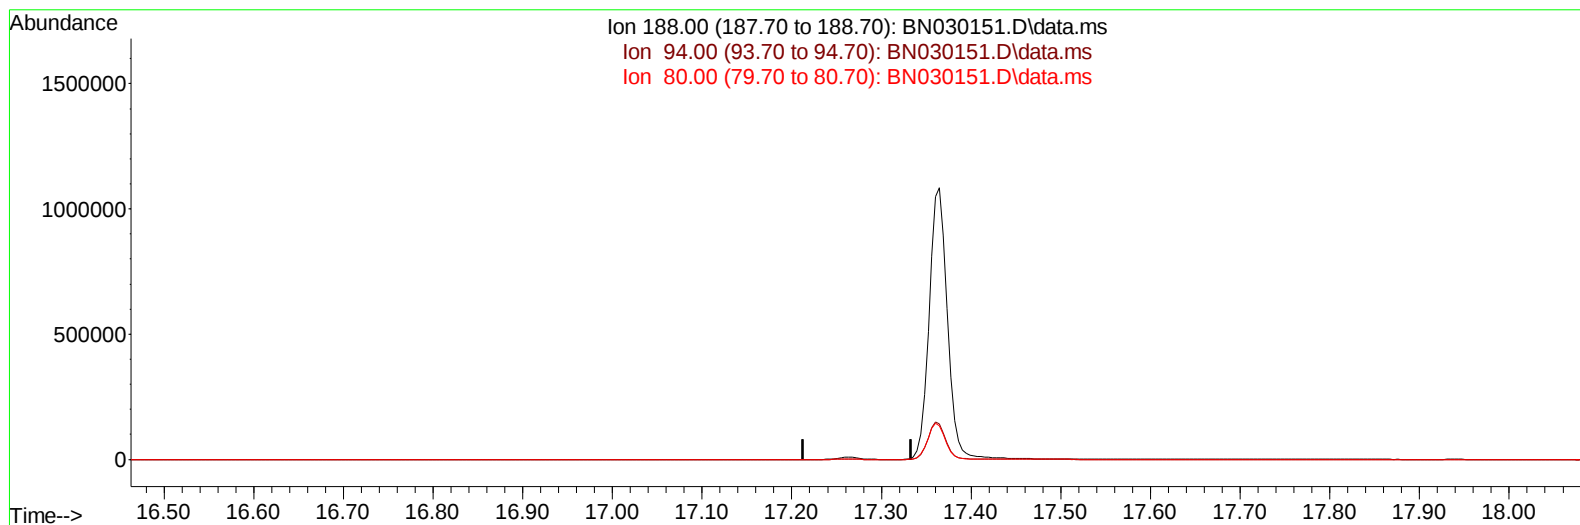

TIC: BN030151.D\data.ms

(13) Phenanthrene-d10 (I)

17.263min (-17.263) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	12.00	0.00#
80.00	13.70	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030151.D
Acq On : 29 Feb 2024 04:39
Operator : MA/JU
Sample : P1494-14
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3W6

Manual IntegrationsAPPROVED

Quant Time: Feb 29 05:13:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/29/2024
Supervised By :mohammad ahmed 03/01/2024

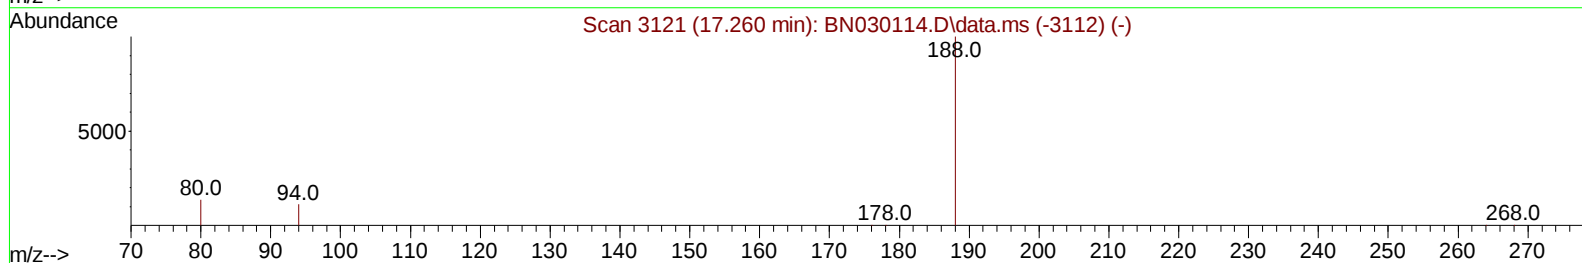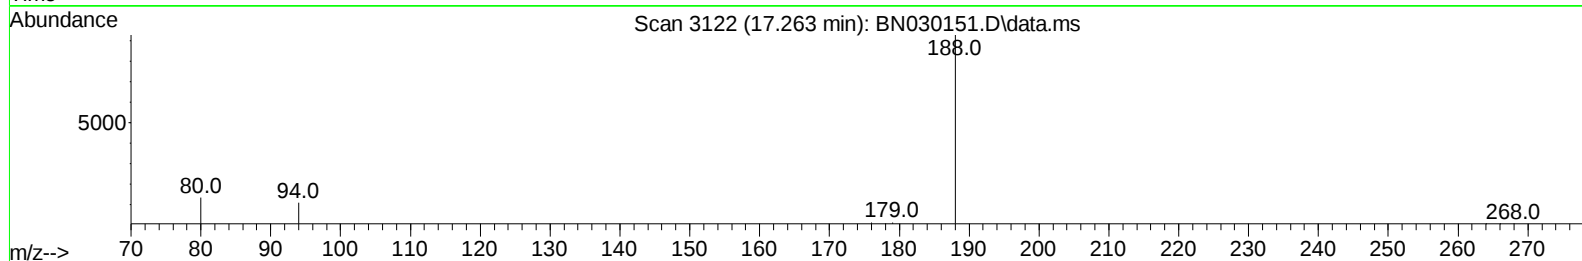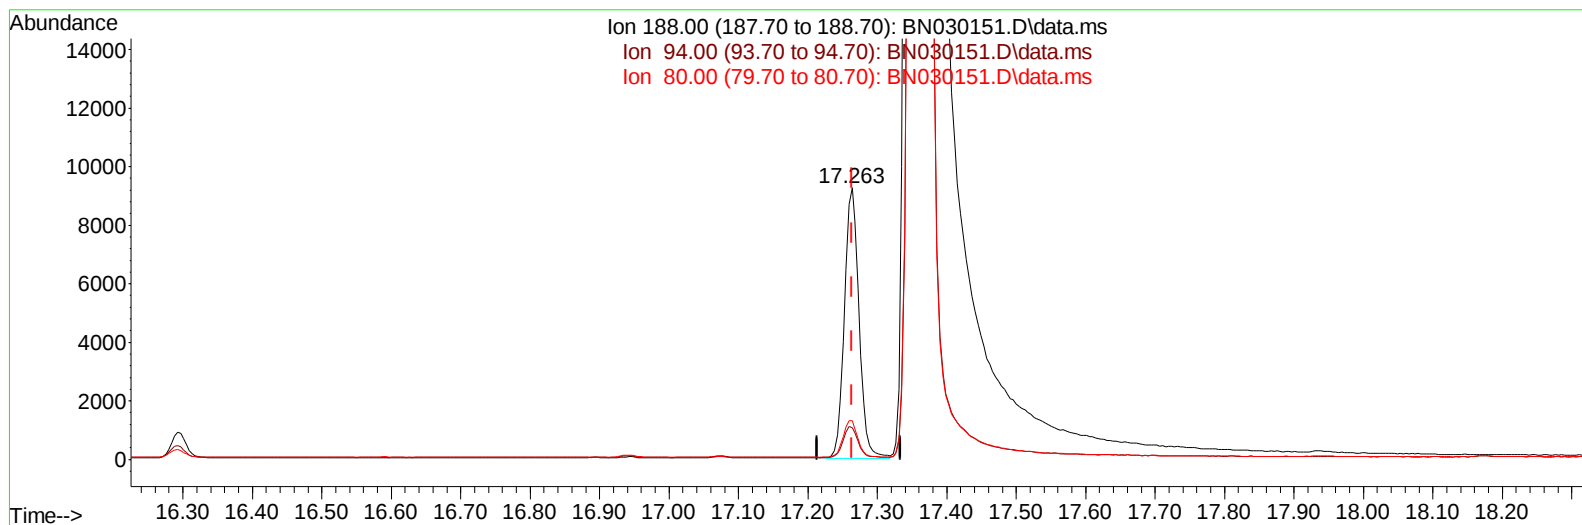

TIC: BN030151.D\data.ms

(13) Phenanthrene-d10 (I)

17.263min (+ 0.000) 0.40 ng/ul m

response 13492

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.00	11.58
80.00	13.70	14.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
 Data File : BN030151.D
 Acq On : 29 Feb 2024 04:39
 Operator : MA/JU
 Sample : P1494-14
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH3W6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/29/2024
 Supervised By :mohammad ahmed 03/01/2024

Quant Time: Feb 29 05:13:39 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 27 23:49:29 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.867	152		4196	0.400	ng/ul	0.01
4) Naphthalene-d8	10.667	136		12977	0.400	ng/ul	0.02
9) Acenaphthene-d10	14.511	164		6841	0.400	ng/ul	# 0.01
13) Phenanthrene-d10	17.263	188		13492m	0.400	ng/ul	0.00
17) Chrysene-d12	21.470	240		7310	0.400	ng/ul	0.00
23) Perylene-d12	23.826	264		8297	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.319	96		27921	5.337	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.262	152		8226	0.498	ng/ul	0.02
18) Fluoranthene-d10	19.295	212		15107	0.629	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030151.D
Acq On : 29 Feb 2024 04:39
Operator : MA/JU
Sample : P1494-14
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3W6

Manual IntegrationsAPPROVED

Quant Time: Feb 29 05:13:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/29/2024
Supervised By :mohammad ahmed 03/01/2024

