




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030154.D
Acq On : 29 Feb 2024 06:27
Operator : MA/JU
Sample : P1494-08
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH410

Manual IntegrationsAPPROVED

Quant Time: Feb 29 06:53:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/29/2024
Supervised By :mohammad ahmed 03/01/2024

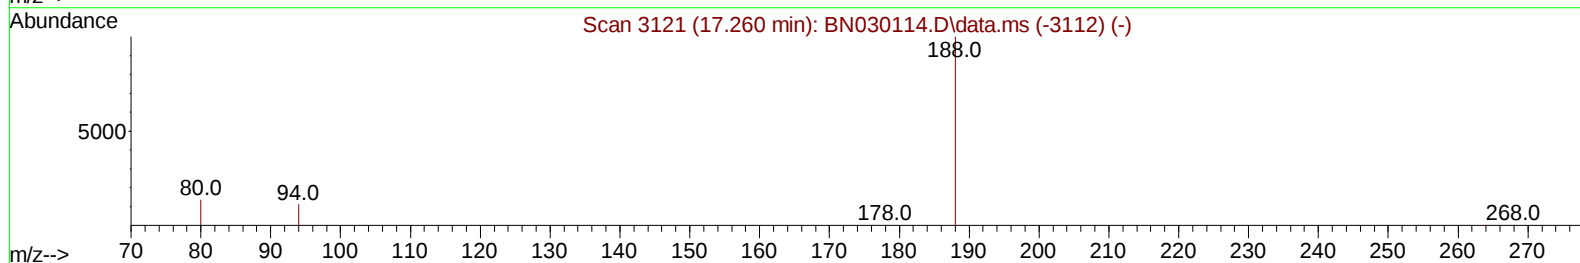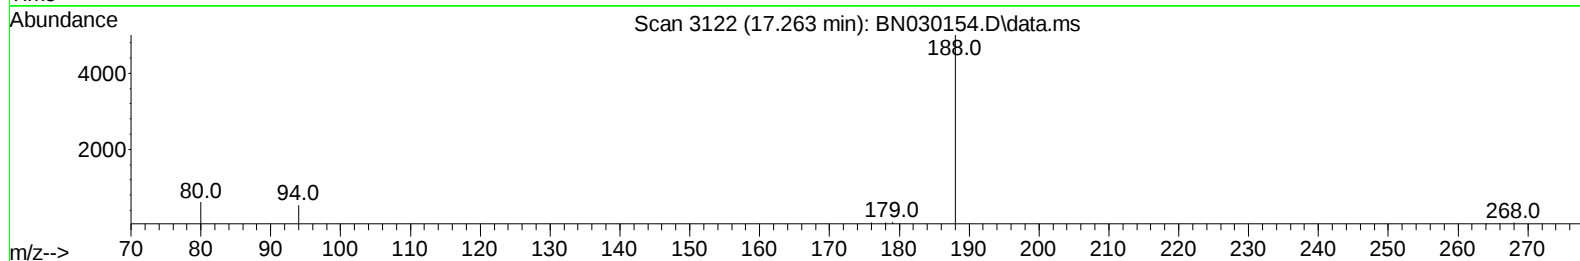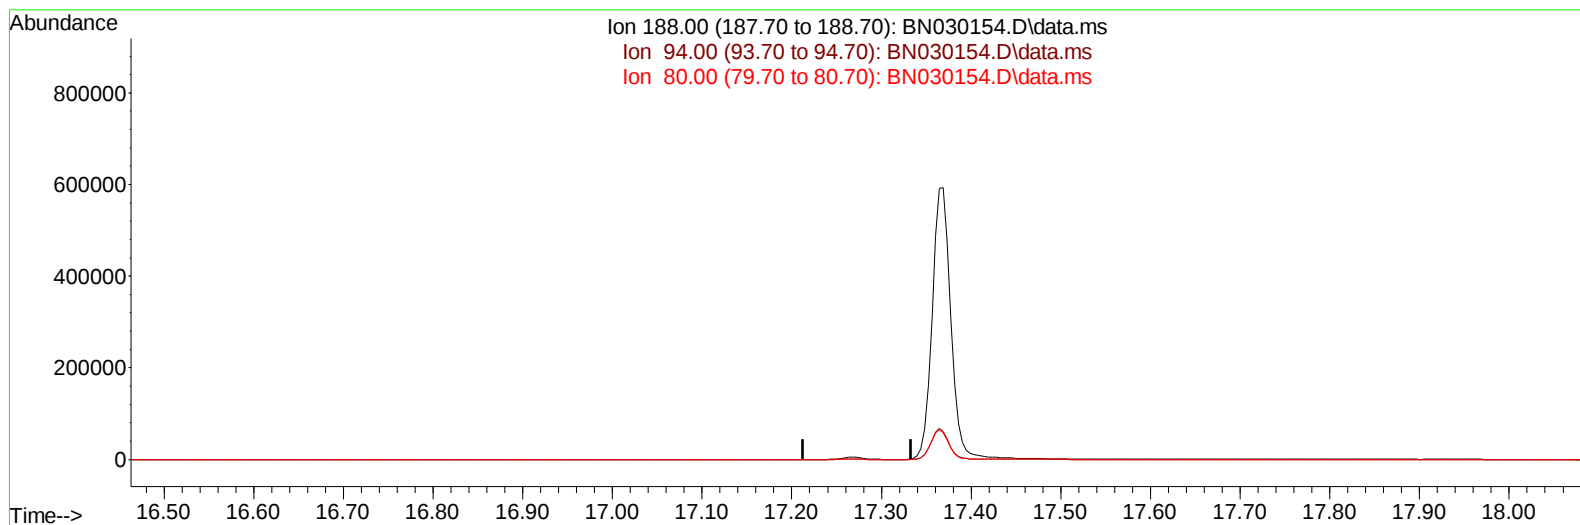

TIC: BN030154.D\data.ms

(13) Phenanthrene-d10 (I)

17.263min (-17.263) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	12.00	0.00#
80.00	13.70	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030154.D
Acq On : 29 Feb 2024 06:27
Operator : MA/JU
Sample : P1494-08
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH410

Manual IntegrationsAPPROVED

Quant Time: Feb 29 06:53:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/29/2024
Supervised By :mohammad ahmed 03/01/2024

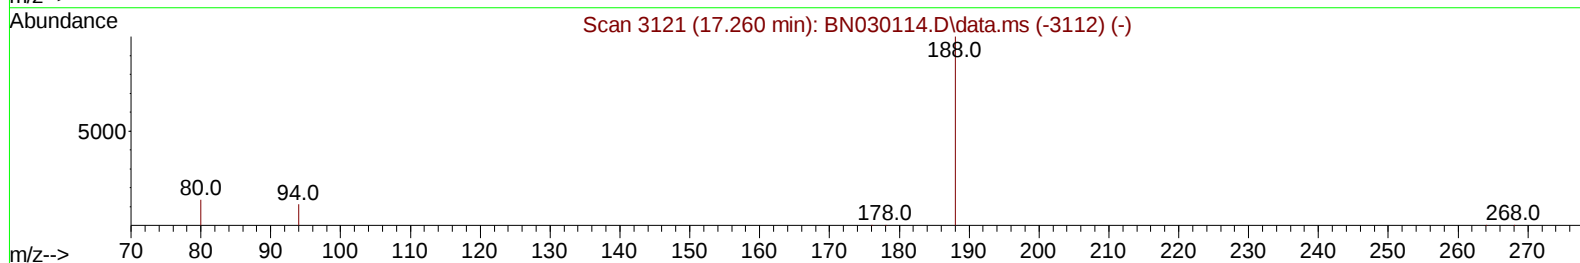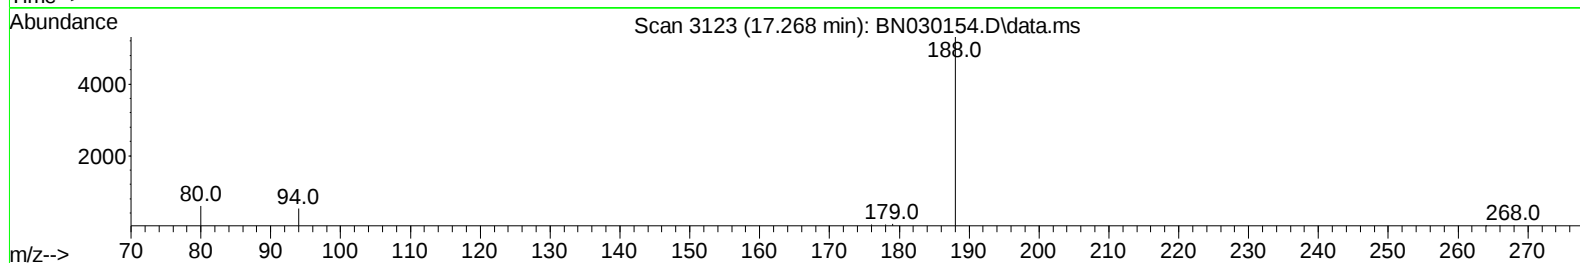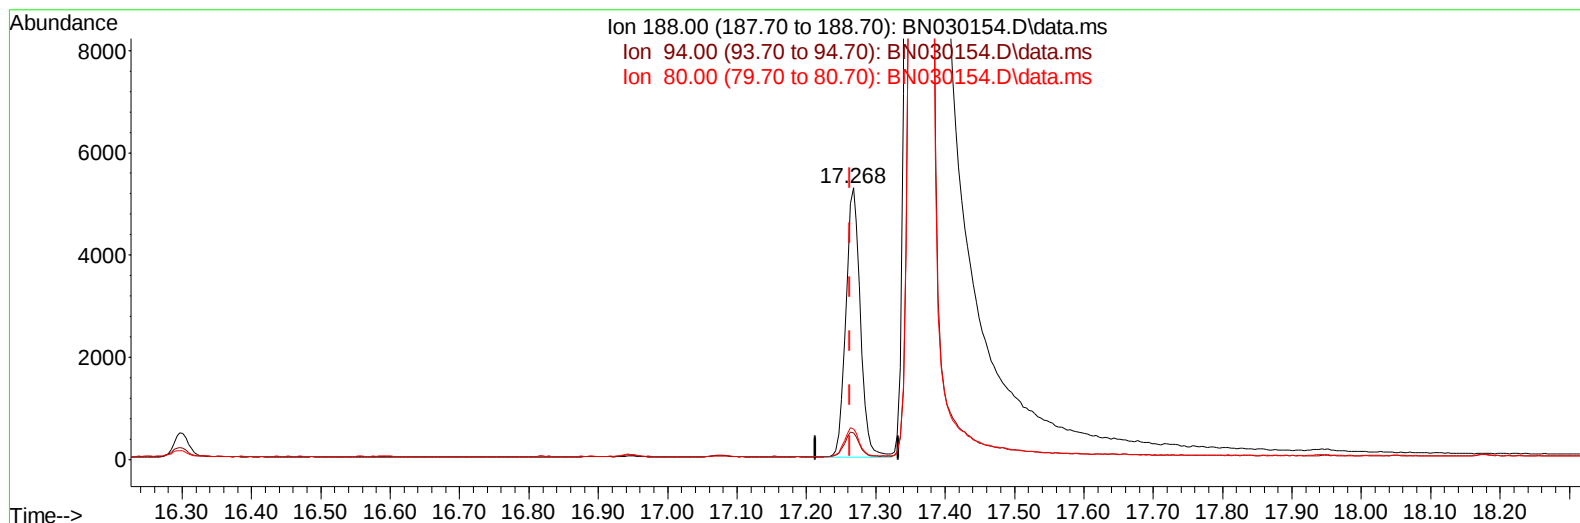

TIC: BN030154.D\data.ms

(13) Phenanthrene-d10 (I)

17.268min (+ 0.005) 0.40 ng/u1 m

response 7683

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.00	9.92
80.00	13.70	11.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
 Data File : BN030154.D
 Acq On : 29 Feb 2024 06:27
 Operator : MA/JU
 Sample : P1494-08
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH410

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/29/2024
 Supervised By :mohammad ahmed 03/01/2024

Quant Time: Feb 29 06:53:49 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 27 23:49:29 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.876	152		2415	0.400	ng/ul	0.02
4) Naphthalene-d8	10.672	136		6796	0.400	ng/ul	0.02
9) Acenaphthene-d10	14.516	164		3714	0.400	ng/ul	# 0.02
13) Phenanthrene-d10	17.268	188		7683m	0.400	ng/ul	0.00
17) Chrysene-d12	21.473	240		5710	0.400	ng/ul	0.00
23) Perylene-d12	23.837	264		7786	0.400	ng/ul	0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.323	96		17543	5.826	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.267	152		4216	0.488	ng/ul	0.02
18) Fluoranthene-d10	19.299	212		9248	0.493	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030154.D
Acq On : 29 Feb 2024 06:27
Operator : MA/JU
Sample : P1494-08
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH410

Manual IntegrationsAPPROVED

Quant Time: Feb 29 06:53:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/29/2024
Supervised By :mohammad ahmed 03/01/2024

