




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030155.D
Acq On : 29 Feb 2024 07:03
Operator : MA/JU
Sample : P1494-09
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH411

Manual IntegrationsAPPROVED

Quant Time: Mar 05 04:03:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 29 14:43:25 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/29/2024
Supervised By :mohammad ahmed 03/01/2024

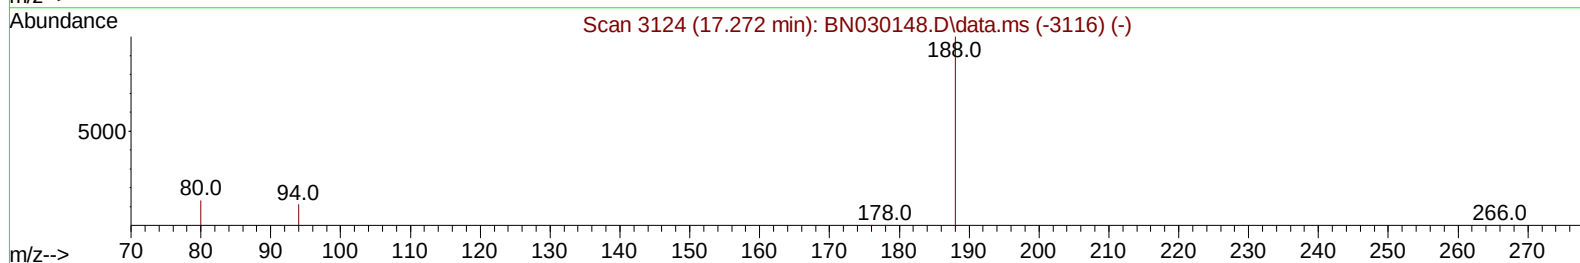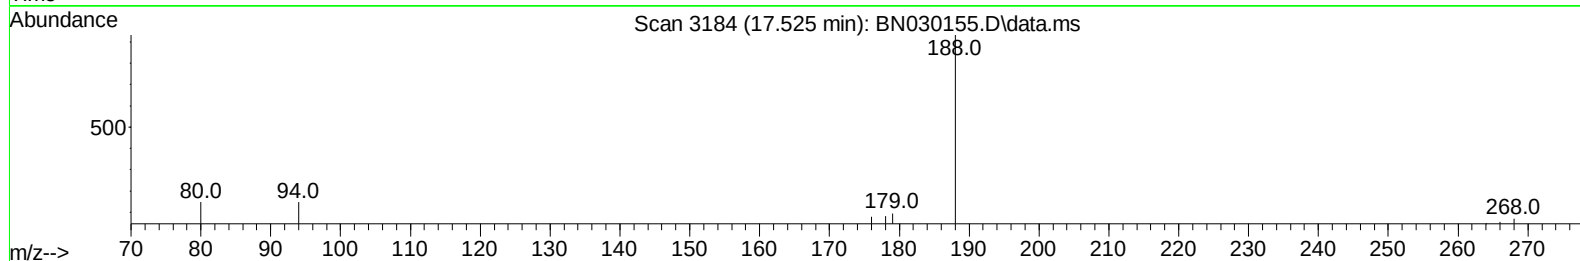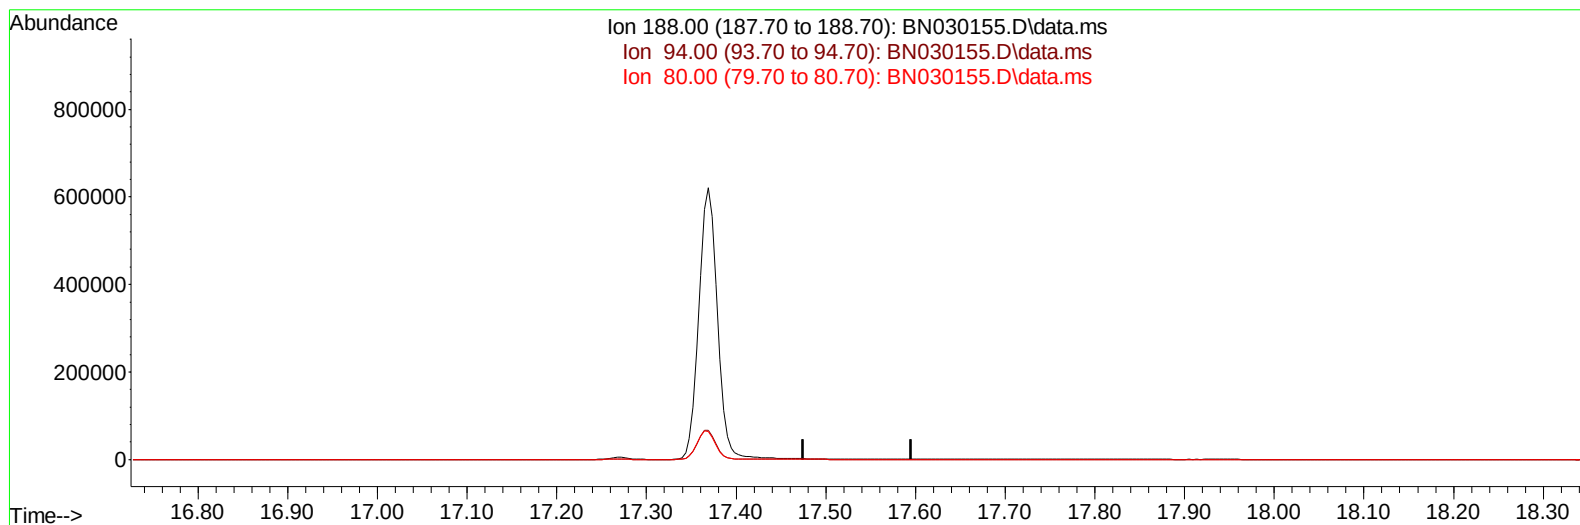

TIC: BN030155.D\data.ms

(13) Phenanthrene-d10 (I)

17.525min (-17.525) 0.00 ng/ul

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	12.00	0.00#
80.00	13.70	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030155.D
Acq On : 29 Feb 2024 07:03
Operator : MA/JU
Sample : P1494-09
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH411

Manual IntegrationsAPPROVED

Quant Time: Feb 29 07:32:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/29/2024
Supervised By :mohammad ahmed 03/01/2024

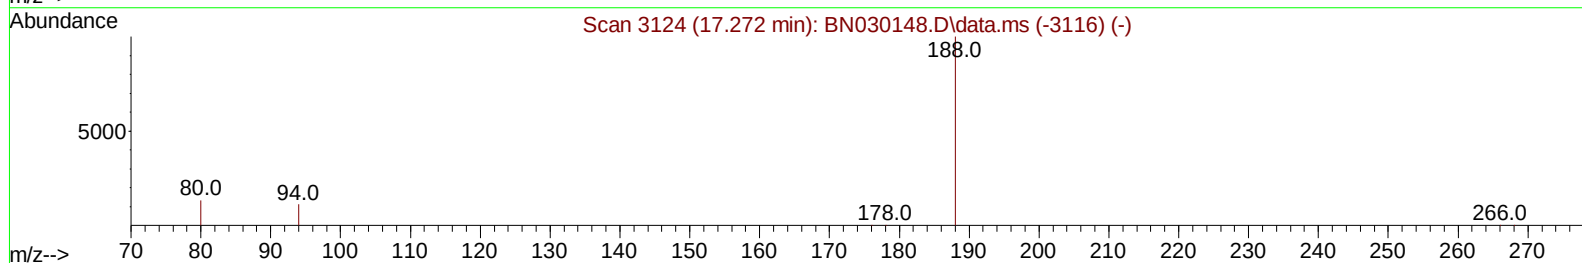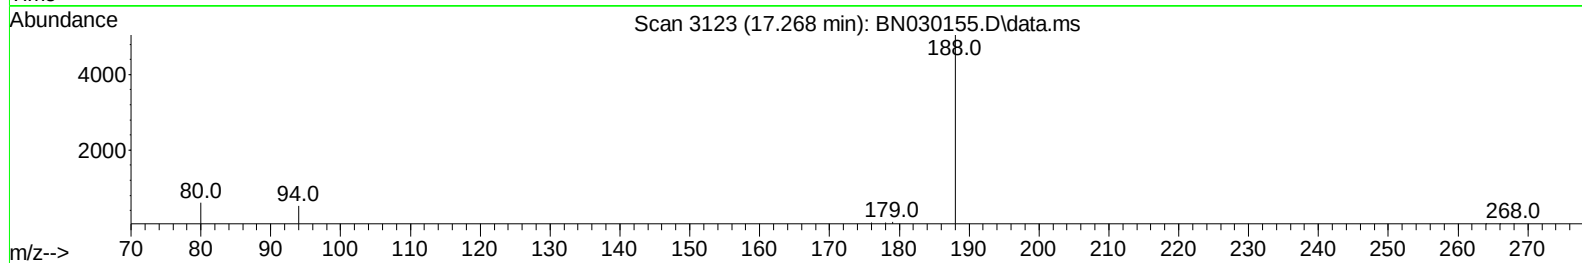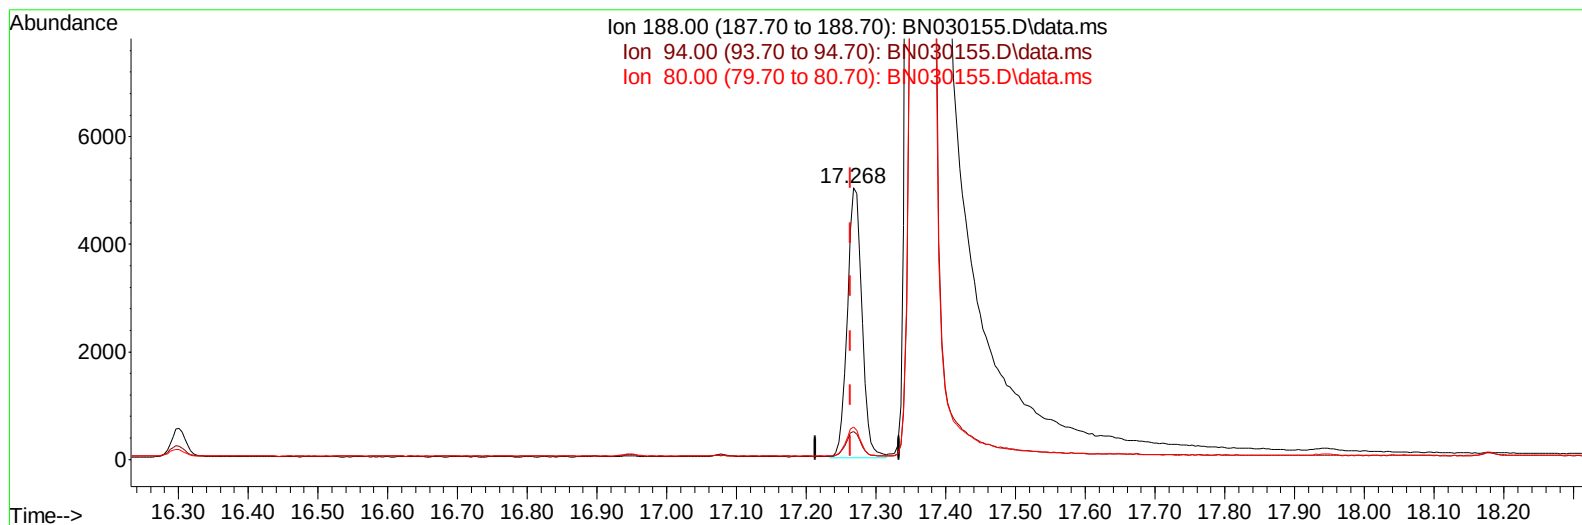

TIC: BN030155.D\data.ms

(13) Phenanthrene-d10 (I)

17.268min (+ 0.004) 0.40 ng/ul m

response 7288

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.00	10.36
80.00	13.70	11.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
 Data File : BN030155.D
 Acq On : 29 Feb 2024 07:03
 Operator : MA/JU
 Sample : P1494-09
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH411

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/29/2024
 Supervised By :mohammad ahmed 03/01/2024

Quant Time: Feb 29 07:32:21 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 27 23:49:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.876	152	2524	0.400	ng/ul	0.02
4) Naphthalene-d8	10.672	136	7257	0.400	ng/ul	0.02
9) Acenaphthene-d10	14.520	164	3720	0.400	ng/ul	# 0.02
13) Phenanthrene-d10	17.268	188	7288m	0.400	ng/ul	0.00
17) Chrysene-d12	21.473	240	5143	0.400	ng/ul	0.00
23) Perylene-d12	23.840	264	6969	0.400	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.323	96	18210	5.786	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.267	152	4905	0.531	ng/ul	0.02
18) Fluoranthene-d10	19.304	212	9295	0.550	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030155.D
Acq On : 29 Feb 2024 07:03
Operator : MA/JU
Sample : P1494-09
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH411

Manual IntegrationsAPPROVED

Quant Time: Feb 29 07:32:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/29/2024
Supervised By :mohammad ahmed 03/01/2024

