




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030156.D
Acq On : 29 Feb 2024 07:39
Operator : MA/JU
Sample : P1494-10
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3W0

Manual IntegrationsAPPROVED

Quant Time: Feb 29 08:07:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/29/2024
Supervised By :mohammad ahmed 03/01/2024

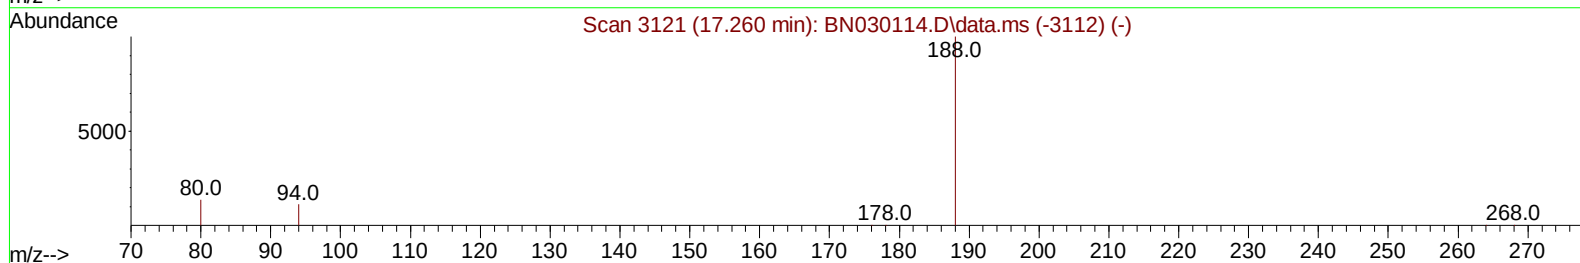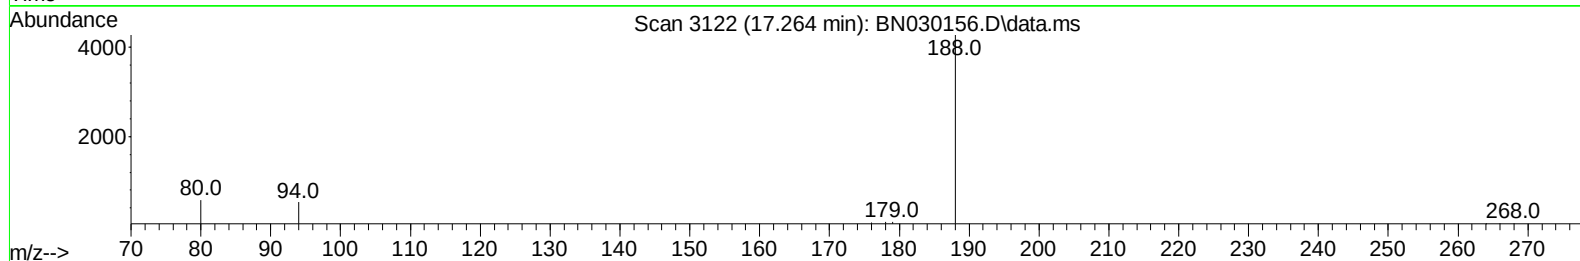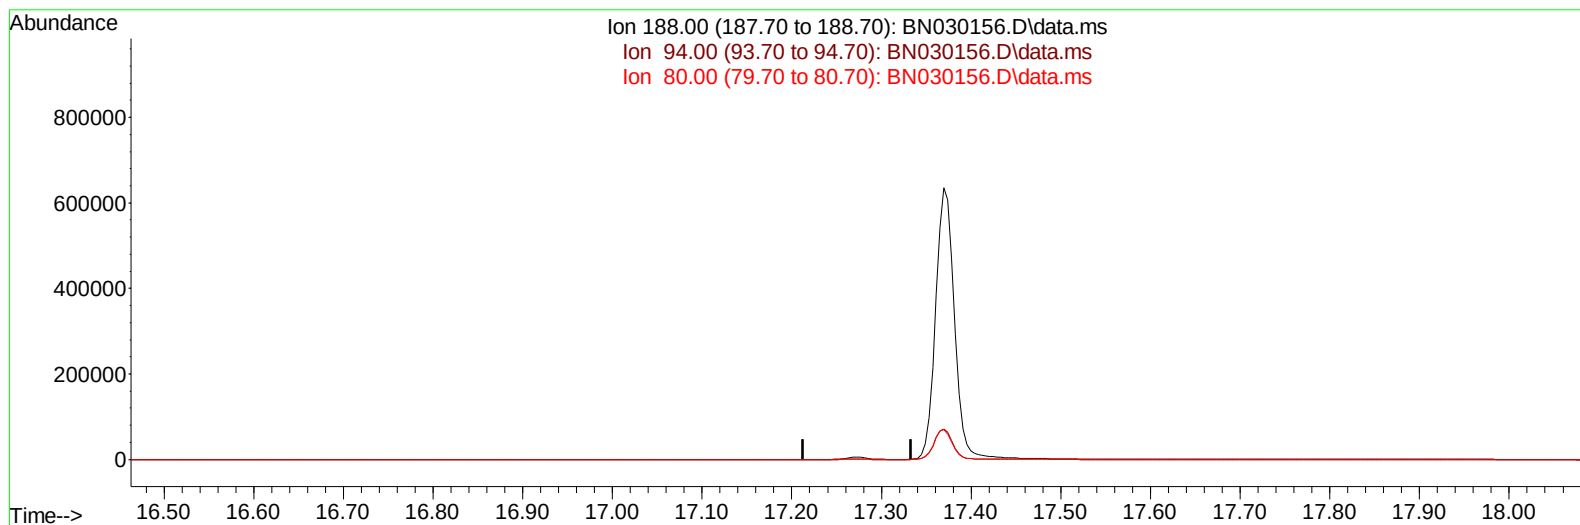

TIC: BN030156.D\data.ms

(13) Phenanthrene-d10 (I)

17.263min (-17.263) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	12.00	0.00#
80.00	13.70	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030156.D
Acq On : 29 Feb 2024 07:39
Operator : MA/JU
Sample : P1494-10
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3W0

Manual IntegrationsAPPROVED

Quant Time: Feb 29 08:07:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/29/2024
Supervised By :mohammad ahmed 03/01/2024

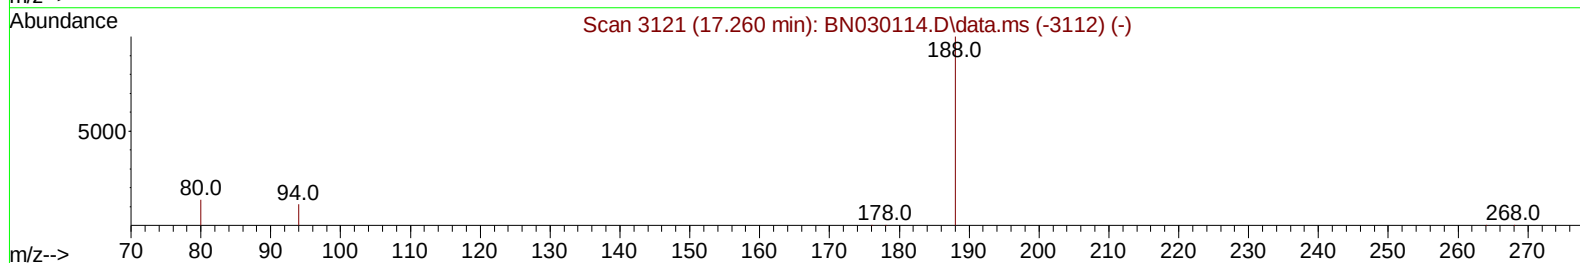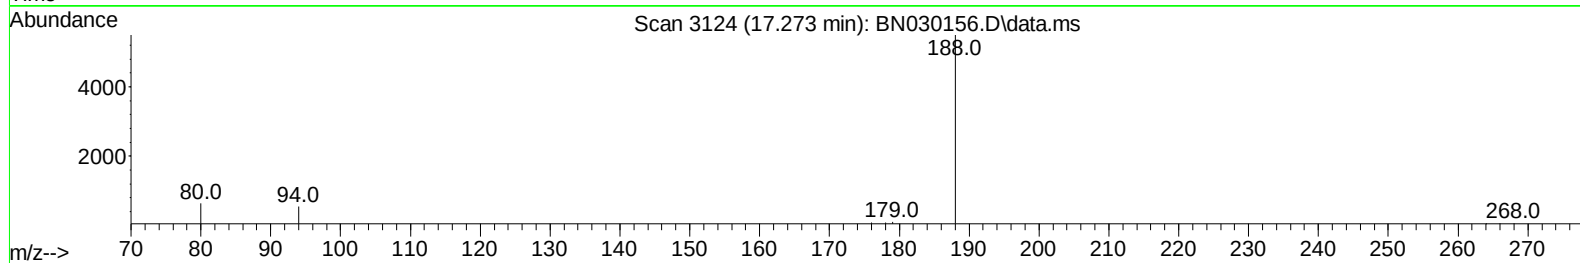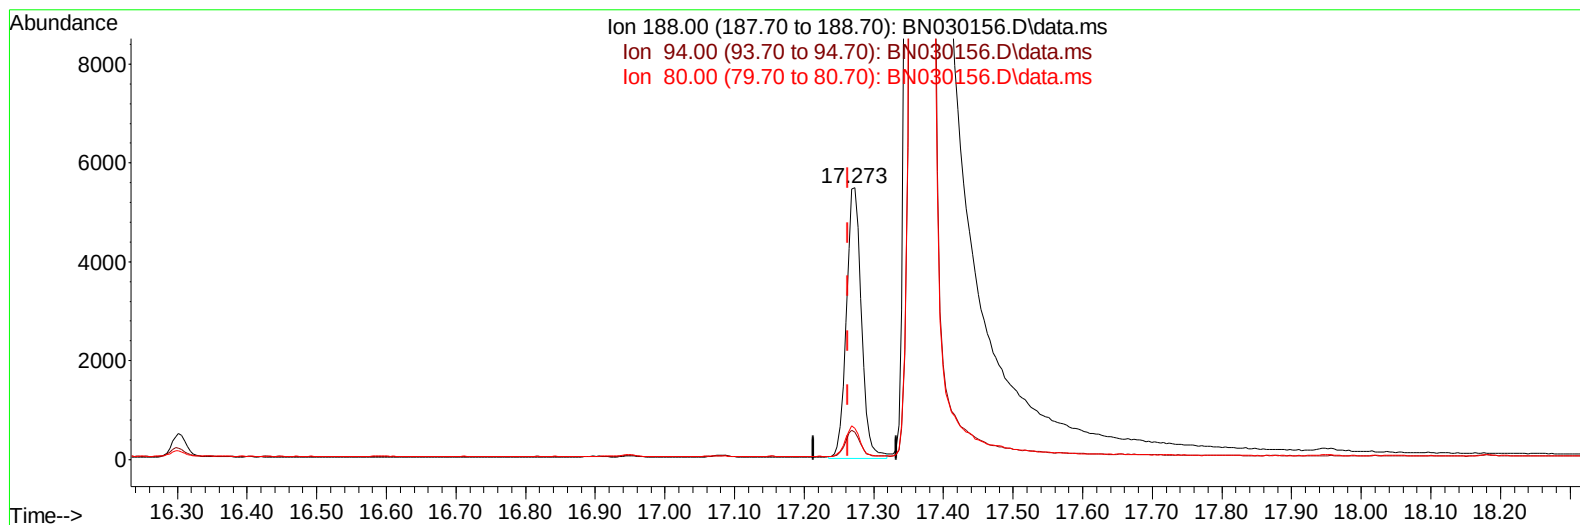

TIC: BN030156.D\data.ms

(13) Phenanthrene-d10 (I)

17.273min (+ 0.009) 0.40 ng/ul m

response 8214

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.00	9.92
80.00	13.70	11.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
 Data File : BN030156.D
 Acq On : 29 Feb 2024 07:39
 Operator : MA/JU
 Sample : P1494-10
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH3W0

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/29/2024
 Supervised By :mohammad ahmed 03/01/2024

Quant Time: Feb 29 08:07:07 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 27 23:49:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.880	152	2524	0.400	ng/ul	0.02
4) Naphthalene-d8	10.672	136	7228	0.400	ng/ul	0.02
9) Acenaphthene-d10	14.521	164	3803	0.400	ng/ul	# 0.02
13) Phenanthrene-d10	17.273	188	8214m	0.400	ng/ul	0.00
17) Chrysene-d12	21.476	240	6035	0.400	ng/ul	0.01
23) Perylene-d12	23.841	264	8577	0.400	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.323	96	14540	4.620	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.272	152	3981	0.433	ng/ul	0.03
18) Fluoranthene-d10	19.305	212	10050	0.507	ng/ul	0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030156.D
Acq On : 29 Feb 2024 07:39
Operator : MA/JU
Sample : P1494-10
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3W0

Manual IntegrationsAPPROVED

Quant Time: Feb 29 08:07:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/29/2024
Supervised By :mohammad ahmed 03/01/2024

