




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030161.D
Acq On : 29 Feb 2024 10:38
Operator : MA/JU
Sample : P1535-01
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AB4

Manual IntegrationsAPPROVED

Quant Time: Feb 29 11:05:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/29/2024
Supervised By :mohammad ahmed 03/01/2024

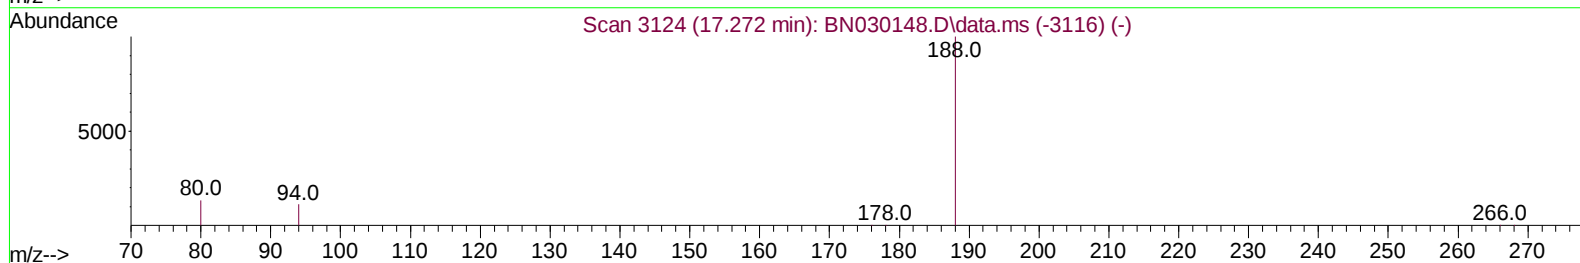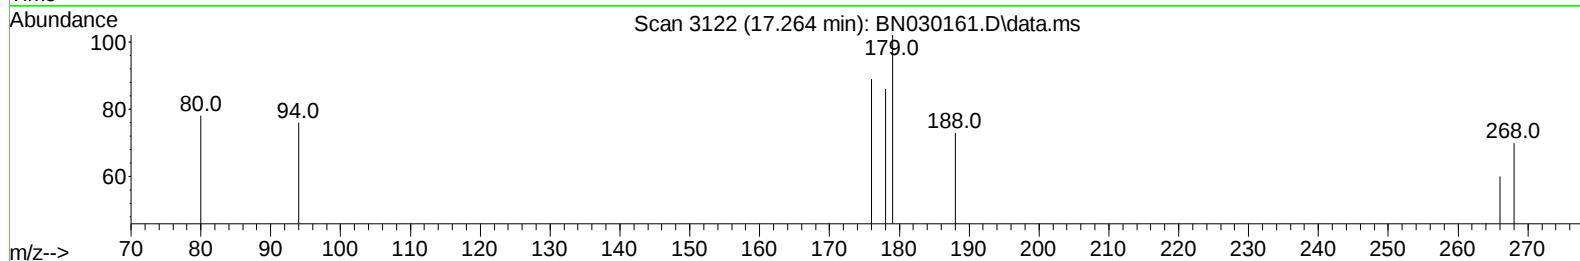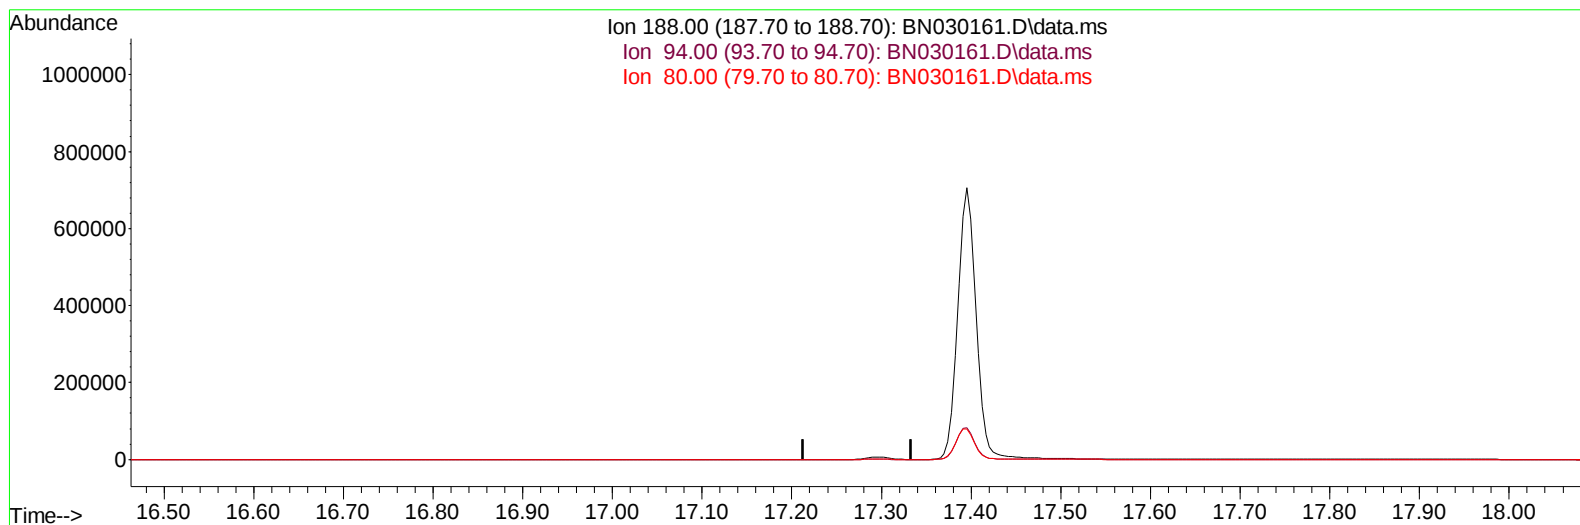

TIC: BN030161.D\data.ms

(13) Phenanthrene-d10 (I)

17.263min (-17.263) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	12.00	0.00#
80.00	13.70	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030161.D
Acq On : 29 Feb 2024 10:38
Operator : MA/JU
Sample : P1535-01
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AB4

Manual IntegrationsAPPROVED

Quant Time: Feb 29 11:05:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/29/2024
Supervised By :mohammad ahmed 03/01/2024

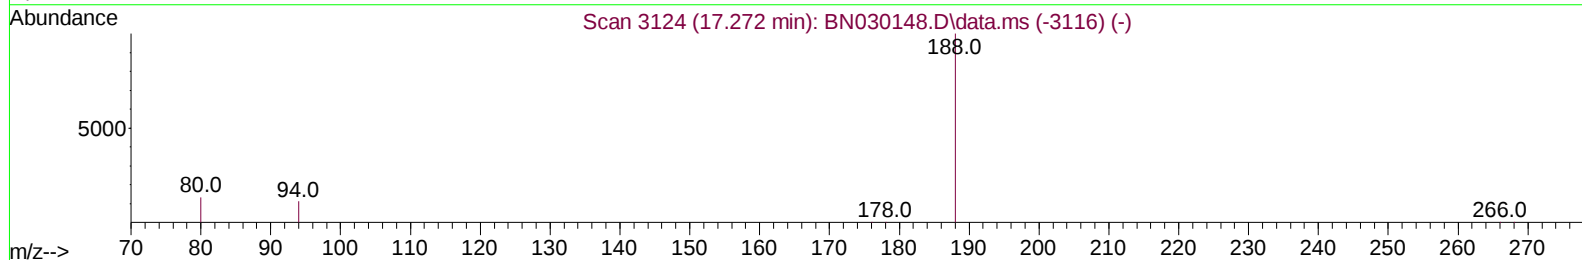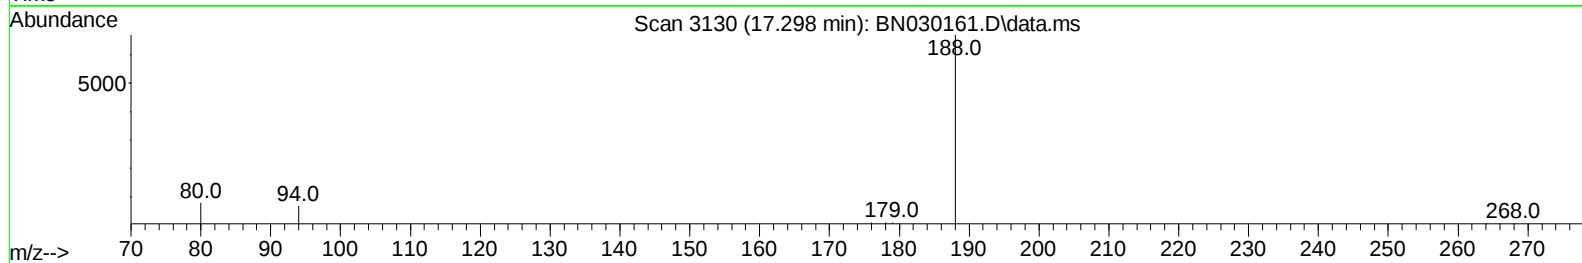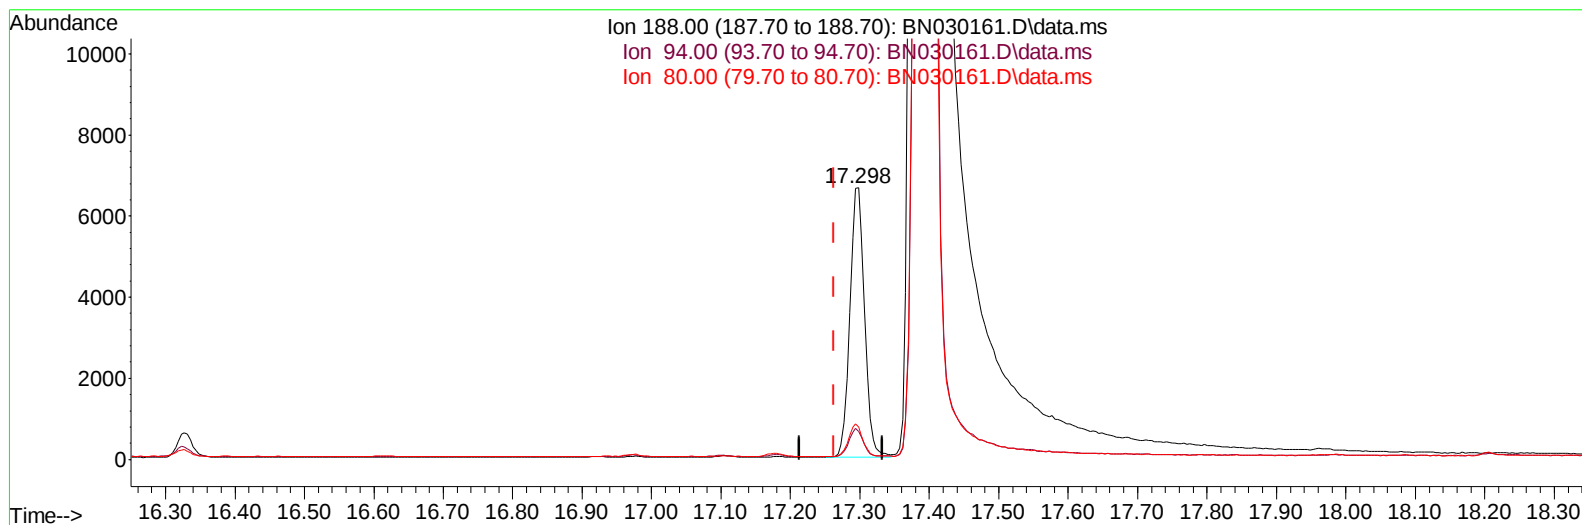

TIC: BN030161.D\data.ms

(13) Phenanthrene-d10 (I)

17.298min (+ 0.035) 0.40 ng/ul m

response 9802

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.00	10.22
80.00	13.70	11.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
 Data File : BN030161.D
 Acq On : 29 Feb 2024 10:38
 Operator : MA/JU
 Sample : P1535-01
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AB4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/29/2024
 Supervised By :mohammad ahmed 03/01/2024

Quant Time: Feb 29 11:05:29 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 27 23:49:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.910	152	2599	0.400	ng/ul	0.05
4) Naphthalene-d8	10.705	136	7344	0.400	ng/ul	0.06
9) Acenaphthene-d10	14.549	164	4829	0.400	ng/ul	# 0.05
13) Phenanthrene-d10	17.298	188	9802m	0.400	ng/ul	0.03
17) Chrysene-d12	21.497	240	8157	0.400	ng/ul	0.03
23) Perylene-d12	23.885	264	8842	0.400	ng/ul	0.06
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.336	96	17118	5.282	ng/ul	0.02
6) 2-Methylnaphthalene-d10	12.306	152	4393	0.470	ng/ul	0.06
18) Fluoranthene-d10	19.328	212	12175	0.454	ng/ul	0.03

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030161.D
Acq On : 29 Feb 2024 10:38
Operator : MA/JU
Sample : P1535-01
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AB4

Manual IntegrationsAPPROVED

Quant Time: Feb 29 11:05:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/29/2024
Supervised By :mohammad ahmed 03/01/2024

